

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
 Data File : BN015723.D
 Acq On : 30 Jul 2021 18:06
 Operator : CG/JU
 Sample : SSTDICC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Quant Time: Jul 30 18:44:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 18:43:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	35194	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	158260	0.400	ng	0.00
13) Acenaphthene-d10	14.421	164	85393	0.400	ng	0.00
19) Phenanthrene-d10	17.163	188	157616	0.400	ng	0.00
29) Chrysene-d12	21.376	240	146110	0.400	ng	0.00
35) Perylene-d12	23.720	264	146636	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	36841	0.389	ng	0.00
5) Phenol-d6	6.951	99	44138	0.369	ng	0.00
8) Nitrobenzene-d5	8.936	82	33943	0.320	ng	0.00
11) 2-Methylnaphthalene-d10	12.167	152	92506	0.372	ng	0.00
14) 2,4,6-Tribromophenol	15.918	330	11955	0.345	ng	0.00
15) 2-Fluorobiphenyl	13.051	172	118983	0.366	ng	0.00
27) Fluoranthene-d10	19.212	212	153605	0.345	ng	0.00
31) Terphenyl-d14	19.817	244	129324	0.348	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.355	88	5898	0.479	ng	100
3) n-Nitrosodimethylamine	3.714	42	8208	0.340	ng	100
6) bis(2-Chloroethyl)ether	7.218	93	37467	0.399	ng	100
9) Naphthalene	10.622	128	159976	0.389	ng	100
10) Hexachlorobutadiene	10.913	225	28049	0.353	ng	# 100
12) 2-Methylnaphthalene	12.238	142	104498	0.376	ng	100
16) Acenaphthylene	14.142	152	135475	0.349	ng	100
17) Acenaphthene	14.484	154	90167	0.373	ng	100
18) Fluorene	15.474	166	109529	0.361	ng	100
20) 4,6-Dinitro-2-methylph...	15.550	198	3342	0.285	ng	100
21) 4-Bromophenyl-phenylether	16.372	248	33846	0.361	ng	100
22) Hexachlorobenzene	16.482	284	38029	0.416	ng	100
23) Atrazine	16.640	200	23938	0.284	ng	100
24) Pentachlorophenol	16.823	266	11993	0.358	ng	100
25) Phenanthrene	17.212	178	167591	0.386	ng	100
26) Anthracene	17.297	178	147741	0.351	ng	100
28) Fluoranthene	19.241	202	181364	0.365	ng	100
30) Pyrene	19.604	202	181217	0.363	ng	100
32) Benzo(a)anthracene	21.355	228	170837	0.344	ng	100
33) Chrysene	21.408	228	176493	0.375	ng	100
34) Bis(2-ethylhexyl)phtha...	21.312	149	75026	0.264	ng	99
36) Indeno(1,2,3-cd)pyrene	26.127	276	194933	0.364	ng	100
37) Benzo(b)fluoranthene	23.012	252	178835	0.360	ng	100
38) Benzo(k)fluoranthene	23.056	252	190216	0.388	ng	100
39) Benzo(a)pyrene	23.618	252	159792	0.356	ng	100
40) Dibenzo(a,h)anthracene	26.147	278	165444	0.367	ng	100
41) Benzo(g,h,i)perylene	26.859	276	169424	0.373	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
 Data File : BN015723.D
 Acq On : 30 Jul 2021 18:06
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jul 30 18:44:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 18:43:48 2021
 Response via : Initial Calibration




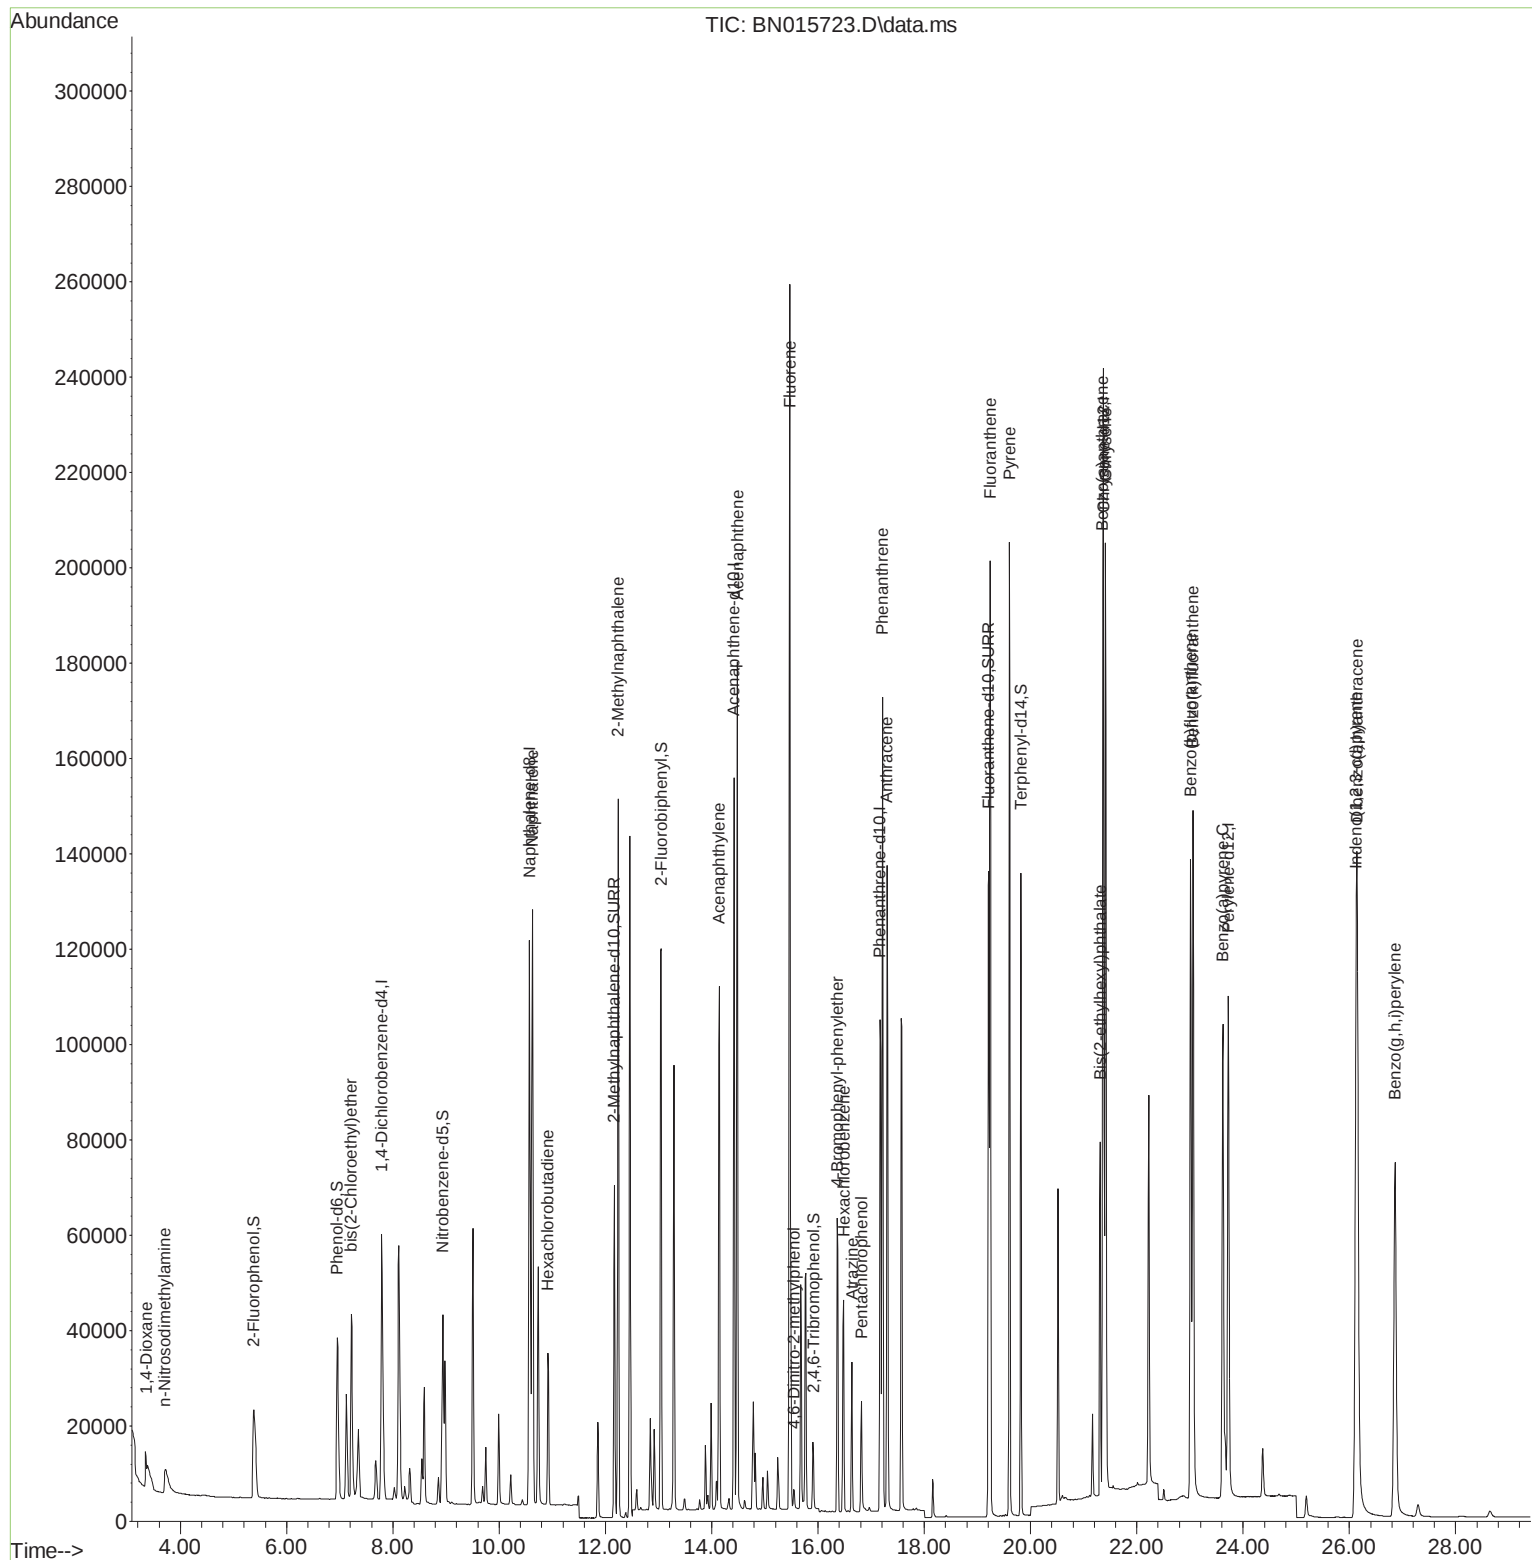


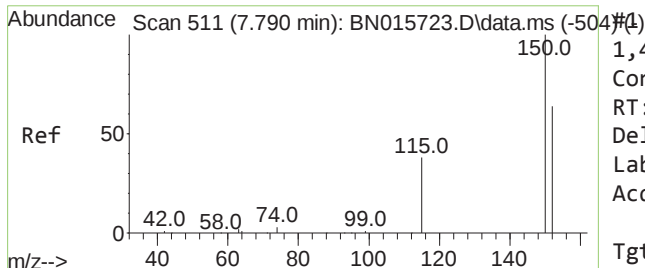

1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.790 min Scan# 511
 Delta R.T. -0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:152 Resp: 35194
 Ion Ratio Lower Upper
 152 100
 150 154.9 123.9 185.9
 115 59.7 47.8 71.6

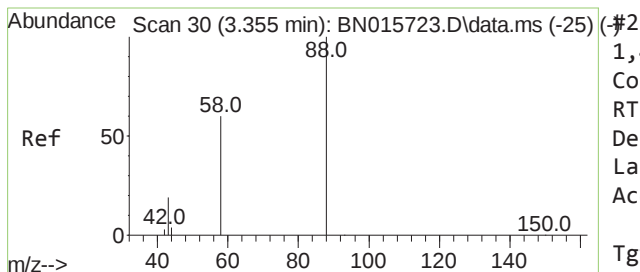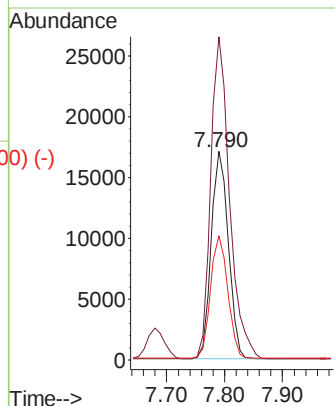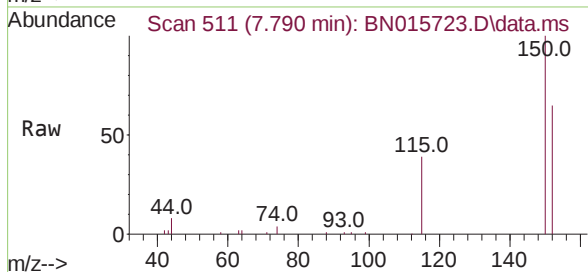

1,4-Dioxane
 Concen: 0.479 ng
 RT: 3.355 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06

Tgt Ion: 88 Resp: 5898
 Ion Ratio Lower Upper
 88 100
 43 21.5 17.2 25.8
 58 77.7 62.2 93.2



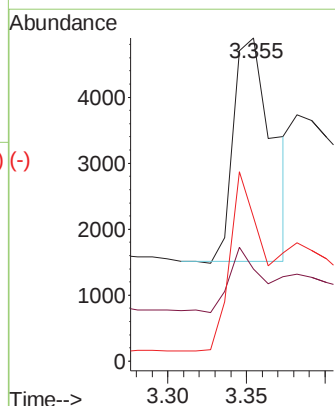



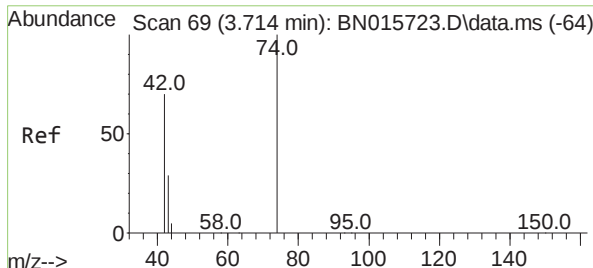

n-Nitrosodimethylamine
 Concen: 0.340 ng
 RT: 3.714 min Scan# 69
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:	42	Resp:	8208
Ion	Ratio	Lower	Upper
42	100		
74	145.2	116.6	174.8
44	8.4	6.6	10.0

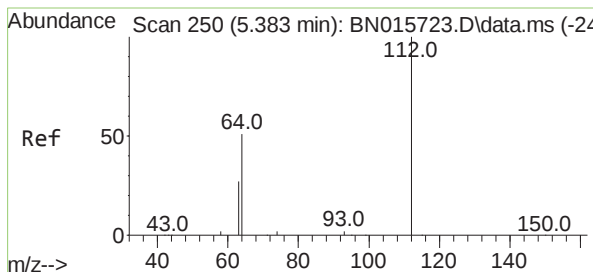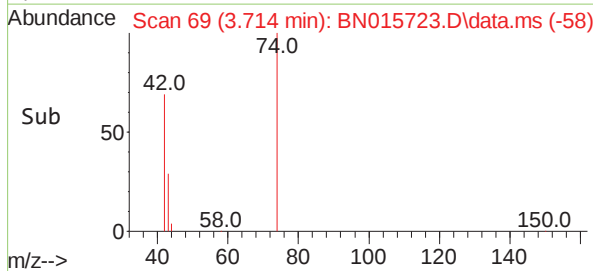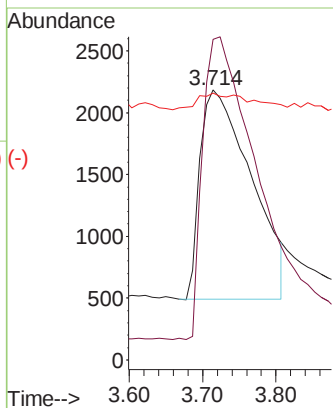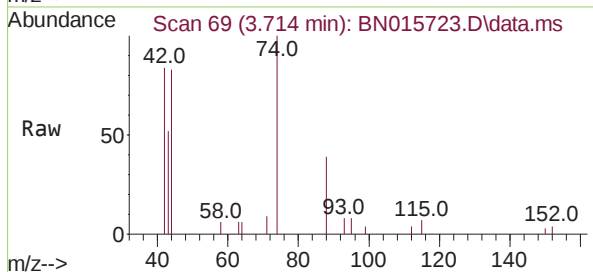

2-Fluorophenol
 Concen: 0.389 ng
 RT: 5.383 min Scan# 250
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06

Tgt Ion:	112	Resp:	36841
Ion	Ratio	Lower	Upper
112	100		
64	52.6	42.1	63.1
63	27.4	21.9	32.9


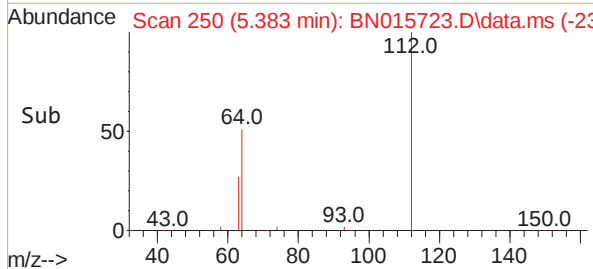

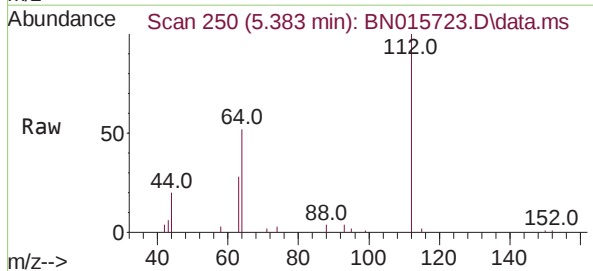


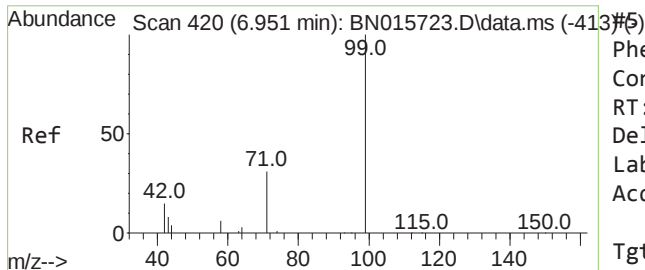

Phenol-d6
 Concen: 0.369 ng
 RT: 6.951 min Scan# 420
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	99	Resp:	44138
Ion	Ratio	Lower	Upper
99	100		
42	16.1	12.9	19.3
71	29.7	23.8	35.6

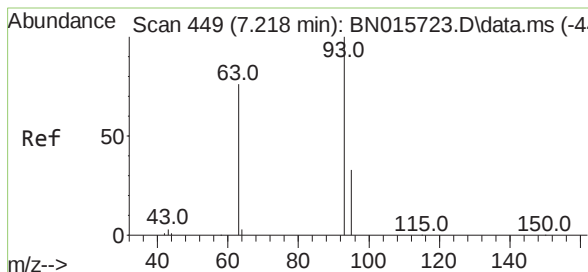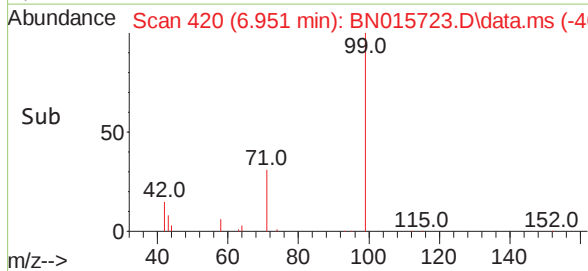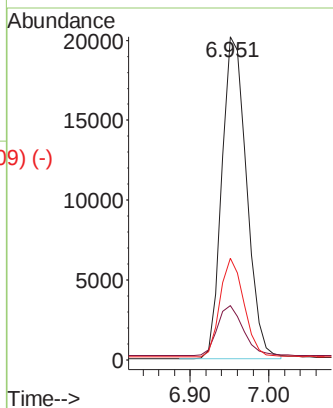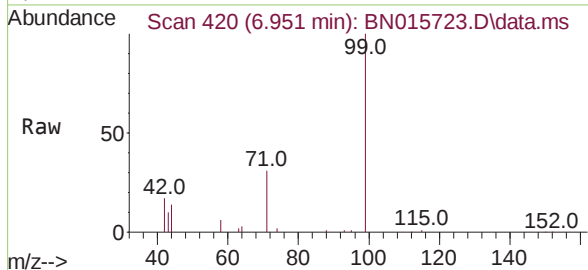


bis(2-Chloroethyl)ether
 Concen: 0.399 ng
 RT: 7.218 min Scan# 449
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06

Tgt Ion:	93	Resp:	37467
Ion	Ratio	Lower	Upper
93	100		
63	73.3	58.6	87.8
95	33.6	26.9	40.3

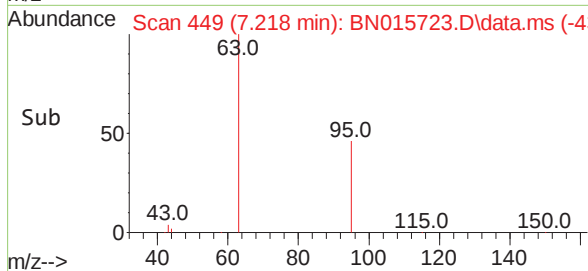



Abundance Scan 746 (10.571 min): BN015723.D\data.ms (-730) (-)

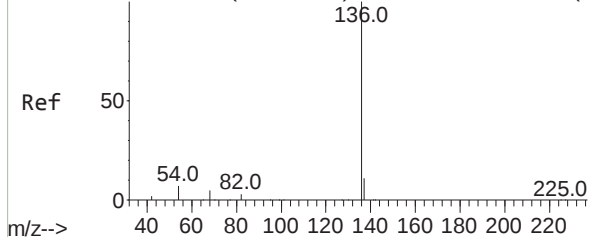


Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	158260
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	6.9	5.5	8.3
68	5.6	4.5	6.7

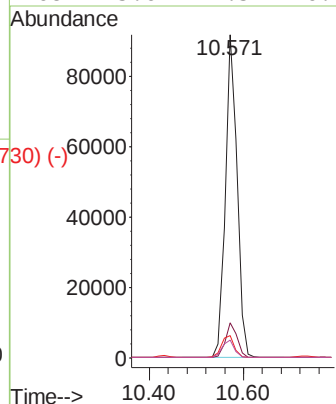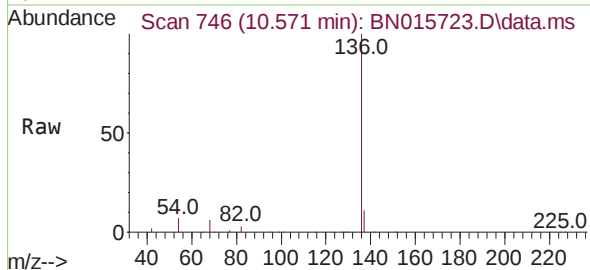

Abundance Scan 746 (10.571 min): BN015723.D\data.ms (-730) (-)


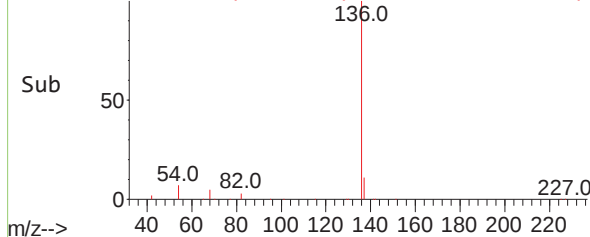


Abundance Scan 617 (8.936 min): BN015723.D\data.ms (-614) (-)

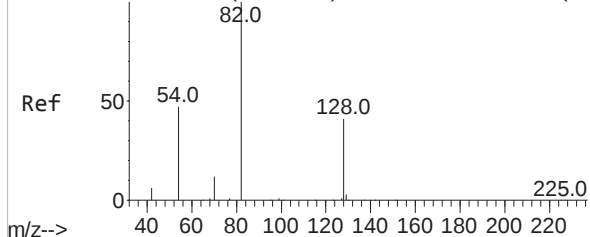



Nitrobenzene-d5
Concen: 0.320 ng
RT: 8.936 min Scan# 617
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	82	Resp:	33943
Ion	Ratio	Lower	Upper
82	100		
128	41.5	33.2	49.8
54	48.0	38.4	57.6

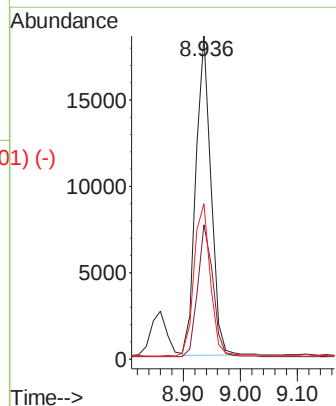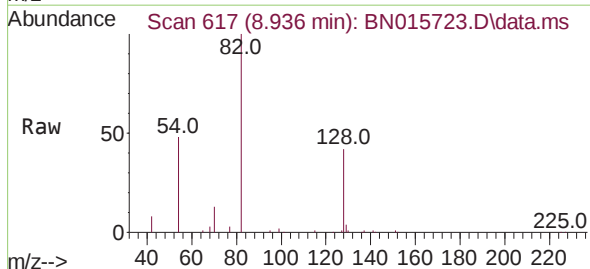

Abundance Scan 617 (8.936 min): BN015723.D\data.ms (-601) (-)




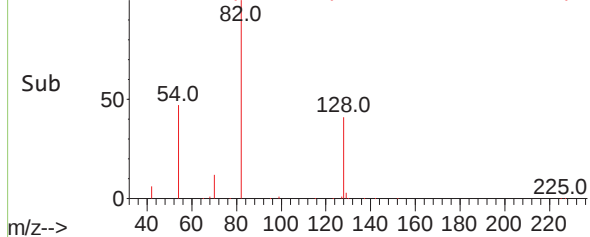


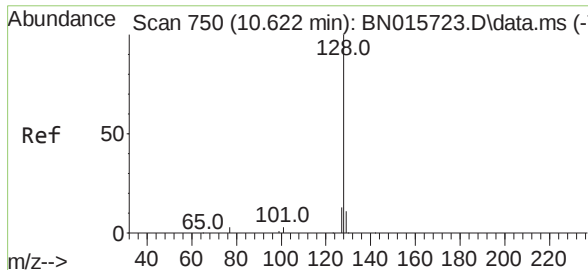

Naphthalene
 Concen: 0.389 ng
 RT: 10.622 min Scan# 750
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	128	Resp:	159976
Ion	Ratio	Lower	Upper
128	100		
129	11.1	8.9	13.3
127	13.0	10.4	15.6

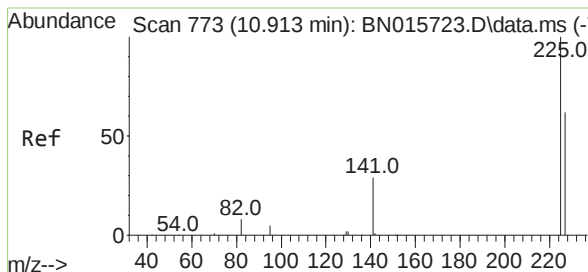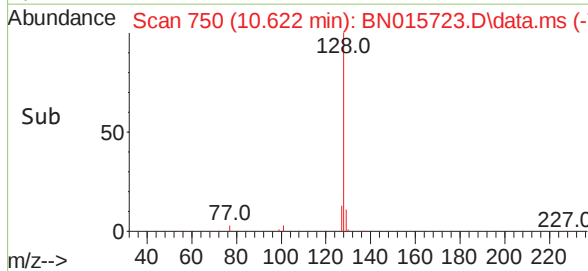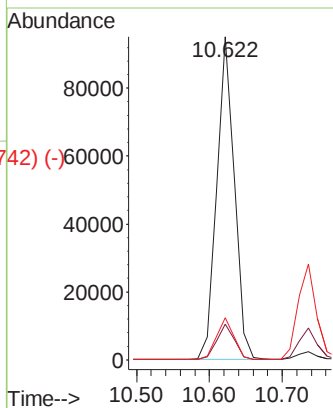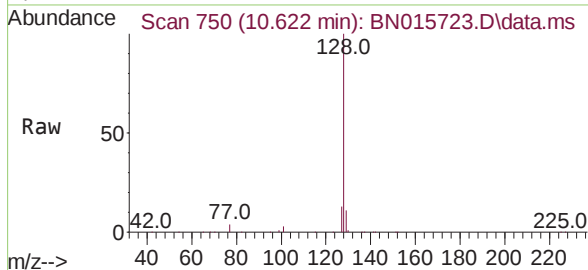


Hexachlorobutadiene
 Concen: 0.353 ng
 RT: 10.913 min Scan# 773
 Delta R.T. 0.000 min
 Lab File: BN015723.D
 Acq: 30 Jul 2021 18:06

Tgt Ion:	225	Resp:	28049
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.7	51.0	76.4

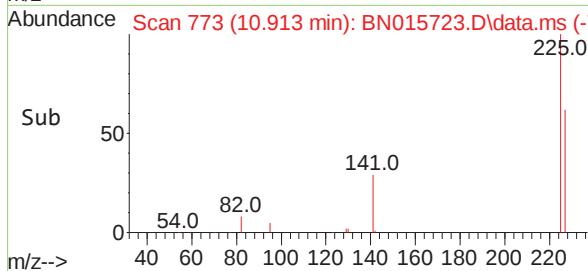



Abundance Scan 968 (12.167 min): BN015723.D\data.ms (-955) #14

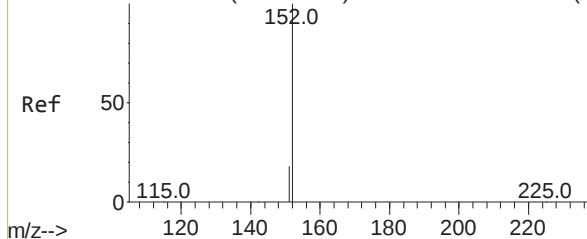


2-Methylnaphthalene-d10
Concen: 0.372 ng
RT: 12.167 min Scan# 968
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 92506
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

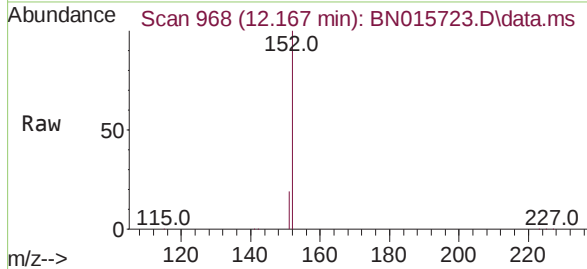

Abundance Scan 968 (12.167 min): BN015723.D\data.ms (-923) (-)


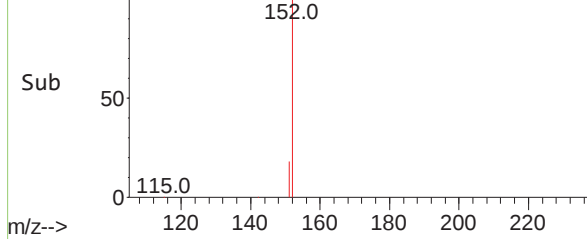


Abundance Scan 984 (12.238 min): BN015723.D\data.ms (-975) #12

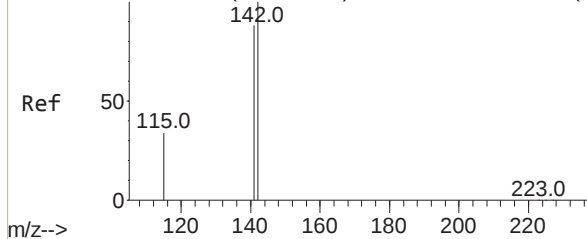


2-Methylnaphthalene
Concen: 0.376 ng
RT: 12.238 min Scan# 984
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:142 Resp: 104498
Ion Ratio Lower Upper
142 100
141 88.1 70.5 105.7
115 34.1 27.3 40.9

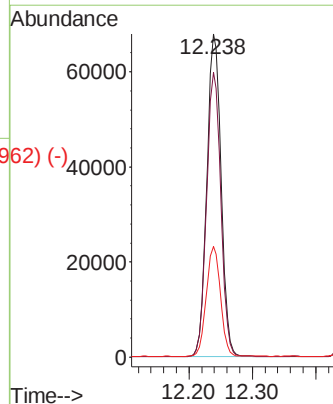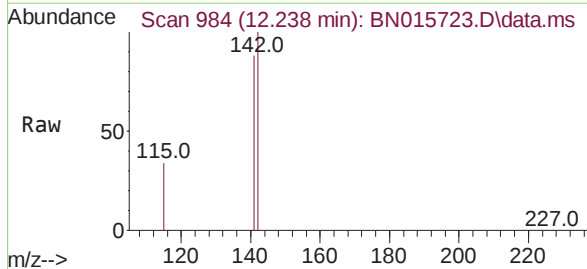


Abundance Scan 984 (12.238 min): BN015723.D\data.ms (-962) (-)

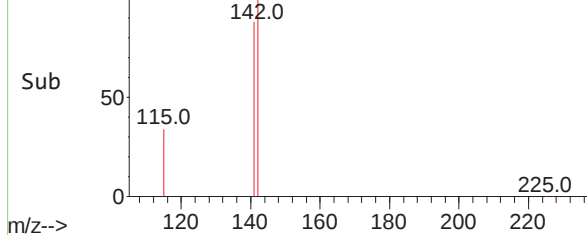




Abundance Scan 1195 (14.421 min): BN015723.D\data.ms (-1195) (-)

Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

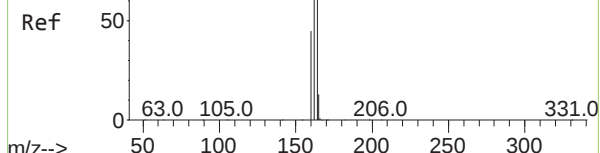





Tgt Ion:	164	Resp:	85393
Ion	Ratio	Lower	Upper
164	100		
162	99.7	79.8	119.6
160	44.7	35.8	53.6

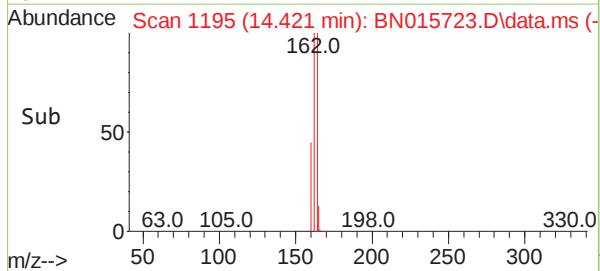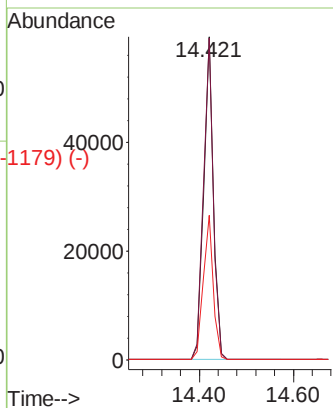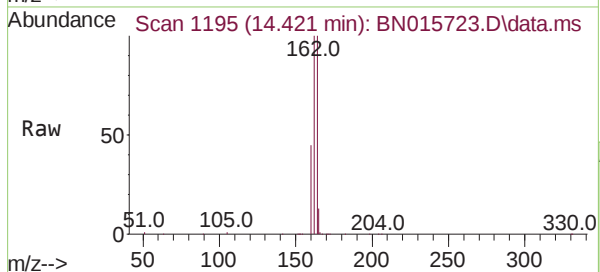


Abundance Scan 1313 (15.918 min): BN015723.D\data.ms (-1313) (-)

2,4,6-Tribromophenol
Concen: 0.345 ng
RT: 15.918 min Scan# 1313
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	330	Resp:	11955
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	36.0	28.8	43.2

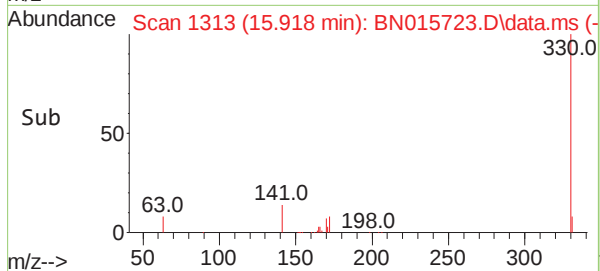
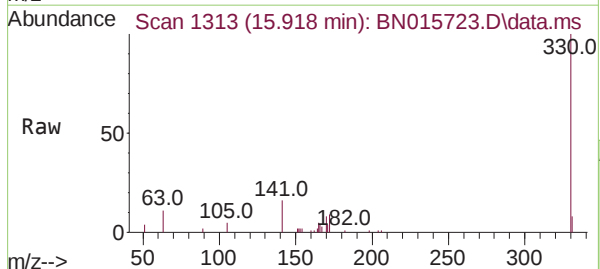

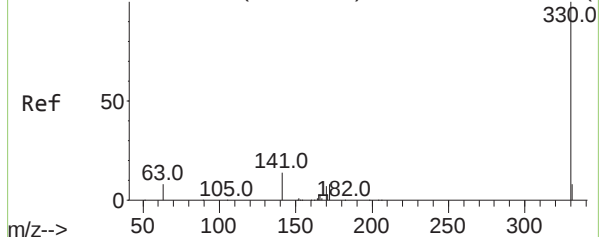


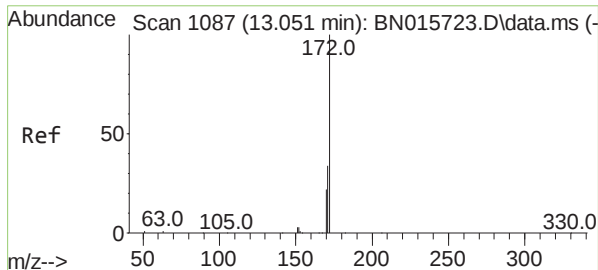

2-Fluorobiphenyl
Concen: 0.366 ng
RT: 13.051 min Scan# 1087
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	172	Resp:	118983
Ion	Ratio	Lower	Upper
172	100		
171	33.6	26.9	40.3
170	21.7	17.4	26.0

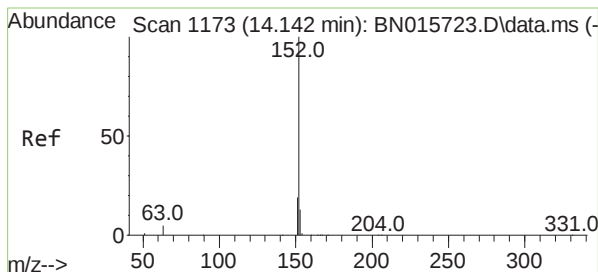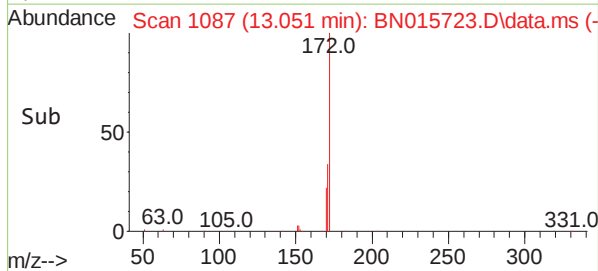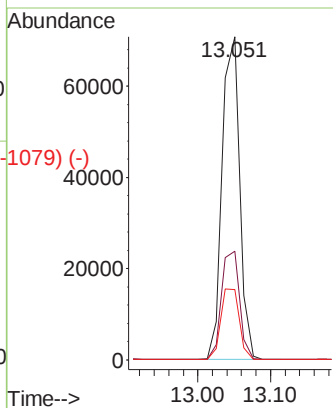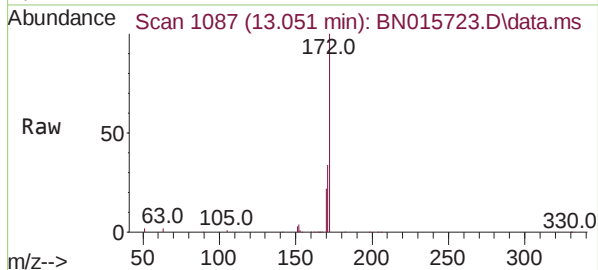


Acenaphthylene
Concen: 0.349 ng
RT: 14.142 min Scan# 1173
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	152	Resp:	135475
Ion	Ratio	Lower	Upper
152	100		
151	19.6	15.7	23.5
153	13.0	10.4	15.6

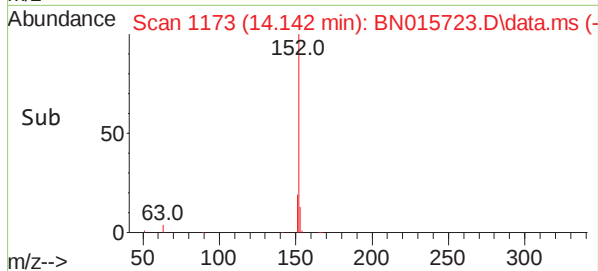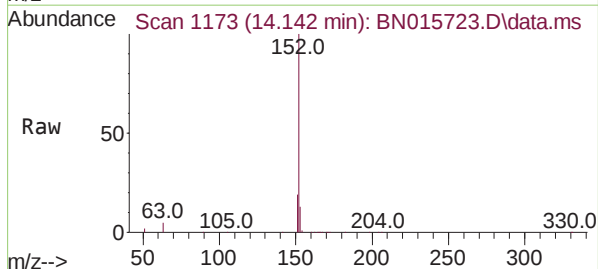




Abundance Scan 1200 (14.484 min): BN015723.D\data.ms (-1197) (-)

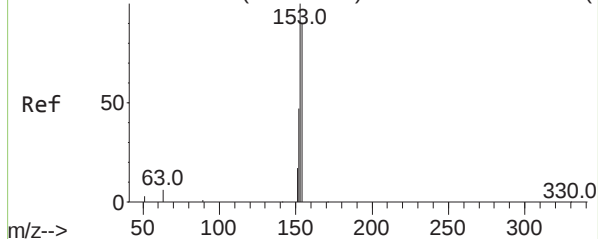


Acenaphthene
Concen: 0.373 ng
RT: 14.484 min Scan# 1200
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:154 Resp: 90167
Ion Ratio Lower Upper
154 100
153 112.1 89.7 134.5
152 54.7 43.8 65.6

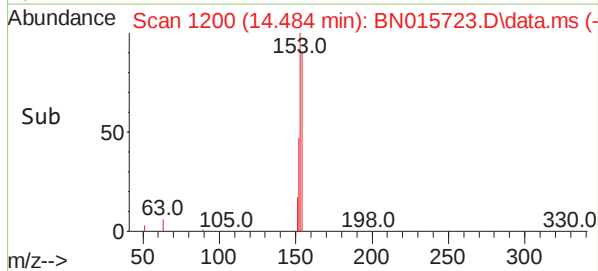
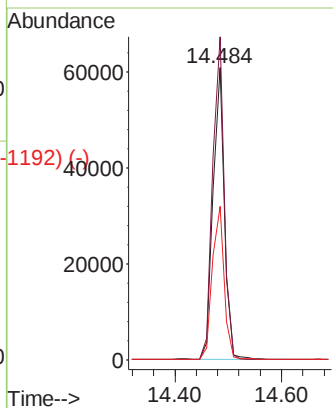
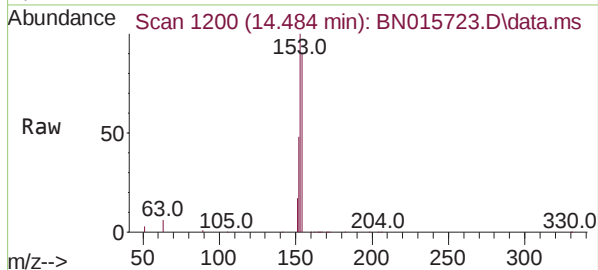


Abundance Scan 1278 (15.474 min): BN015723.D\data.ms (-1213) (-)

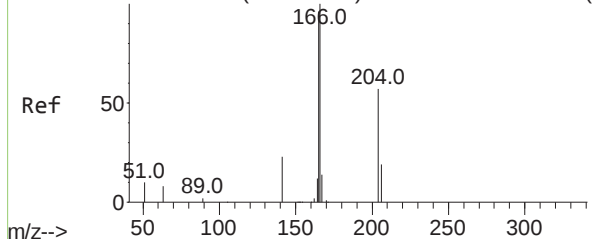

Fluorene
Concen: 0.361 ng
RT: 15.474 min Scan# 1278
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06


Tgt Ion:166 Resp: 109529
Ion Ratio Lower Upper
166 100
165 97.6 78.1 117.1
167 13.5 10.8 16.2

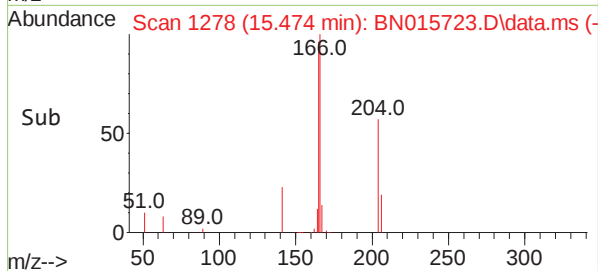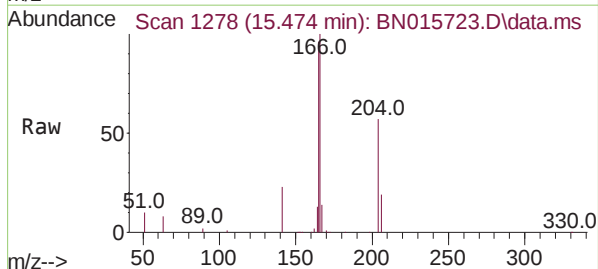



Abundance Scan 1415 (17.163 min): BN015723.D\data.ms (-1419) (-)

Phenanthrene-d10
Concen: 0.400 ng
RT: 17.163 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

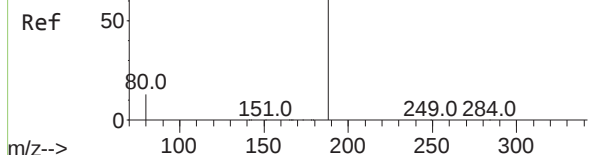

Tgt Ion:	188	Resp:	157616
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.8	10.2	15.4

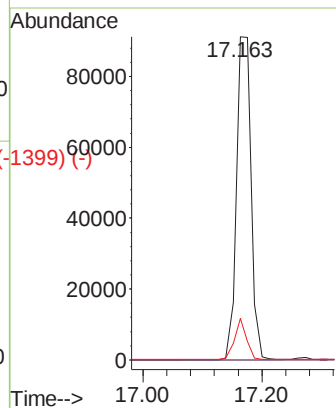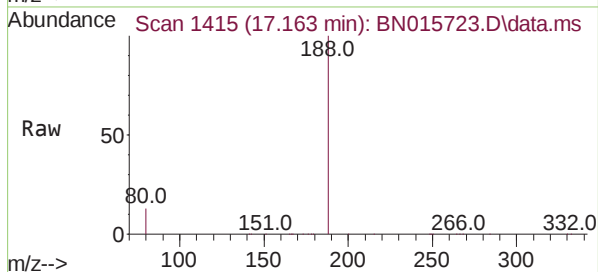



Abundance Scan 1415 (17.163 min): BN015723.D\data.ms (-1399) (-)

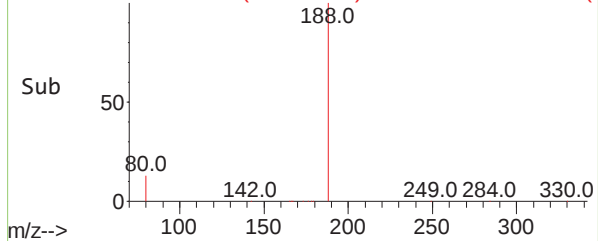


Abundance Scan 1284 (15.550 min): BN015723.D\data.ms (-1278) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.285 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06


Tgt Ion:	198	Resp:	3342
Ion	Ratio	Lower	Upper
198	100		
182	11.7	9.4	14.0
77	0.0	0.0	0.0

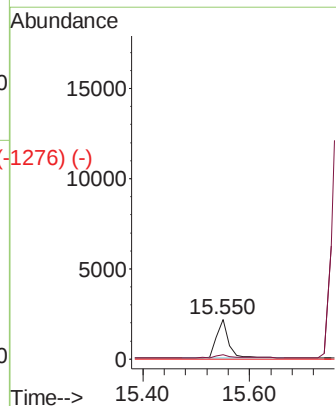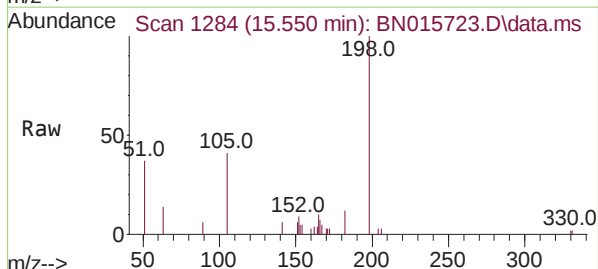

Abundance Scan 1284 (15.550 min): BN015723.D\data.ms (-1276) (-)

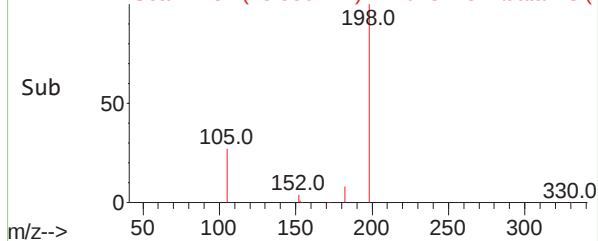



Abundance Scan 1350 (16.372 min): BN015723.D\data.ms (-1342) (-)

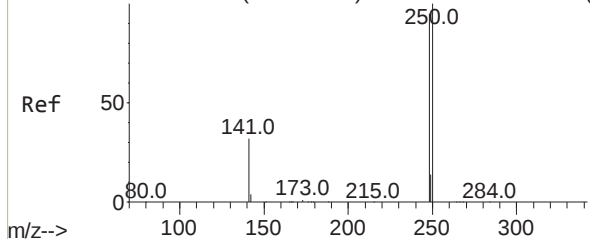


4-Bromophenyl-phenylether
Concen: 0.361 ng
RT: 16.372 min Scan# 1350
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	248	Resp:	33846
Ion	Ratio	Lower	Upper
248	100		
250	104.9	83.9	125.9
141	33.6	26.9	40.3

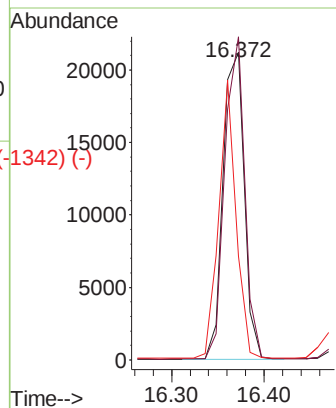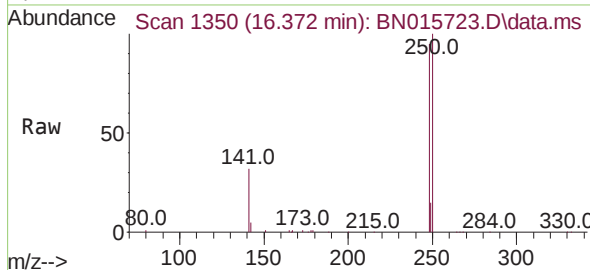

Abundance Scan 1350 (16.372 min): BN015723.D\data.ms (-1342) (-)


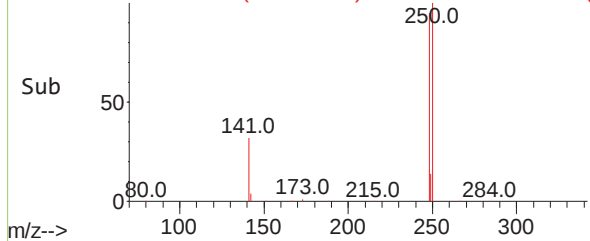


Abundance Scan 1359 (16.482 min): BN015723.D\data.ms (-1322) (-)

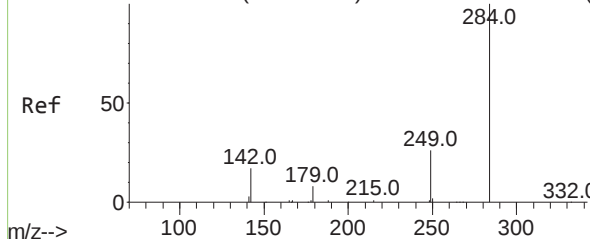


Hexachlorobenzene
Concen: 0.416 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	284	Resp:	38029
Ion	Ratio	Lower	Upper
284	100		
142	36.7	29.4	44.0
249	29.7	23.8	35.6

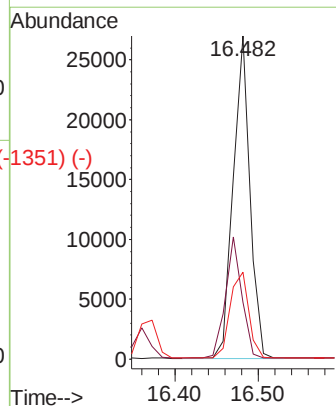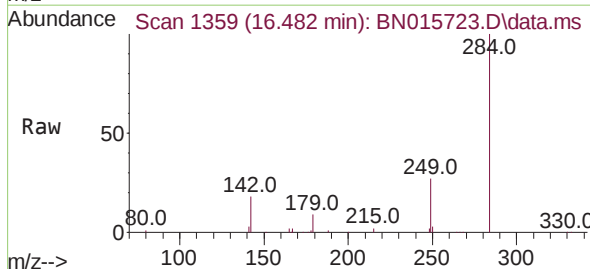


Abundance Scan 1359 (16.482 min): BN015723.D\data.ms (-1351) (-)

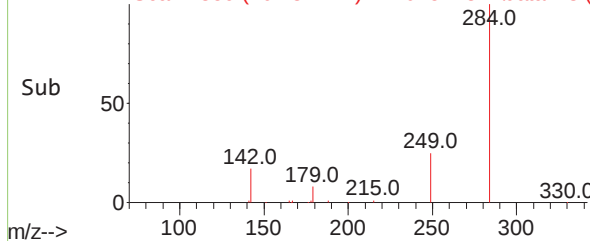




Abundance Scan 1372 (16.640 min): BN015723.D\data.ms (-1325) (-)

Atrazine
Concen: 0.284 ng
RT: 16.640 min Scan# 1372
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

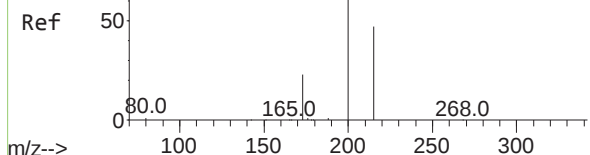


Tgt Ion:	200	Resp:	23938
Ion	Ratio	Lower	Upper
200	100		
173	23.6	18.9	28.3
215	47.6	38.1	57.1

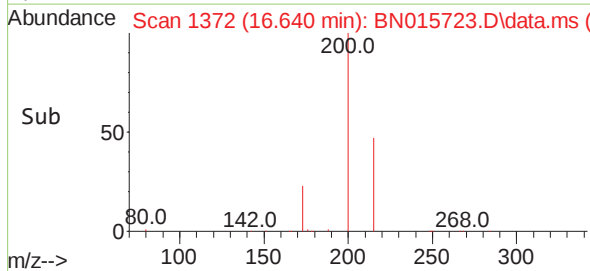
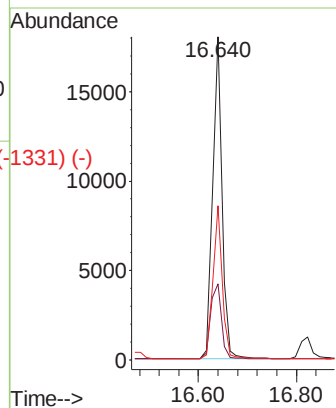
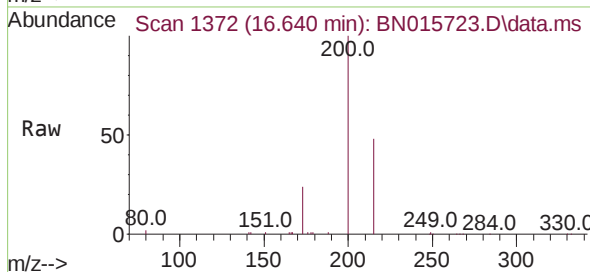


Abundance Scan 1387 (16.823 min): BN015723.D\data.ms (-1324) (-)


Pentachlorophenol
Concen: 0.358 ng
RT: 16.823 min Scan# 1387
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

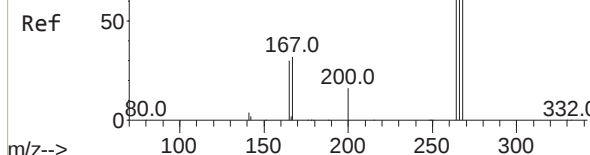

Tgt Ion:	266	Resp:	11993
Ion	Ratio	Lower	Upper
266	100		
264	62.7	50.2	75.2
268	64.2	51.1	76.7

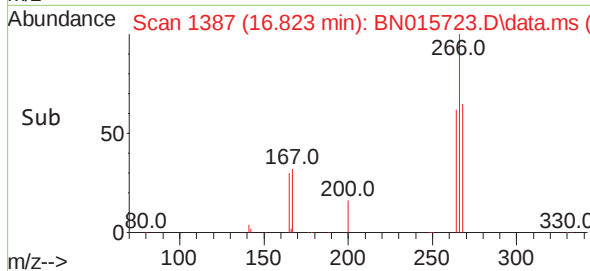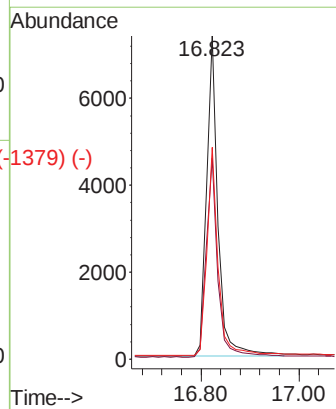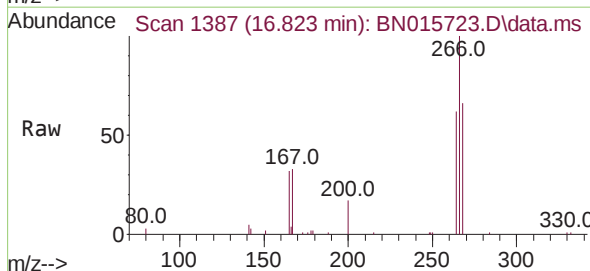



Abundance Scan 1419 (17.212 min): BN015723.D\data.ms (-1425) (-)

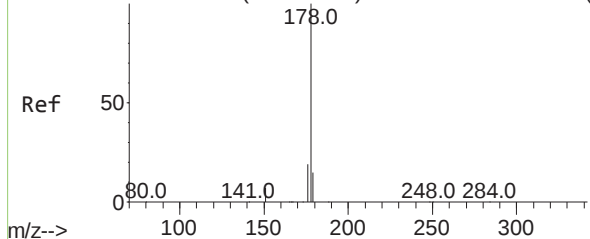


Phenanthrene
Concen: 0.386 ng
RT: 17.212 min Scan# 1419
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 167591
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.5 12.4 18.6

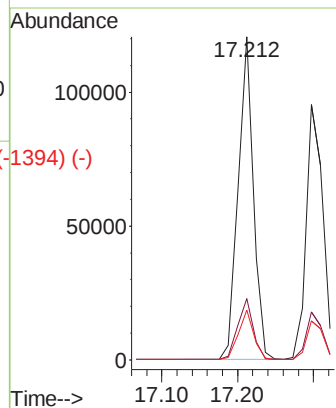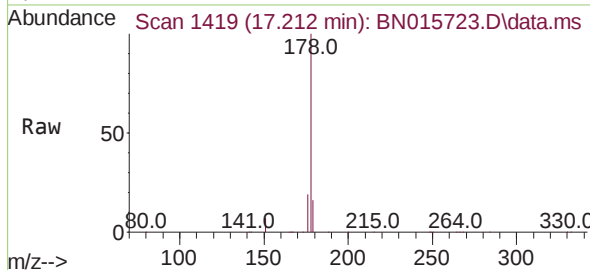

Abundance Scan 1419 (17.212 min): BN015723.D\data.ms (-1394) (-)


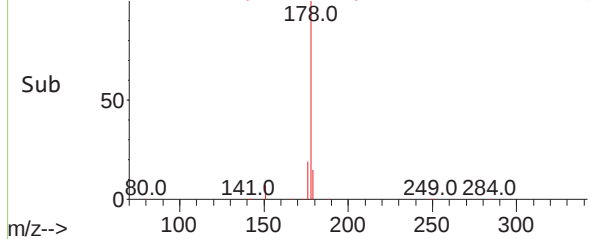


Abundance Scan 1426 (17.297 min): BN015723.D\data.ms (-1425) (-)

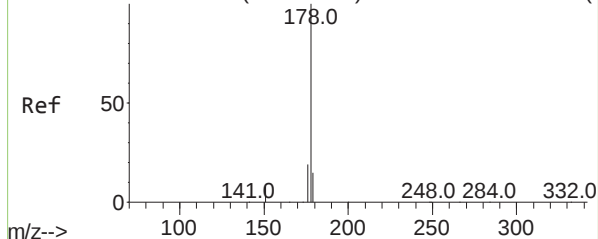


Anthracene
Concen: 0.351 ng
RT: 17.297 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06


Tgt Ion:178 Resp: 147741
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.3 12.2 18.4

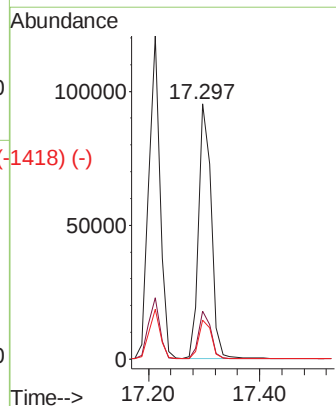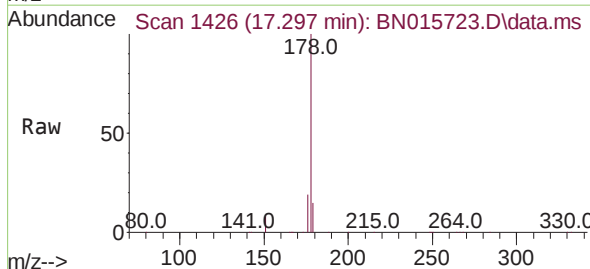

Abundance Scan 1426 (17.297 min): BN015723.D\data.ms (-1418) (-)

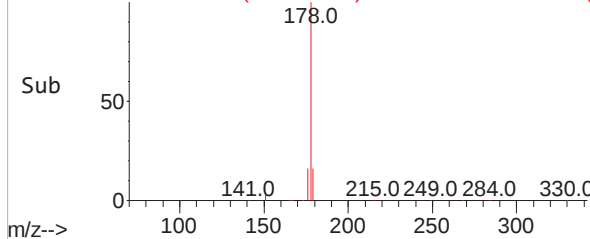




Abundance Scan 1726 (19.212 min): BN015723.D\data.ms (-1706) (-)

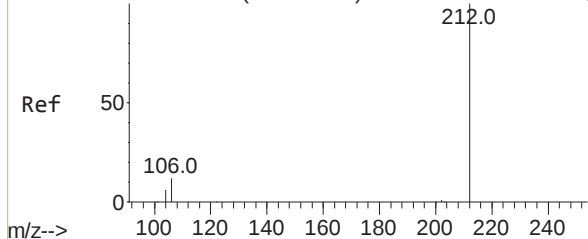


Fluoranthene-d10
Concen: 0.345 ng
RT: 19.212 min Scan# 1726
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:212 Resp: 153605
Ion Ratio Lower Upper
212 100
106 13.3 10.6 16.0
104 7.4 5.9 8.9



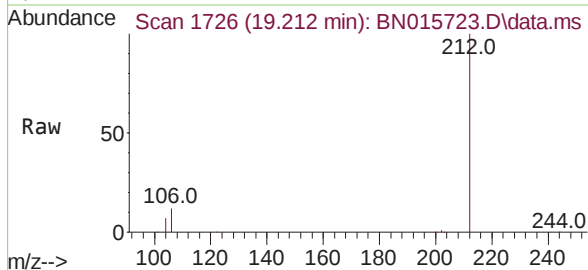


Abundance Scan 1732 (19.241 min): BN015723.D\data.ms (-1724) (-)

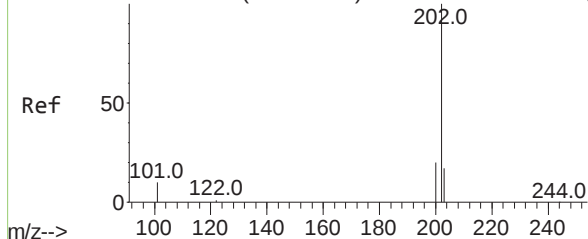


Fluoranthene
Concen: 0.365 ng
RT: 19.241 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:202 Resp: 181364
Ion Ratio Lower Upper
202 100
101 11.3 9.0 13.6
203 17.3 13.8 20.8

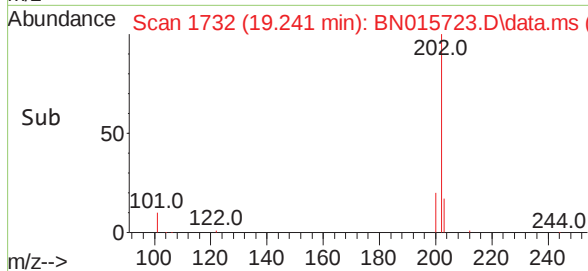




Abundance Scan 2015 (21.376 min): BN015723.D\data.ms (-1996) (-)

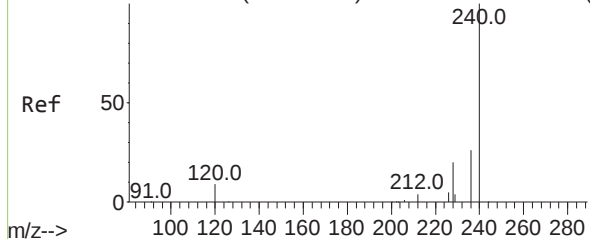


Chrysene-d12
Concen: 0.400 ng
RT: 21.376 min Scan# 2015
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	240	Resp:	146110
Ion	Ratio	Lower	Upper
240	100		
120	9.2	7.4	11.0
236	26.1	20.9	31.3

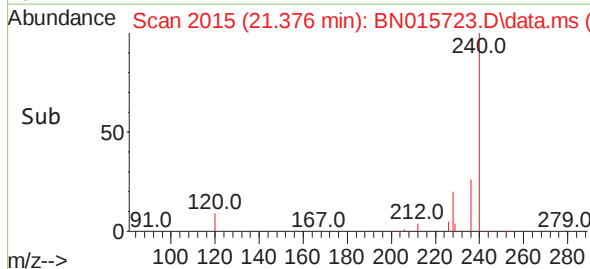
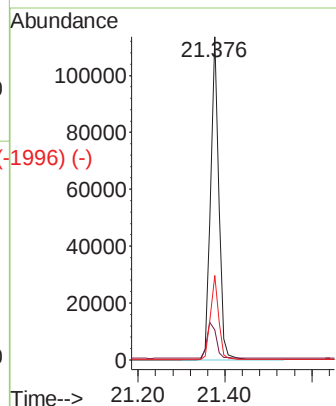
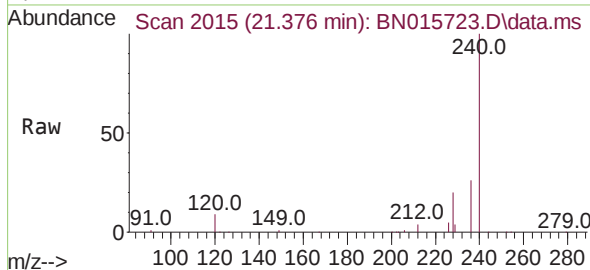


Abundance Scan 1805 (19.604 min): BN015723.D\data.ms (-1734) (-)

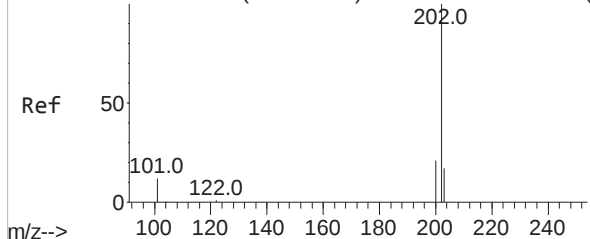


Pyrene
Concen: 0.363 ng
RT: 19.604 min Scan# 1805
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	202	Resp:	181217
Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.5	24.7
203	17.5	14.0	21.0

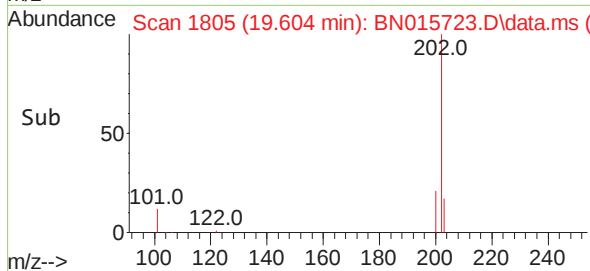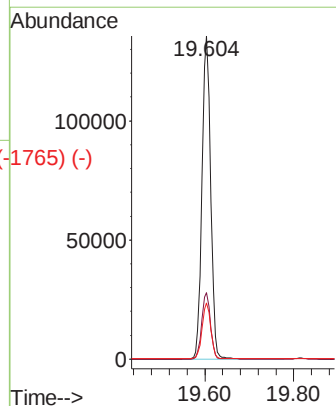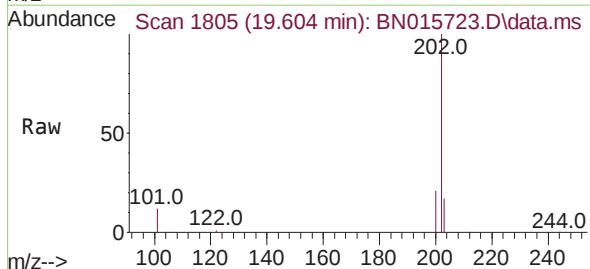




Abundance Scan 1848 (19.817 min): BN015723.D\data.ms (-1818) (-)

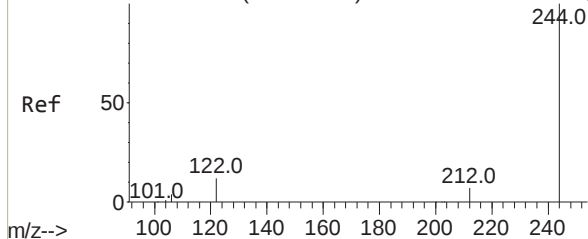


Terphenyl-d14
Concen: 0.348 ng
RT: 19.817 min Scan# 1848
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	244	Resp:	129324
Ion	Ratio	Lower	Upper
244	100		
212	7.4	5.9	8.9
122	12.0	9.6	14.4



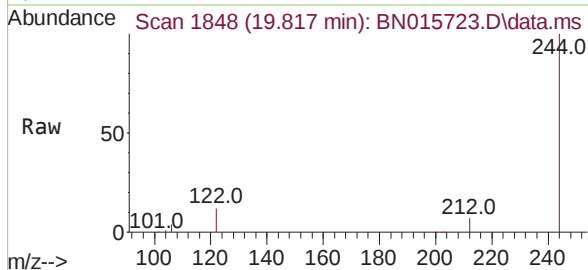


Abundance Scan 2013 (21.355 min): BN015723.D\data.ms (-1994) (-)

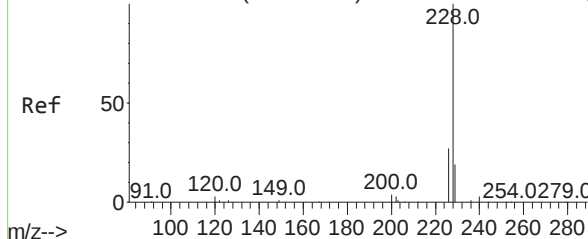


Benzo(a)anthracene
Concen: 0.344 ng
RT: 21.355 min Scan# 2013
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	228	Resp:	170837
Ion	Ratio	Lower	Upper
228	100		
226	27.4	21.9	32.9
229	19.2	15.4	23.0

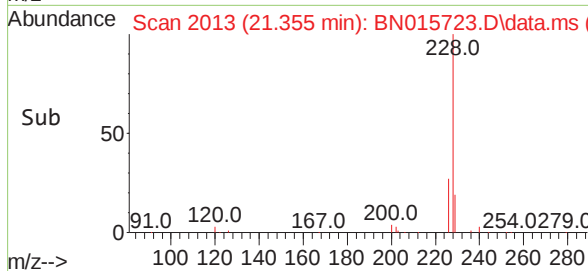



Abundance Scan 2018 (21.408 min): BN015723.D\data.ms (-2009) (-)

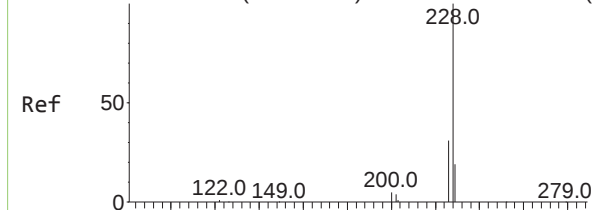


Chrysene
Concen: 0.375 ng
RT: 21.408 min Scan# 2018
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	228	Resp:	176493
Ion	Ratio	Lower	Upper
228	100		
226	30.4	24.3	36.5
229	19.1	15.3	22.9

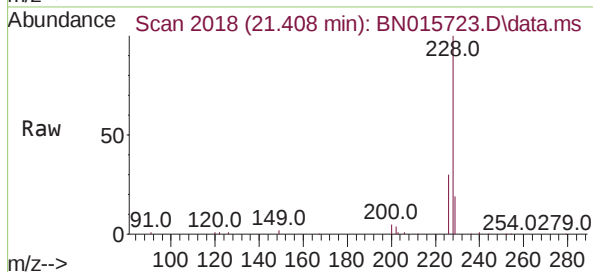

Abundance Scan 2018 (21.408 min): BN015723.D\data.ms (-2009) (-)


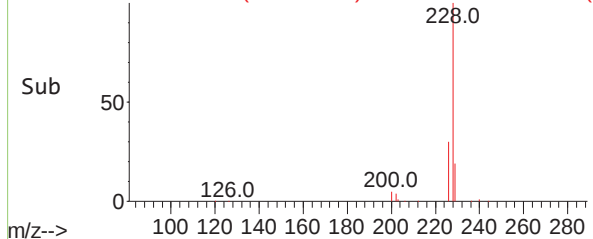


Abundance Scan 2009 (21.312 min): BN015723.D\data.ms (-2009) (-)

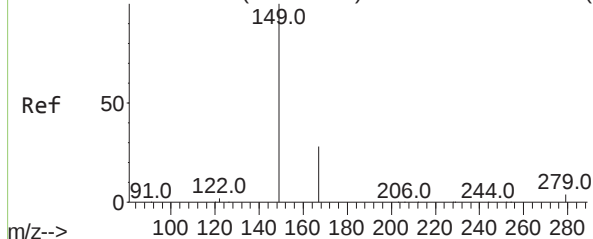


Bis(2-ethylhexyl)phthalate
Concen: 0.264 ng
RT: 21.312 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	149	Resp:	75026
Ion	Ratio	Lower	Upper
149	100		
167	26.5	21.5	32.3
279	3.9	3.2	4.8

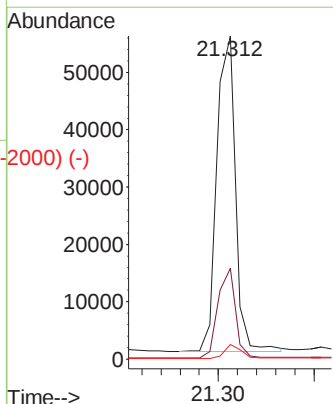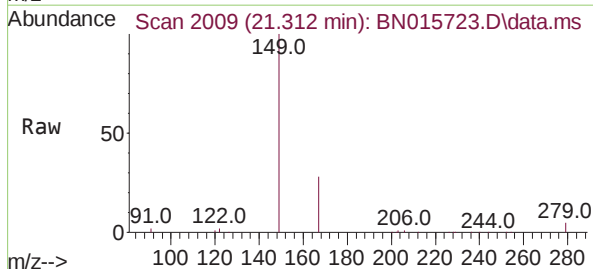


Abundance Scan 2009 (21.312 min): BN015723.D\data.ms (-2000) (-)

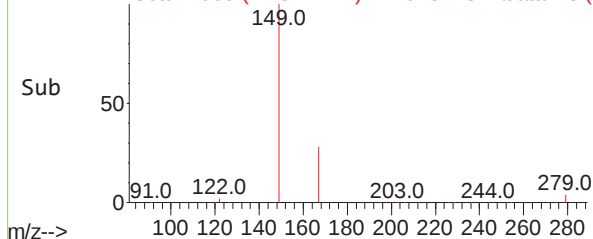




Abundance Scan 2496 (23.720 min): BN015723.D\data.ms (-2452) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.720 min Scan# 2496
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

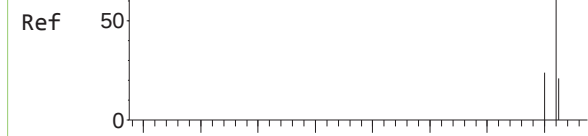





Tgt Ion:	264	Resp:	146636
Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.4	29.2
265	24.9	19.9	29.9

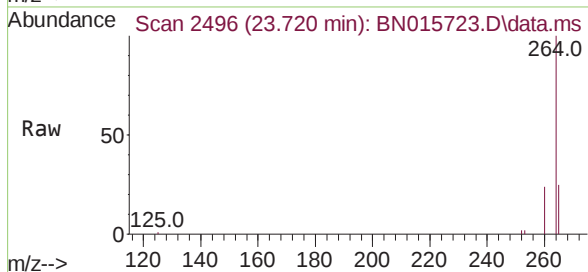


Abundance Scan 3199 (26.127 min): BN015723.D\data.ms (-3170) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.364 ng
RT: 26.127 min Scan# 3199
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	276	Resp:	194933
Ion	Ratio	Lower	Upper
276	100		
138	25.7	20.6	30.8
277	25.1	20.1	30.1

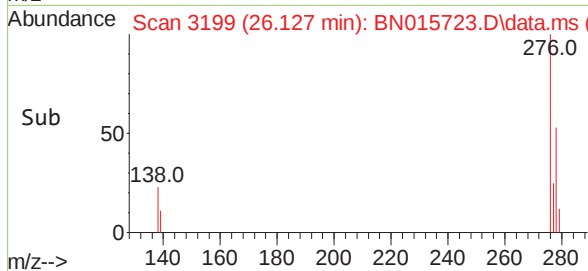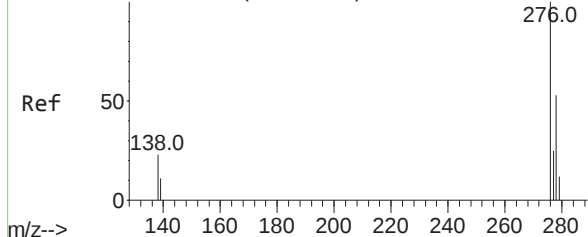



Abundance Scan 2289 (23.012 min): BN015723.D\data.ms (-2231) (-)

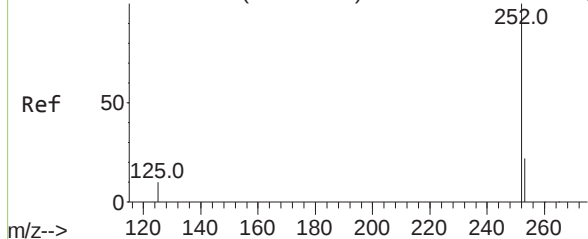


Benzo(b)fluoranthene
Concen: 0.360 ng
RT: 23.012 min Scan# 2289
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	252	Resp:	178835
Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.1	27.1
125	10.4	8.3	12.5

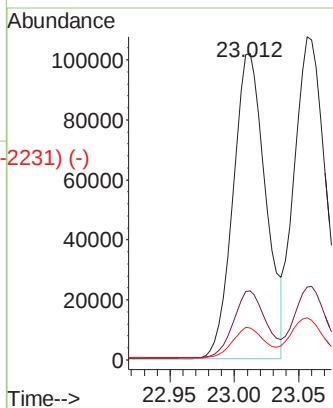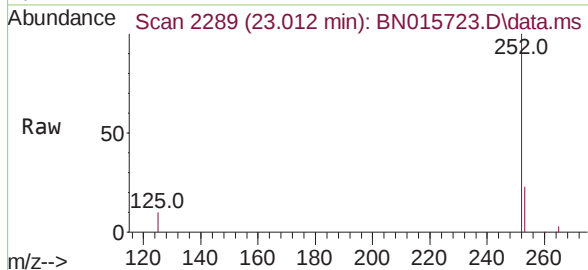

Abundance Scan 2289 (23.012 min): BN015723.D\data.ms (-2231) (-)


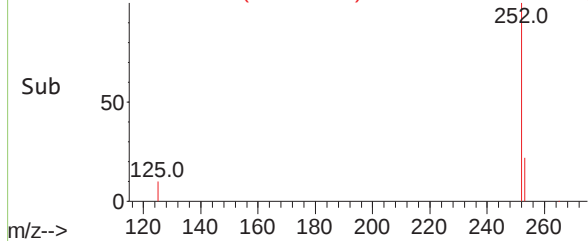


Abundance Scan 2302 (23.056 min): BN015723.D\data.ms (-2231) (-)

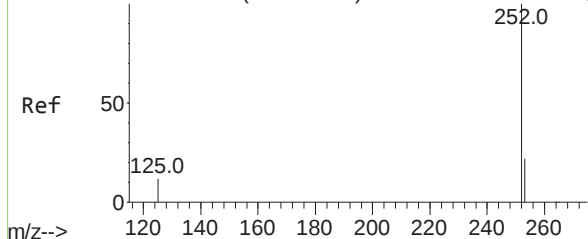


Benzo(k)fluoranthene
Concen: 0.388 ng
RT: 23.056 min Scan# 2302
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Tgt Ion:	252	Resp:	190216
Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.1	27.1
125	13.0	10.4	15.6




Abundance Scan 2302 (23.056 min): BN015723.D\data.ms (-2214) (-)

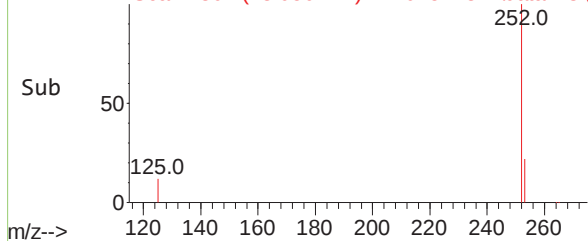



Abundance Scan 2466 (23.618 min): BN015723.D\data.ms (-2408) (-)

Benzo(a)pyrene
Concen: 0.356 ng
RT: 23.618 min Scan# 2466
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

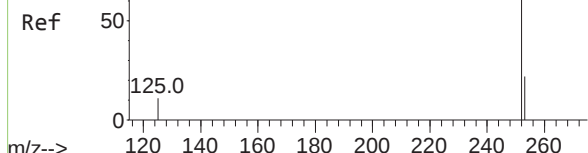

Tgt Ion:	252	Resp:	159792
Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.1	27.1
125	11.5	9.2	13.8

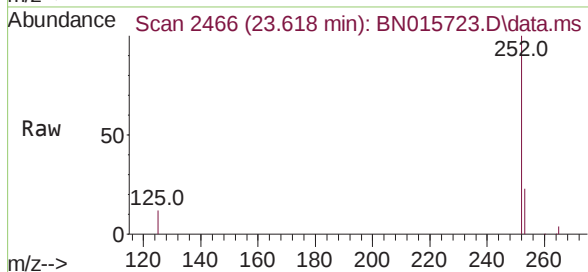




Abundance Scan 2466 (23.618 min): BN015723.D\data.ms (-2408) (-)

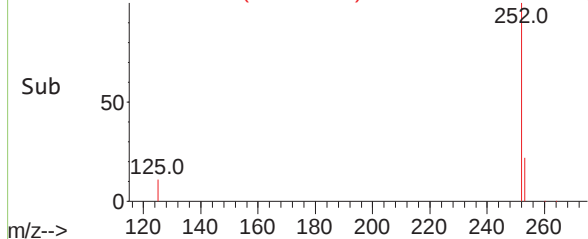


Abundance Scan 3205 (26.147 min): BN015723.D\data.ms (-3182) (-)

Dibenzo(a,h)anthracene
Concen: 0.367 ng
RT: 26.147 min Scan# 3205
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06


Tgt Ion:	278	Resp:	165444
Ion	Ratio	Lower	Upper
278	100		
139	20.0	16.0	24.0
279	24.0	19.2	28.8

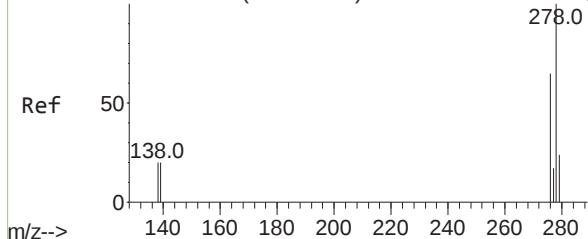

Abundance Scan 3205 (26.147 min): BN015723.D\data.ms (-3182) (-)

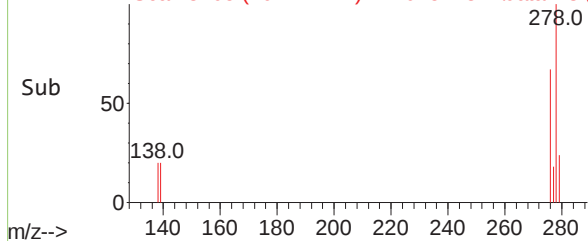


Abundance Scan 3413 (26.859 min): BN015723.D\data.ms (-3355) (-)

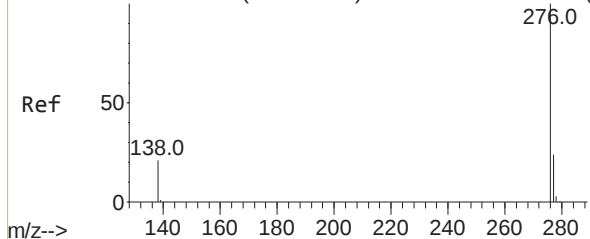

Benzo(g,h,i)perylene
Concen: 0.373 ng
RT: 26.859 min Scan# 3413
Delta R.T. 0.000 min
Lab File: BN015723.D
Acq: 30 Jul 2021 18:06

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

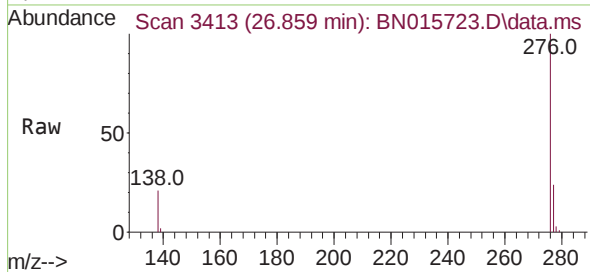

Tgt Ion:	276	Resp:	169424
Ion	Ratio	Lower	Upper
276	100		
277	24.0	19.2	28.8
138	21.0	16.8	25.2

