
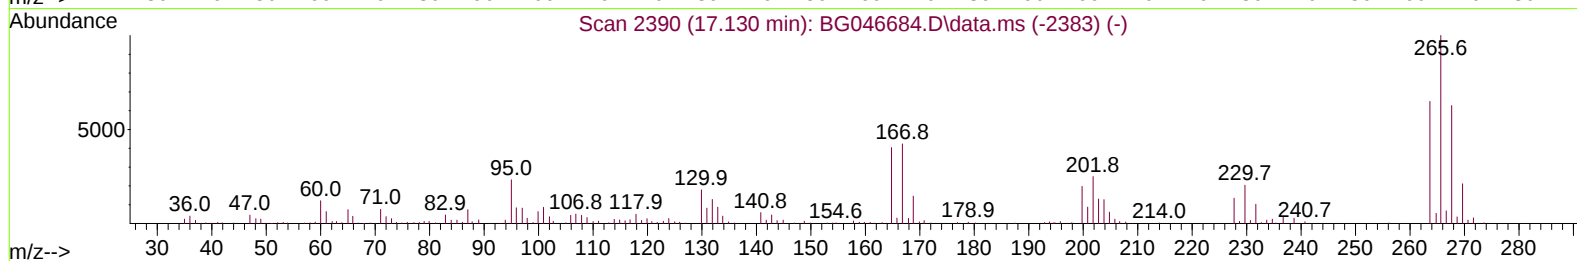
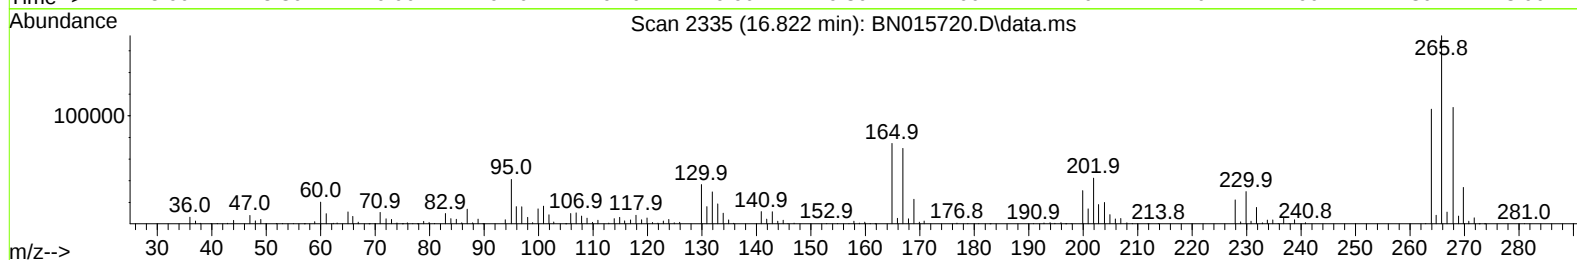


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
 Data File : BN015720.D
 Acq On : 30 Jul 2021 16:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 08:50:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 07:20:03 2021
 Response via : Initial Calibration

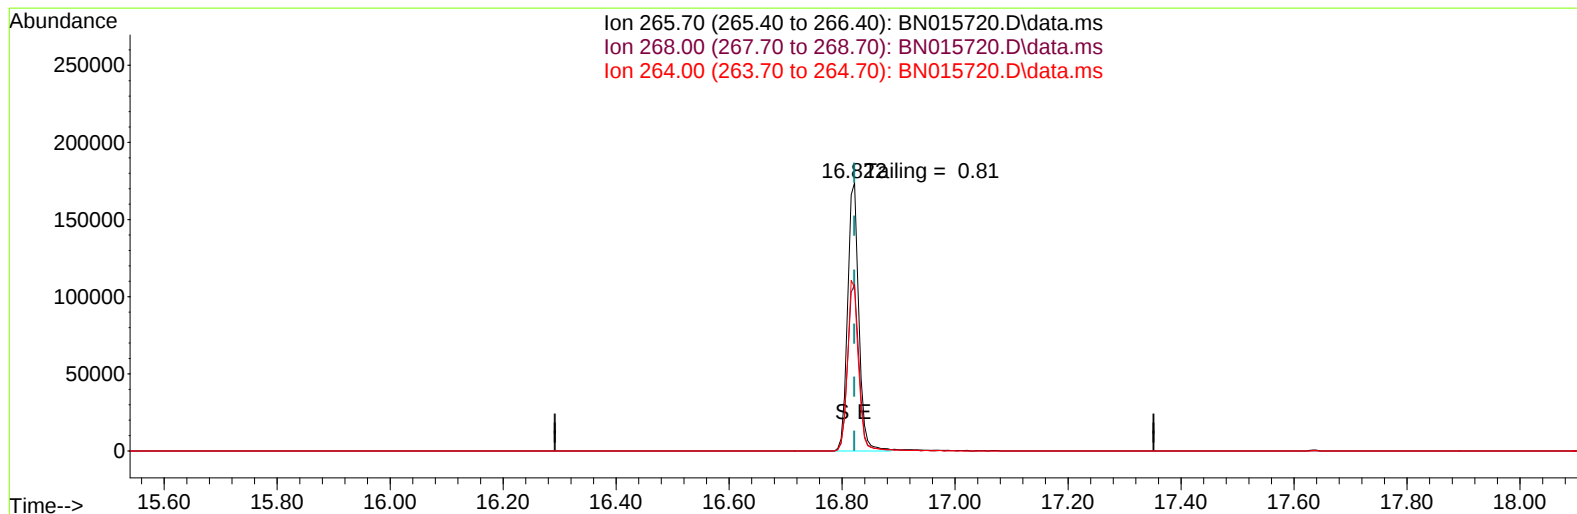

TIC: BN015720.D\data.ms

(70) Pentachlorophenol (C)




16.822min (+ 0.000) 21874.40 ng

response 240159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.98
264.00	61.60	61.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
Data File : BN015720.D
Acq On : 30 Jul 2021 16:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 08:50:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

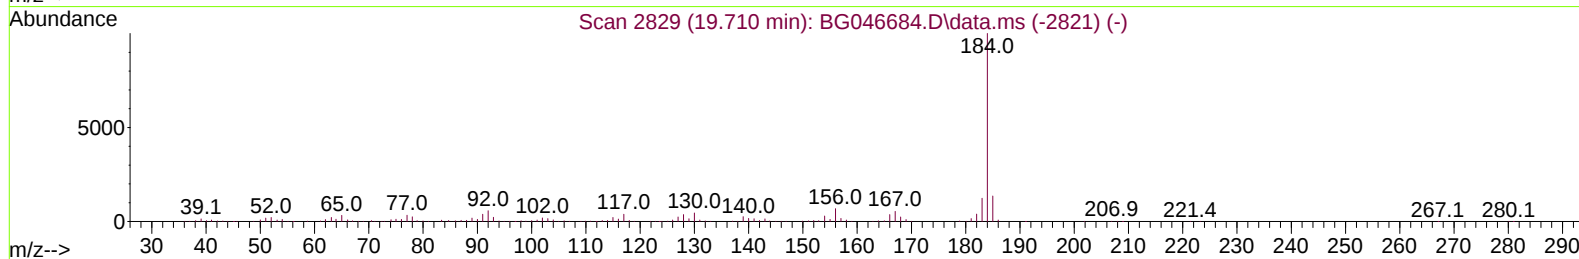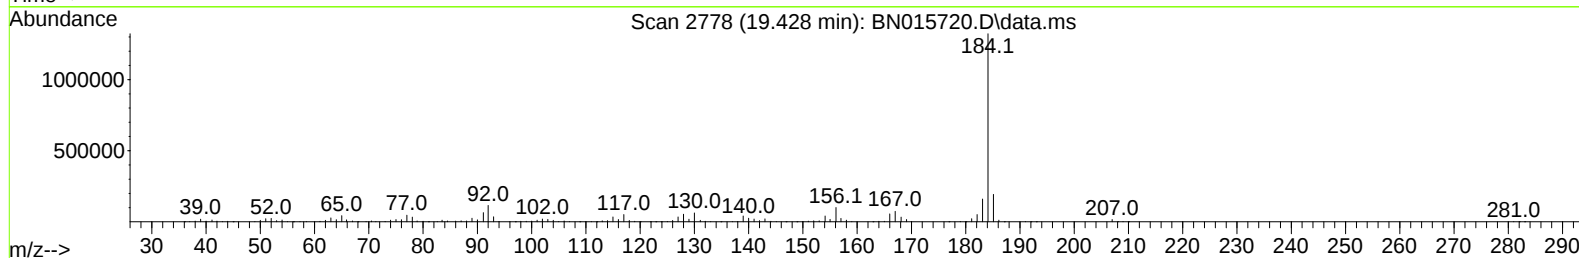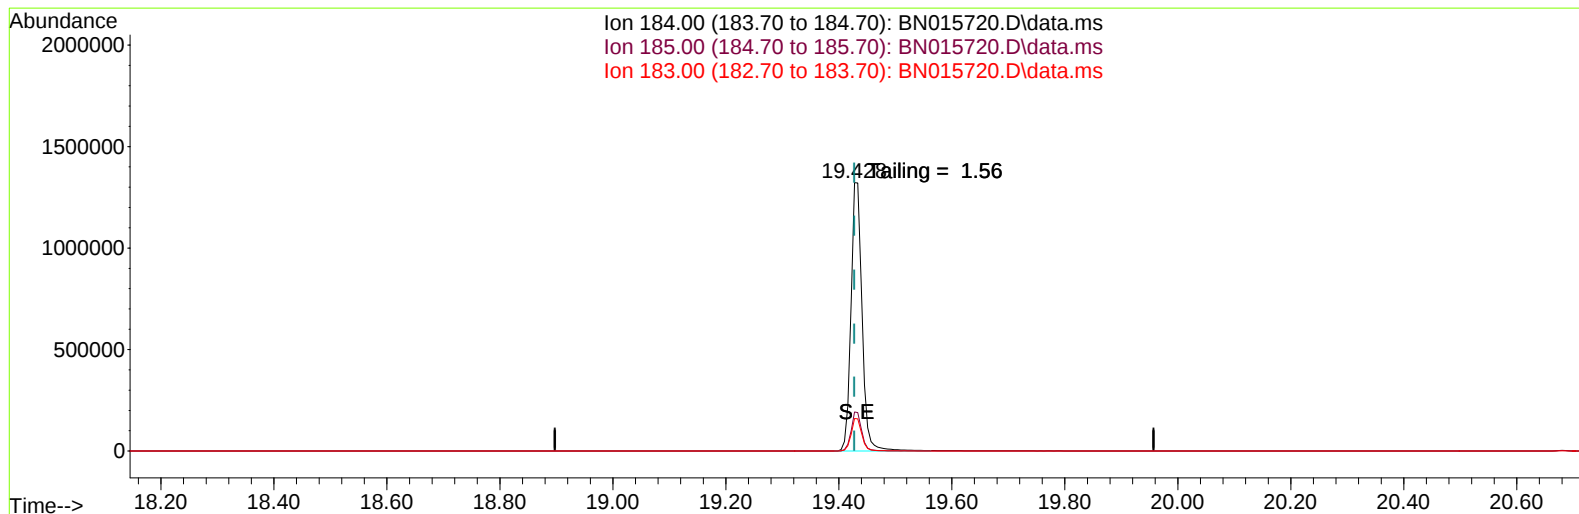

TIC: BN015720.D\data.ms

(77) Benzidine**19.428min (+ 0.000) 0.00 ng****response 1813999**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	12.13
0.00	0.00	0.00