


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
 Data File : BN015720.D
 Acq On : 30 Jul 2021 16:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 31 04:53:33 2021

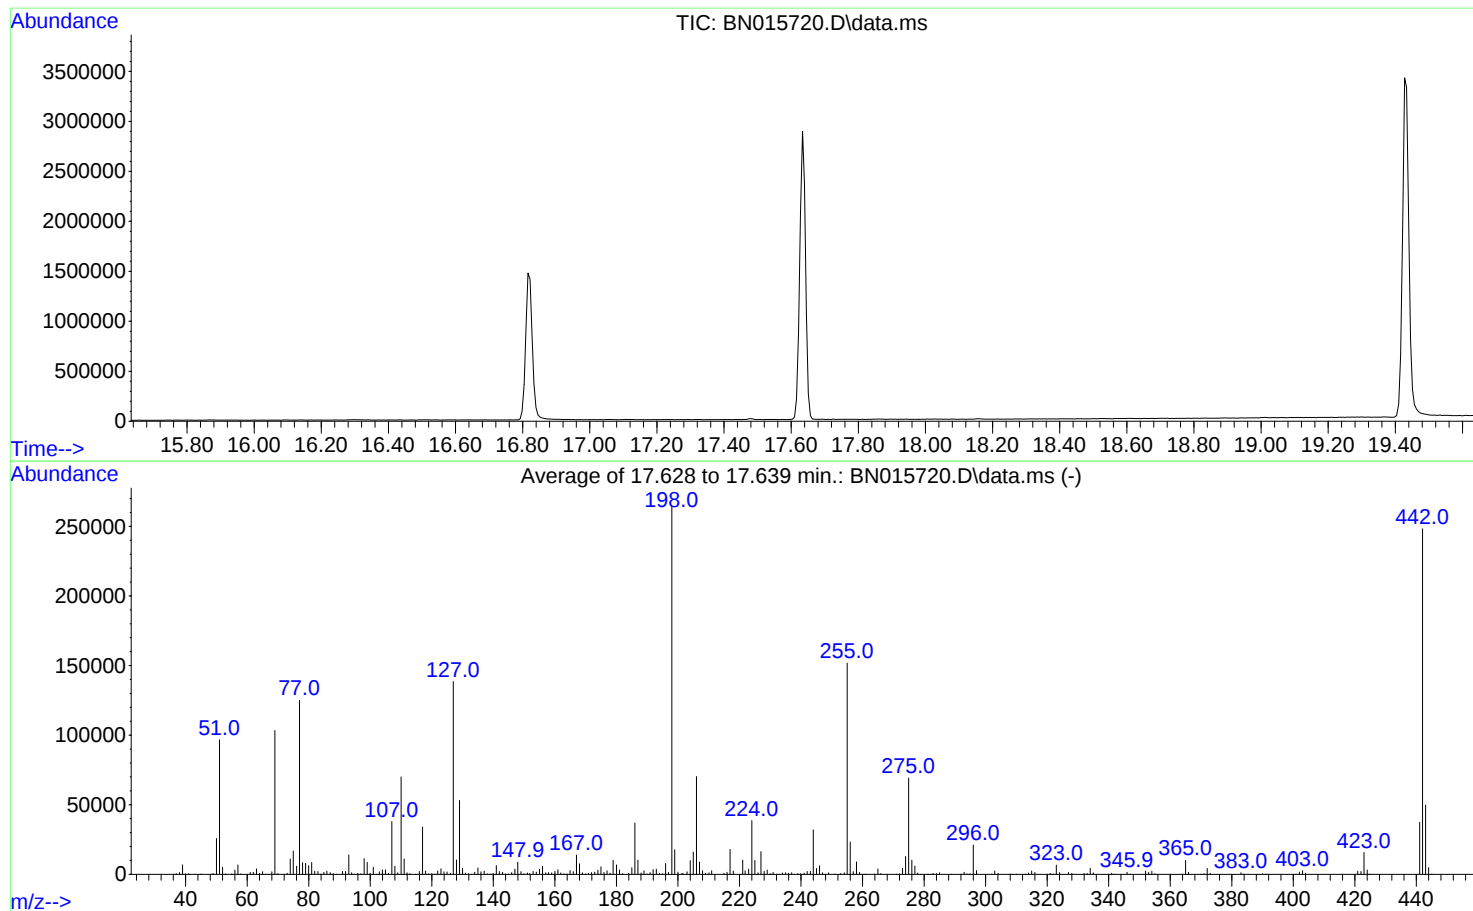




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	96728	PASS
68	69	0.00	2	1.8	1827	PASS
69	198	0.00	100	39.1	103307	PASS
70	69	0.00	2	0.6	576	PASS
127	198	10	80	52.4	138501	PASS
197	198	0.00	2	0.5	1389	PASS
198	198	100	100	100.0	264299	PASS
199	198	5	9	6.7	17769	PASS
275	198	10	60	26.2	69184	PASS
365	198	1	100	3.8	10017	PASS
441	198	0.01	100	14.1	37336	PASS
442	442	50	100	100.0	248277	PASS
443	442	15	24	20.1	49813	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
Data File : BN015720.D
Acq On : 30 Jul 2021 16:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 31 08:50:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

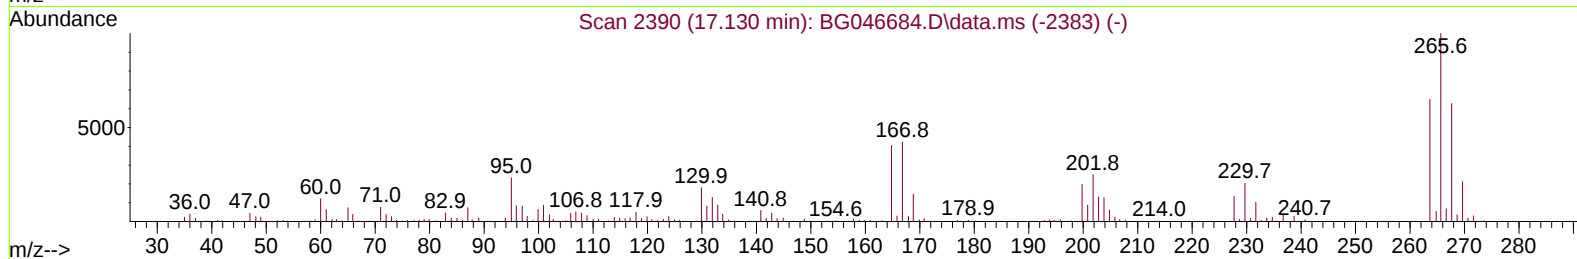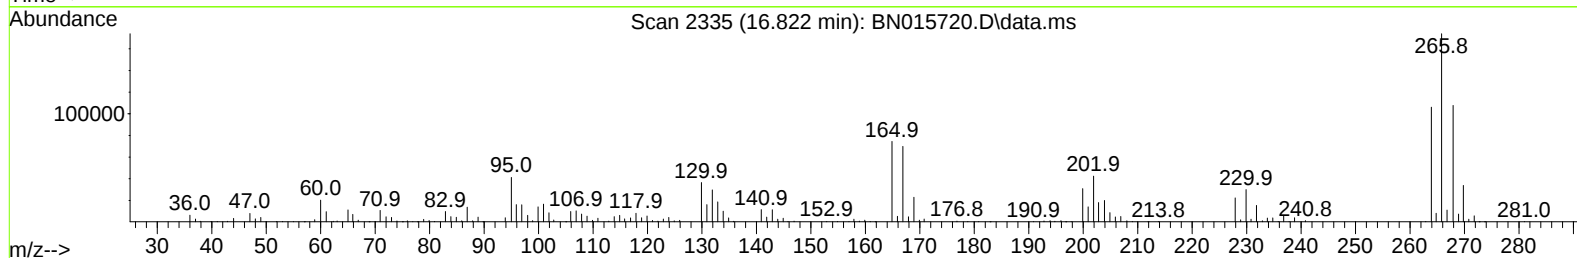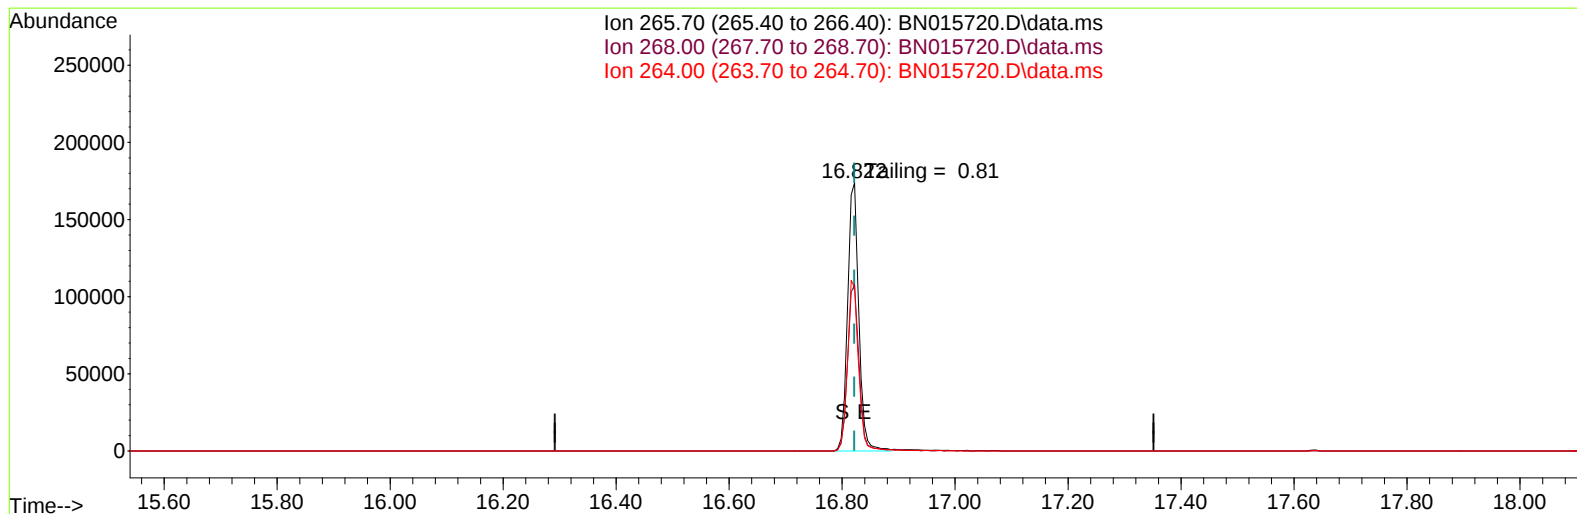

TIC: BN015720.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.000) 21874.40 ng




response 240159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.98
264.00	61.60	61.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073021\
Data File : BN015720.D
Acq On : 30 Jul 2021 16:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 31 08:50:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

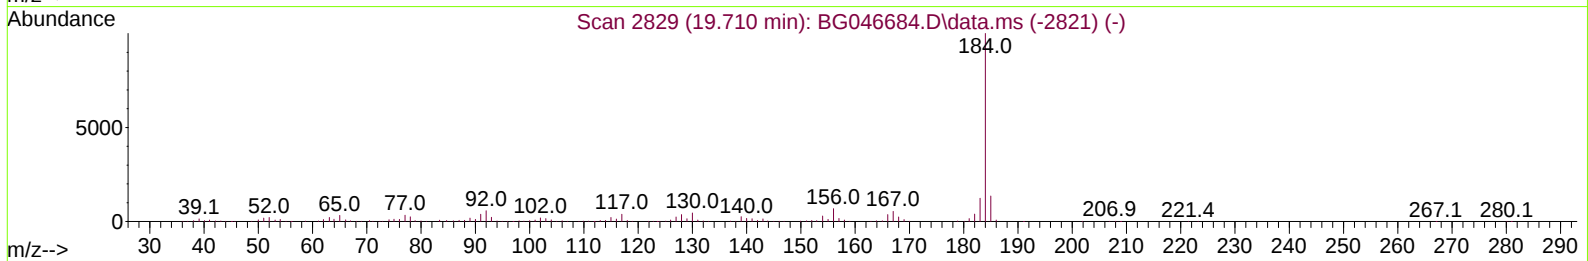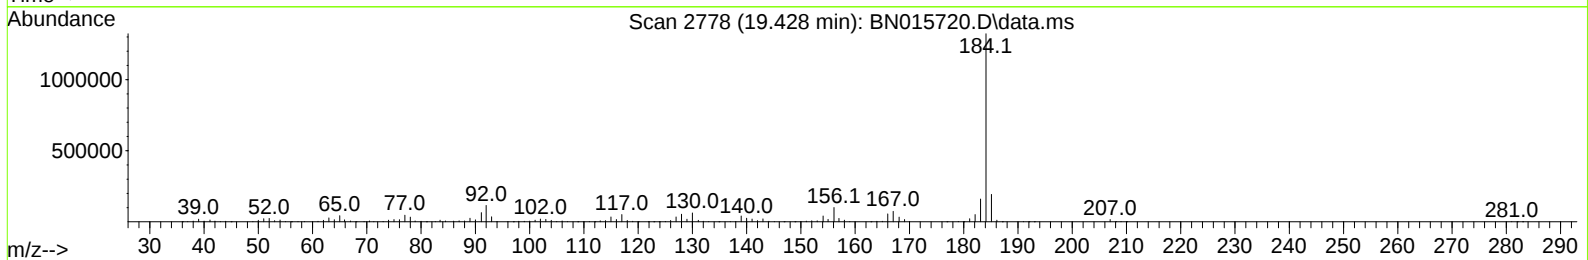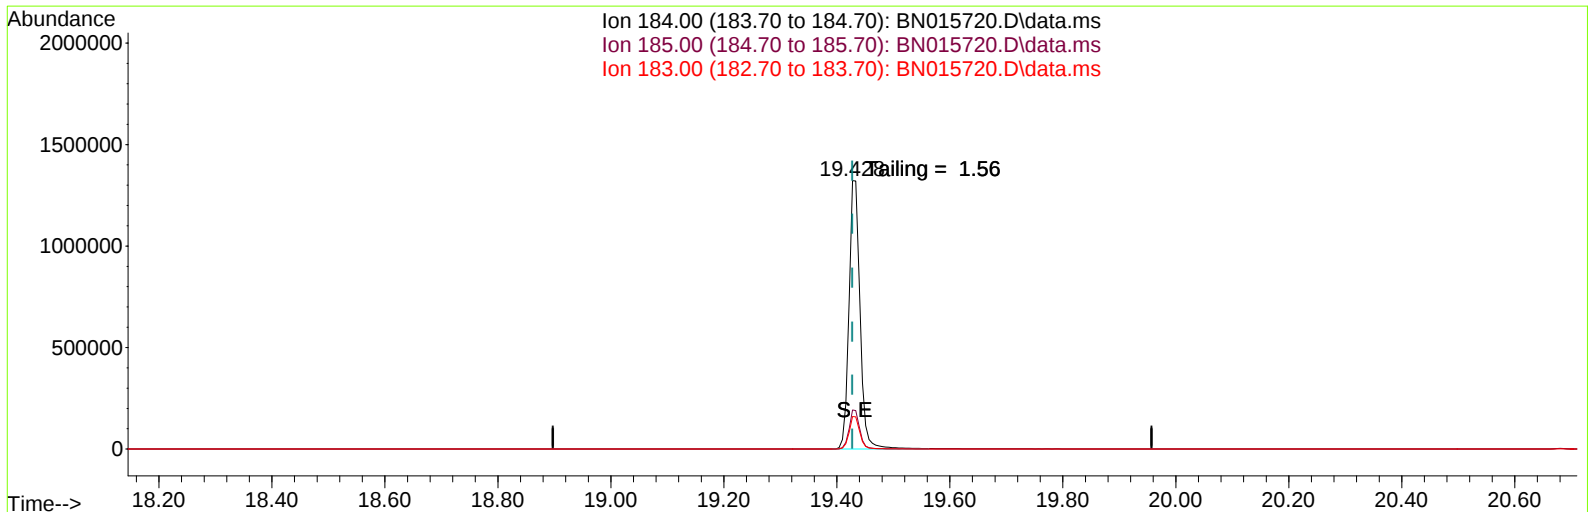

TIC: BN015720.D\data.ms

(77) Benzidine

19.428min (+ 0.000) 0.00 ng

response 1813999

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/30/2021	BNA_N	<u>BN015720.D</u>
Compound Name	Response	Retention Time
DDT	694471	20.68
DDD	2244	20.239
DDE	897	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3141	697612	0.45

Instrument :
BNA_N
ClientSampleId :
DFTPP