

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073024\
 Data File : BN033074.D
 Acq On : 29 Jul 2024 19:02
 Operator : MA/JU
 Sample : P3347-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AX3

Quant Time: Jul 29 23:07:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 29 23:04:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.507	152	1752	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.262	136	6366	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.148	164	4143	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.004	188	718966	0.400	ng/ul	0.06
17) Chrysene-d12	21.148	240	8242	0.400	ng/ul	-0.01
23) Perylene-d12	23.323	264	18837	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.056	96	10302	4.649	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.901	152	2765	0.266	ng/ul	-0.01
18) Fluoranthene-d10	18.958	212	9810	0.420	ng/ul	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.090	88	130	0.051	ng/ul#	46
20) Pyrene	19.316	202	1857	0.064	ng/ul#	1
26) Benzo(a)pyrene	23.168	252	4272	0.082	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073024\
Data File : BN033074.D
Acq On : 29 Jul 2024 19:02
Operator : MA/JU
Sample : P3347-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX3


Quant Time: Jul 29 23:07:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 29 23:04:40 2024
Response via : Initial Calibration

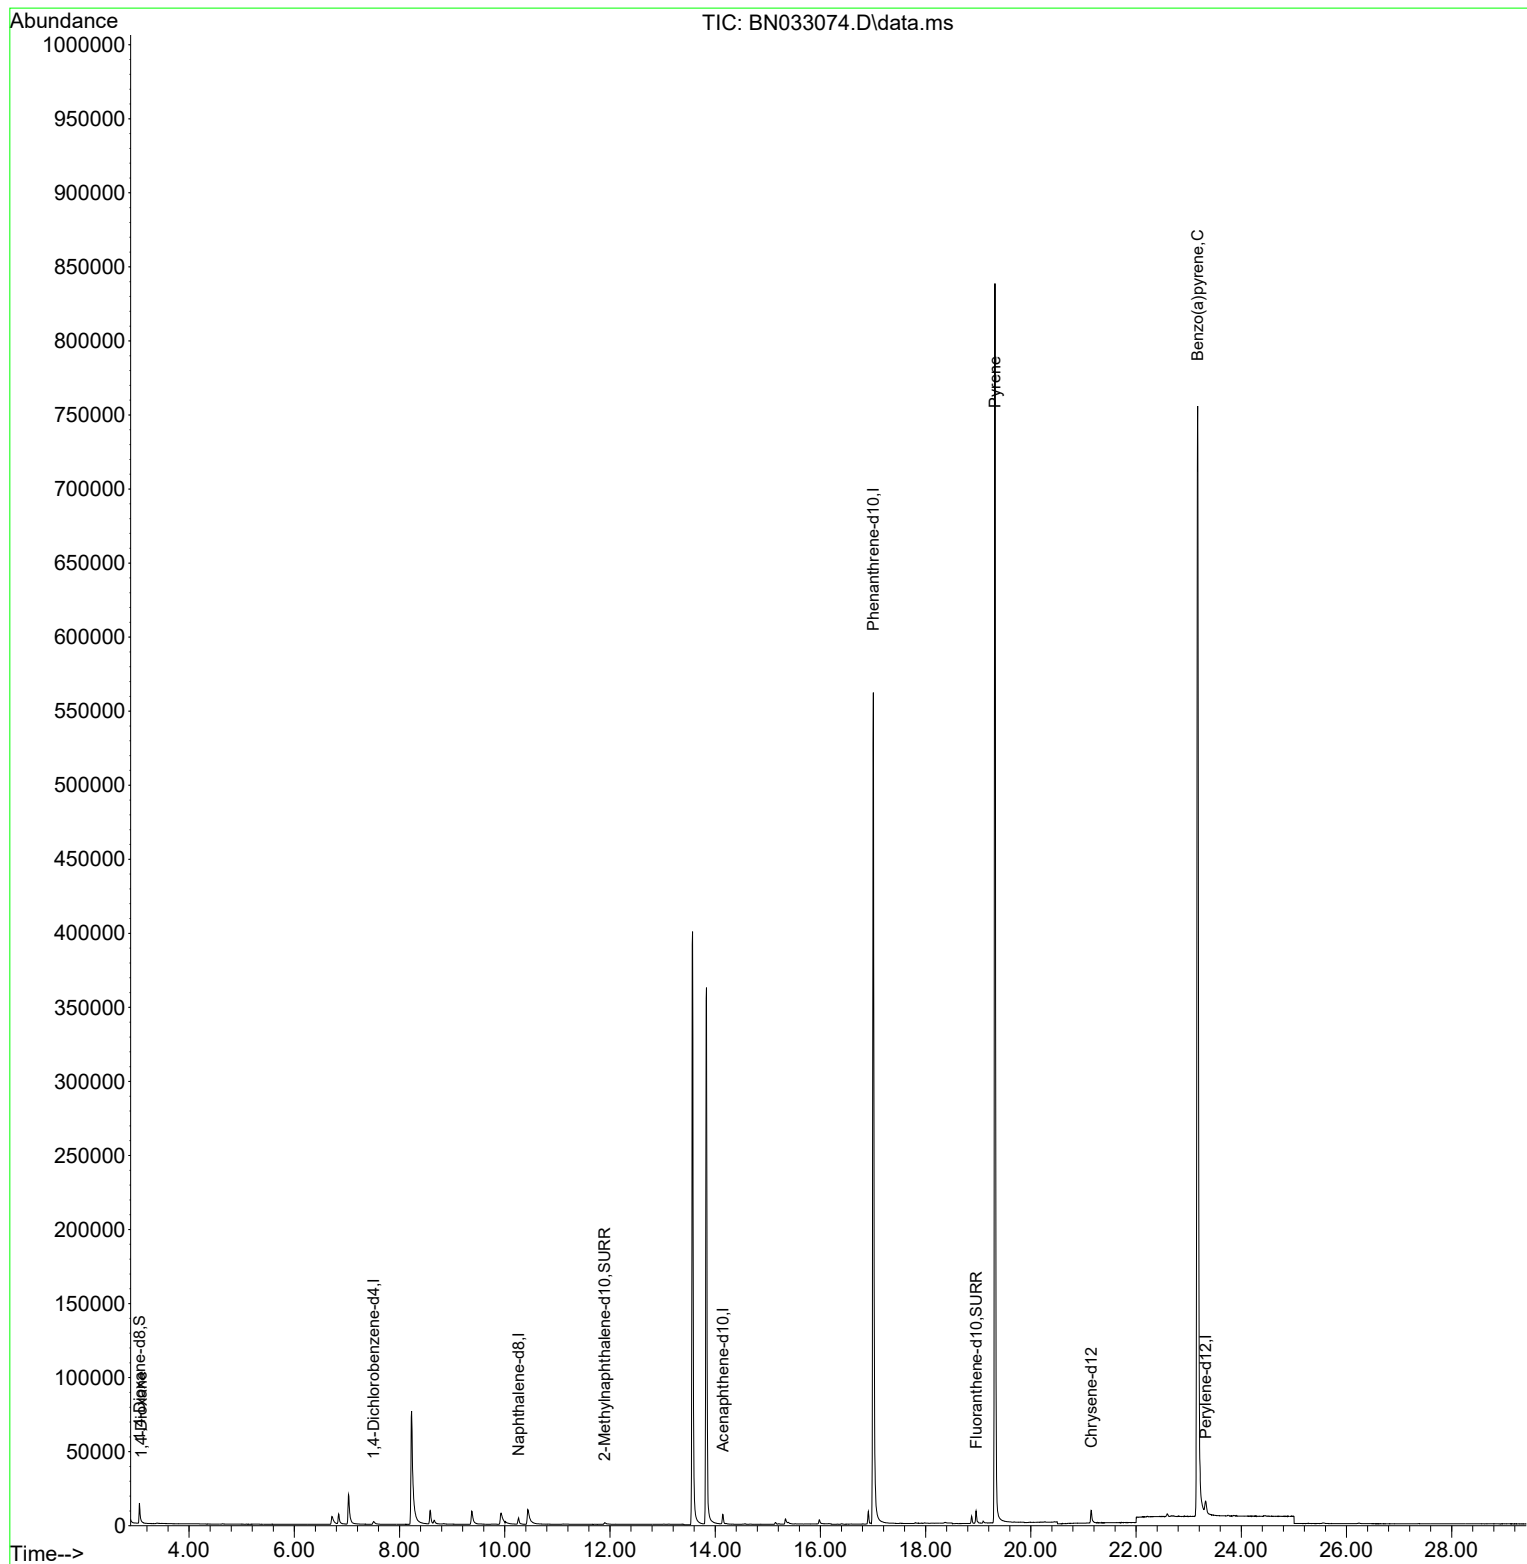



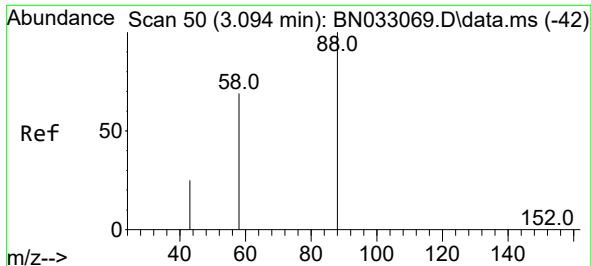


#2
1,4-Dioxane
Concen: 0.051 ng/ul
RT: 3.090 min Scan# 49
Delta R.T. -0.013 min
Lab File: BN033074.D
Acq: 29 Jul 2024 19:02


Instrument :
BNA_N
ClientSampleId :
C0AX3

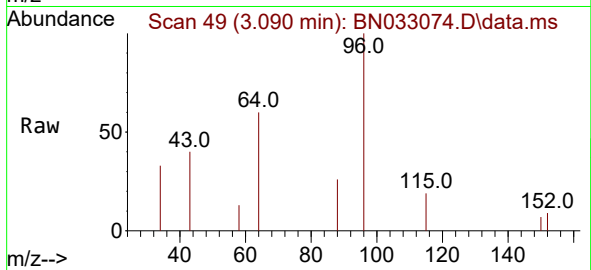



Tgt Ion: 88 Resp: 130
Ion Ratio Lower Upper
88 100
43 151.3 63.4 95.2#
58 47.7 49.4 74.0#

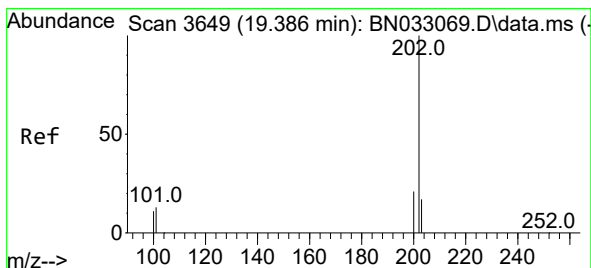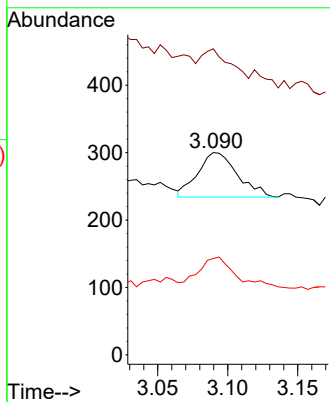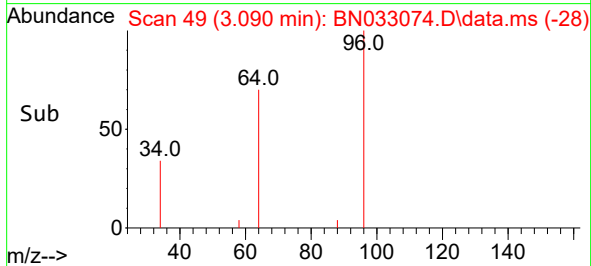


#20
Pyrene
Concen: 0.064 ng/ul
RT: 19.316 min Scan# 3634
Delta R.T. -0.065 min
Lab File: BN033074.D
Acq: 29 Jul 2024 19:02

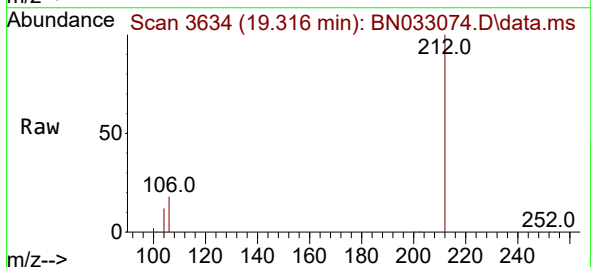


Tgt Ion: 202 Resp: 1857
Ion Ratio Lower Upper
202 100
101 162.5 12.6 18.8#
100 1155.5 9.9 14.9#

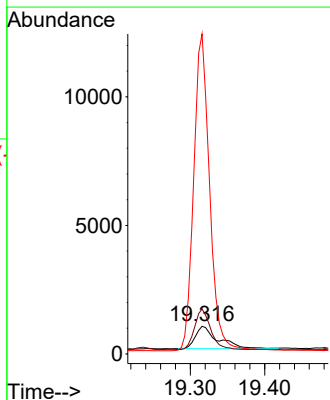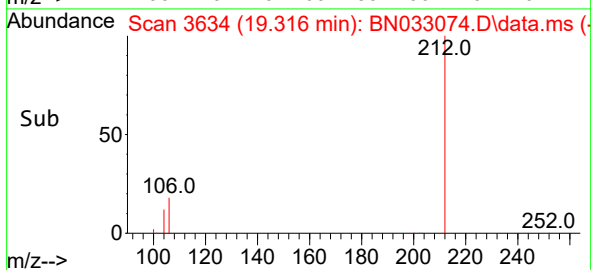

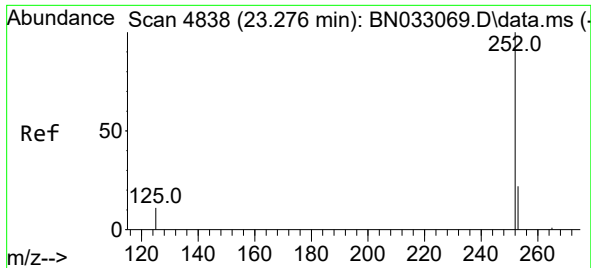

#26
Benzo(a)pyrene
Concen: 0.082 ng/ul
RT: 23.168 min Scan# 41
Delta R.T. -0.094 min
Lab File: BN033074.D
Acq: 29 Jul 2024 19:02

Instrument :
BNA_N
ClientSampleId :
C0AX3

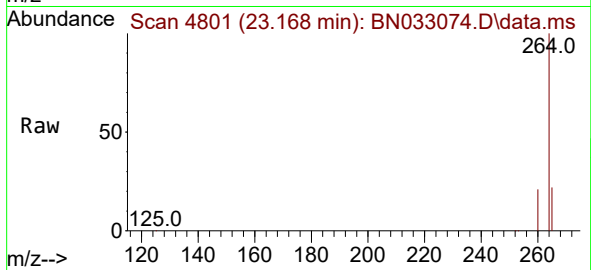

Tgt Ion:252 Resp: 4272
Ion Ratio Lower Upper
252 100
253 57.2 27.5 41.3#
125 57.4 27.0 40.6#

