

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073024\
 Data File : BN033074.D
 Acq On : 29 Jul 2024 19:02
 Operator : MA/JU
 Sample : P3347-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AX3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 07/31/2024

Quant Time: Jul 29 23:07:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 29 23:04:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.507	152	1752	0.400	ng/u1	-0.02
4) Naphthalene-d8	10.262	136	6366	0.400	ng/u1	-0.04
9) Acenaphthene-d10	14.148	164	4143	0.400	ng/u1	#-0.02
13) Phenanthrene-d10	16.911	188	10073m	0.400	ng/u1	-0.03
17) Chrysene-d12	21.148	240	10237m	0.400	ng/u1	-0.01
23) Perylene-d12	23.323	264	9333m	0.400	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.056	96	10302	4.649	ng/u1	-0.01
6) 2-Methylnaphthalene-d10	11.901	152	2765	0.266	ng/u1	-0.01
18) Fluoranthene-d10	18.958	212	9810	0.338	ng/u1	-0.02
Target Compounds						Qvalue
16) Anthracene	17.042	178	2082m	0.086	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073024\
Data File : BN033074.D
Acq On : 29 Jul 2024 19:02
Operator : MA/JU
Sample : P3347-11
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AX3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 07/31/2024


Quant Time: Jul 29 23:07:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 29 23:04:40 2024
Response via : Initial Calibration

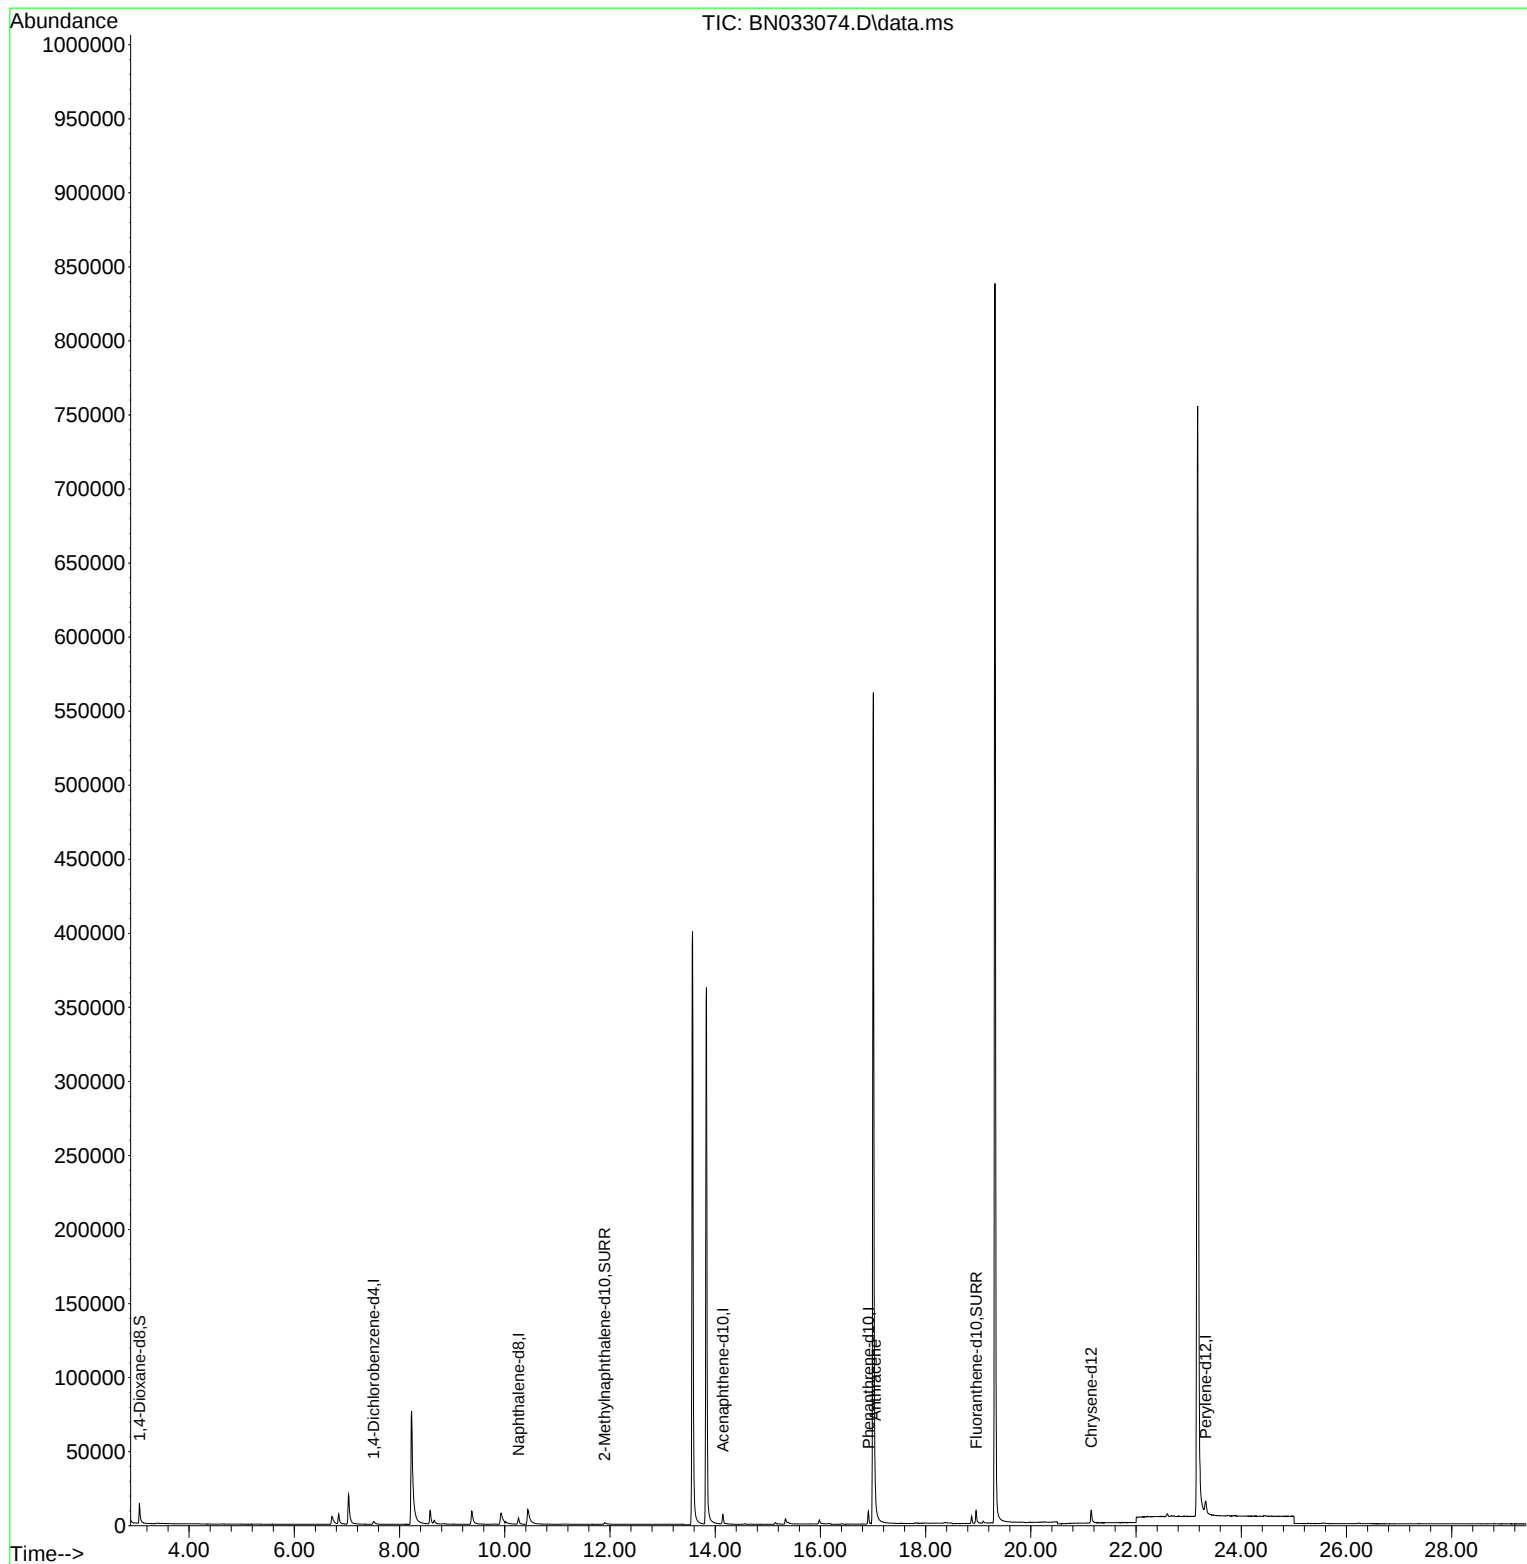

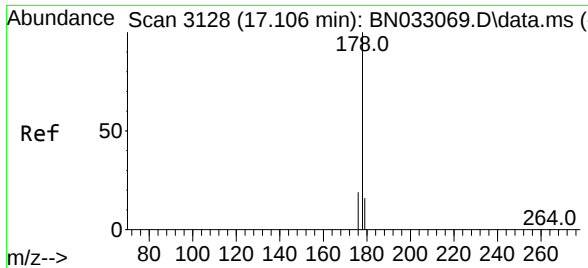

#16
Anthracene
Concen: 0.086 ng/ul m
RT: 17.042 min Scan# 31
Delta R.T. -0.042 min
Lab File: BN033074.D
Acq: 29 Jul 2024 19:02

Instrument :
BNA_N
ClientSampleId :
C0AX3

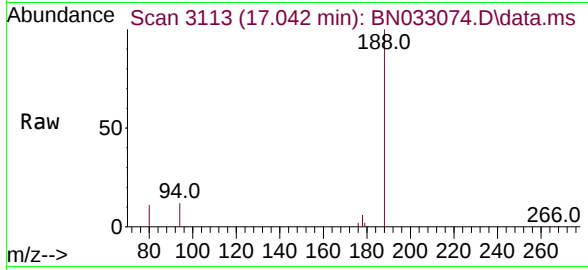

Tgt Ion:178 Resp: 208
Ion Ratio Lower Upper
178 100
179 31.2 14.3 21.5
176 27.6 15.8 23.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 07/31/2024

