


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073118\
 Data File : BN002200.D
 Acq On : 31 Jul 2018 07:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 30 16:17:29 2018

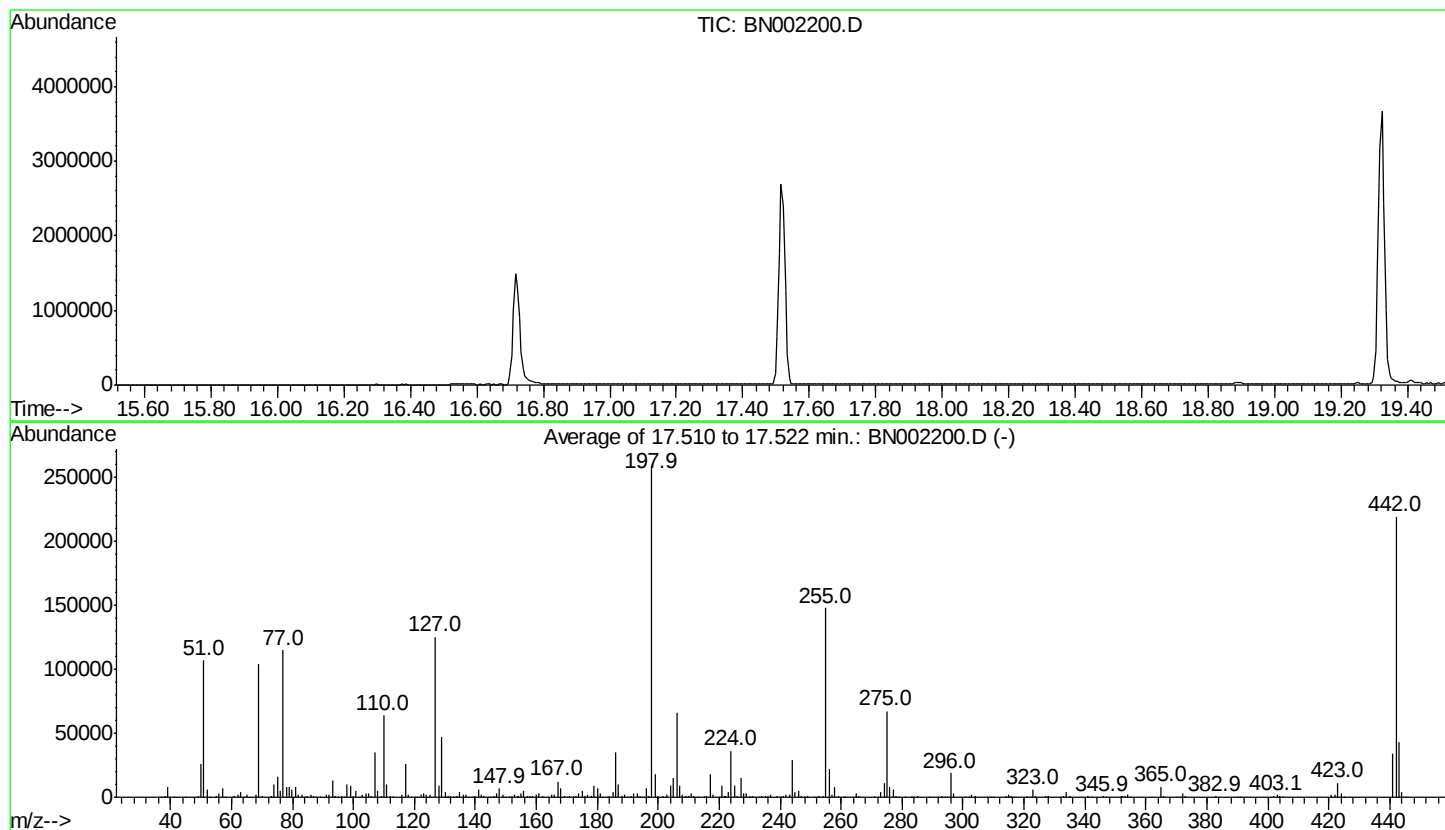

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	106640	PASS
68	69	0.00	2	1.7	1761	PASS
69	198	0.00	100	40.3	104445	PASS
70	69	0.00	2	0.5	557	PASS
127	198	10	80	48.4	125546	PASS
197	198	0.00	2	0.3	828	PASS
198	198	100	100	100.0	259221	PASS
199	198	5	9	6.8	17700	PASS
275	198	10	60	25.9	67197	PASS
365	198	1	100	3.1	8058	PASS
441	198	0.01	100	13.0	33760	PASS
442	198	50	100	84.5	219157	PASS
443	442	15	24	19.7	43162	PASS