
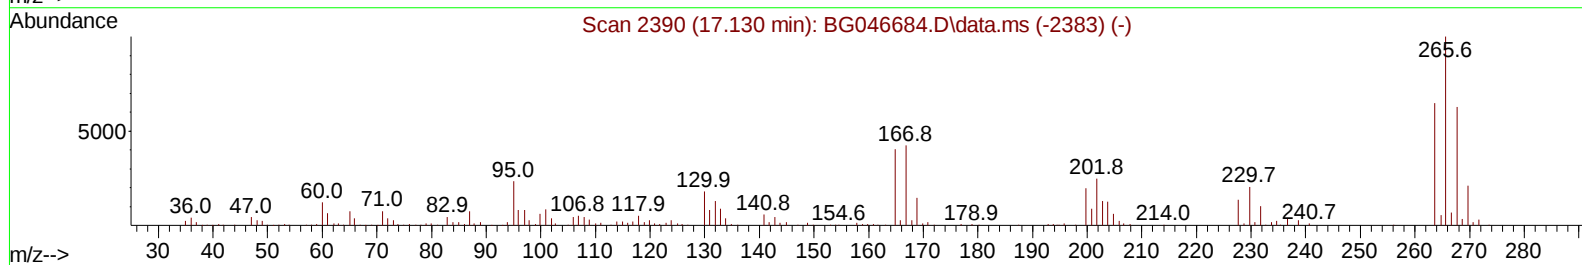
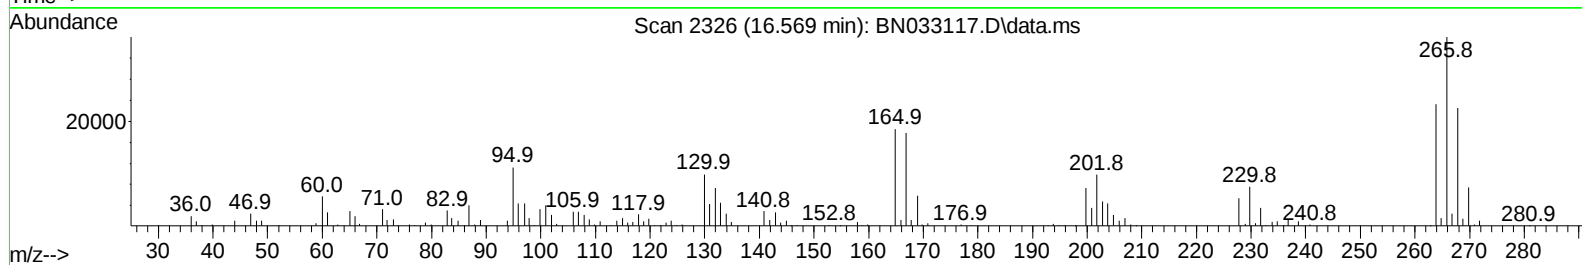


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073124\
Data File : BN033117.D
Acq On : 30 Jul 2024 22:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jul 31 04:17:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 04:17:18 2024
Response via : Initial Calibration

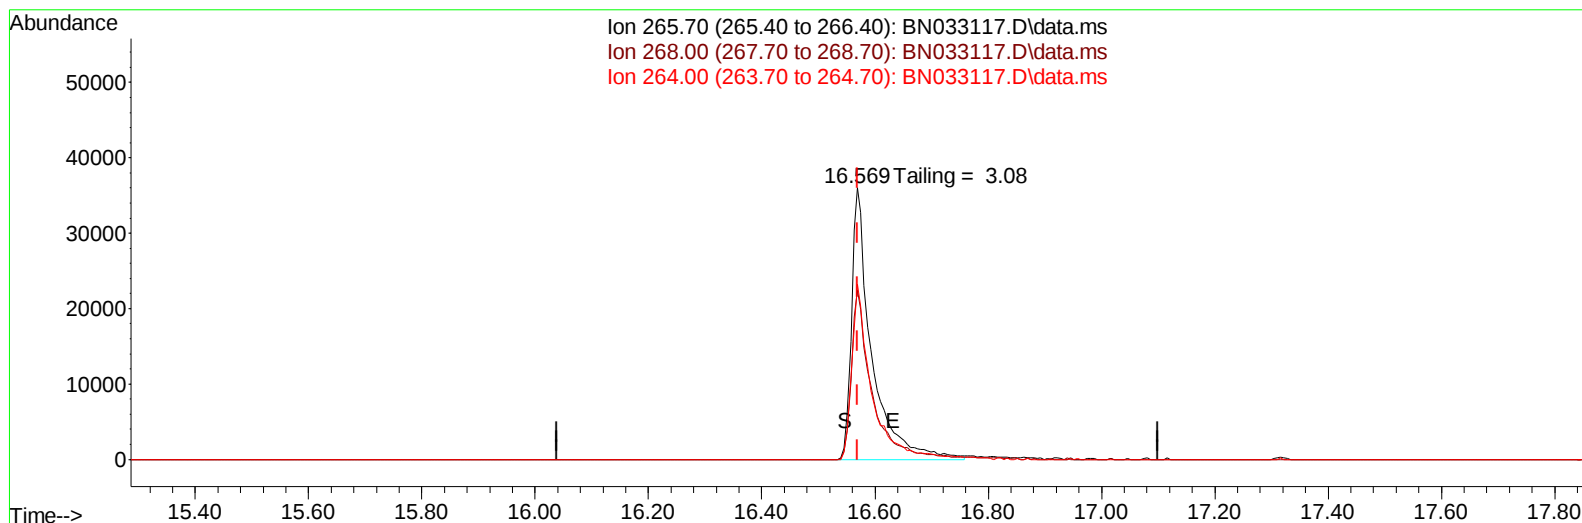




TIC: BN033117.D\data.ms

(70) Pentachlorophenol (C)**16.569min (0.000) 16889.42 ng****response 87479**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.42
264.00	61.60	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073124\
Data File : BN033117.D
Acq On : 30 Jul 2024 22:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jul 31 04:17:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 04:17:18 2024
Response via : Initial Calibration

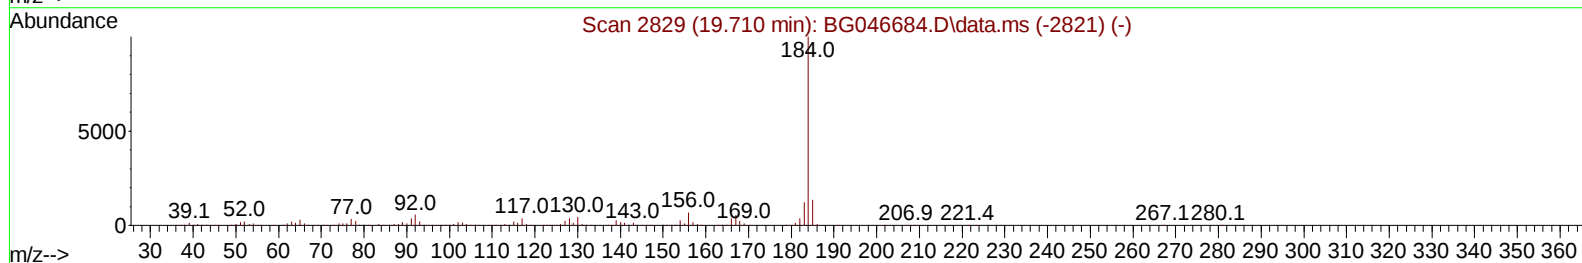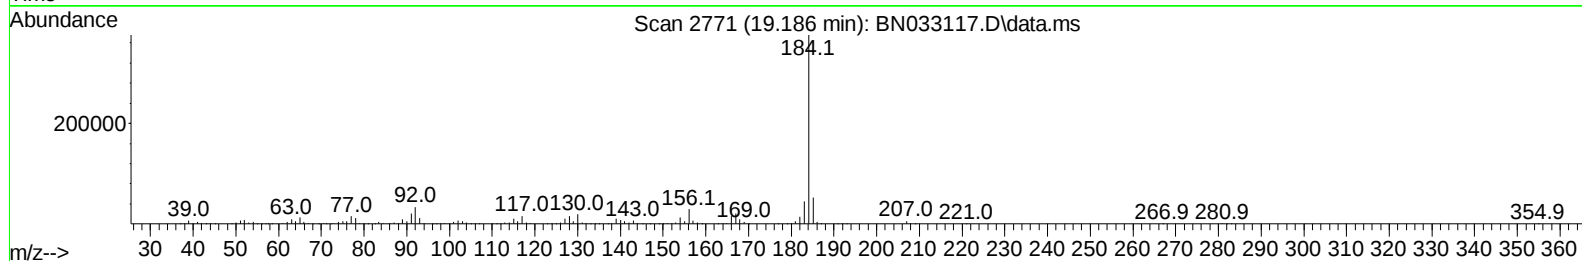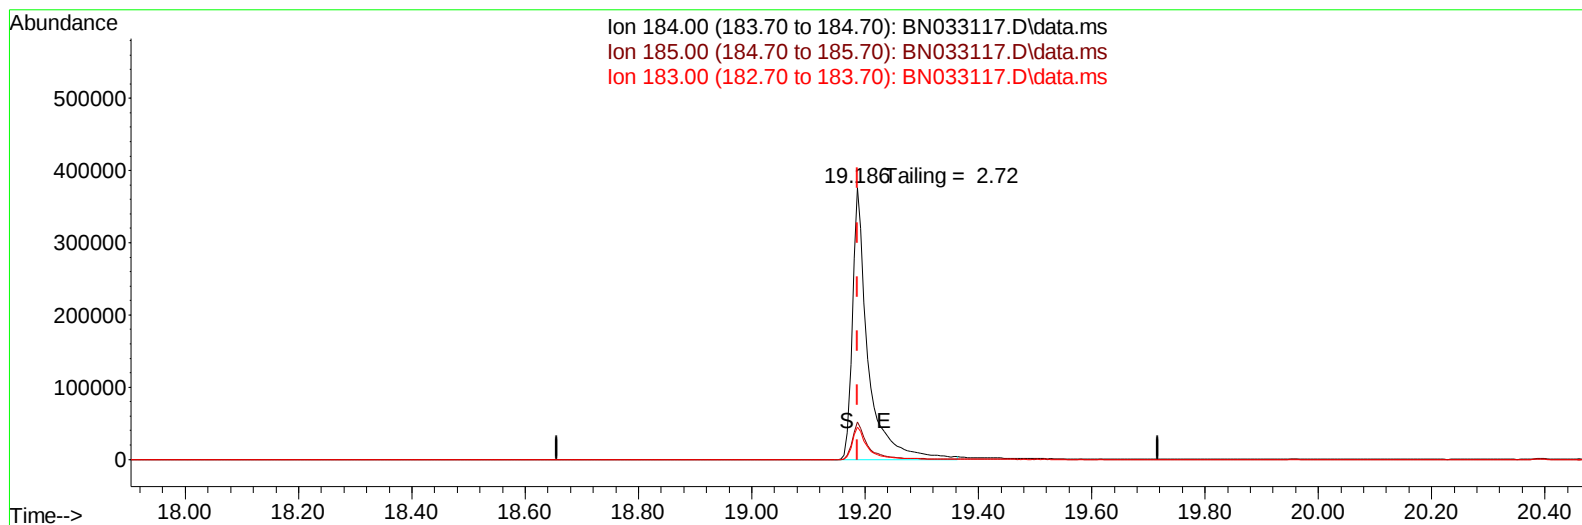

TIC: BN033117.D\data.ms

(77) Benzidine

19.186min (0.000) 0.00 ng

response 732781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	11.90
0.00	0.00	0.00