


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073124\
Data File : BN033117.D
Acq On : 30 Jul 2024 22:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 29 10:37:08 2024

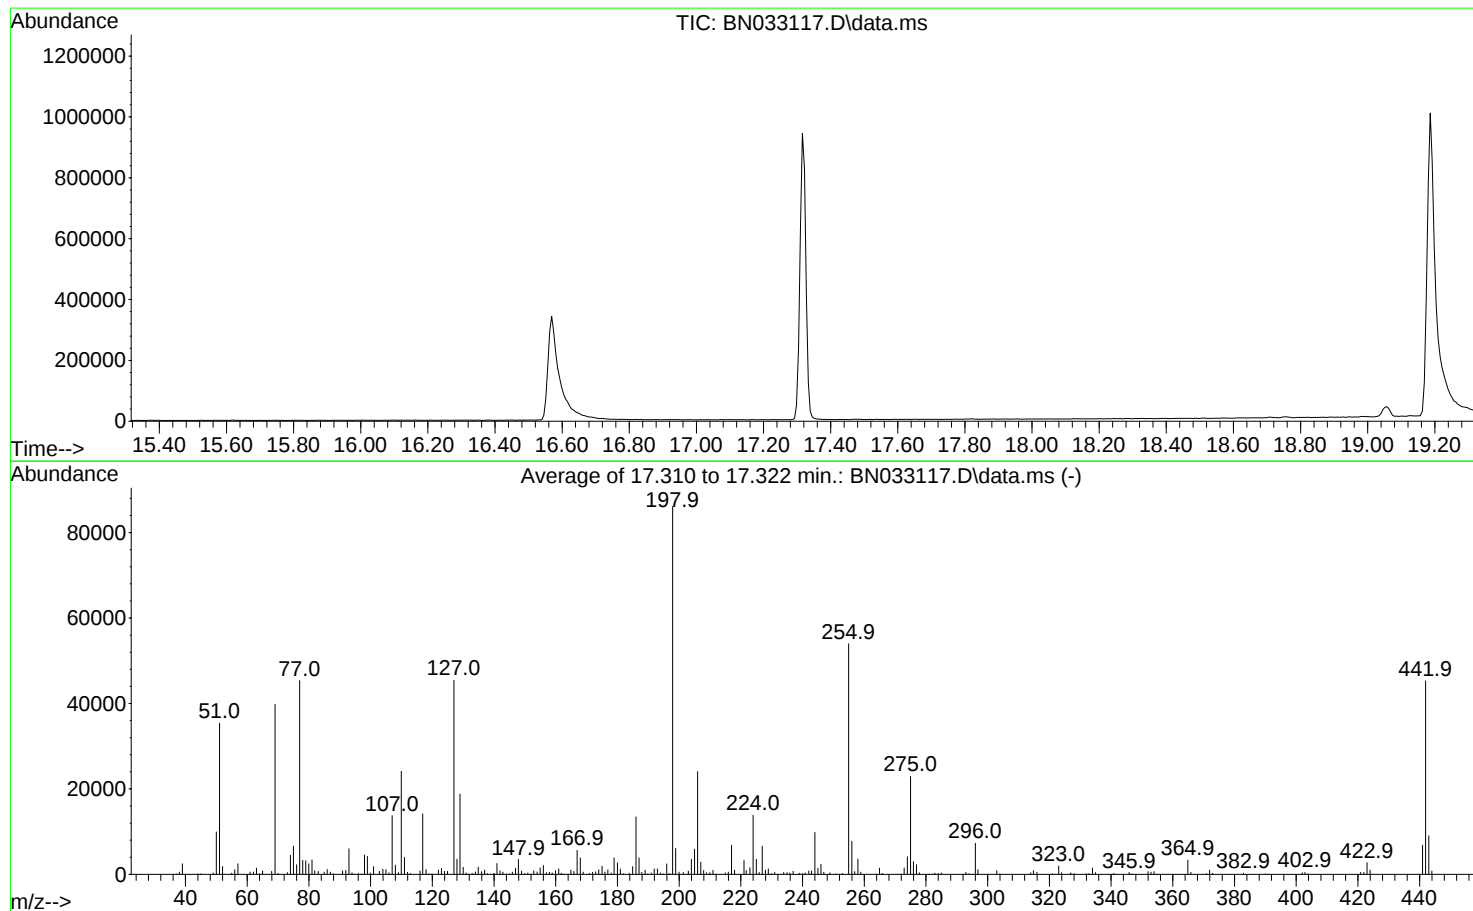




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	35397	PASS
68	69	0.00	2	1.8	698	PASS
69	198	0.00	100	46.2	39765	PASS
70	69	0.00	2	0.6	222	PASS
127	198	10	80	52.8	45435	PASS
197	198	0.00	2	0.2	166	PASS
198	198	100	100	100.0	86104	PASS
199	198	5	9	7.0	6058	PASS
275	198	10	60	26.6	22936	PASS
365	198	1	100	3.9	3352	PASS
441	198	0.01	100	7.9	6832	PASS
442	442	50	100	100.0	45299	PASS
443	442	15	24	19.9	9028	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073124\
Data File : BN033117.D
Acq On : 30 Jul 2024 22:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 31 04:17:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 04:17:18 2024
Response via : Initial Calibration

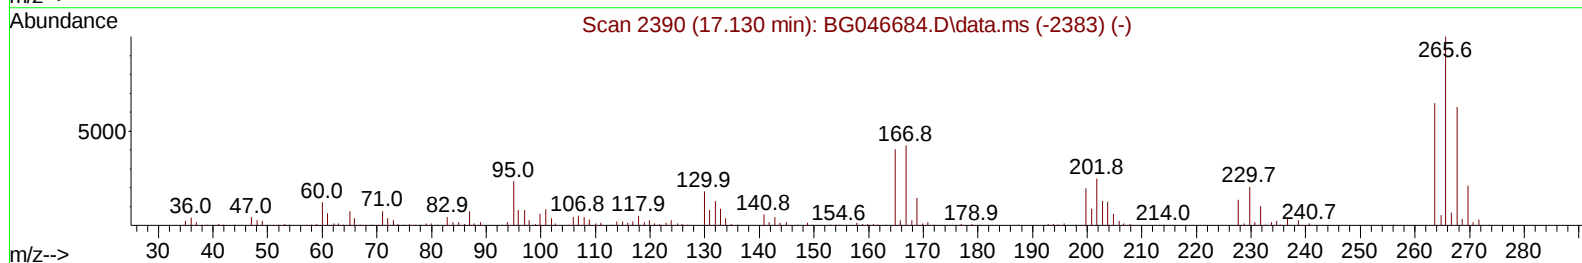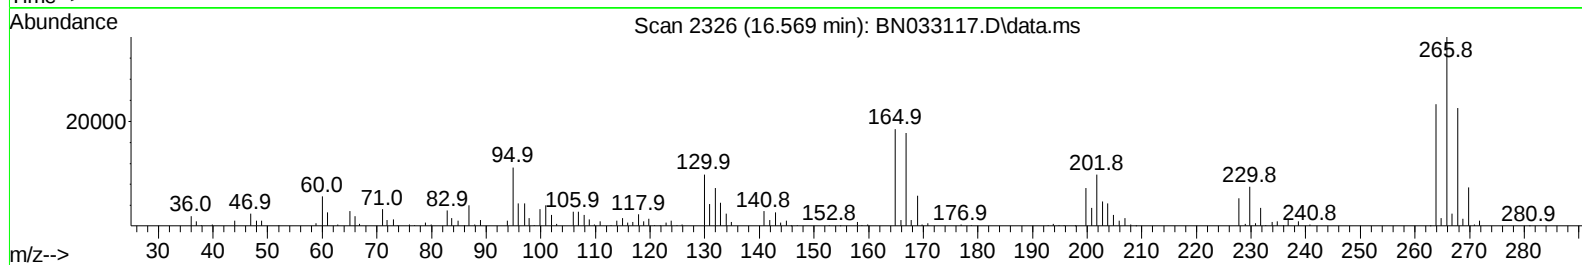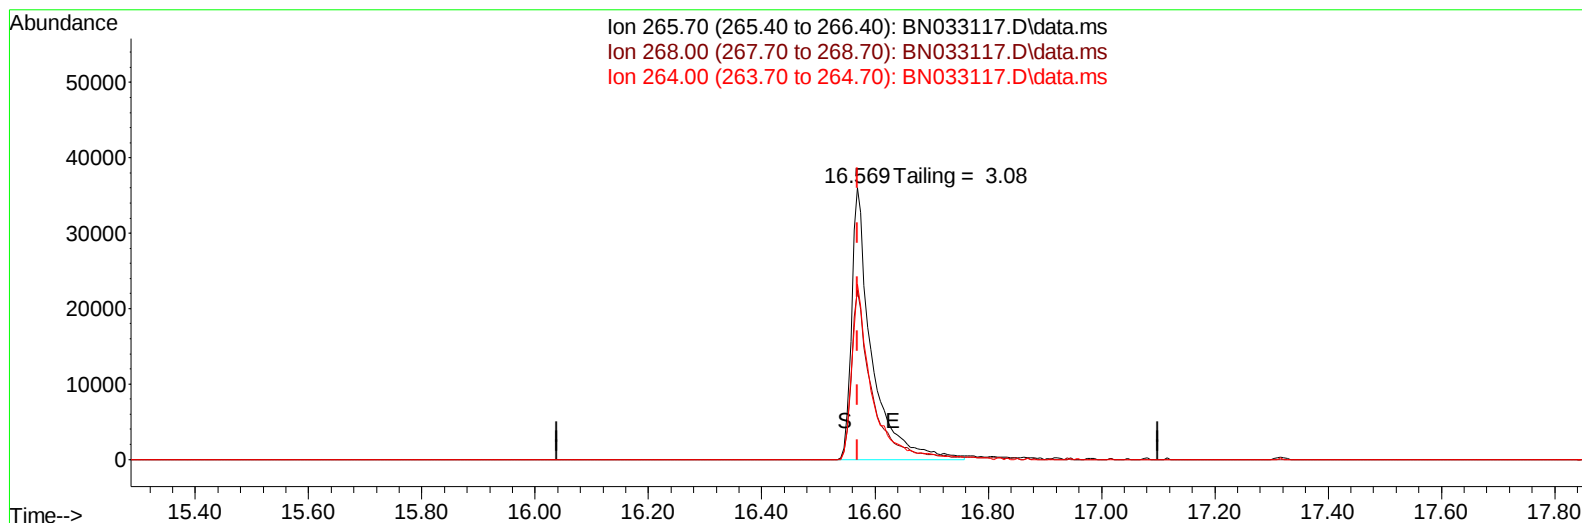

TIC: BN033117.D\data.ms

(70) Pentachlorophenol (C)

16.569min (0.000) 16889.42 ng




response 87479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.42
264.00	61.60	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073124\
Data File : BN033117.D
Acq On : 30 Jul 2024 22:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 31 04:17:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 04:17:18 2024
Response via : Initial Calibration

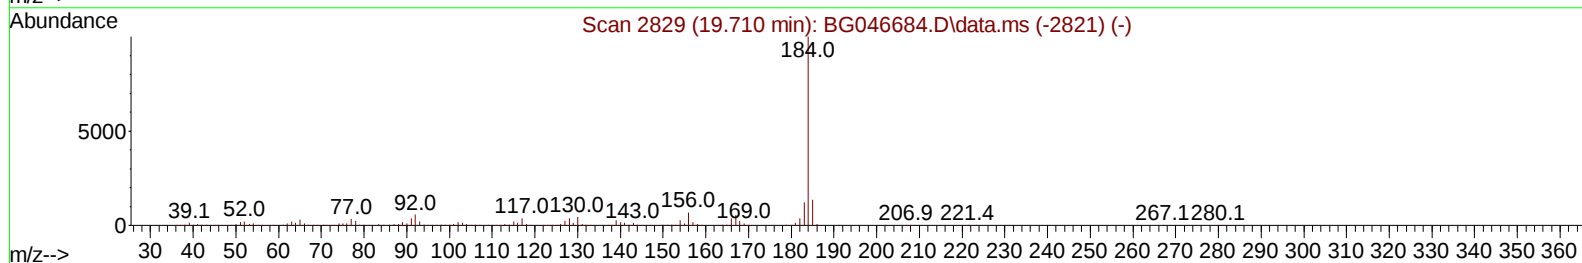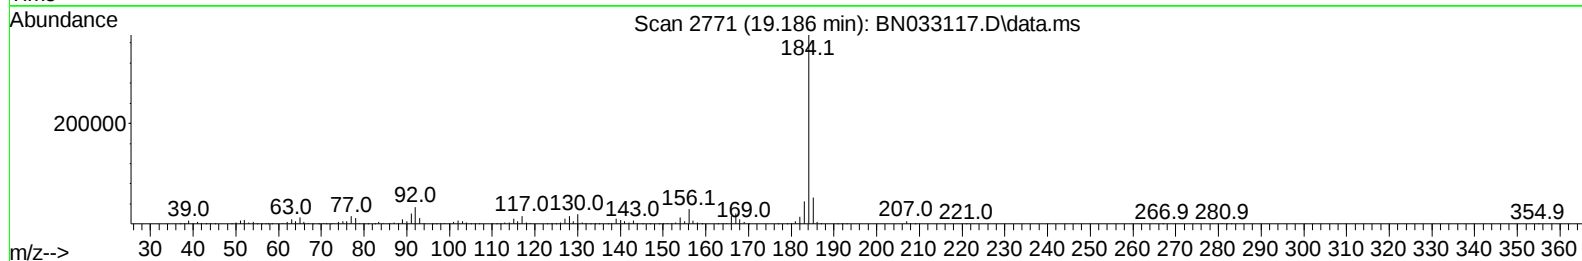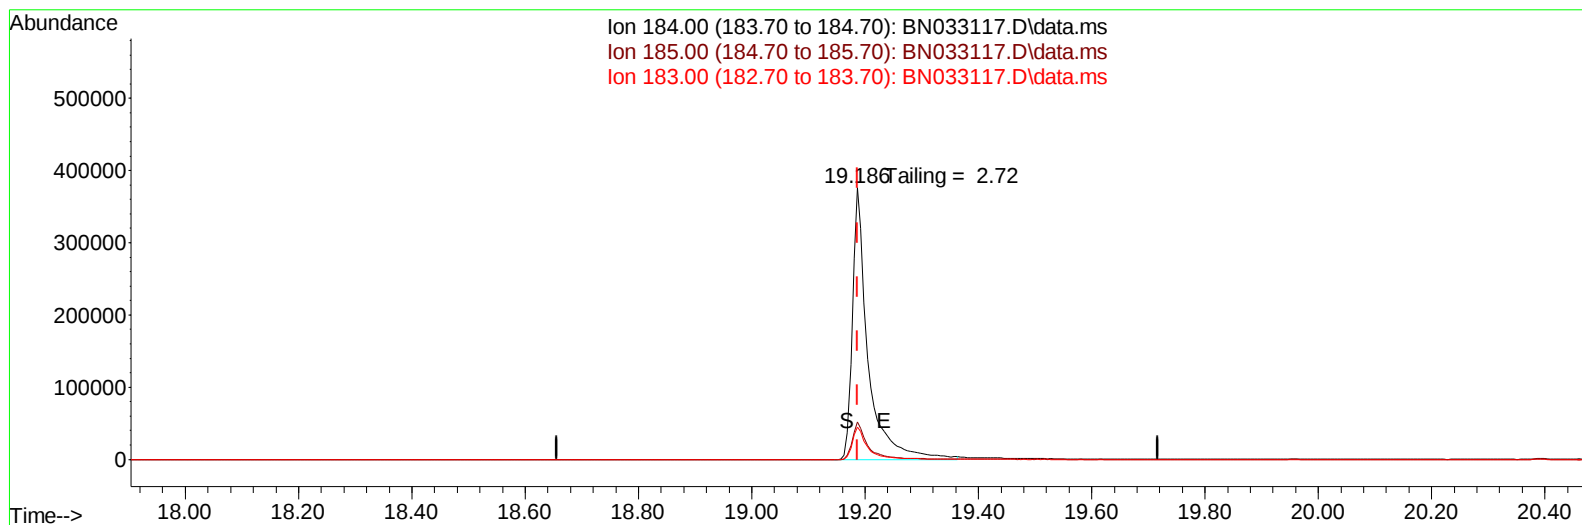

TIC: BN033117.D\data.ms

(77) Benzidine

19.186min (0.000) 0.00 ng

response 732781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2024	BNA_N	<u>BN033117.D</u>
Compound Name	Response	Retention Time
DDT	249153	20.392
DDD	58168	19.963
DDE	6362	19.439
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
64530	313683	20.57

Instrument :
BNA_N
ClientSampleId :
DFTPP