


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080123\
Data File : BN026772.D
Acq On : 01 Aug 2023 07:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 00:35:47 2023

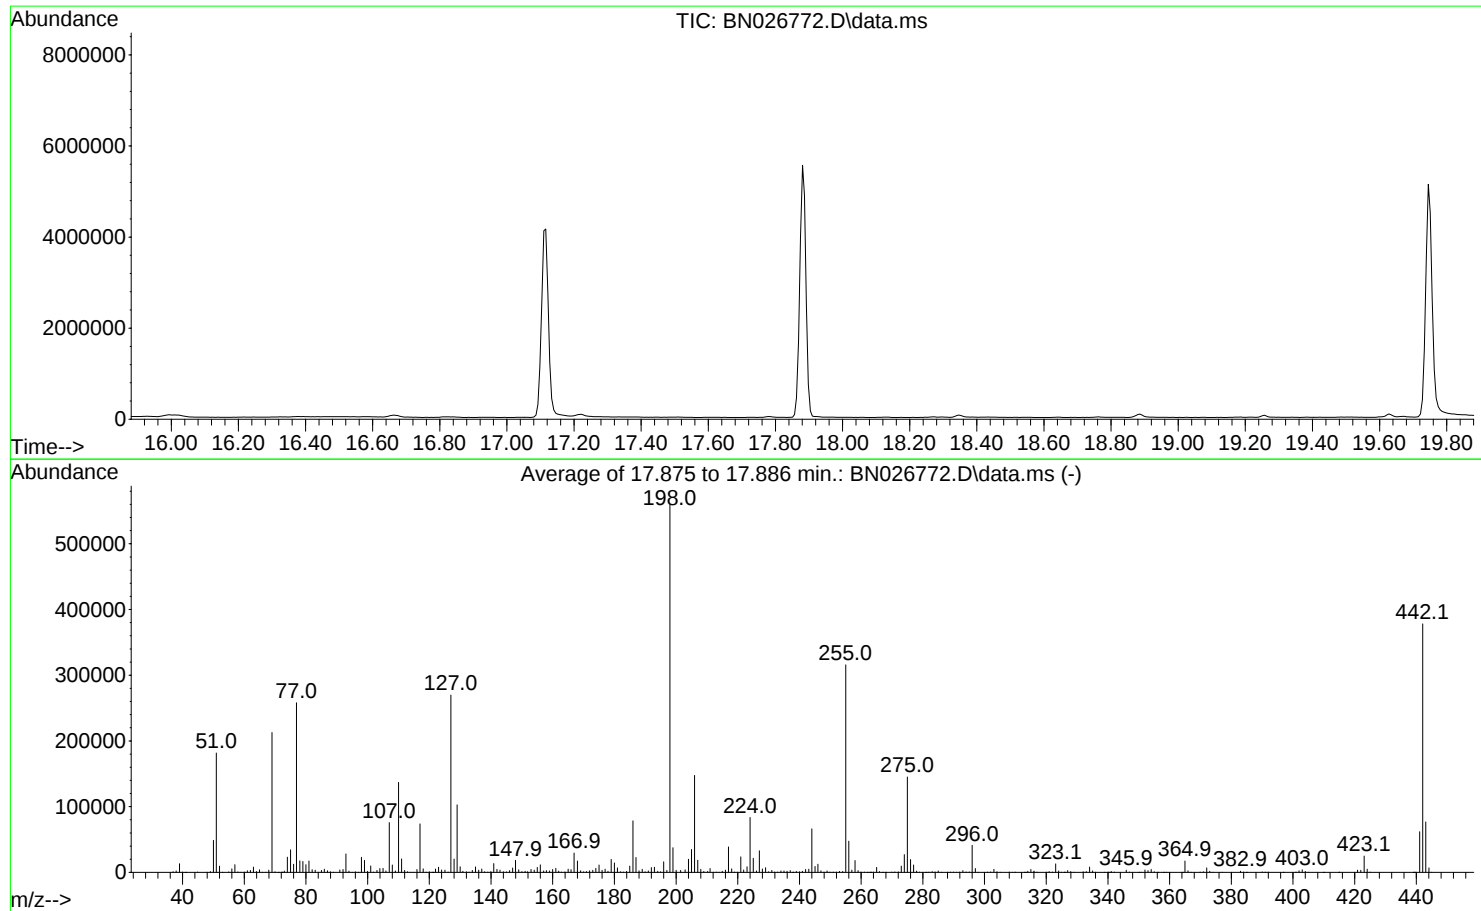




AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	181639	PASS
68	69	0.00	2	1.7	3539	PASS
69	198	0.00	100	38.0	212795	PASS
70	69	0.00	2	0.5	991	PASS
127	198	10	80	48.2	269909	PASS
197	198	0.00	2	0.5	2887	PASS
198	198	100	100	100.0	559765	PASS
199	198	5	9	6.7	37515	PASS
275	198	10	60	25.9	145037	PASS
365	198	1	100	3.1	17376	PASS
441	198	0.01	100	11.1	61939	PASS
442	442	50	100	100.0	378176	PASS
443	442	15	24	20.3	76720	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080123\
Data File : BN026772.D
Acq On : 01 Aug 2023 07:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 01:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 01:19:36 2023
Response via : Initial Calibration

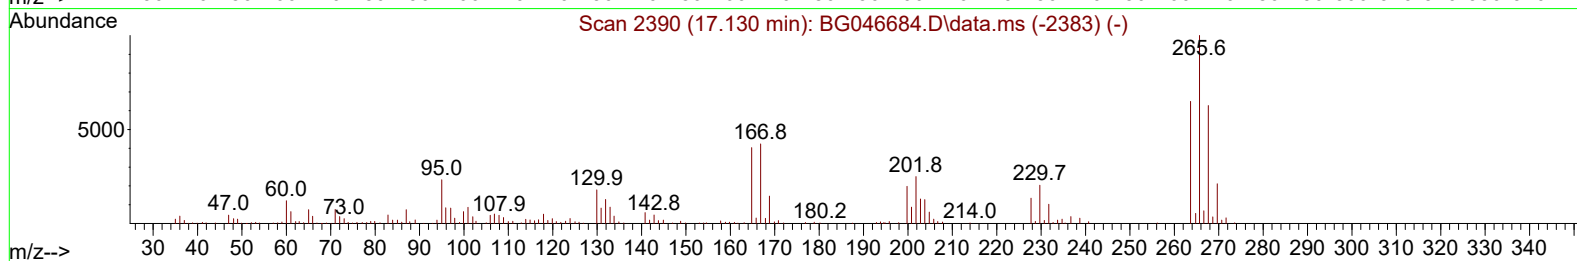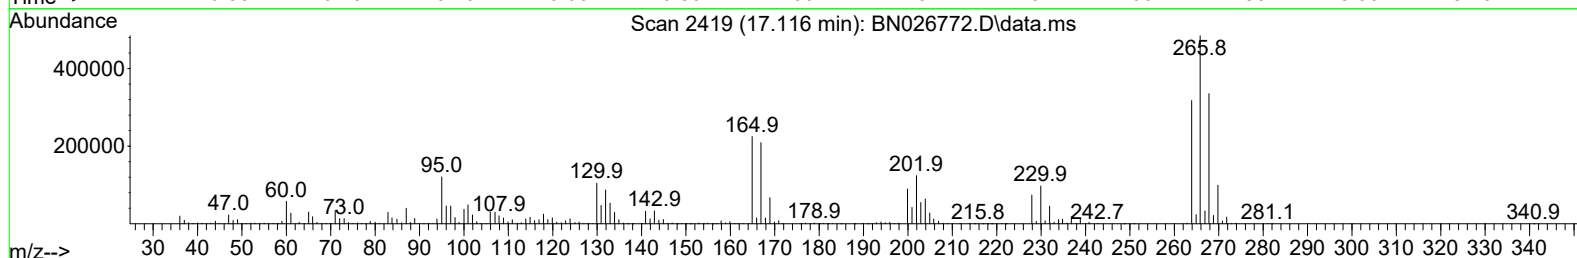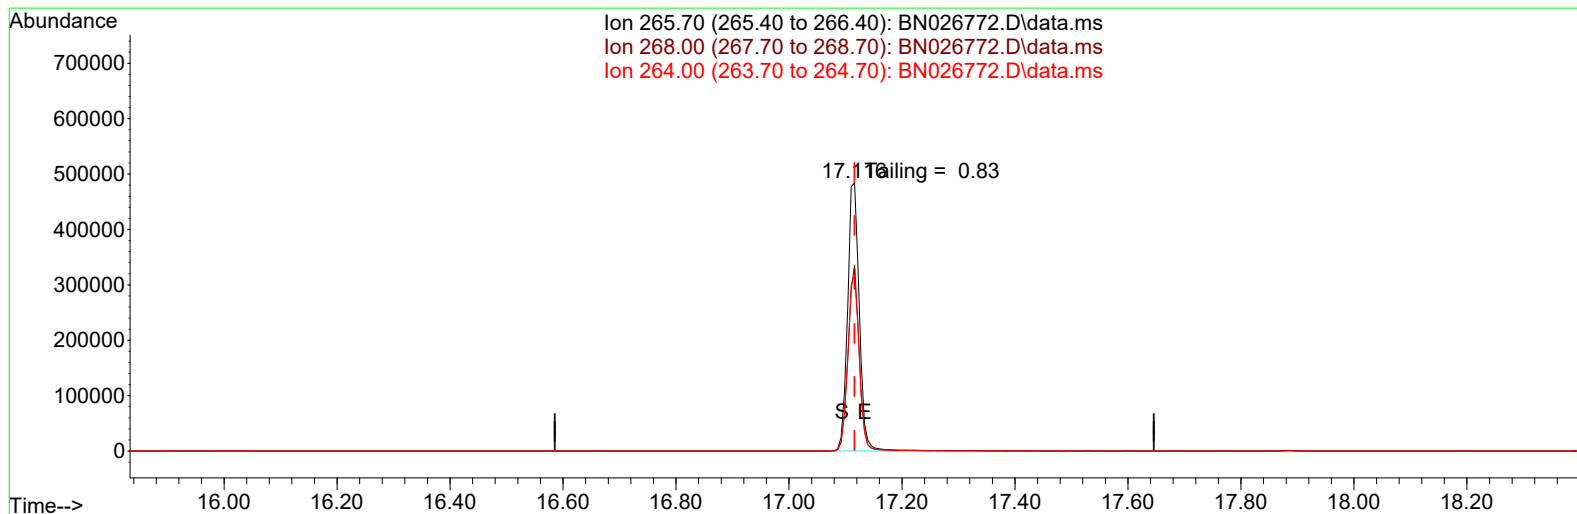

TIC: BN026772.D\data.ms

(70) Pentachlorophenol (C)

17.116min (0.000) 25386.37 ng




response 701275

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.21
264.00	61.60	65.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080123\
Data File : BN026772.D
Acq On : 01 Aug 2023 07:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 01:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 01:19:36 2023
Response via : Initial Calibration

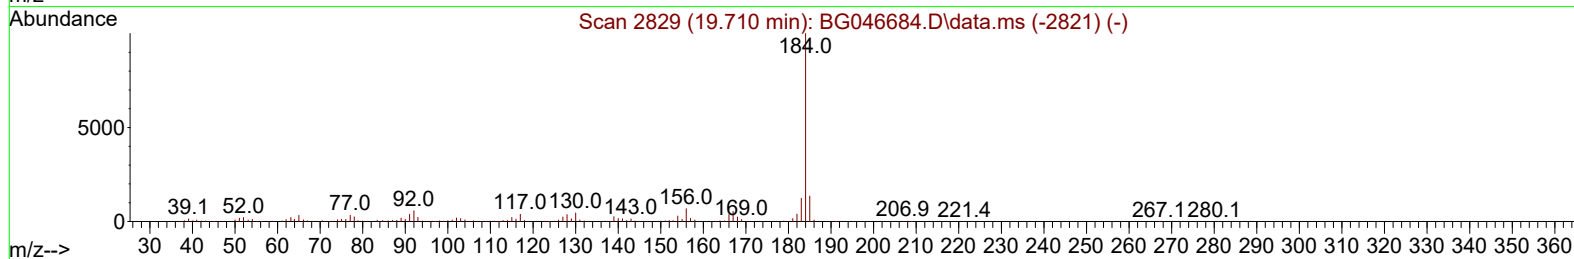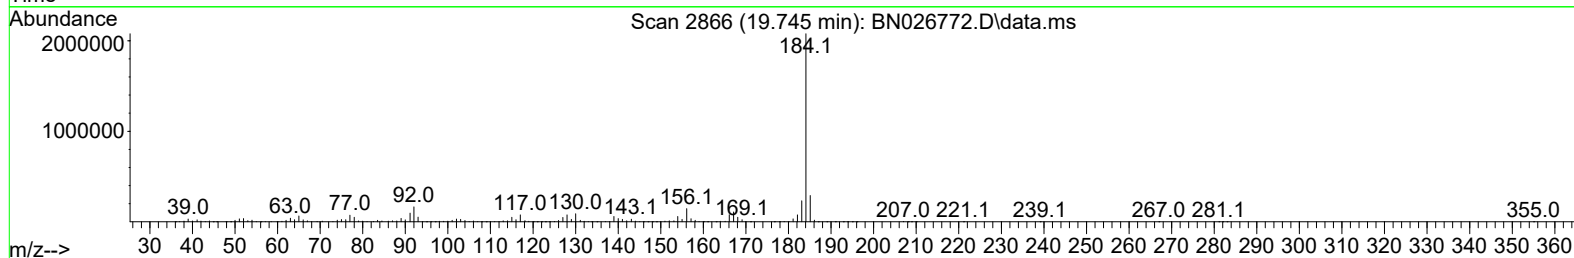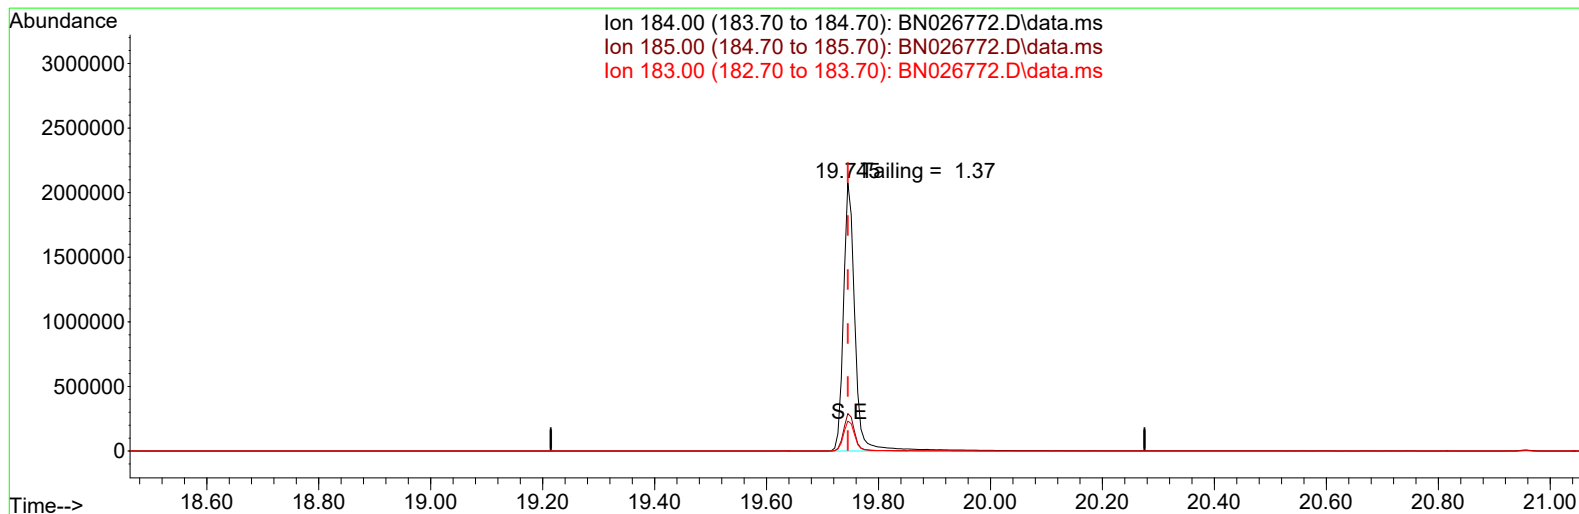

TIC: BN026772.D\data.ms

(77) Benzidine

19.745min (0.000) 0.00 ng

response 2997095

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/1/2023	BNA_N	<u>BN026772.D</u>
Compound Name	Response	Retention Time
DDT	1749815	20.957
DDD	15420	20.563
DDE	662	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16082	1765897	0.91

Instrument :
BNA_N
ClientSampleId :
DFTPP