
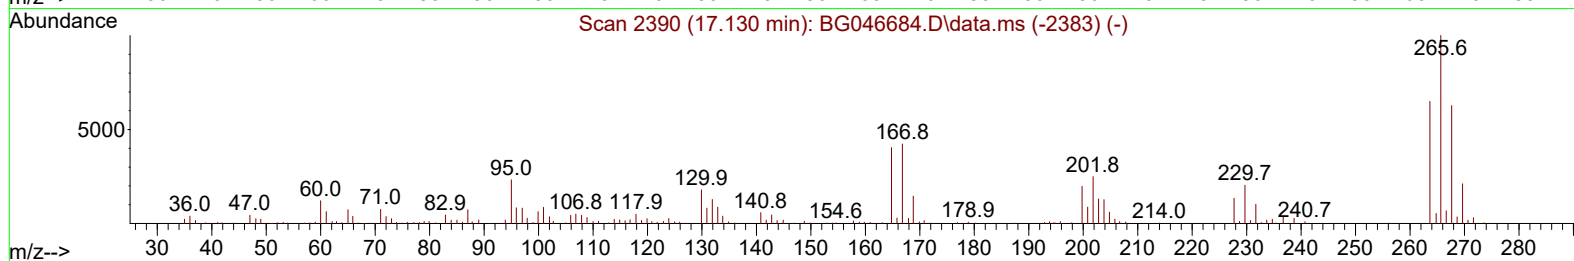
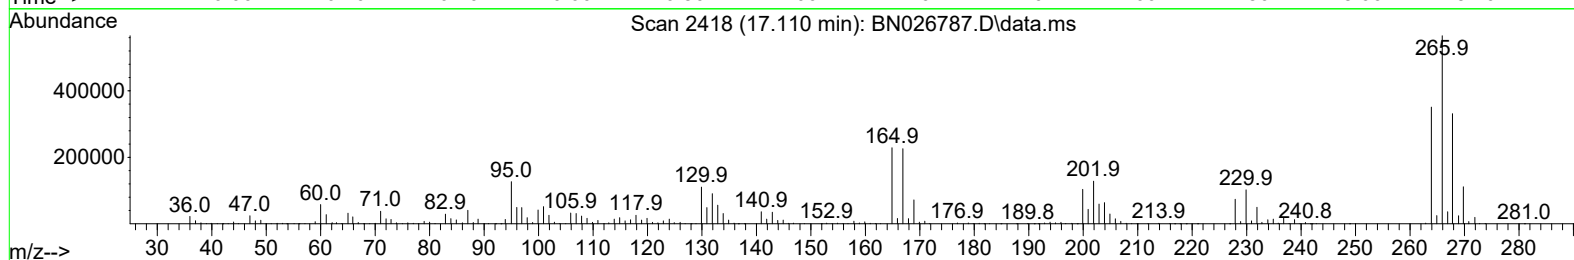


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN080223\  
Data File : BN026787.D  
Acq On : 02 Aug 2023 07:16  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 01:33:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 03 01:33:44 2023  
Response via : Initial Calibration

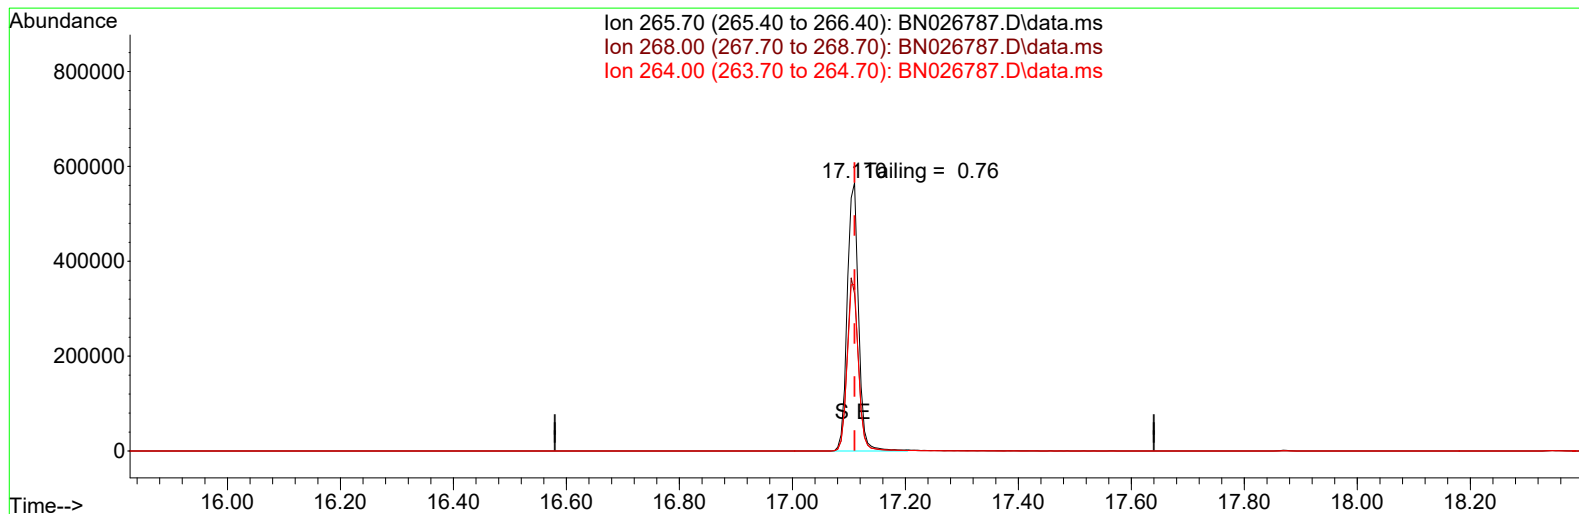

TIC: BN026787.D\data.ms

**(70) Pentachlorophenol (C)**




17.110min ( 0.000) 27541.78 ng

response 785240

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 58.61  |
| 264.00 | 61.60  | 62.09  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN080223\  
Data File : BN026787.D  
Acq On : 02 Aug 2023 07:16  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 01:33:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 03 01:33:44 2023  
Response via : Initial Calibration

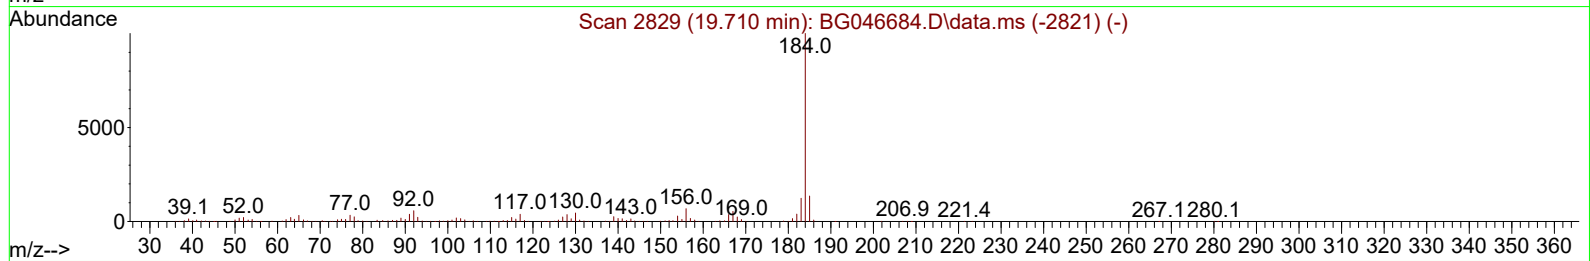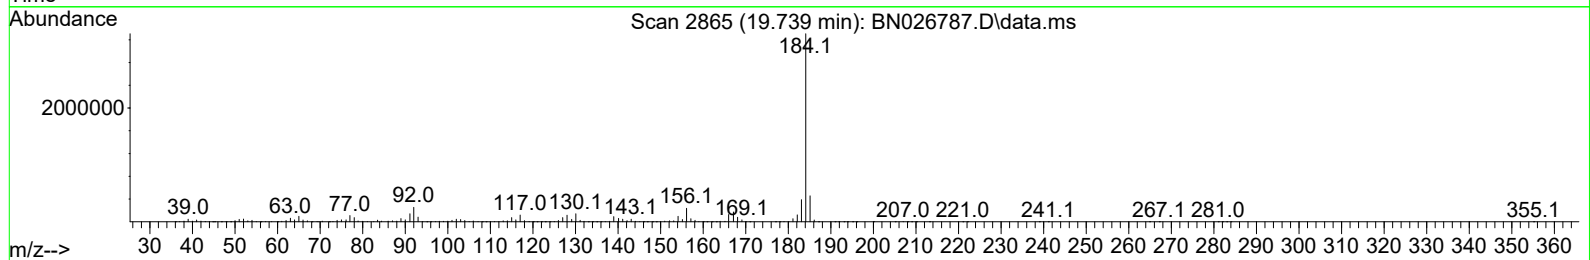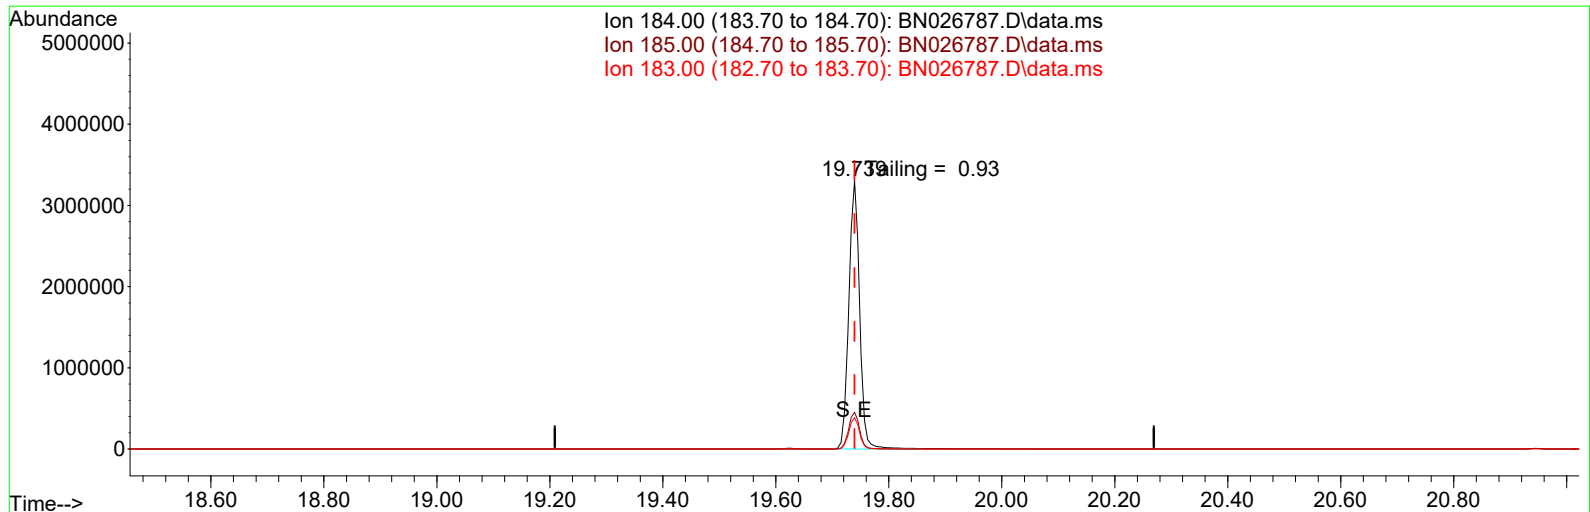

TIC: BN026787.D\data.ms

**(77) Benzidine****19.739min ( 0.000) 124787.70 ng****response 4396695**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.75  |
| 183.00 | 13.20  | 11.71  |
| 0.00   | 0.00   | 0.00   |