
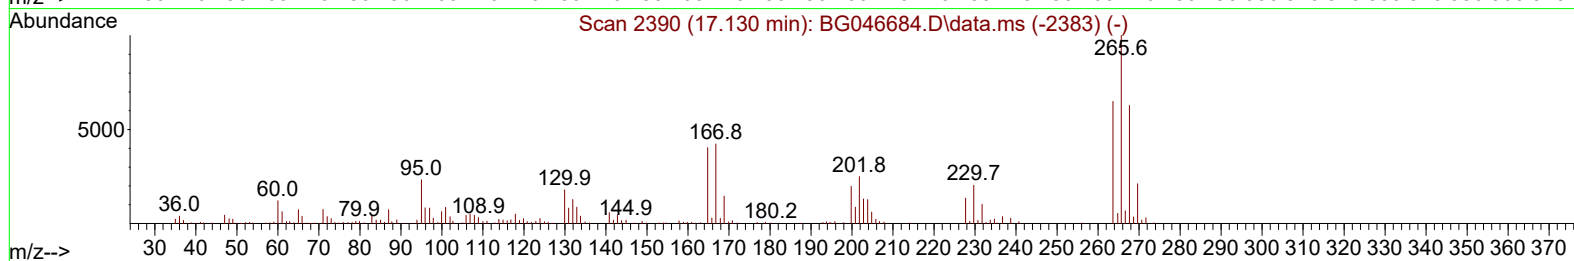
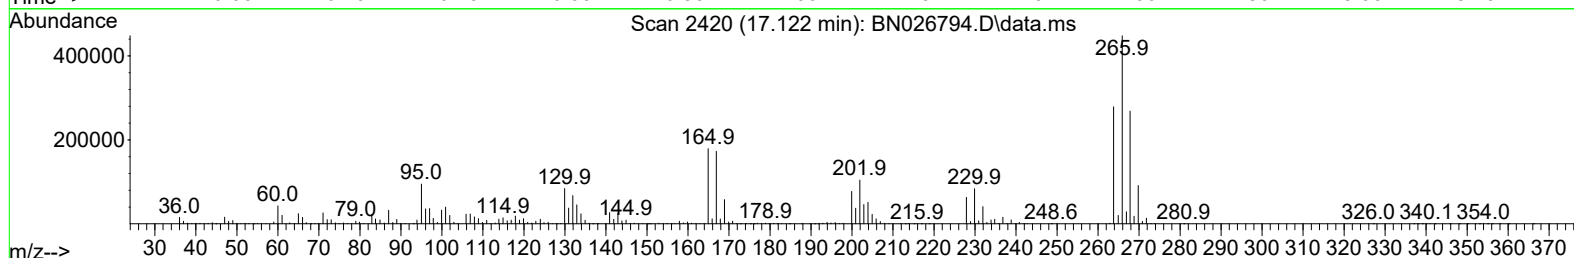


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026794.D
Acq On : 02 Aug 2023 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 01:35:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 01:33:44 2023
Response via : Initial Calibration

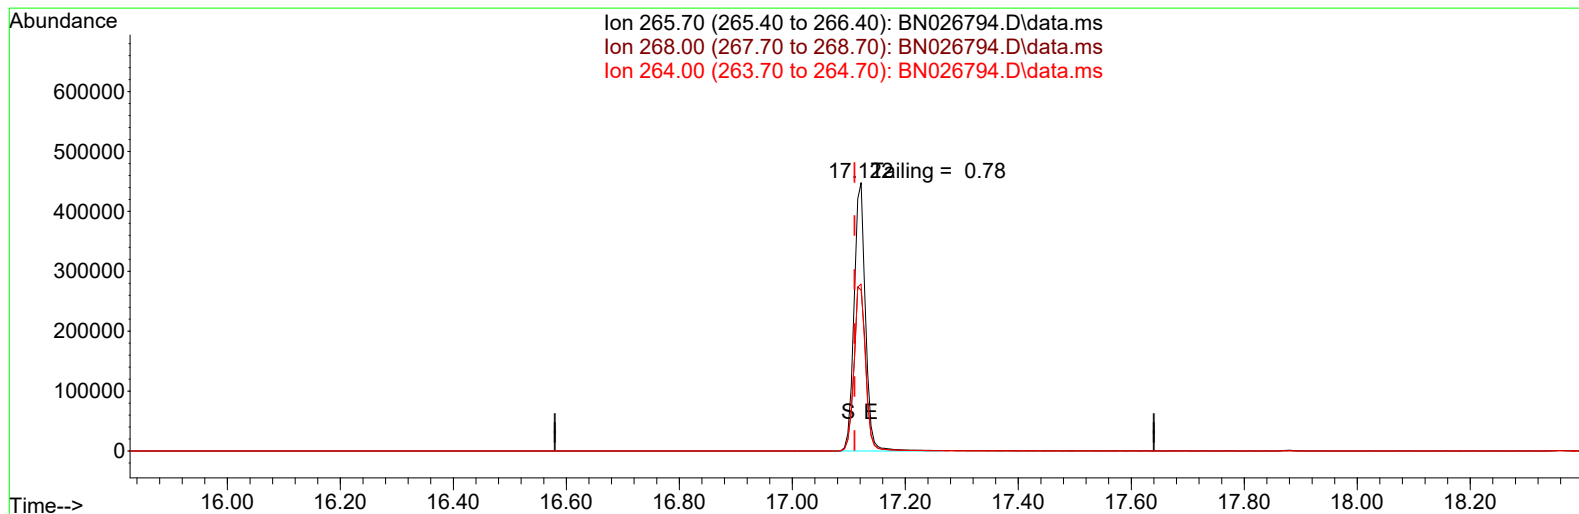

TIC: BN026794.D\data.ms

(70) Pentachlorophenol (C)




17.122min (+ 0.012) 23656.20 ng

response 630646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.93
264.00	61.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026794.D
Acq On : 02 Aug 2023 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 01:35:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 01:33:44 2023
Response via : Initial Calibration

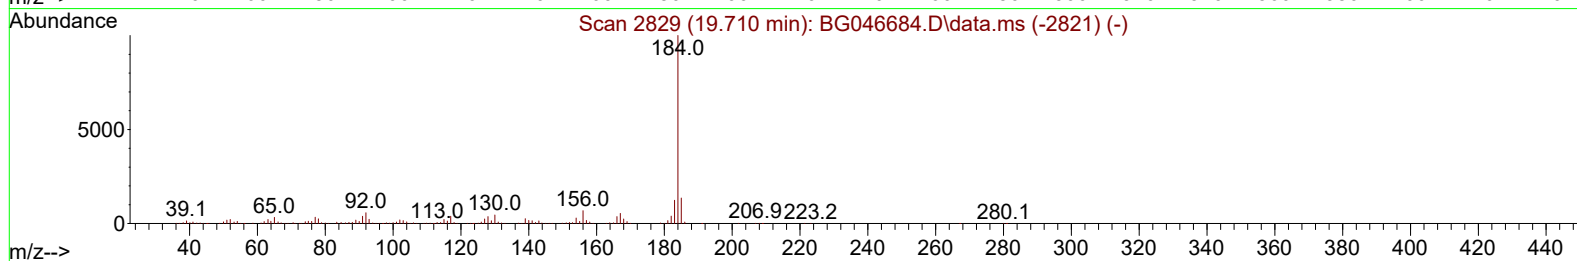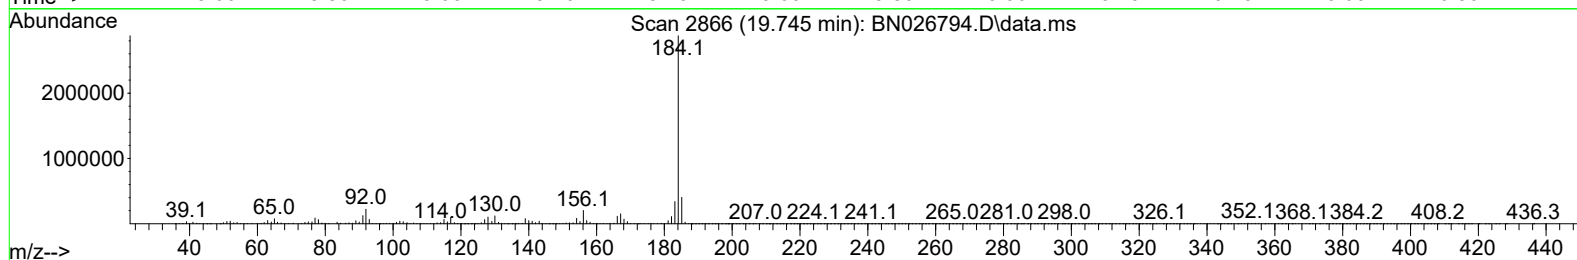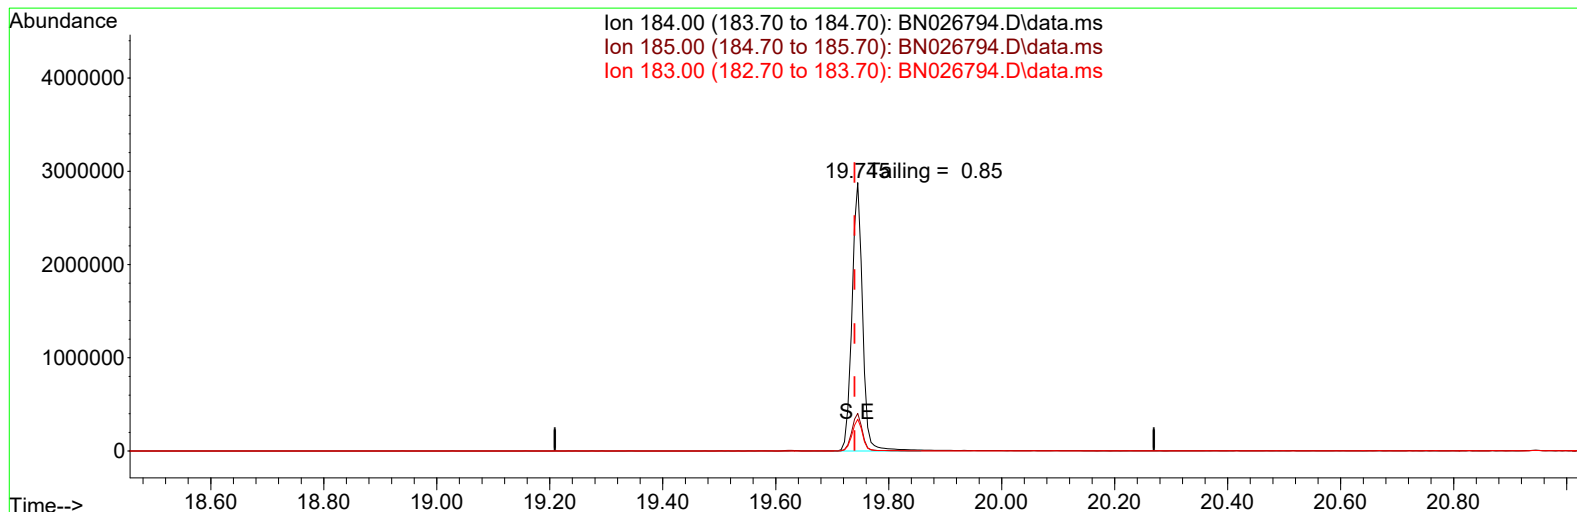

TIC: BN026794.D\data.ms

(77) Benzidine**19.745min (+ 0.006) 465522.66 ng****response 3788376**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	11.86
0.00	0.00	0.00