


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026787.D
Acq On : 02 Aug 2023 07:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 00:35:47 2023

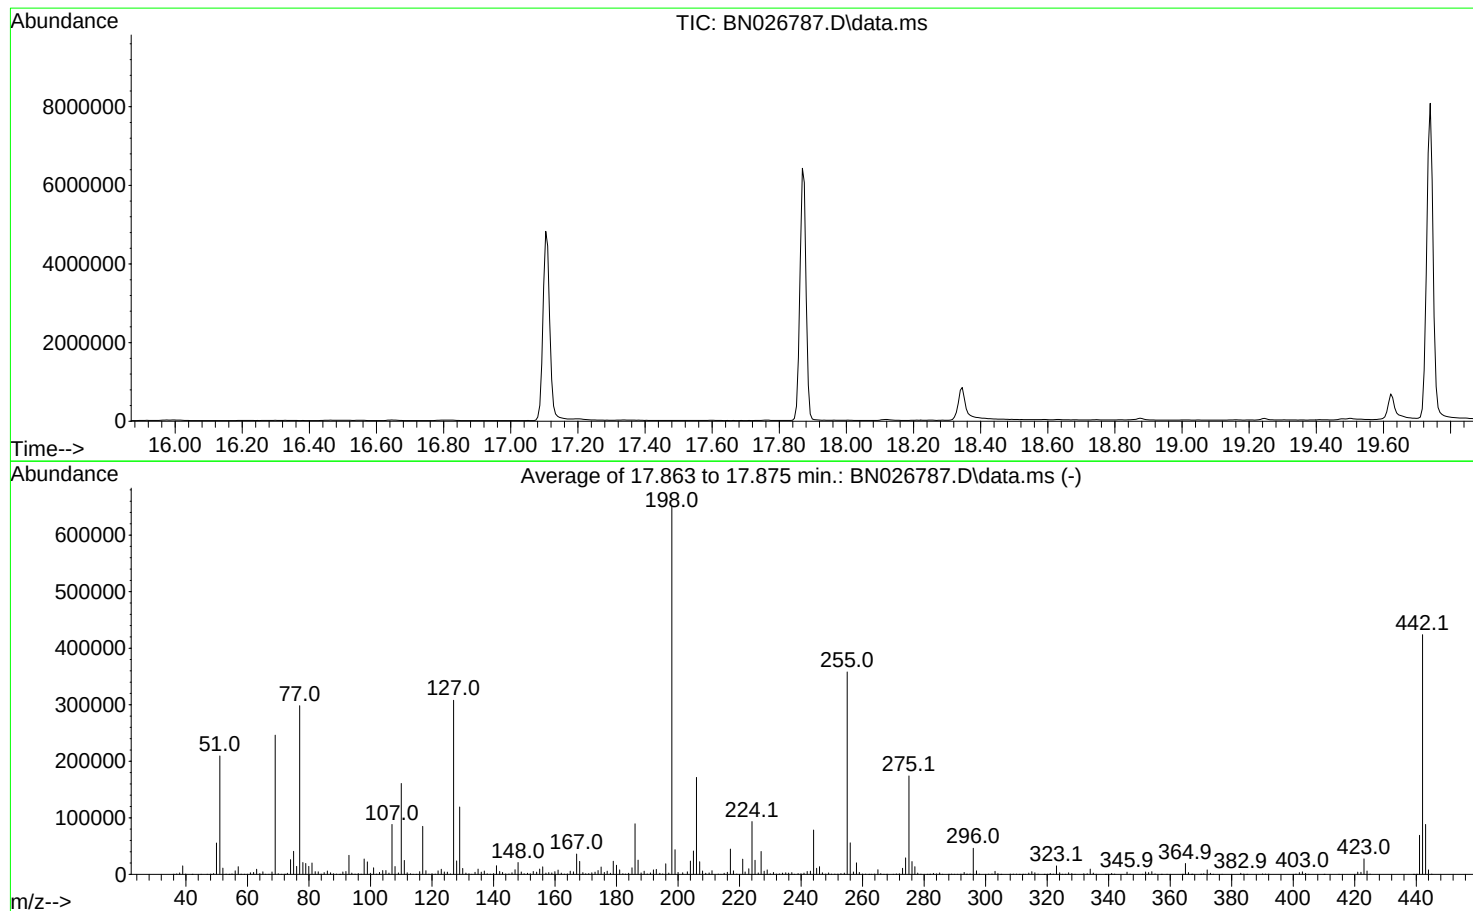




AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	209334	PASS
68	69	0.00	2	1.7	4181	PASS
69	198	0.00	100	37.9	246266	PASS
70	69	0.00	2	0.5	1160	PASS
127	198	10	80	47.3	307947	PASS
197	198	0.00	2	0.4	2345	PASS
198	198	100	100	100.0	650624	PASS
199	198	5	9	6.7	43707	PASS
275	198	10	60	26.7	173939	PASS
365	198	1	100	3.0	19422	PASS
441	198	0.01	100	10.6	69035	PASS
442	442	50	100	100.0	423829	PASS
443	442	15	24	20.8	88181	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026787.D
Acq On : 02 Aug 2023 07:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 01:33:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 01:33:44 2023
Response via : Initial Calibration

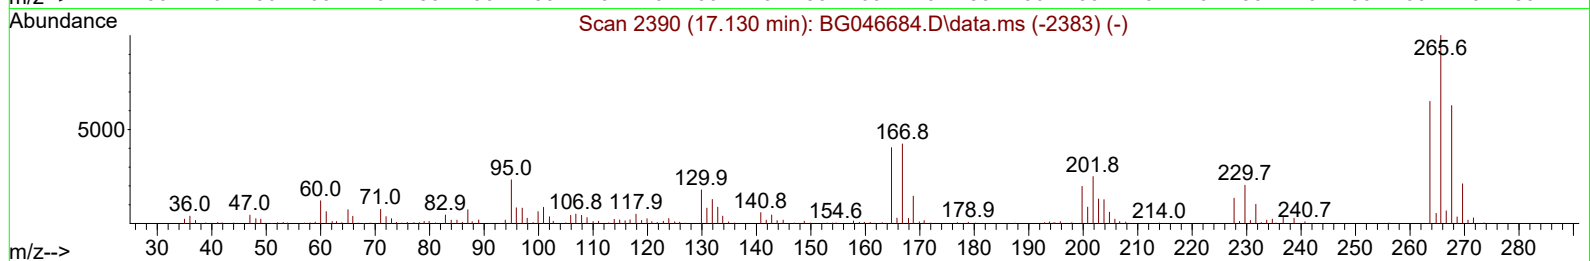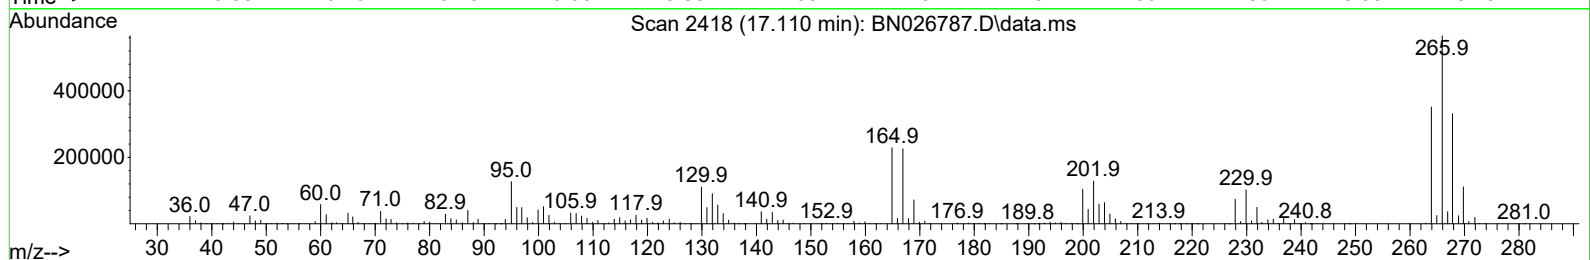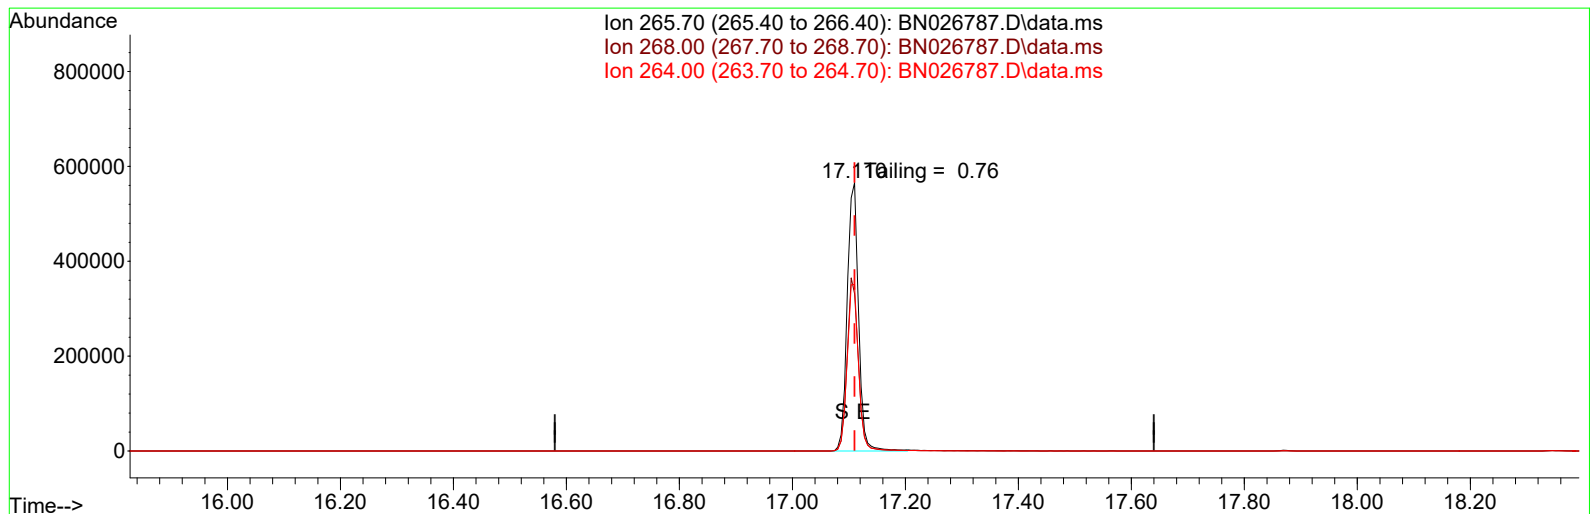

TIC: BN026787.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 27541.78 ng




response 785240

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.61
264.00	61.60	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
 Data File : BN026787.D
 Acq On : 02 Aug 2023 07:16
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 01:33:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 03 01:33:44 2023
 Response via : Initial Calibration

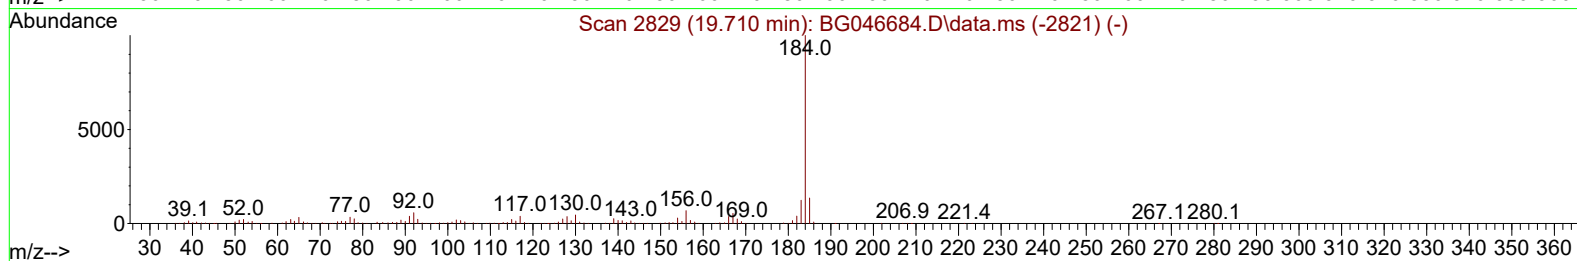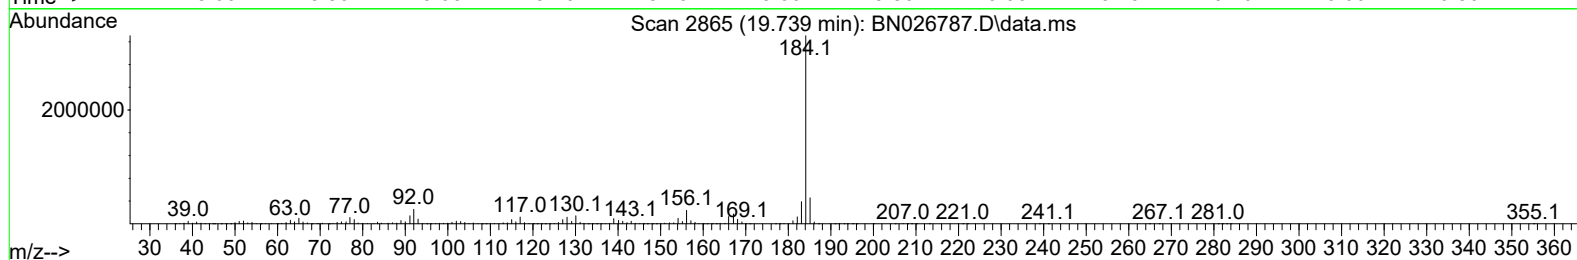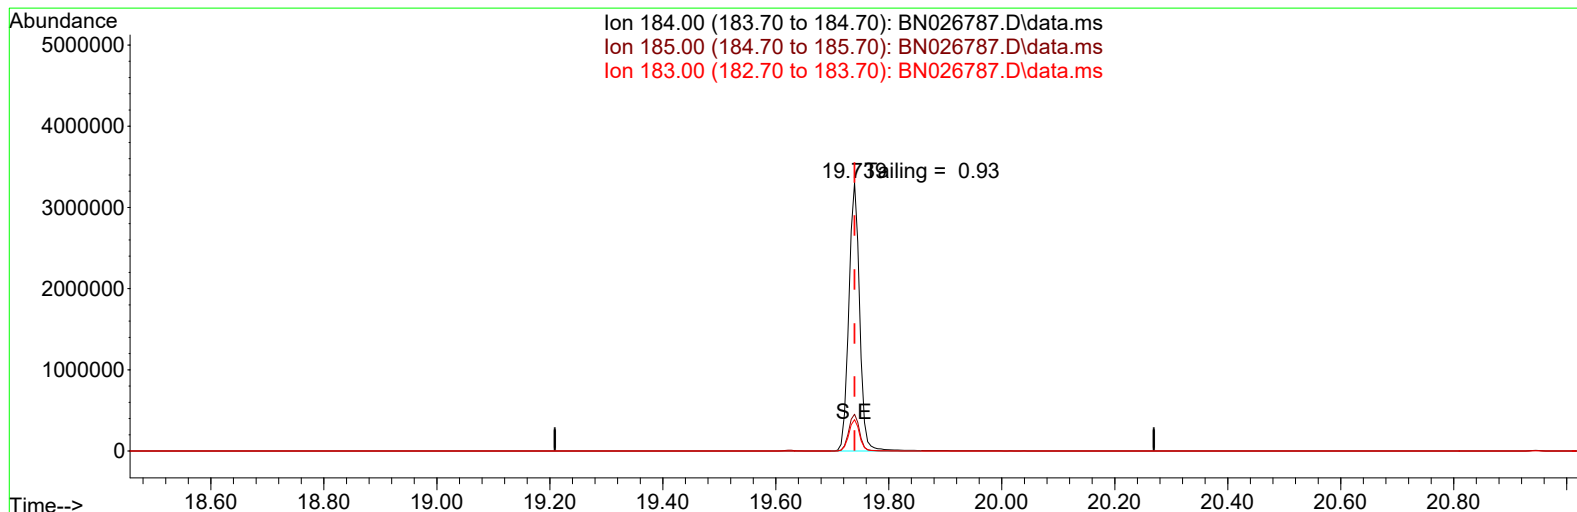

TIC: BN026787.D\data.ms

(77) Benzidine

19.739min (0.000) 124787.70 ng

response 4396695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_N	<u>BN026787.D</u>
Compound Name	Response	Retention Time
DDT	1960955	20.945
DDD	44883	20.504
DDE	2568	19.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47451	2008406	2.36

Instrument :
BNA_N
ClientSampleId :
DFTPP