
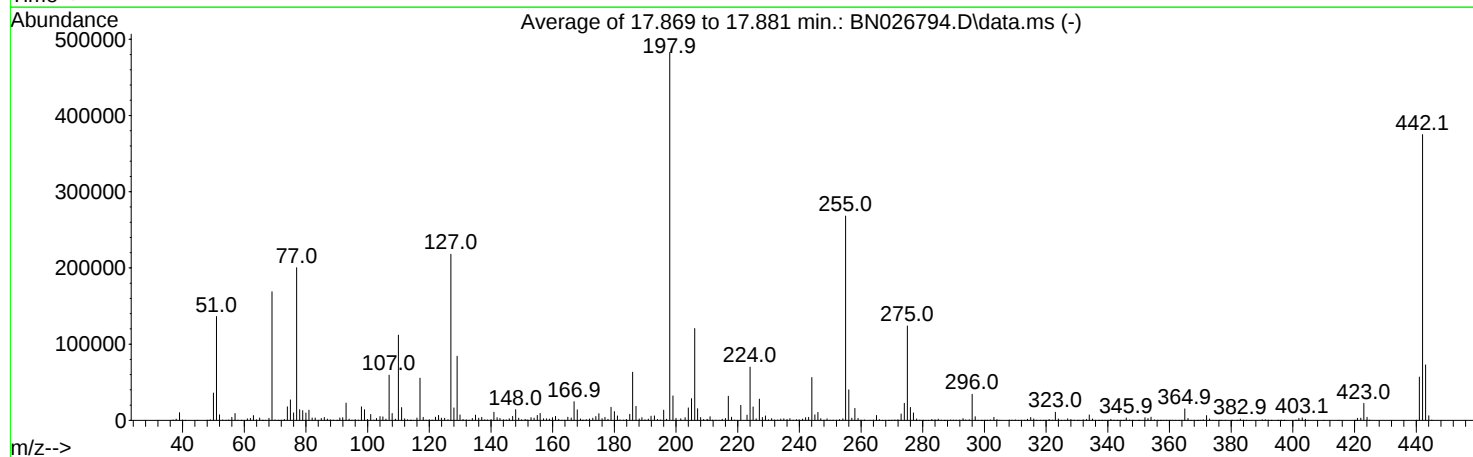


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026794.D
Acq On : 02 Aug 2023 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 00:35:47 2023

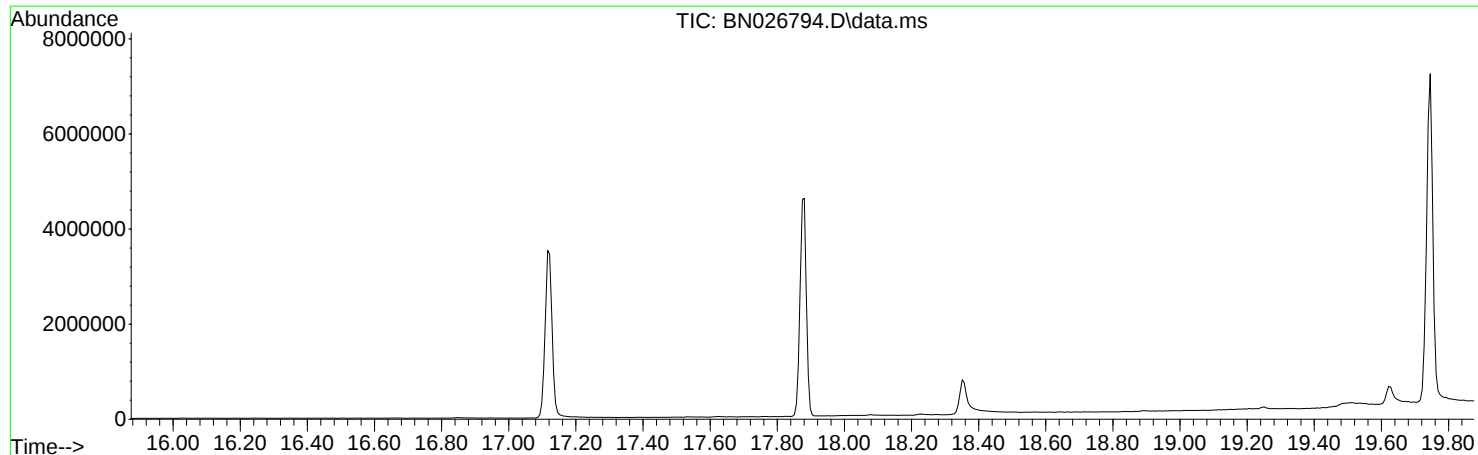




AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	136208	PASS
68	69	0.00	2	1.6	2722	PASS
69	198	0.00	100	35.0	168863	PASS
70	69	0.00	2	0.4	663	PASS
127	198	10	80	45.1	217899	PASS
197	198	0.00	2	0.3	1526	PASS
198	198	100	100	100.0	482645	PASS
199	198	5	9	6.7	32179	PASS
275	198	10	60	25.7	123941	PASS
365	198	1	100	3.1	15041	PASS
441	198	0.01	100	11.8	56808	PASS
442	442	50	100	100.0	374933	PASS
443	442	15	24	19.4	72792	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026794.D
Acq On : 02 Aug 2023 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 01:35:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 01:33:44 2023
Response via : Initial Calibration

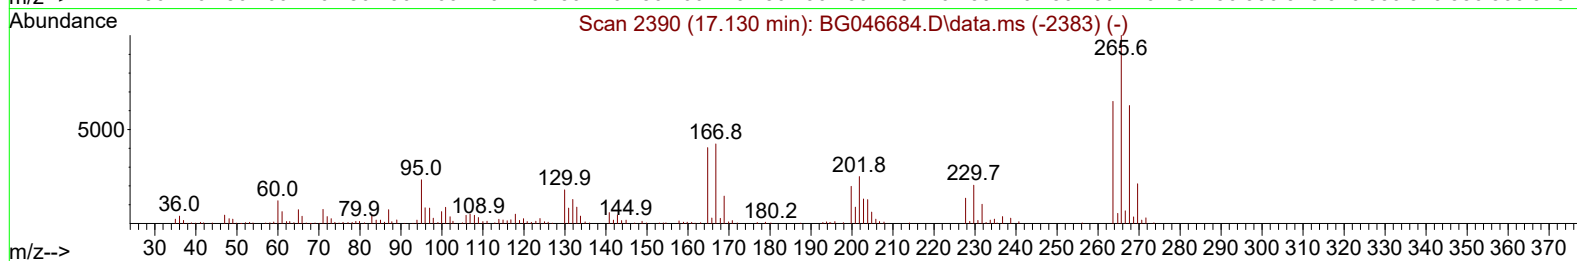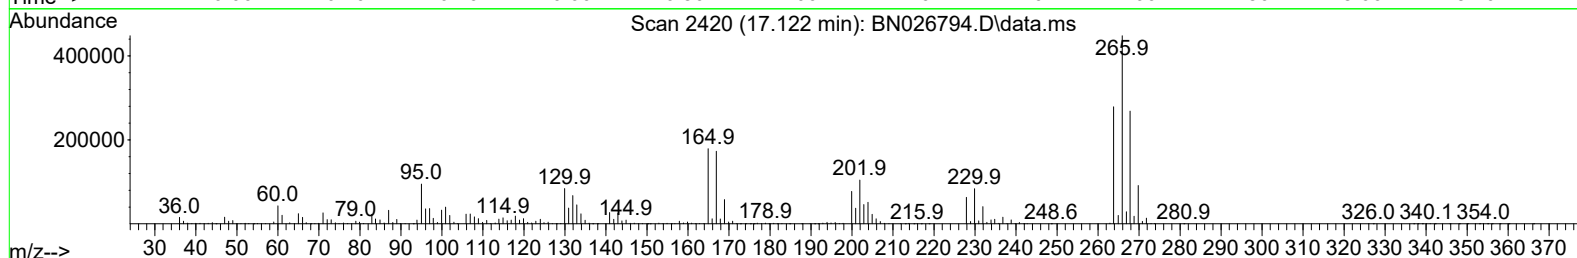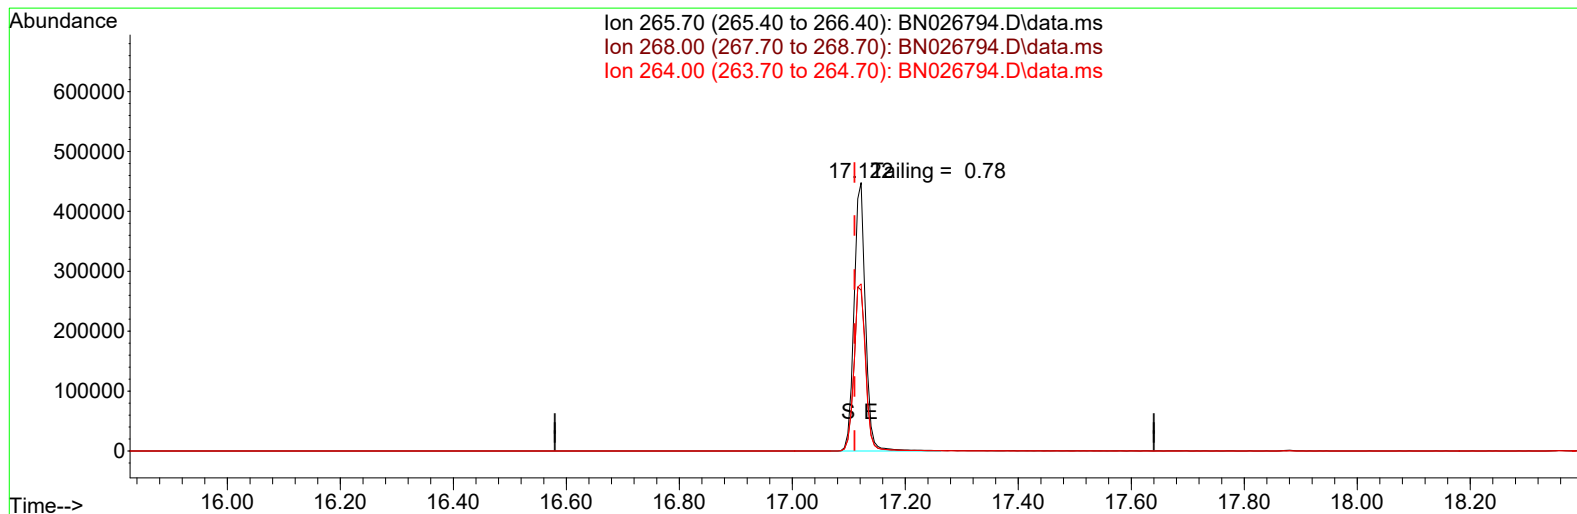

TIC: BN026794.D\data.ms

(70) Pentachlorophenol (C)

17.122min (+ 0.012) 23656.20 ng




response 630646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.93
264.00	61.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080223\
Data File : BN026794.D
Acq On : 02 Aug 2023 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 03 01:35:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 01:33:44 2023
Response via : Initial Calibration

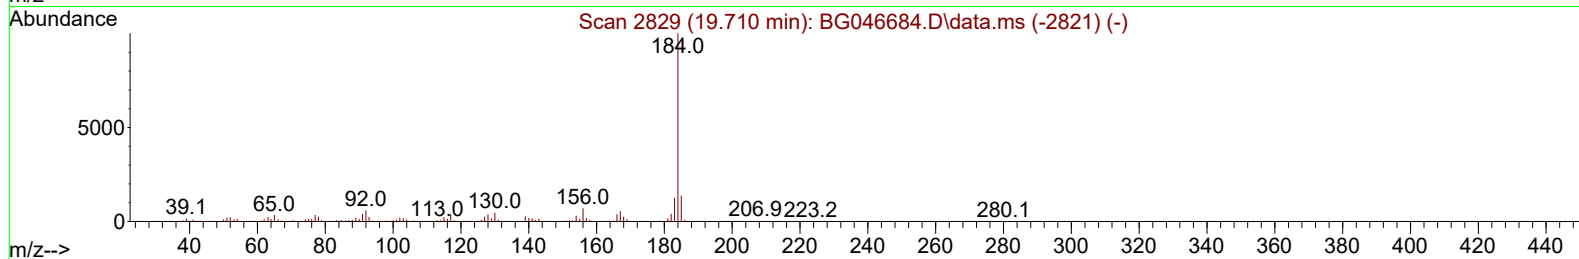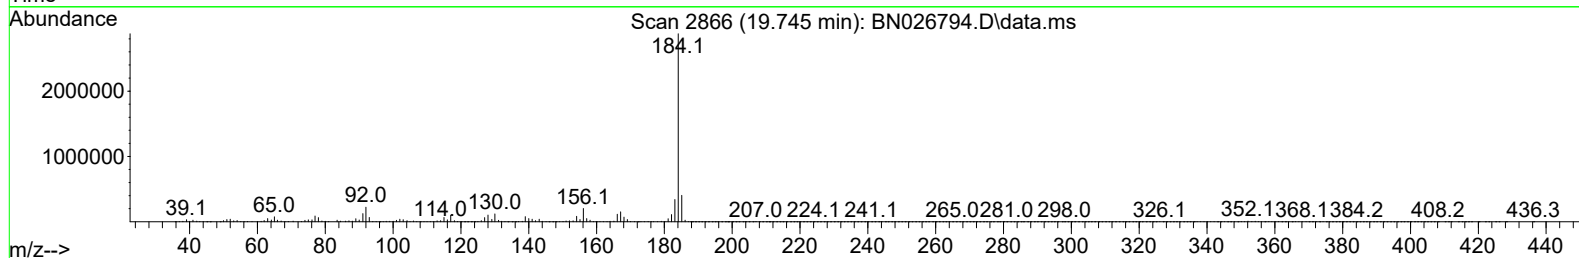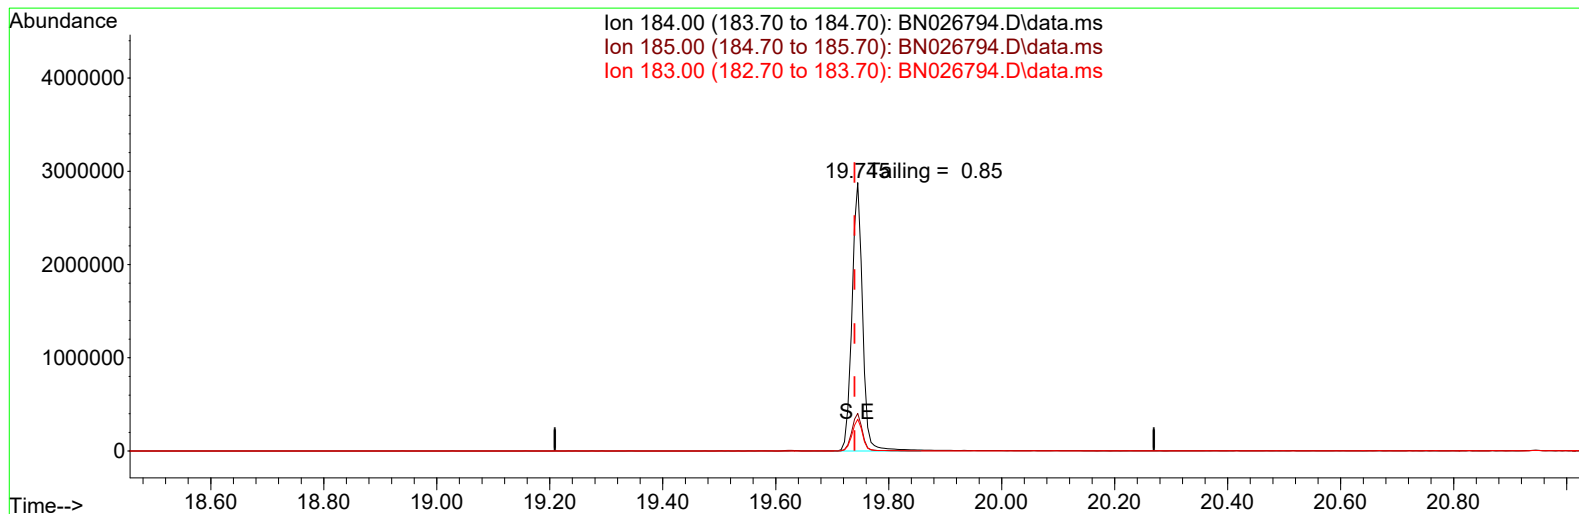

TIC: BN026794.D\data.ms

(77) Benzidine

19.745min (+ 0.006) 465522.66 ng

response 3788376

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_N	<u>BN026794.D</u>
Compound Name	Response	Retention Time
DDT	1652260	20.945
DDD	24828	20.557
DDE	3906	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28734	1680994	1.71

Instrument :
BNA_N
ClientSampleId :
DFTPP