

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080318\
 Data File : BN002218.D
 Acq On : 03 Aug 2018 12:12
 Operator : JU/SJ
 Sample : J4206-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JJ1J5

Quant Time: Aug 03 15:40:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 15:22:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	329635	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1526192	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	889142	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1850012	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1404680	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1203282	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	28795	3.94	ng/uL	0.00
5) Phenol-d5	6.87	99	682755	21.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	456348	24.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	541403	22.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	579846	23.19	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	297252	23.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	310579	21.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	554792	21.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	753863	25.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1808120	23.99	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	2301237	24.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	249452	17.32	ng/ul	0.00
57) Fluorene-d10	15.32	176	1569852	24.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	217181	18.02	ng/ul	0.00
70) Anthracene-d10	17.16	188	2328033	25.81	ng/ul	0.00
78) Pyrene-d10	19.46	212	2409078	32.99	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	1734761	26.70	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.78	163	143665	1.946	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080318\
Data File : BN002218.D
Acq On : 03 Aug 2018 12:12
Operator : JU/SJ
Sample : J4206-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JJ1J5

Quant Time: Aug 03 15:40:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 15:22:46 2018
Response via : Initial Calibration

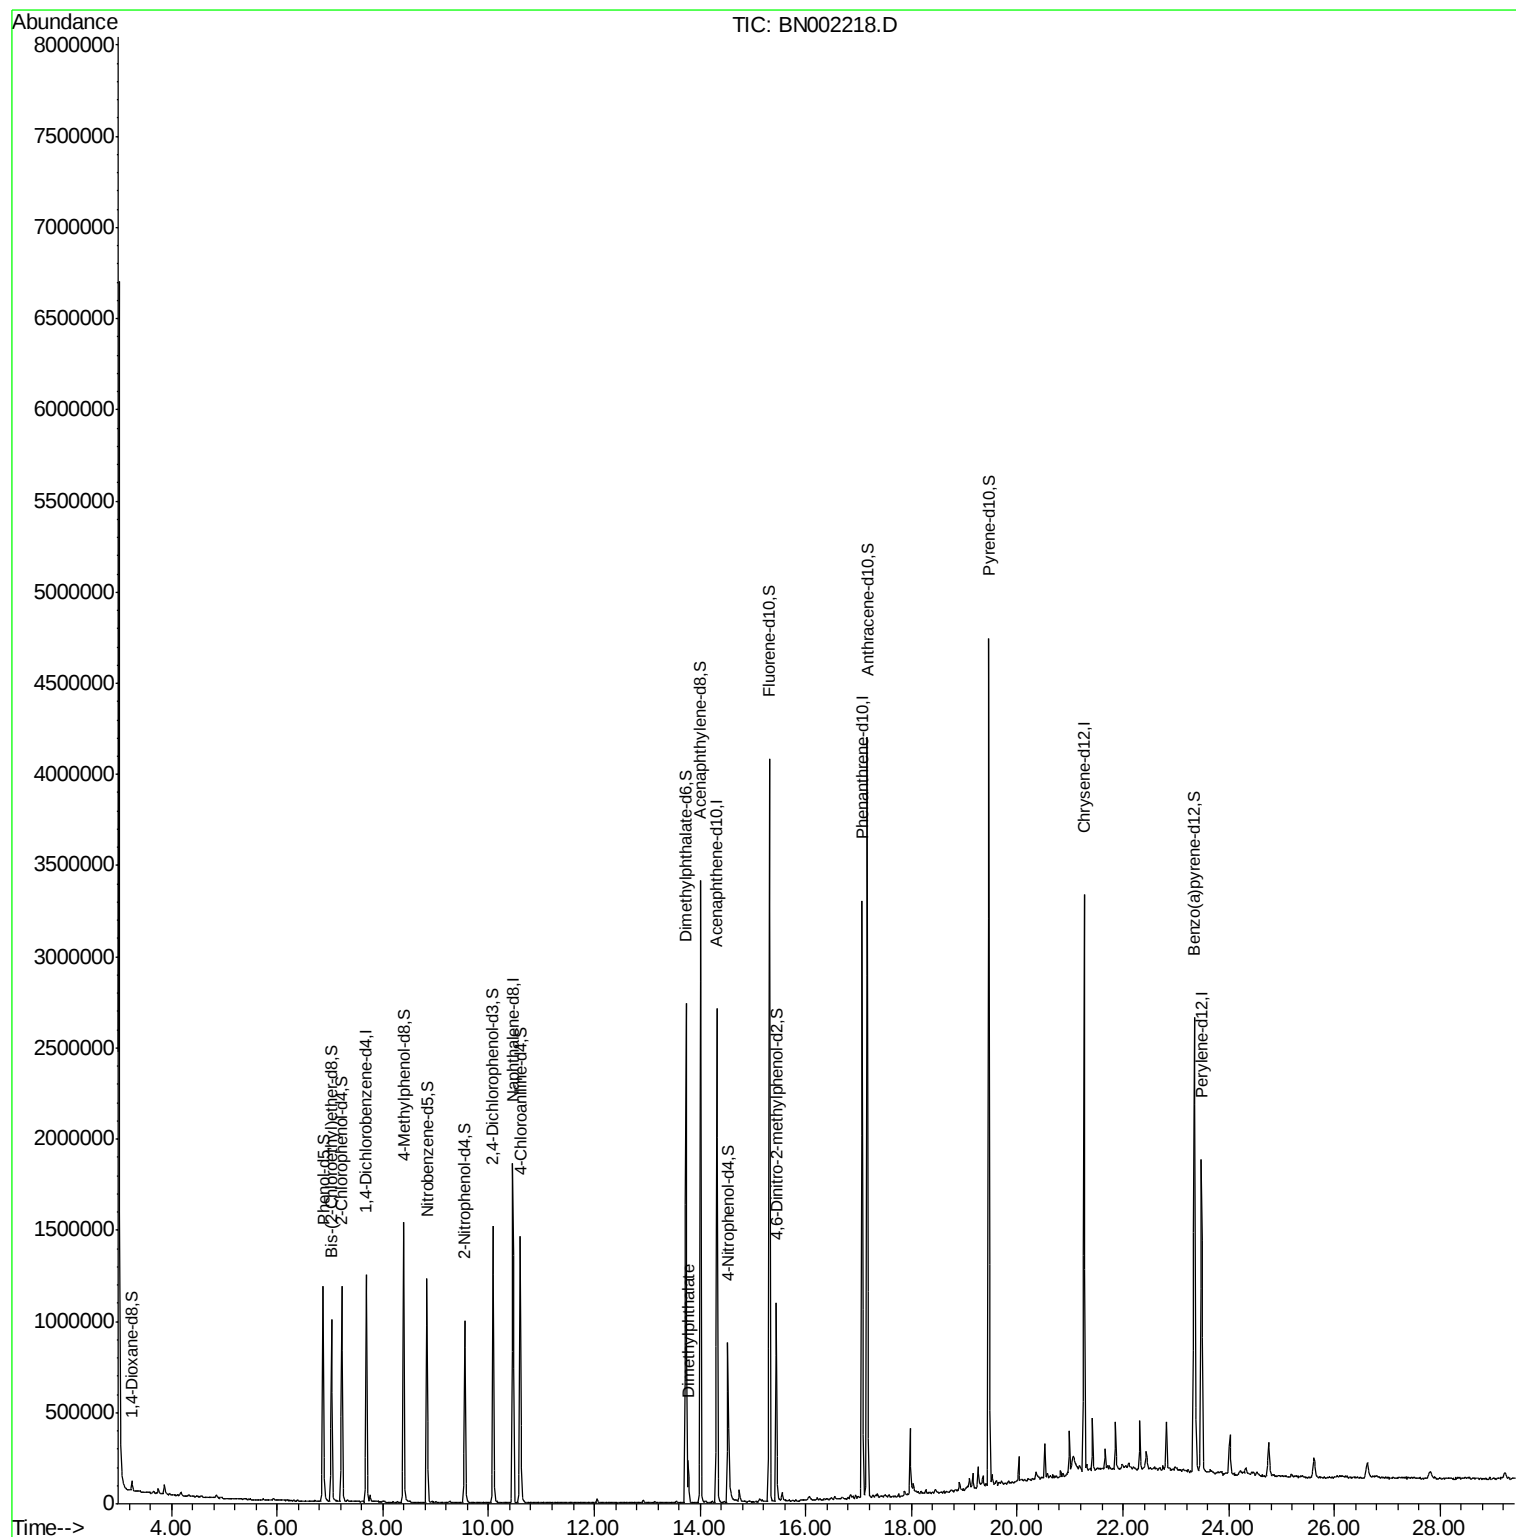

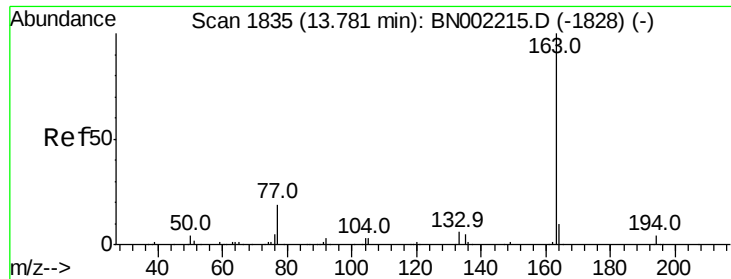

#44

Dimethylphthalate

Concen: 1.946 ng/ul

RT: 13.78 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BN002218.D

Acq: 03 Aug 2018 12:12

Instrument :

BNA_N

ClientSampleId :

JJ1J5


Tot Ion:163 Resp: 143665

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.6 7.8 11.8

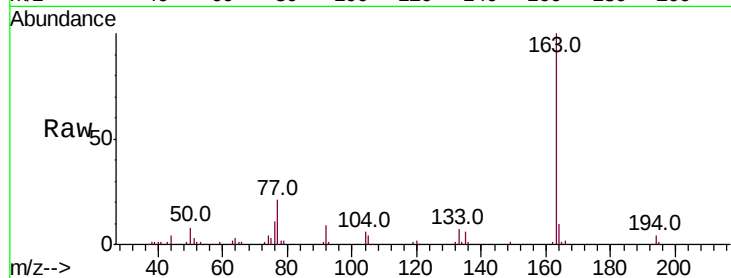

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

