

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080318\
 Data File : BN002219.D
 Acq On : 03 Aug 2018 12:47
 Operator : JU/SJ
 Sample : J4206-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JJ1J7

Quant Time: Aug 03 15:49:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 15:22:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	269084	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1208392	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	650014	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1225383	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	961989	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	973951	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	19149	3.21	ng/uL	0.00
5) Phenol-d5	6.86	99	419441	16.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	282588	18.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	339822	16.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	347150	17.01	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	179976	17.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	186723	16.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	326255	15.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	416328	17.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1002387	18.19	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1302406	19.00	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	102320	9.72	ng/ul	0.00
57) Fluorene-d10	15.32	176	845410	17.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	87213	10.93	ng/ul	0.00
70) Anthracene-d10	17.16	188	1168294	19.55	ng/ul	0.00
78) Pyrene-d10	19.46	212	1156769	23.13	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	1044006	19.85	ng/ul	0.00


Target Compounds				Ovalue		
6) Phenol	6.89	94	35244	1.385	ng/ul#	85
44) Dimethylphthalate	13.77	163	107033	1.983	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080318\
Data File : BN002219.D
Acq On : 03 Aug 2018 12:47
Operator : JU/SJ
Sample : J4206-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JJ1J7

Quant Time: Aug 03 15:49:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 15:22:46 2018
Response via : Initial Calibration

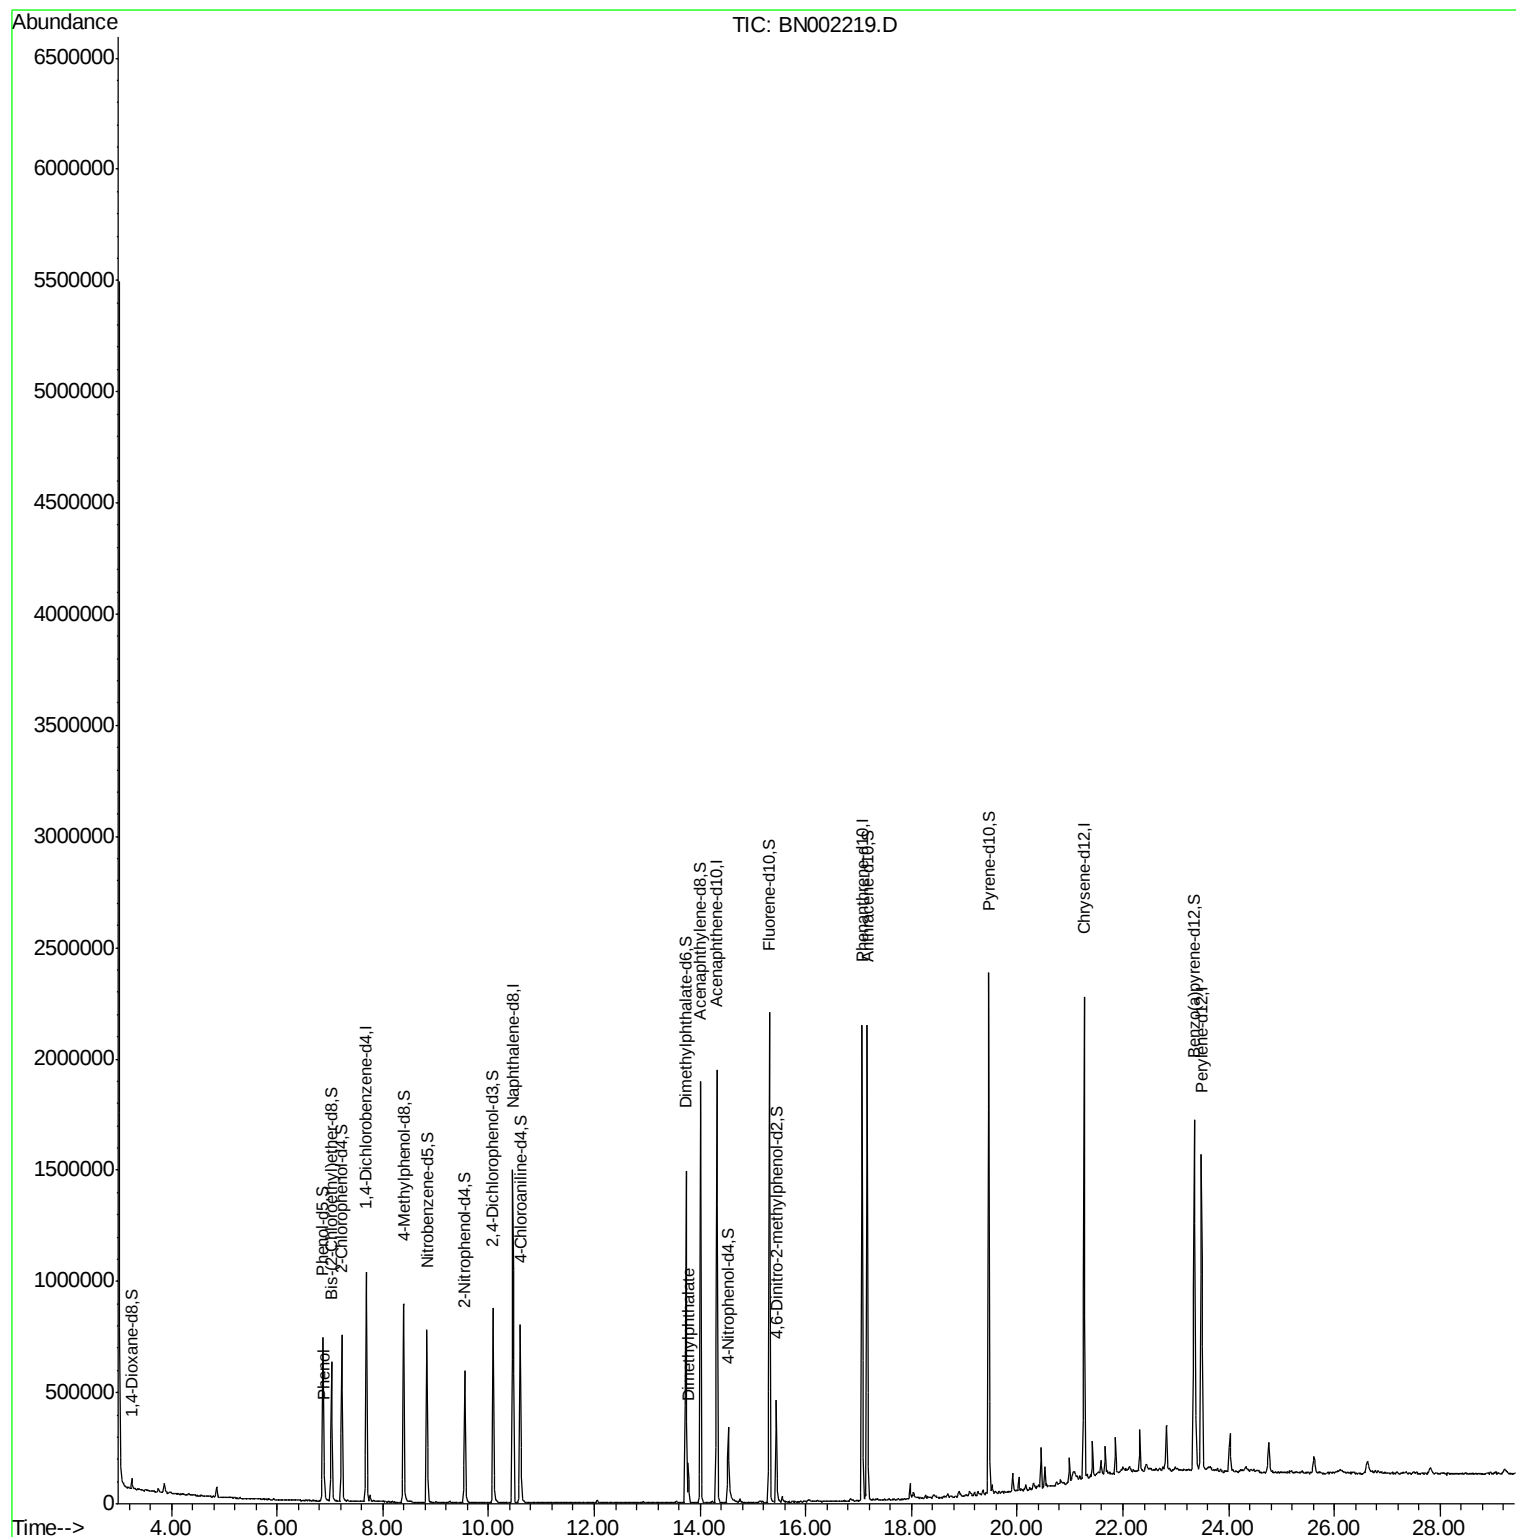

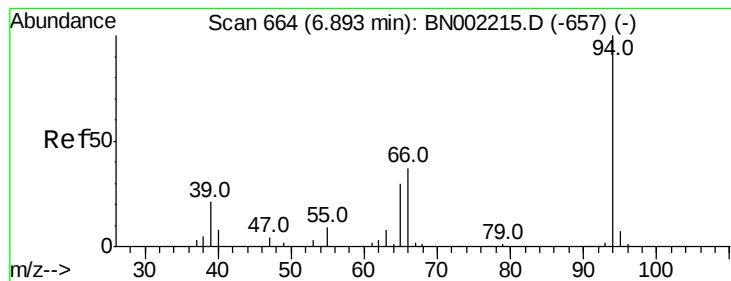





#6

Phenol

Concen: 1.385 ng/ul
 RT: 6.89 min Scan# 664
 Delta R.T. 0.00 min
 Lab File: BN002219.D
 Acq: 03 Aug 2018 12:47

Instrument :
 BNA_N
 ClientSampled :
 JJ1J7

Tot Ion: 94 Resp: 35244
 Ion Ratio Lower Upper
 94 100
 65 32.4 21.0 31.6#
 66 47.0 29.3 43.9#

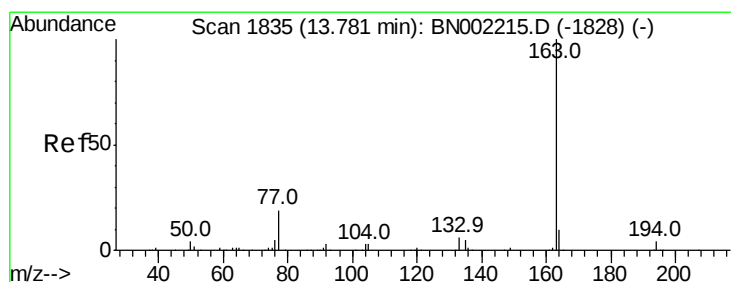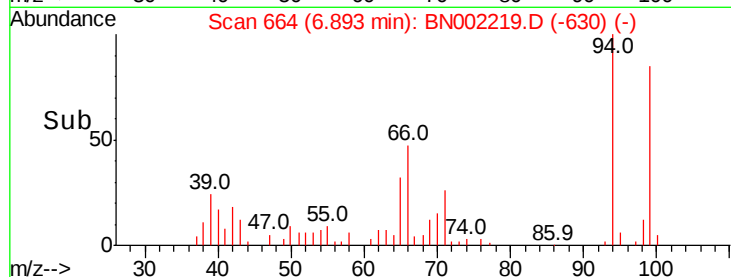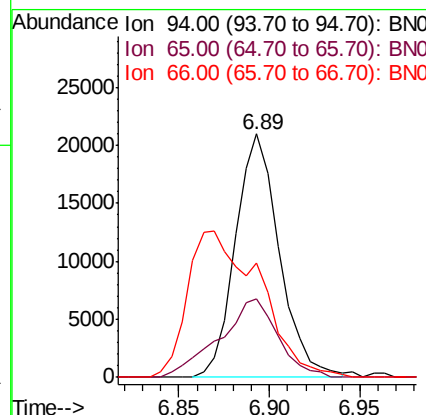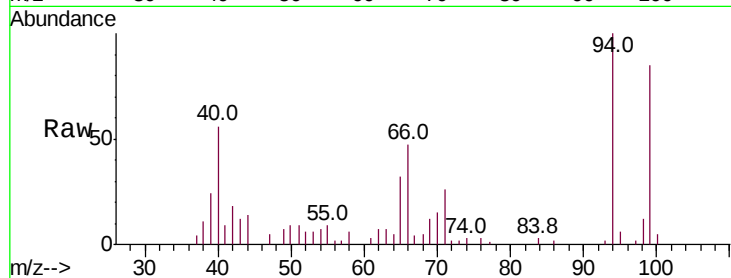

#44

Dimethylphthalate

Concen: 1.983 ng/ul
 RT: 13.77 min Scan# 1834
 Delta R.T. -0.01 min
 Lab File: BN002219.D
 Acq: 03 Aug 2018 12:47

Tgt Ion:163 Resp: 107033
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.2 4.8
 164 10.1 7.8 11.8

