

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080318\
 Data File : BN002220.D
 Acq On : 03 Aug 2018 13:23
 Operator : JU/SJ
 Sample : J4206-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JJ1J8

Quant Time: Aug 03 16:18:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 15:22:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	255791	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1162275	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	651546	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1261356	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	923148	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	898793	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	22980	4.05	ng/uL	0.00
5) Phenol-d5	6.86	99	526842	21.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	335312	22.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	417381	21.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	436163	22.48	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	214326	22.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	224337	20.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	404488	20.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	310213	13.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1242505	22.50	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1589129	23.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	138616	13.14	ng/ul	0.00
57) Fluorene-d10	15.32	176	1045810	22.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	114092	13.89	ng/ul	0.00
70) Anthracene-d10	17.16	188	1448919	23.56	ng/ul	0.00
78) Pyrene-d10	19.46	212	1333492	27.79	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	1102606	22.72	ng/ul	0.00
Target Compounds						
6) Phenol	6.89	94	43028	1.779	ng/ul	93
44) Dimethylphthalate	13.77	163	130433	2.411	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080318\
Data File : BN002220.D
Acq On : 03 Aug 2018 13:23
Operator : JU/SJ
Sample : J4206-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JJ1J8

Quant Time: Aug 03 16:18:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 15:22:46 2018
Response via : Initial Calibration

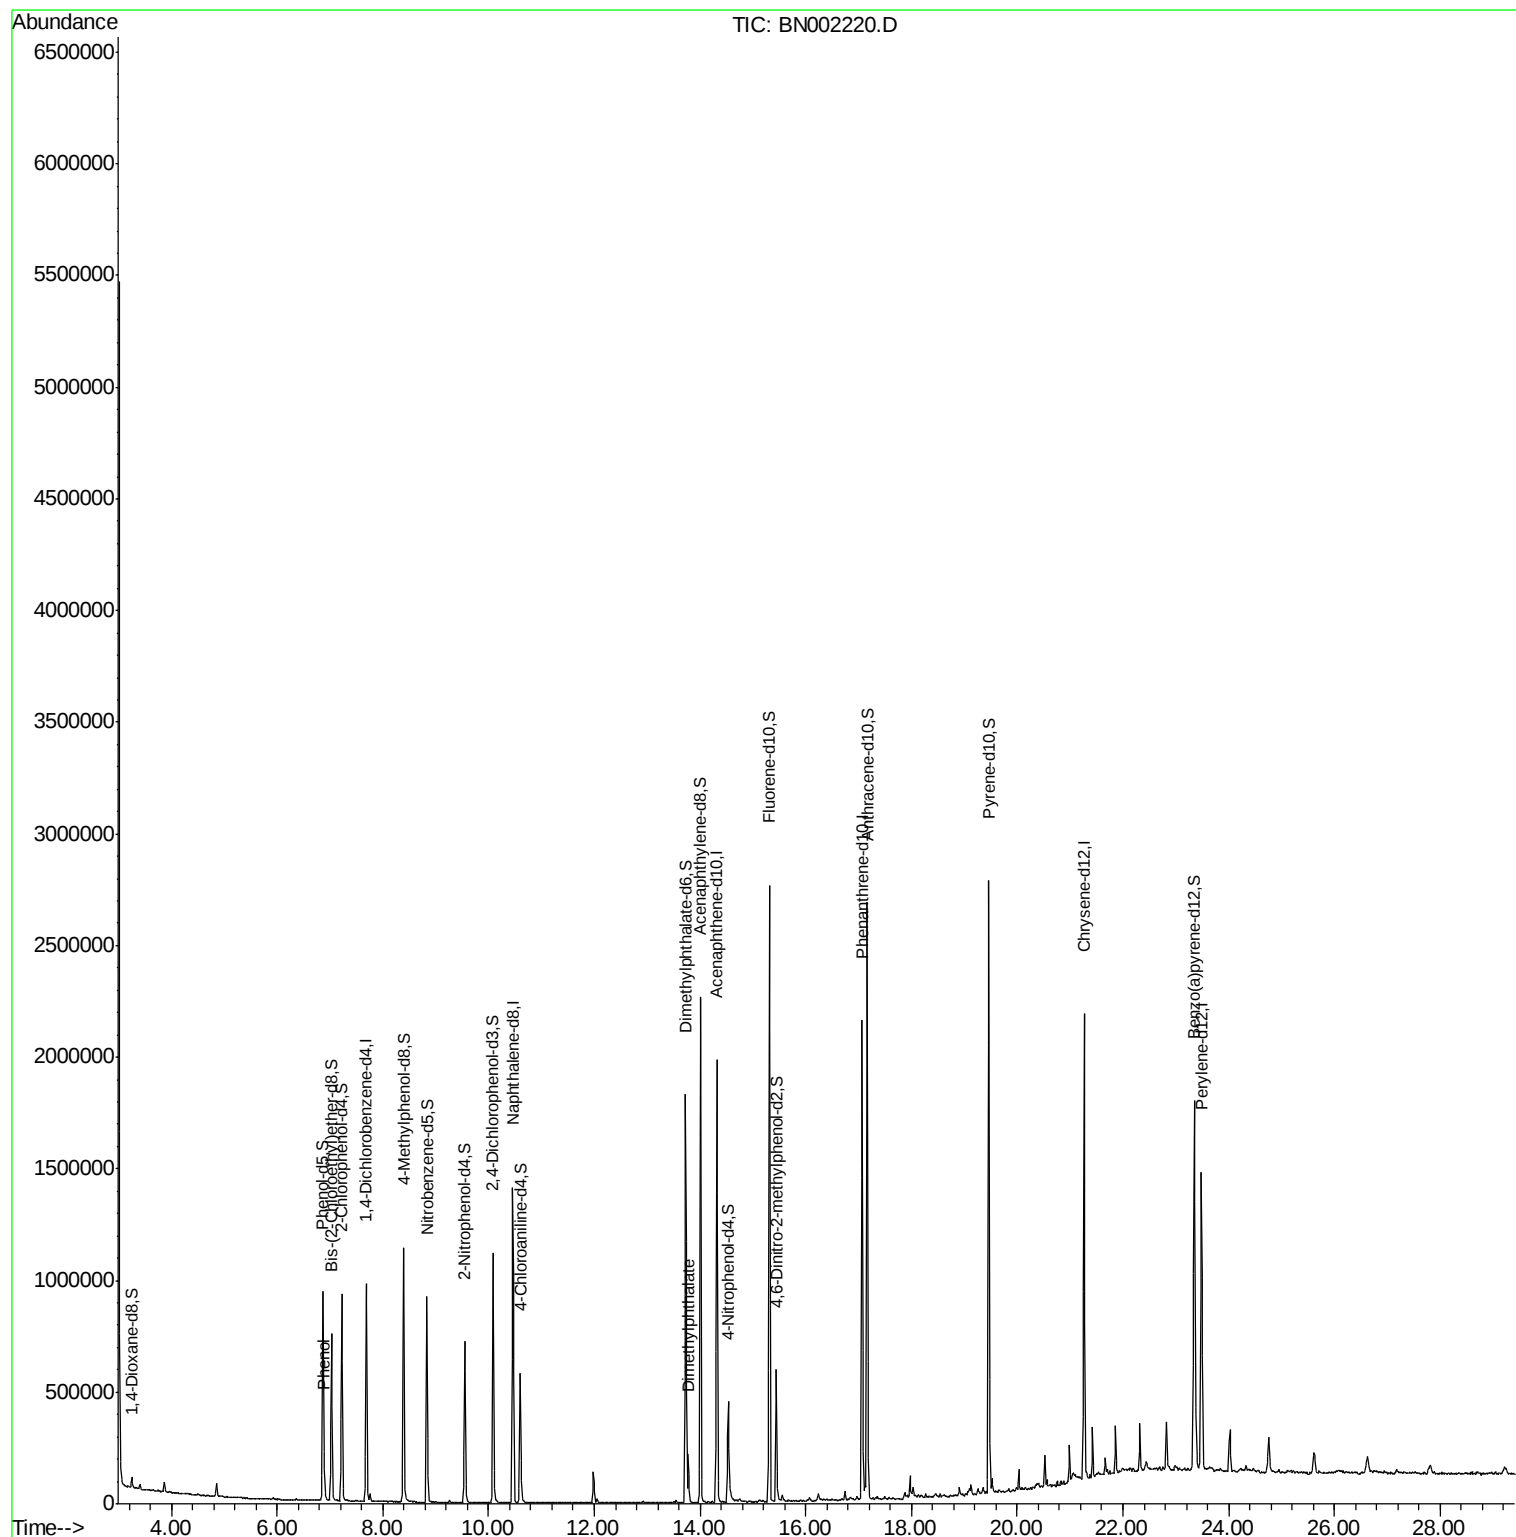

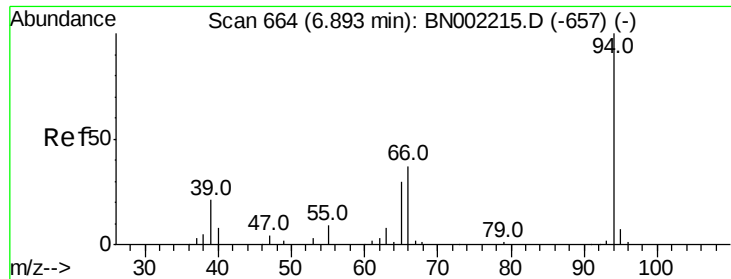


#6

Phenol




Concen: 1.779 ng/ul
 RT: 6.89 min Scan# 664
 Delta R.T. 0.00 min
 Lab File: BN002220.D
 Acq: 03 Aug 2018 13:23

Instrument :
 BNA_N
 ClientSampleId :
 JJ1J8

Tot Ion: 94 Resp: 43028
 Ion Ratio Lower Upper
 94 100
 65 28.5 21.0 31.6
 66 41.5 29.3 43.9

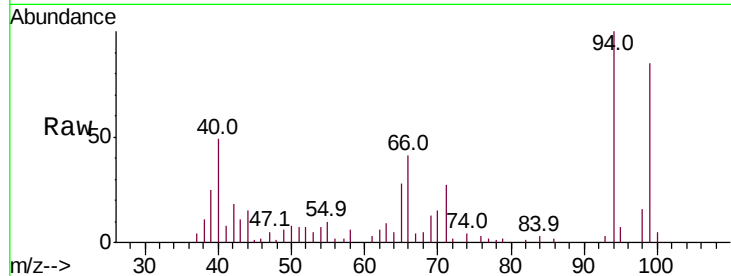

Abundance Ion 94.00 (93.70 to 94.70): BN0
 Ion 65.00 (64.70 to 65.70): BN0
 Ion 66.00 (65.70 to 66.70): BN0

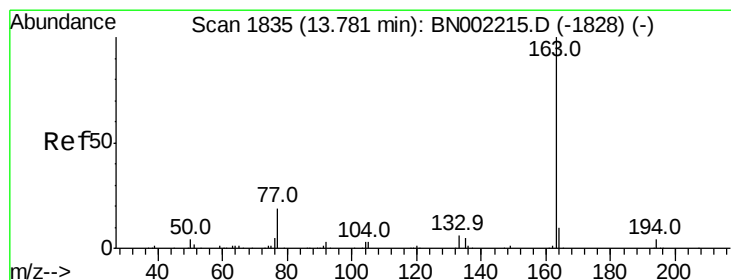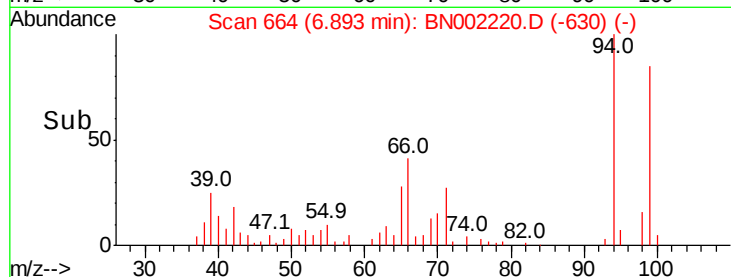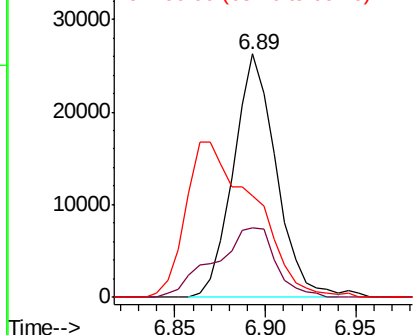


#44

Dimethylphthalate

Concen: 2.411 ng/ul
 RT: 13.77 min Scan# 1834
 Delta R.T. -0.01 min
 Lab File: BN002220.D
 Acq: 03 Aug 2018 13:23

Tgt Ion:163 Resp: 130433
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.2 4.8
 164 10.1 7.8 11.8

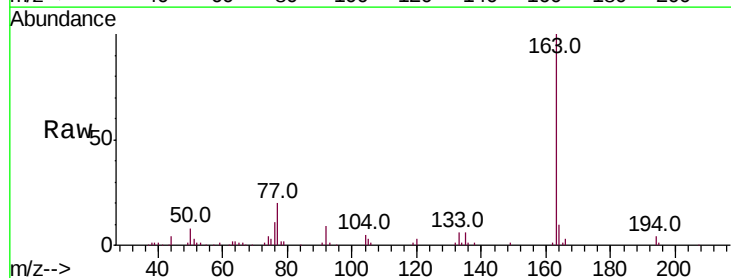

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

