

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080318\
 Data File : BN002221.D
 Acq On : 03 Aug 2018 13:58
 Operator : JU/SJ
 Sample : J4206-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JJ1J6

Quant Time: Aug 03 16:21:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 15:22:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	221427	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	930824	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	484834	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1004238	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	980168	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1025190	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	16242	3.31	ng/uL	0.00
5) Phenol-d5	6.86	99	312755	15.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	216410	17.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	263944	16.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	241283	14.37	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	132222	17.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	131979	15.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	232019	14.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	281307	15.50	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	688383	16.75	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	875543	17.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	60446	7.70	ng/ul	0.00
57) Fluorene-d10	15.32	176	611407	17.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	61613	9.42	ng/ul	0.00
70) Anthracene-d10	17.16	188	904733	18.48	ng/ul	0.00
78) Pyrene-d10	19.46	212	979909	19.23	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	998479	18.04	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.89	94	22453	1.072	ng/ul 96
44) Dimethylphthalate	13.77	163	67613	1.680	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080318\
Data File : BN002221.D
Acq On : 03 Aug 2018 13:58
Operator : JU/SJ
Sample : J4206-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JJ1J6

Quant Time: Aug 03 16:21:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 15:22:46 2018
Response via : Initial Calibration

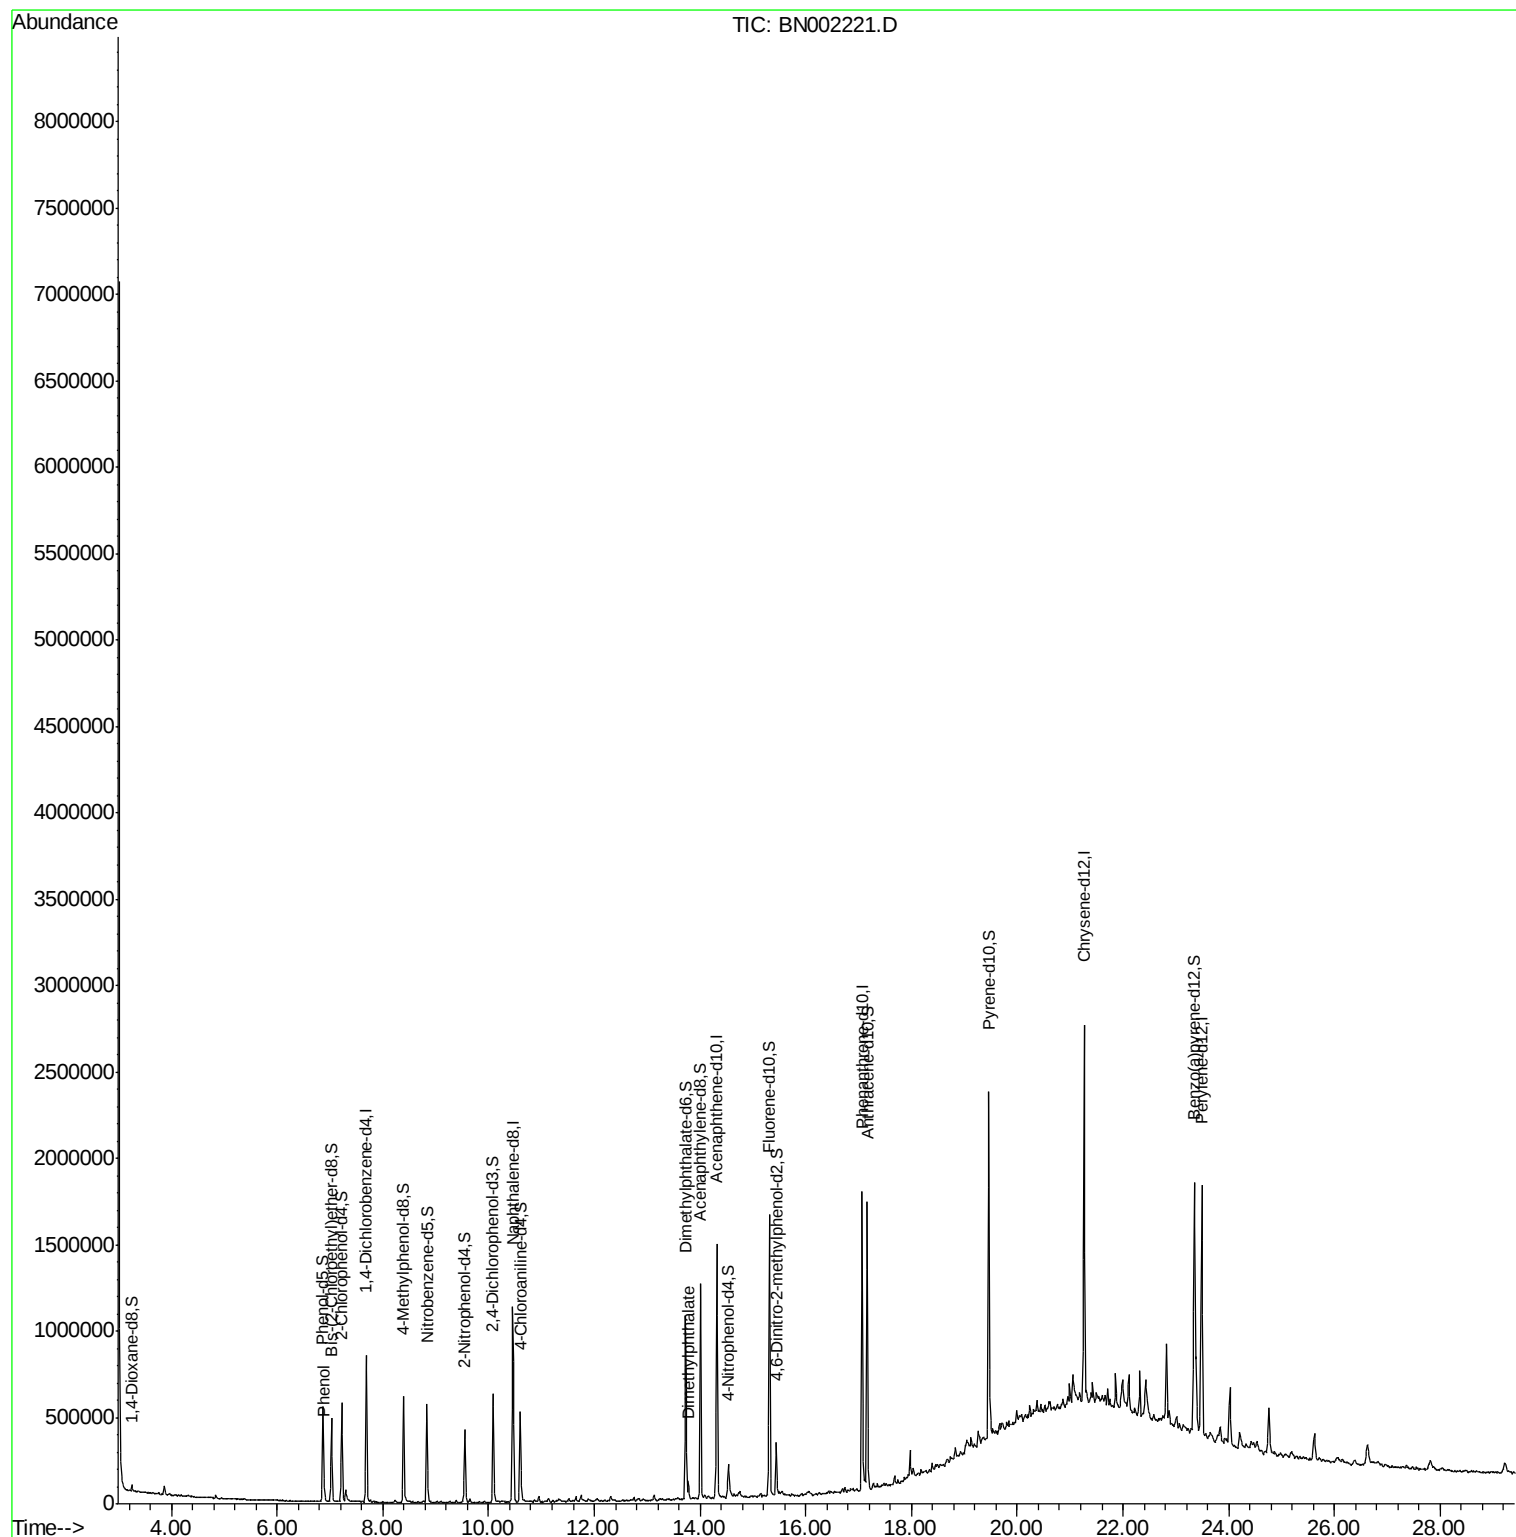

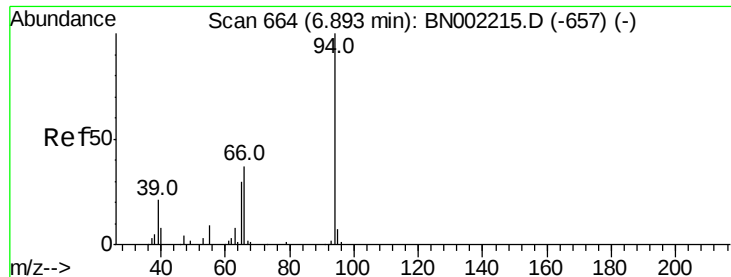

#6

Phenol

Concen: 1.072 ng/ul

RT: 6.89 min Scan# 664

Delta R.T. 0.00 min

Lab File: BN002221.D

Acq: 03 Aug 2018 13:58

Instrument :

BNA_N

ClientSampleId :

JJ1J6





Tot Ion: 94 Resp: 22453

Ion Ratio Lower Upper

94 100

65 30.0 21.0 31.6

66 37.6 29.3 43.9

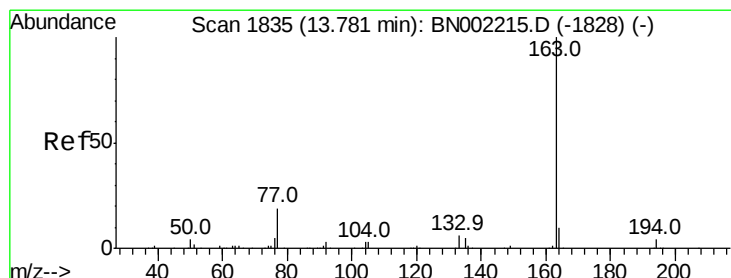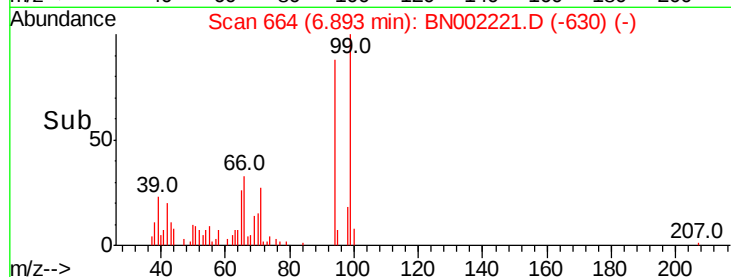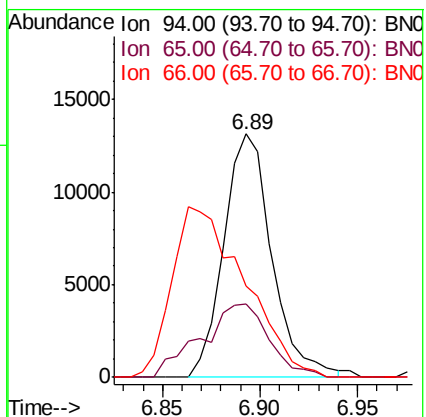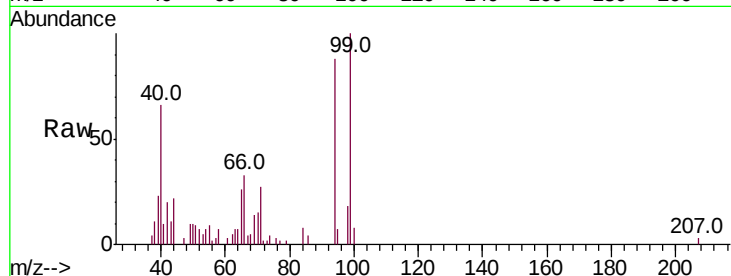

#44

Dimethylphthalate

Concen: 1.680 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BN002221.D

Acq: 03 Aug 2018 13:58

Tgt Ion:163 Resp: 67613

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.5 7.8 11.8

