

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080318\
 Data File : BN002222.D
 Acq On : 03 Aug 2018 14:34
 Operator : JU/SJ
 Sample : J4206-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JJ1K0

Quant Time: Aug 03 16:26:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 15:22:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	232430	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	978026	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	520263	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1076106	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1038185	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1079136	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	30473	5.92	ng/uL	0.00
5) Phenol-d5	6.86	99	609147	27.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	403125	30.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	503990	29.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	466474	26.46	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	253167	31.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	269059	29.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	460538	27.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	597393	31.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1371451	31.10	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1780313	32.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	152152	18.06	ng/ul	0.00
57) Fluorene-d10	15.32	176	1172579	30.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	135154	19.28	ng/ul	0.00
70) Anthracene-d10	17.16	188	1731536	33.00	ng/ul	0.00
78) Pyrene-d10	19.46	212	1860310	34.47	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	1847552	31.71	ng/ul	0.00
Target Compounds						
6) Phenol	6.89	94	43539	1.981	ng/ul#	93
44) Dimethylphthalate	13.78	163	161281	3.734	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080318\
Data File : BN002222.D
Acq On : 03 Aug 2018 14:34
Operator : JU/SJ
Sample : J4206-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JJ1K0

Quant Time: Aug 03 16:26:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 15:22:46 2018
Response via : Initial Calibration

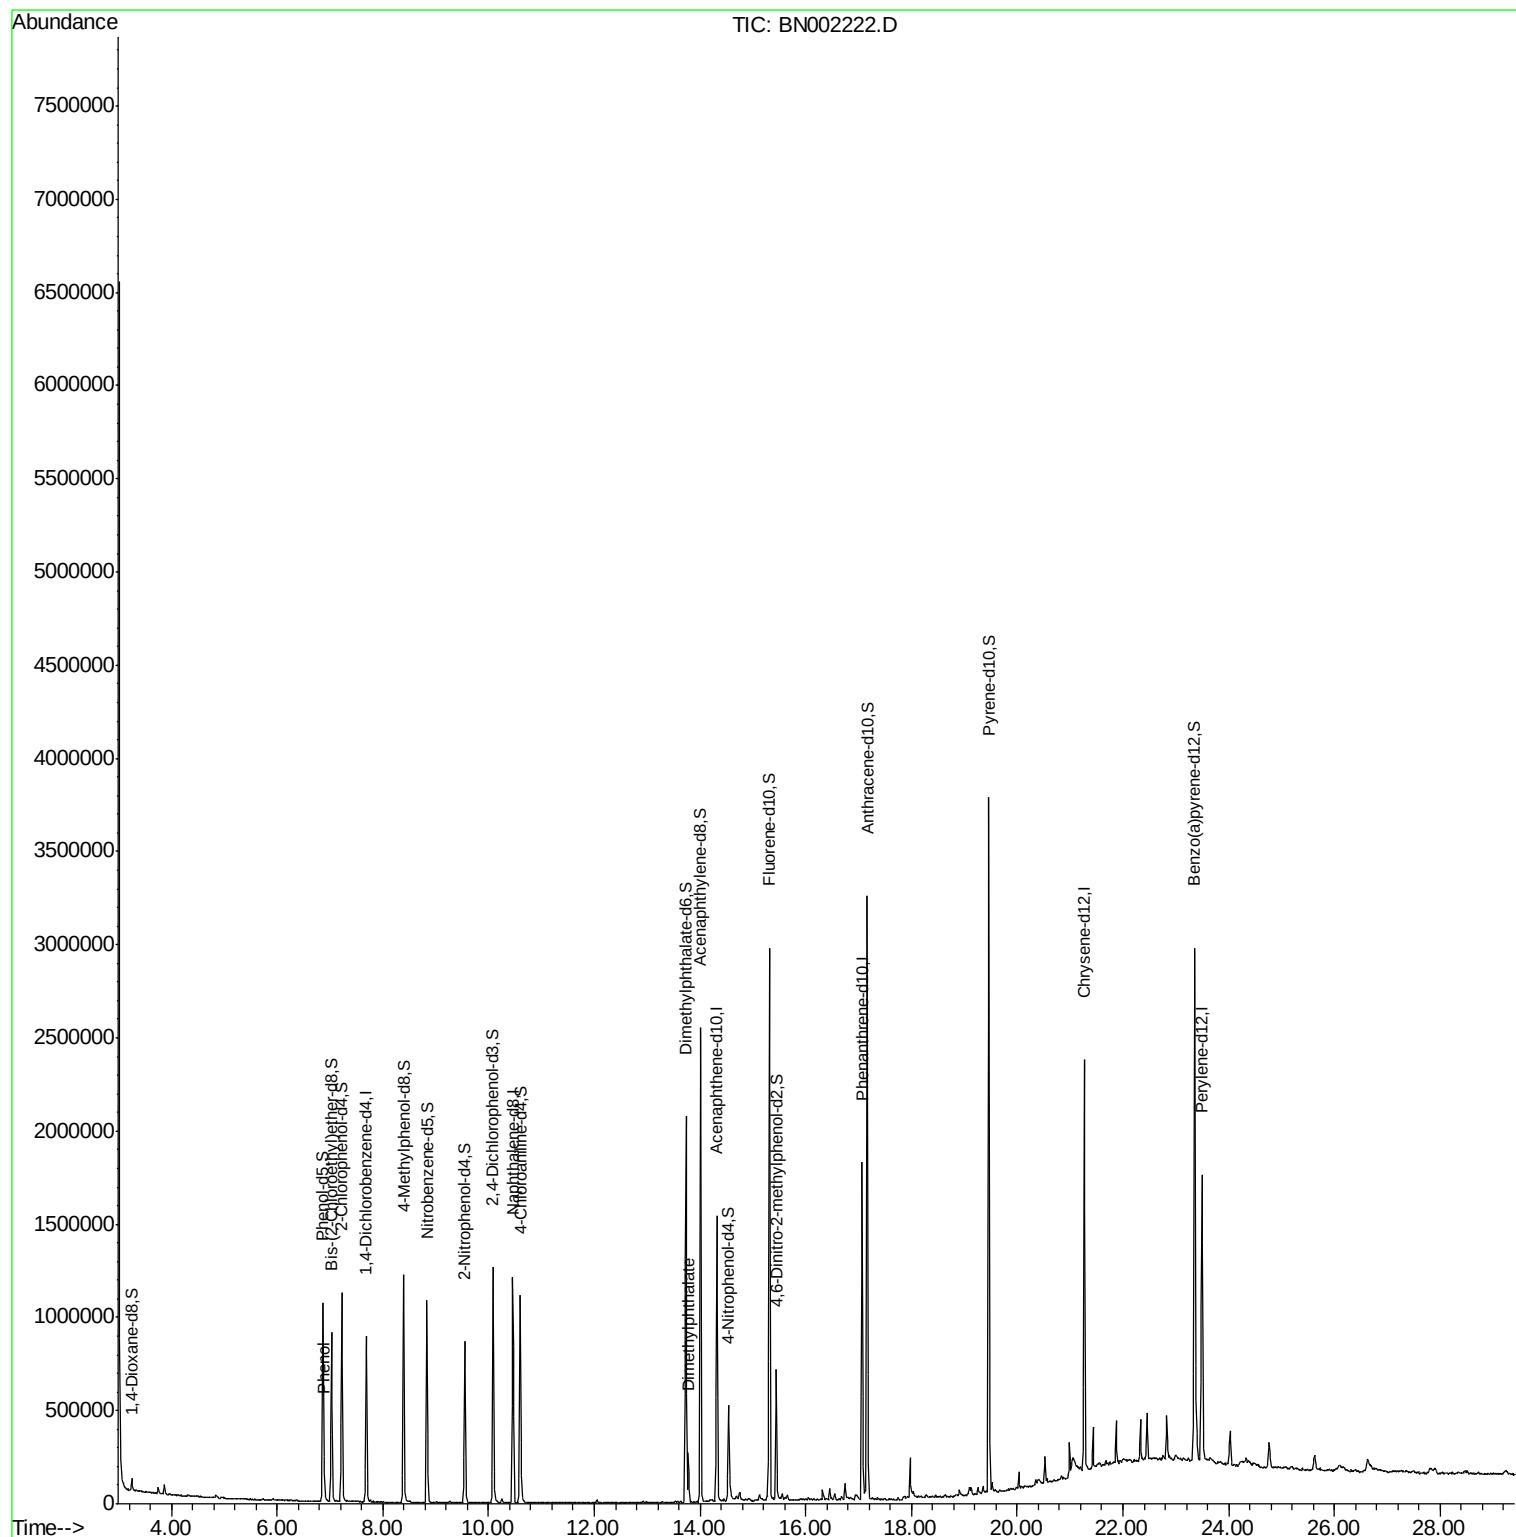

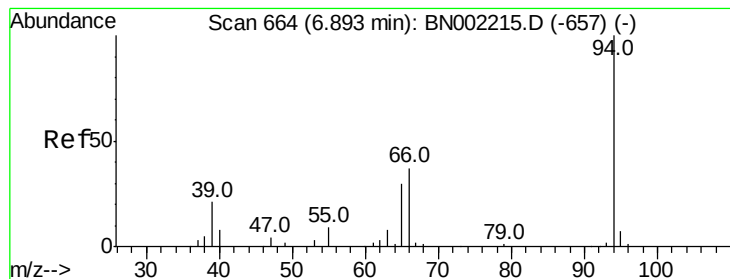





#6

Phenol

Concen: 1.981 ng/ul
 RT: 6.89 min Scan# 664
 Delta R.T. 0.00 min
 Lab File: BN002222.D
 Acq: 03 Aug 2018 14:34

Instrument :
 BNA_N
 ClientSampleId :
 JJ1K0

Tot Ion: 94 Resp: 43539
 Ion Ratio Lower Upper
 94 100
 65 31.9 21.0 31.6#
 66 39.1 29.3 43.9

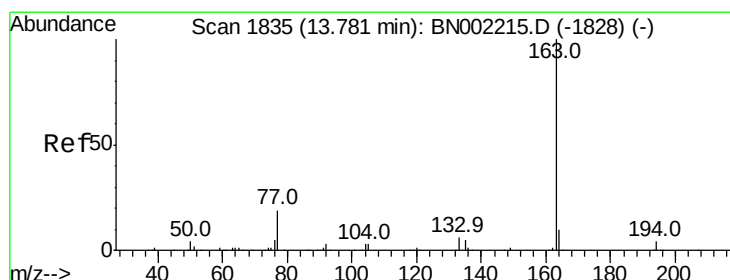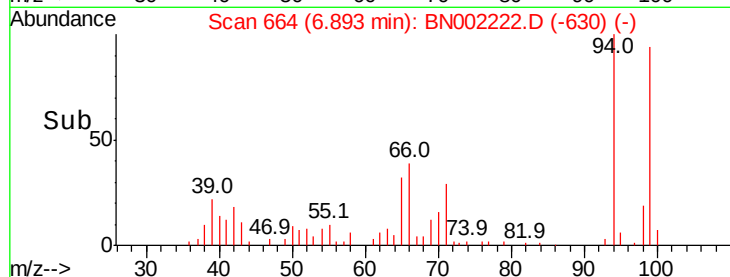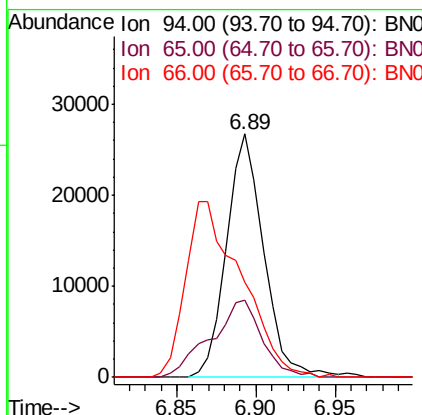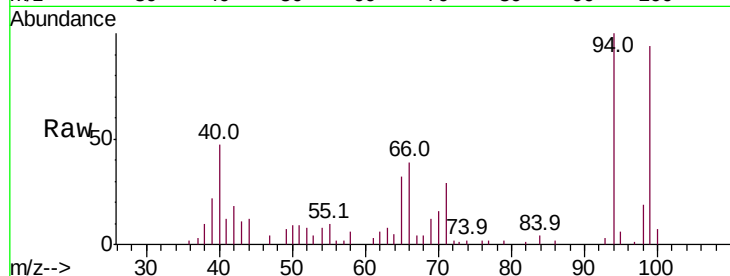

#44

Dimethylphthalate

Concen: 3.734 ng/ul
 RT: 13.78 min Scan# 1835
 Delta R.T. 0.00 min
 Lab File: BN002222.D
 Acq: 03 Aug 2018 14:34

Tgt Ion:163 Resp: 161281
 Ion Ratio Lower Upper
 163 100
 194 4.5 3.2 4.8
 164 9.4 7.8 11.8

