

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080318\
 Data File : BN002224.D
 Acq On : 03 Aug 2018 15:45
 Operator : JU/SJ
 Sample : J4206-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JJ1L0

Quant Time: Aug 03 16:49:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 15:22:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	249264	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1096918	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	571325	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1069543	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	891074	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	912701	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	17800	3.22	ng/uL	0.00
5) Phenol-d5	6.86	99	388747	16.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	266892	18.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	322490	17.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	323265	17.10	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	167948	18.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	176118	17.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	302273	16.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	418632	19.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	885800	18.29	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1156741	19.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	74249	8.03	ng/ul	0.00
57) Fluorene-d10	15.32	176	743039	17.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	80877	11.61	ng/ul	0.00
70) Anthracene-d10	17.16	188	1013471	19.43	ng/ul	0.00
78) Pyrene-d10	19.46	212	1025653	22.14	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	958641	19.45	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.77	163	84784	1.787	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080318\
Data File : BN002224.D
Acq On : 03 Aug 2018 15:45
Operator : JU/SJ
Sample : J4206-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JJ1L0

Quant Time: Aug 03 16:49:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 15:22:46 2018
Response via : Initial Calibration

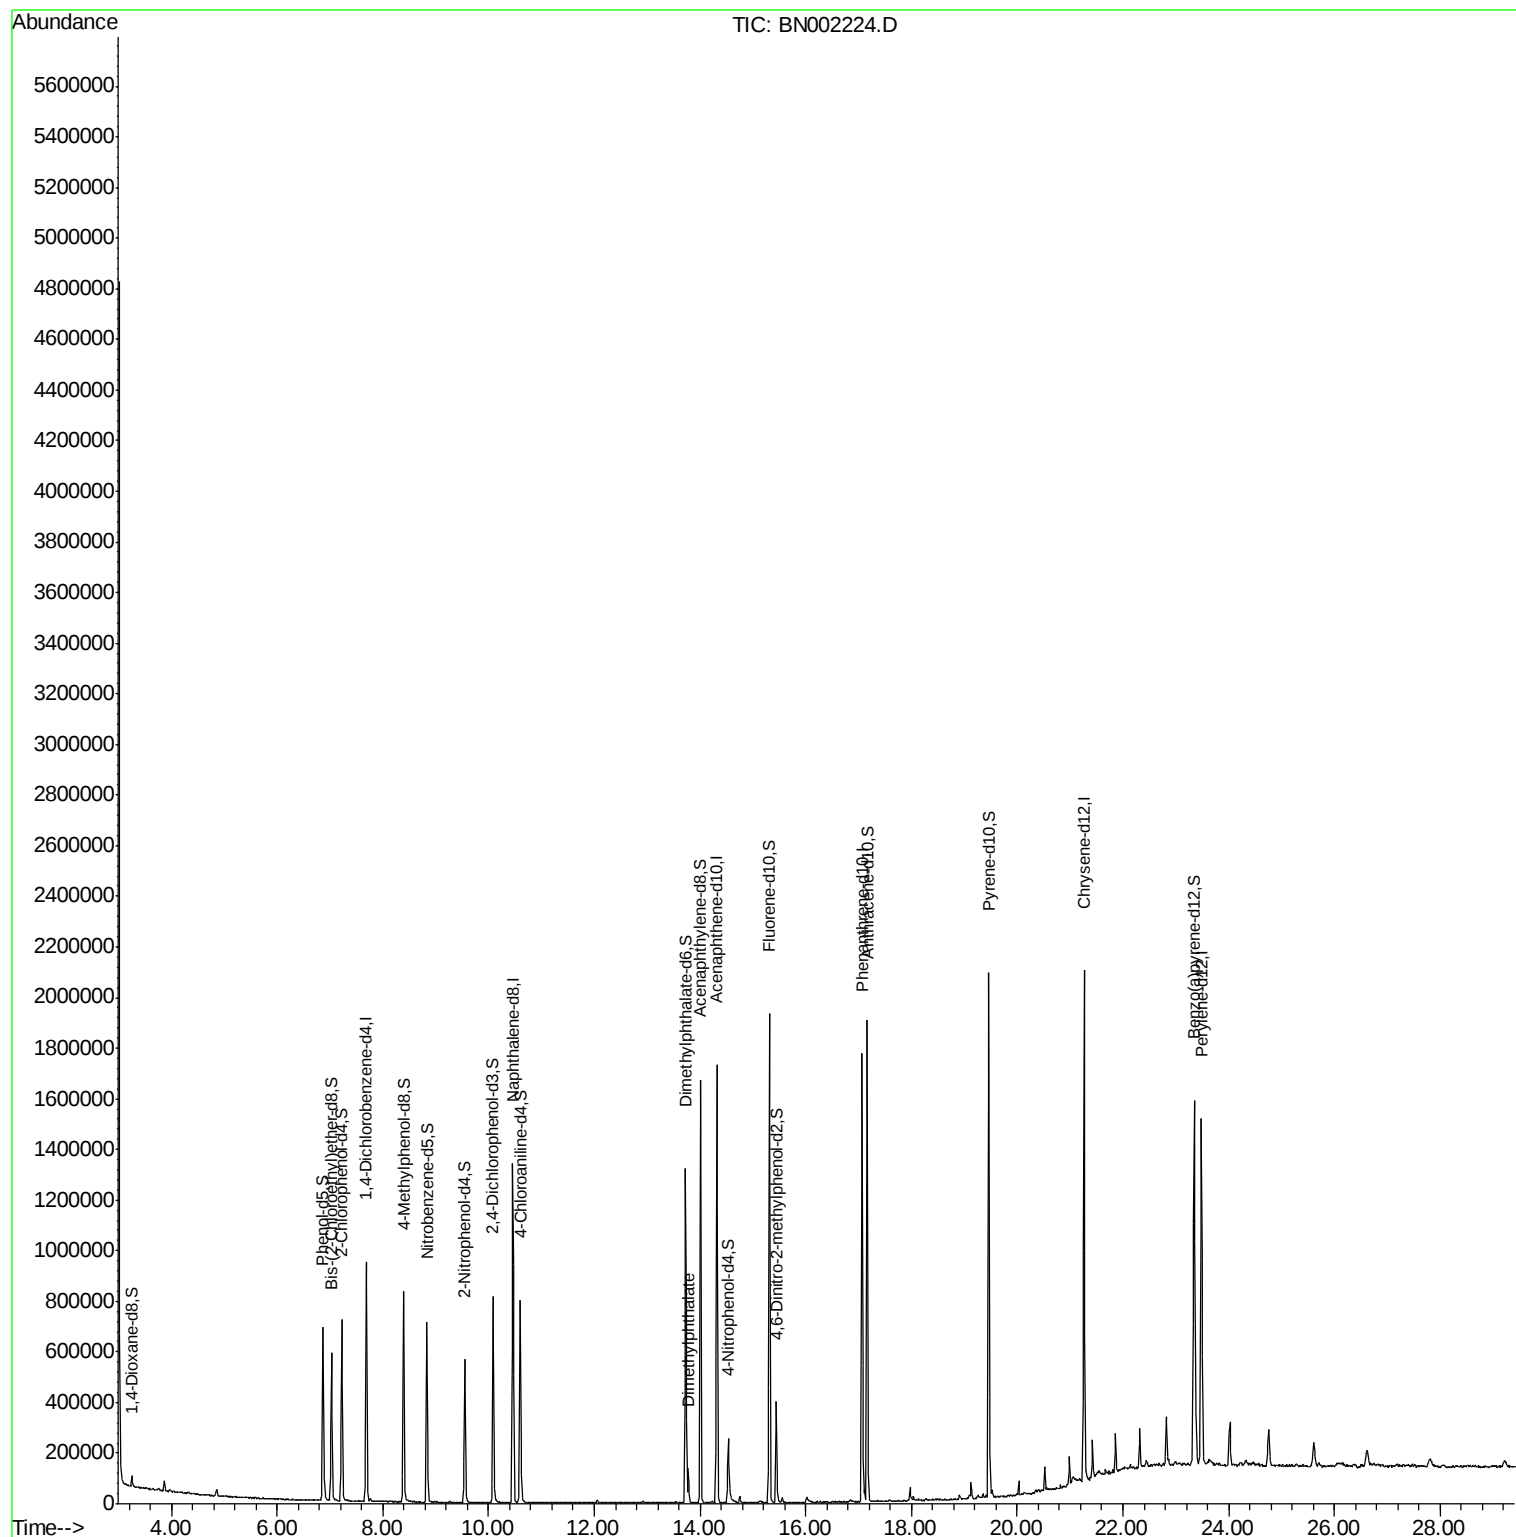

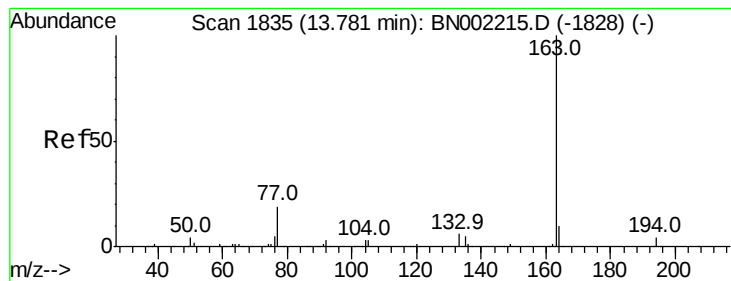

#44

Dimethylphthalate

Concen: 1.787 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BN002224.D

Acq: 03 Aug 2018 15:45

Instrument :

BNA_N

ClientSampleId :

JJ1L0


Tot Ion:163 Resp: 84784

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.7 7.8 11.8

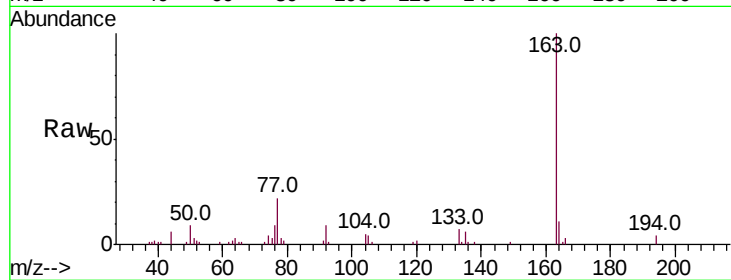

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

