
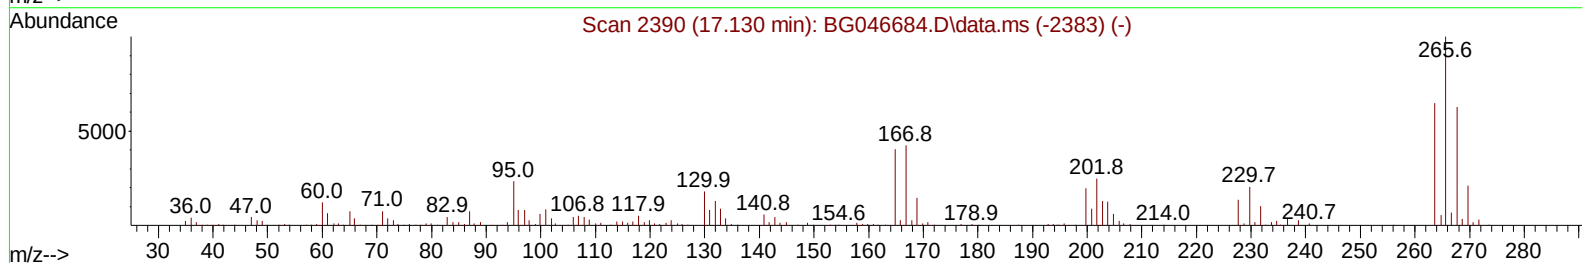
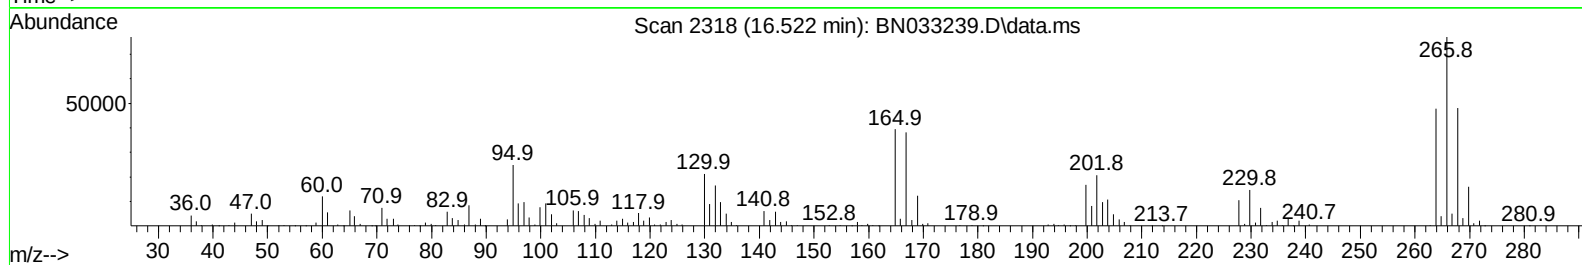


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080524\
Data File : BN033239.D
Acq On : 05 Aug 2024 16:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 08:54:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

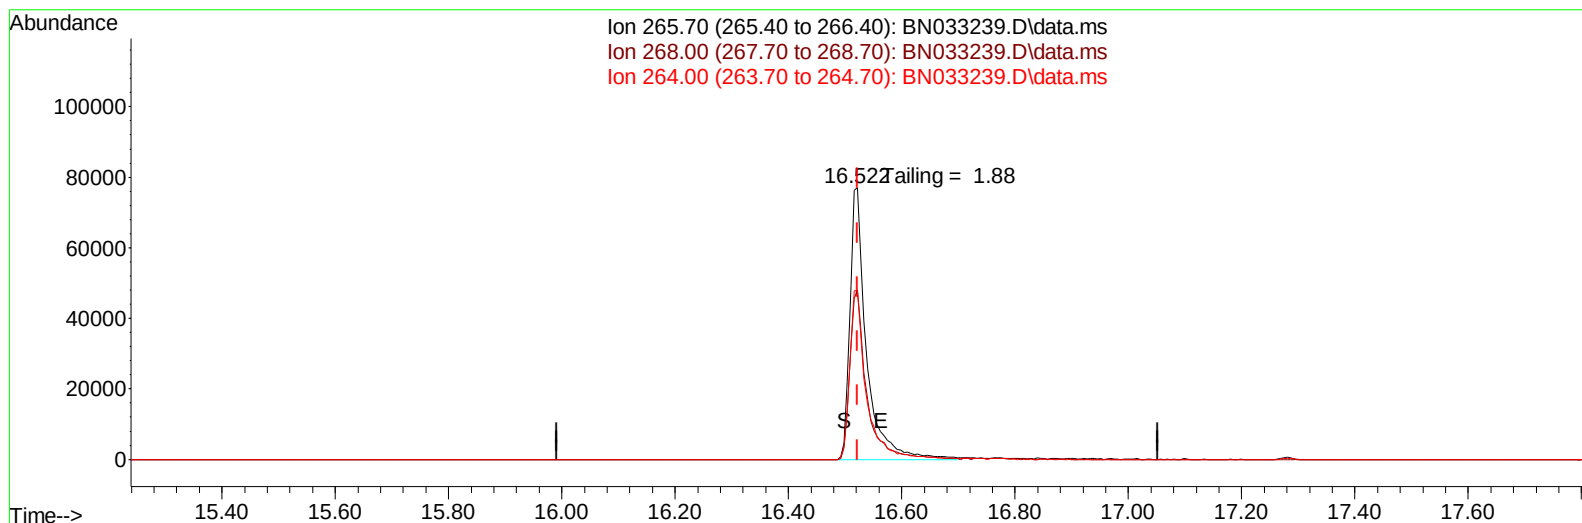

TIC: BN033239.D\data.ms




(70) Pentachlorophenol (C)

16.522min (0.000) 16240.58 ng

response 159315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.36
264.00	61.60	62.10
0.00	0.00	0.00

Quant Time: Aug 06 08:54:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

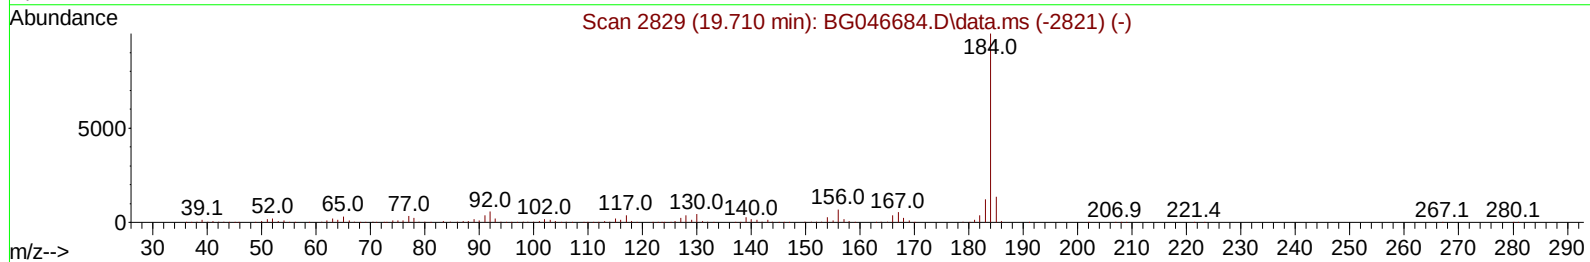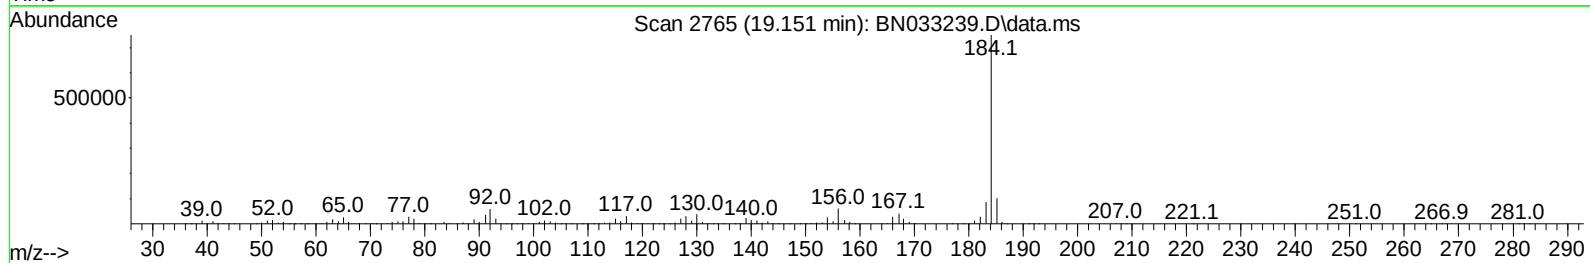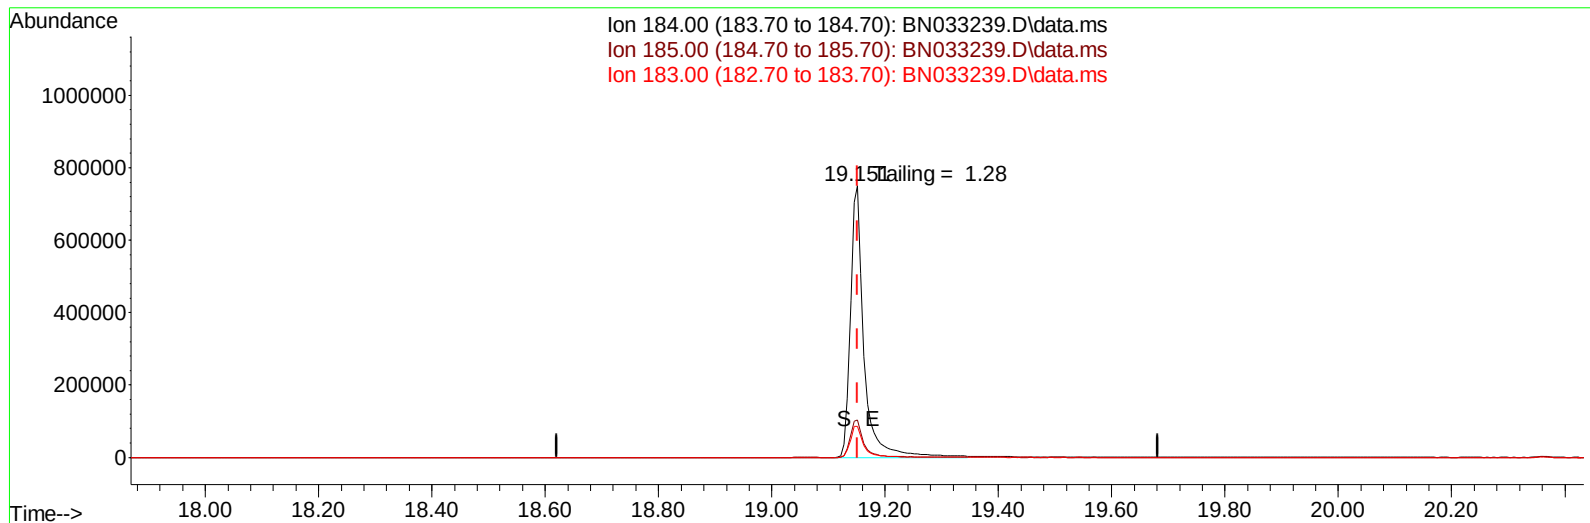

TIC: BN033239.D\data.ms

(77) Benzidine

19.151min (0.000) 0.00 ng

response **1263871**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.48
0.00	0.00	0.00