
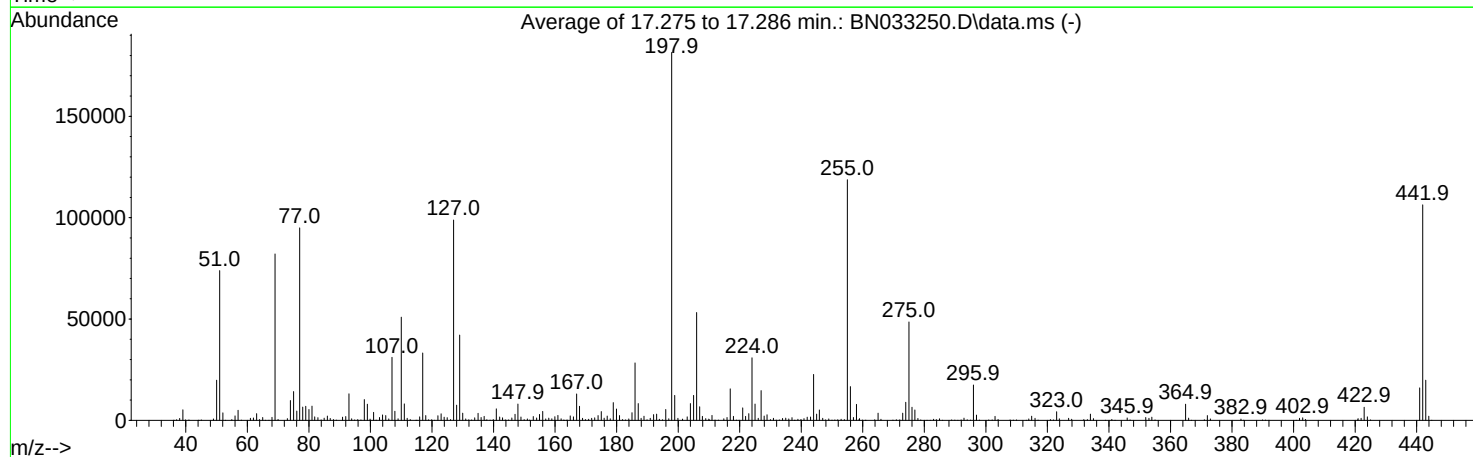


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080524\
Data File : BN033250.D
Acq On : 06 Aug 2024 00:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 05 23:57:48 2024

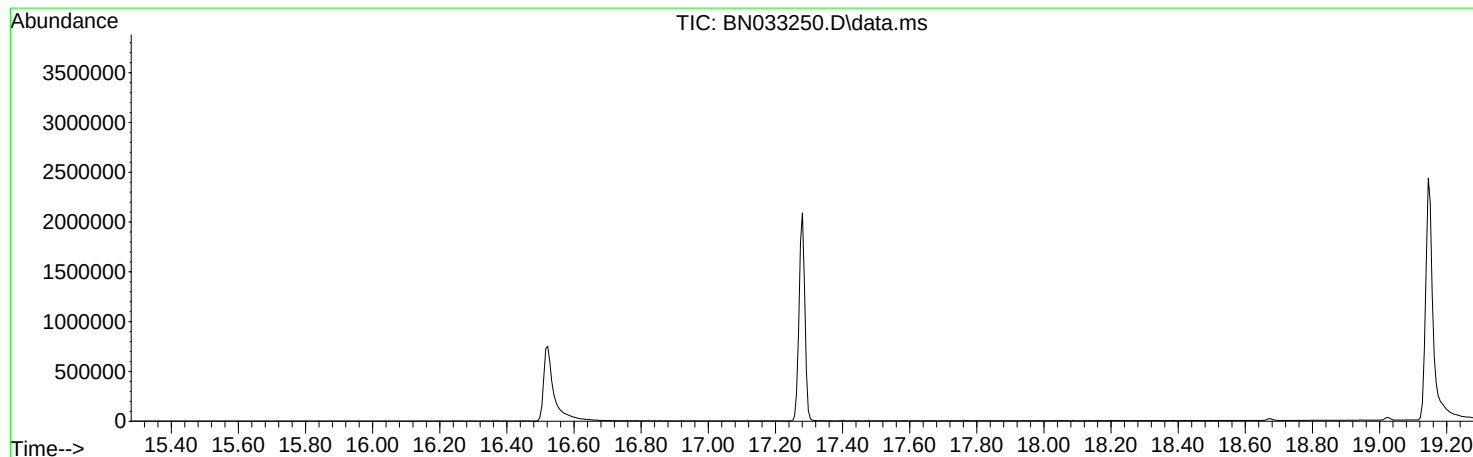




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	73899	PASS
68	69	0.00	2	1.8	1507	PASS
69	198	0.00	100	45.2	82088	PASS
70	69	0.00	2	0.6	473	PASS
127	198	10	80	54.4	98813	PASS
197	198	0.00	2	0.4	766	PASS
198	198	100	100	100.0	181483	PASS
199	198	5	9	6.8	12280	PASS
275	198	10	60	26.7	48523	PASS
365	198	1	100	4.4	7971	PASS
441	198	0.01	100	8.8	16046	PASS
442	442	50	100	100.0	106331	PASS
443	442	15	24	18.7	19845	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080524\
Data File : BN033250.D
Acq On : 06 Aug 2024 00:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 08:56:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

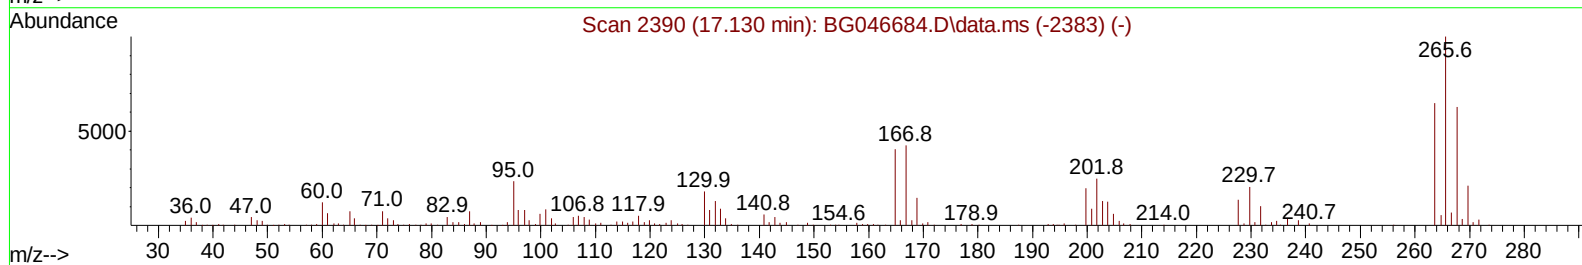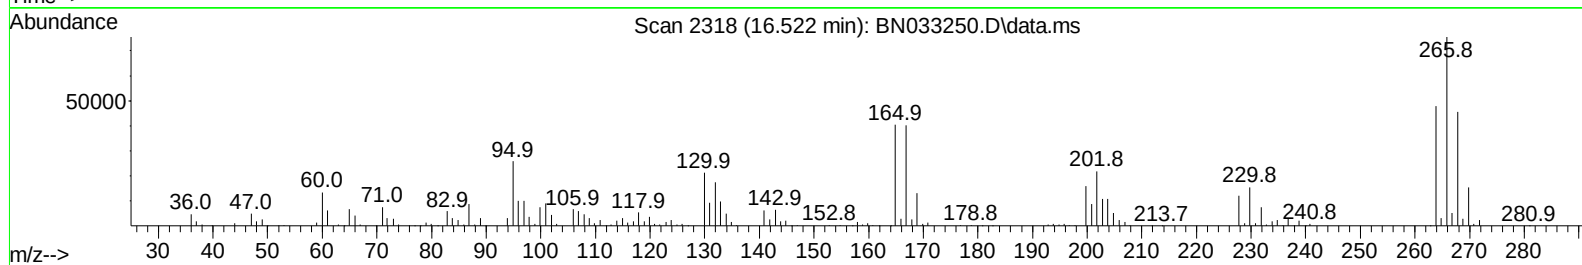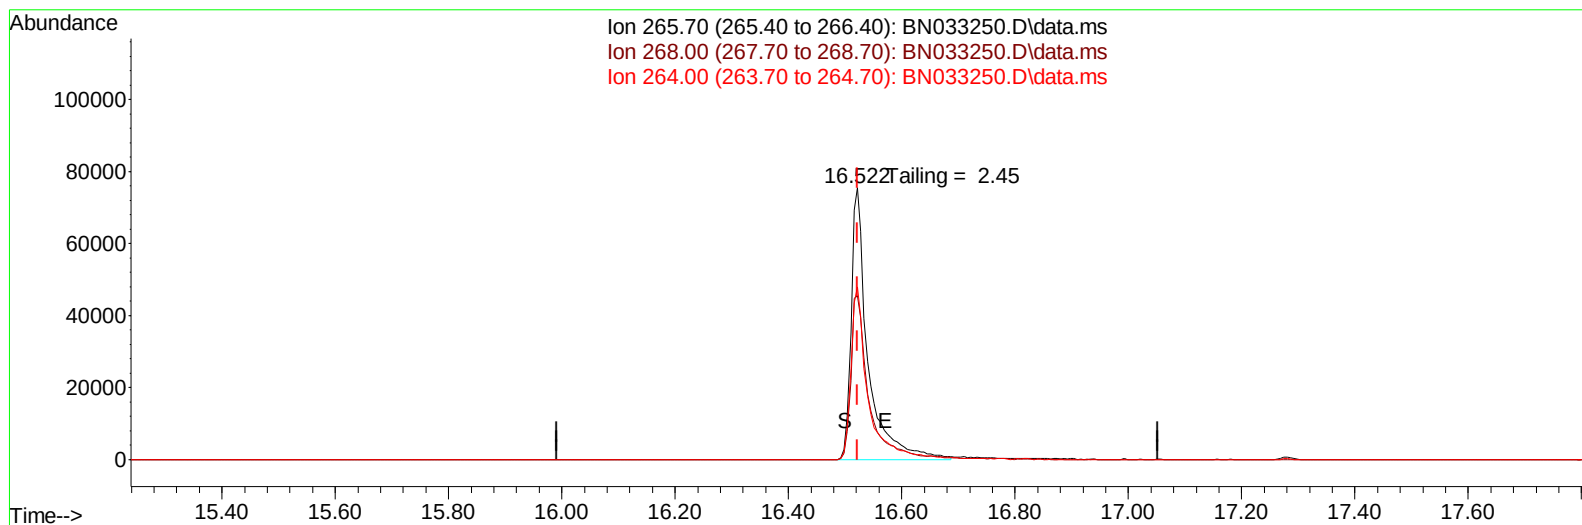

TIC: BN033250.D\data.ms

(70) Pentachlorophenol (C)

16.522min (-0.000) 13670.53 ng




response 157384

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.27
264.00	61.60	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080524\
Data File : BN033250.D
Acq On : 06 Aug 2024 00:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 08:56:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

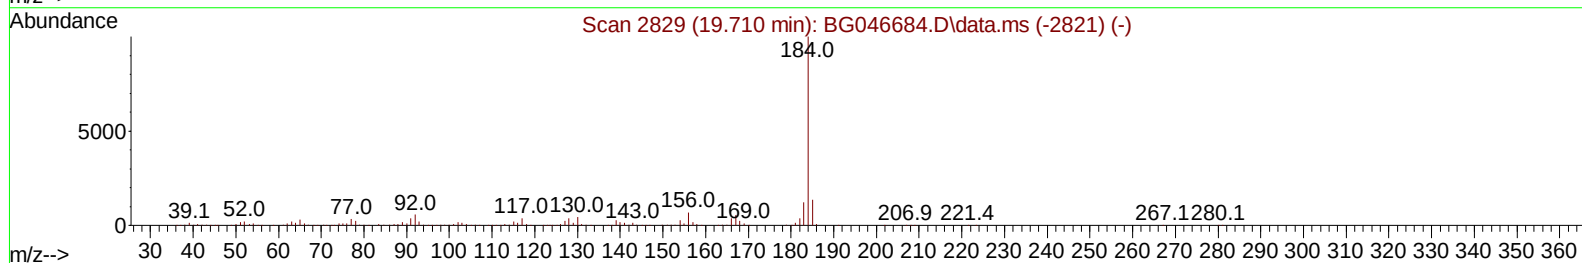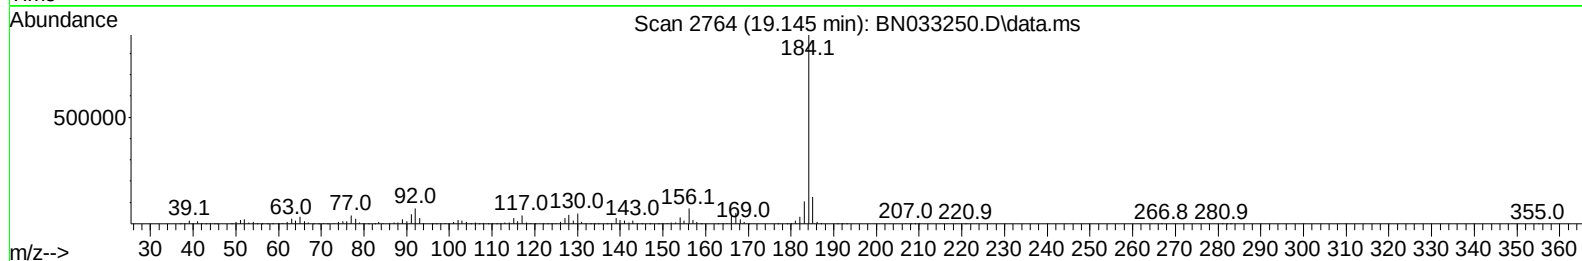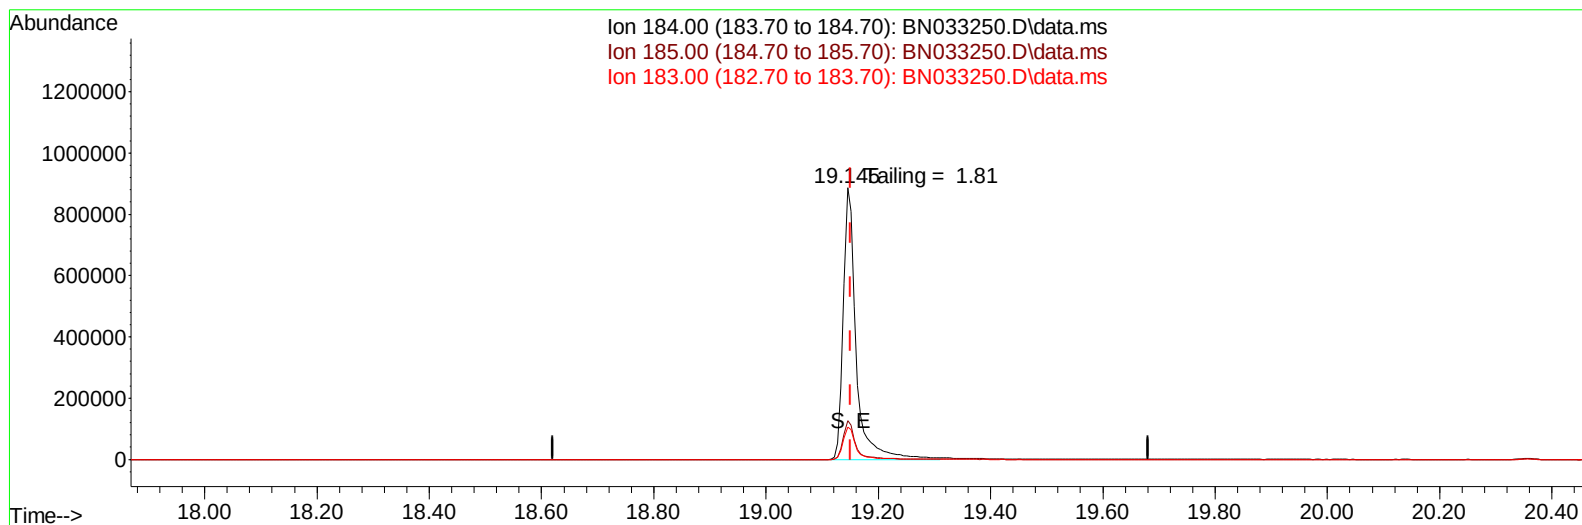

TIC: BN033250.D\data.ms

(77) Benzidine

19.145min (-0.006) 0.00 ng

response 1435972

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2024	BNA_N	<u>BN033250.D</u>
Compound Name	Response	Retention Time
DDT	750394	20.357
DDD	8802	19.963
DDE	807	19.41
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9609	760003	1.26

Instrument :
BNA_N
ClientSampleId :
DFTPP