


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080625\
Data File : BN037569.D
Acq On : 06 Aug 2025 13:11
Operator : RC/JU
Sample : DFTPP381
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP381

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
Title : SVOA CALIBRATION
Last Update : Fri Jul 18 16:22:45 2025

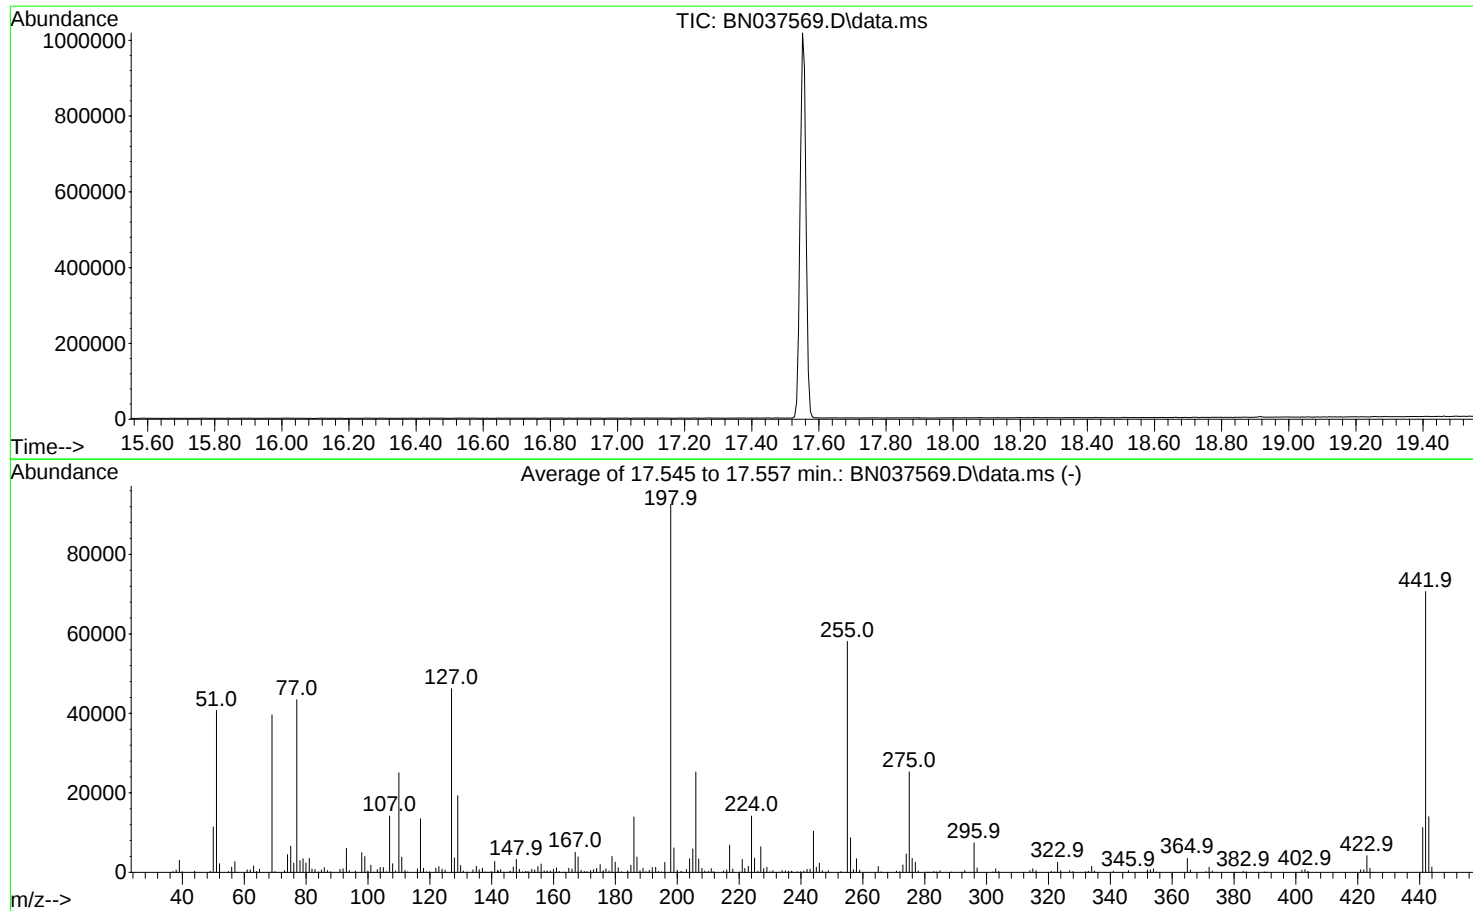

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	40733	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.9	39672	PASS
70	69	0.00	2	0.5	198	PASS
127	198	10	80	49.9	46227	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92557	PASS
199	198	5	9	6.7	6170	PASS
275	198	10	60	27.3	25291	PASS
365	198	1	100	3.8	3505	PASS
441	198	0.01	100	12.2	11305	PASS
442	198	50	100	76.3	70637	PASS
443	442	15	24	19.9	14031	PASS