
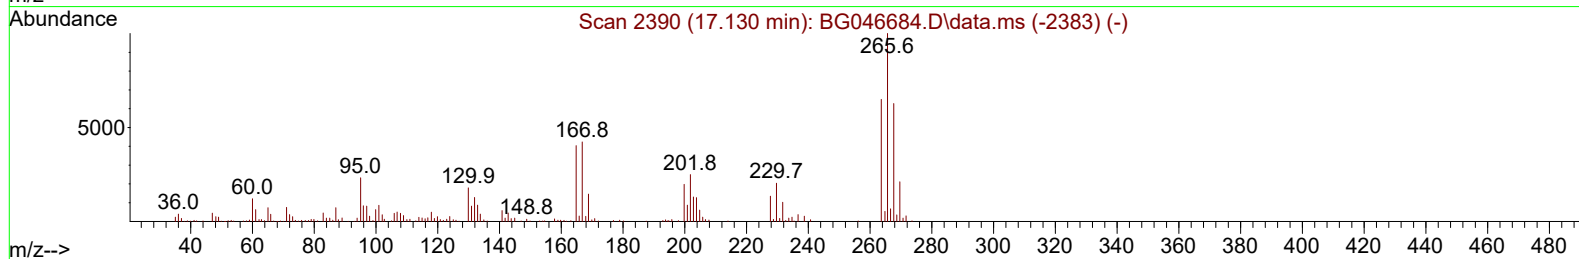
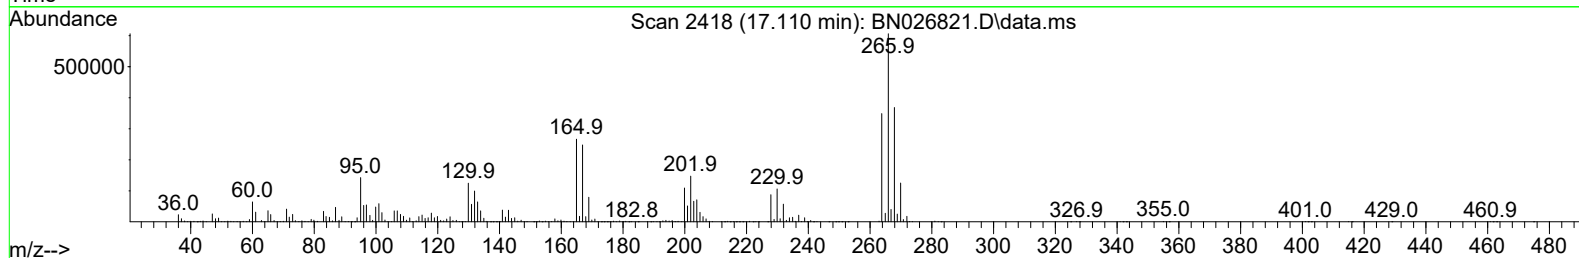


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080723\
Data File : BN026821.D
Acq On : 07 Aug 2023 08:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 09:25:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 09:25:41 2023
Response via : Initial Calibration

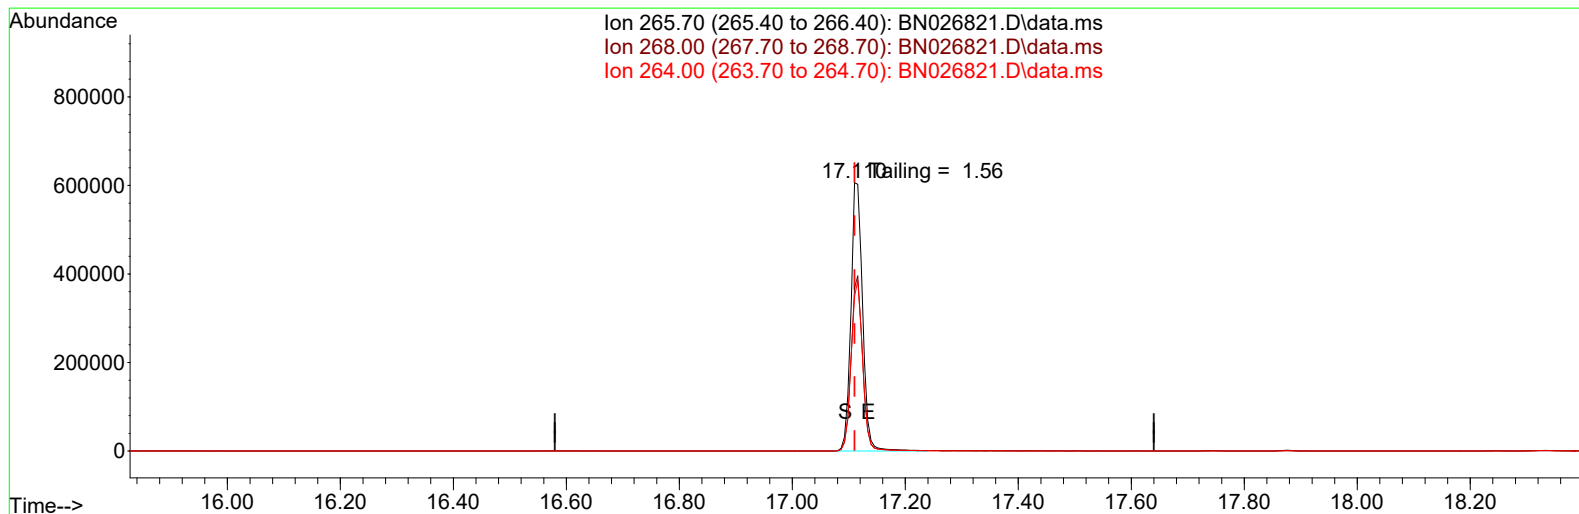

TIC: BN026821.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 26558.46 ng

response 880175

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.82
264.00	61.60	57.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080723\
Data File : BN026821.D
Acq On : 07 Aug 2023 08:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 09:25:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 09:25:41 2023
Response via : Initial Calibration

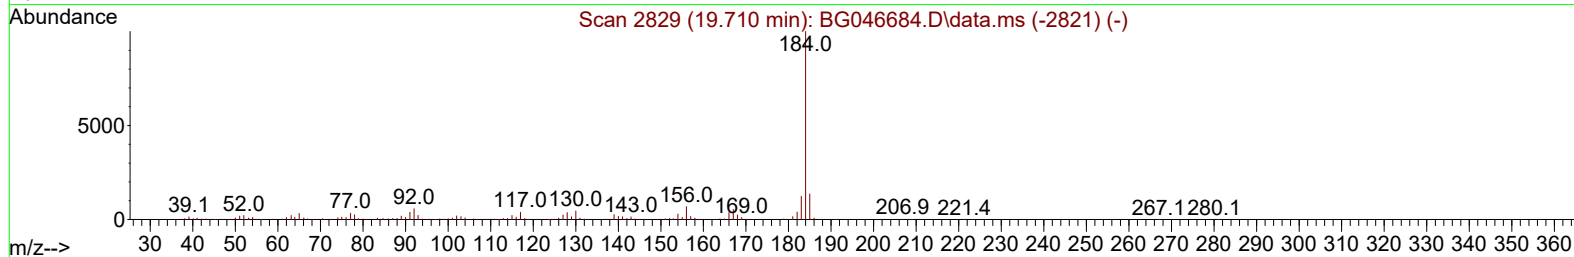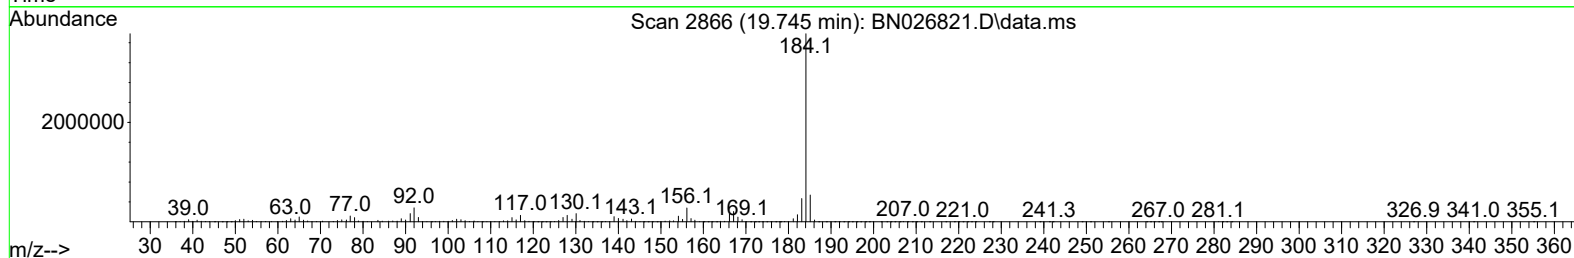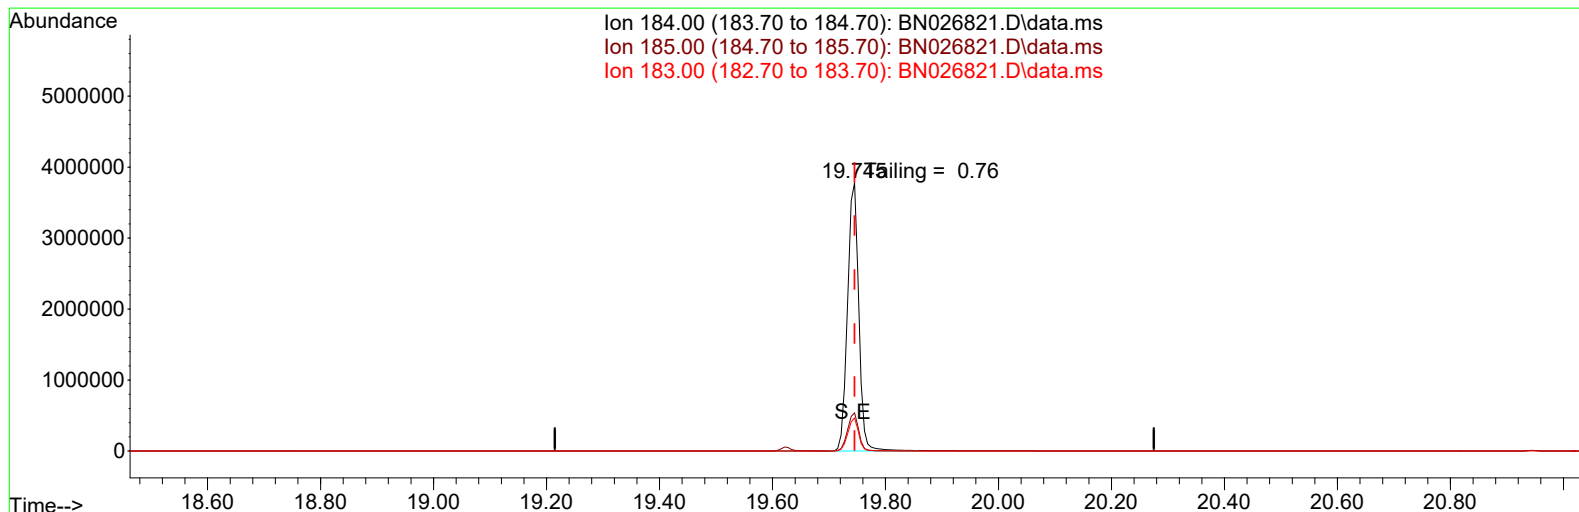

TIC: BN026821.D\data.ms

(77) Benzidine**19.745min (0.000) 1335663.38 ng****response 5270057**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	12.34
0.00	0.00	0.00