

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
 Data File : BN033294.D
 Acq On : 07 Aug 2024 22:24
 Operator : MA/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Aug 08 04:32:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 08 04:24:54 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	4461	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	13219	0.400	ng	0.00
13) Acenaphthene-d10	14.222	164	8372	0.400	ng	0.00
19) Phenanthrene-d10	16.970	188	18799	0.400	ng	0.00
29) Chrysene-d12	21.178	240	18827	0.400	ng	0.00
35) Perylene-d12	23.358	264	21395	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.206	112	34375	2.710	ng	0.00
5) Phenol-d6	6.759	99	47645	2.864	ng	0.00
8) Nitrobenzene-d5	8.717	82	25151	2.290	ng	0.00
11) 2-Methylnaphthalene-d10	11.950	152	63062	2.995	ng	0.00
14) 2,4,6-Tribromophenol	15.716	330	10374	2.585	ng	0.00
15) 2-Fluorobiphenyl	12.843	172	97795	3.079	ng	0.00
27) Fluoranthene-d10	19.011	212	161413	3.155	ng	0.00
31) Terphenyl-d14	19.628	244	97575	2.120	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.198	88	14645	2.681	ng	# 92
3) n-Nitrosodimethylamine	3.487	42	19337	3.725	ng	# 98
6) bis(2-Chloroethyl)ether	7.026	93	41546	2.901	ng	99
9) Naphthalene	10.404	128	114285	3.211	ng	96
10) Hexachlorobutadiene	10.703	225	20850	3.352	ng	# 99
12) 2-Methylnaphthalene	12.026	142	79078	3.252	ng	98
16) Acenaphthylene	13.934	152	126902	3.288	ng	100
17) Acenaphthene	14.286	154	81352	3.275	ng	99
18) Fluorene	15.281	166	107124	3.228	ng	99
20) 4,6-Dinitro-2-methylph...	15.345	198	4744	1.463	ng	# 27
21) 4-Bromophenyl-phenylether	16.175	248	35018	3.284	ng	97
22) Hexachlorobenzene	16.287	284	36939	3.342	ng	99
23) Atrazine	16.461	200	29177	2.987	ng	98
24) Pentachlorophenol	16.622	266	14393	2.625	ng	99
25) Phenanthrene	17.007	178	169141	3.242	ng	100
26) Anthracene	17.106	178	165514	3.419	ng	100
28) Fluoranthene	19.038	202	215119	3.401	ng	100
30) Pyrene	19.401	202	225330	3.012	ng	100
32) Benzo(a)anthracene	21.160	228	226536	3.194	ng	100
33) Chrysene	21.214	228	218946	3.266	ng	100
34) Bis(2-ethylhexyl)phtha...	21.151	149	118211	2.442	ng	100
36) Indeno(1,2,3-cd)pyrene	25.542	276	302258	3.787	ng	100
37) Benzo(b)fluoranthene	22.712	252	250636	3.214	ng	98
38) Benzo(k)fluoranthene	22.759	252	243911	3.308	ng	97
39) Benzo(a)pyrene	23.268	252	223769	3.326	ng	97
40) Dibenzo(a,h)anthracene	25.572	278	238179	3.788	ng	97
41) Benzo(g,h,i)perylene	26.200	276	258703	3.828	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033294.D
Acq On : 07 Aug 2024 22:24
Operator : MA/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Aug 08 04:32:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:24:54 2024
Response via : Initial Calibration




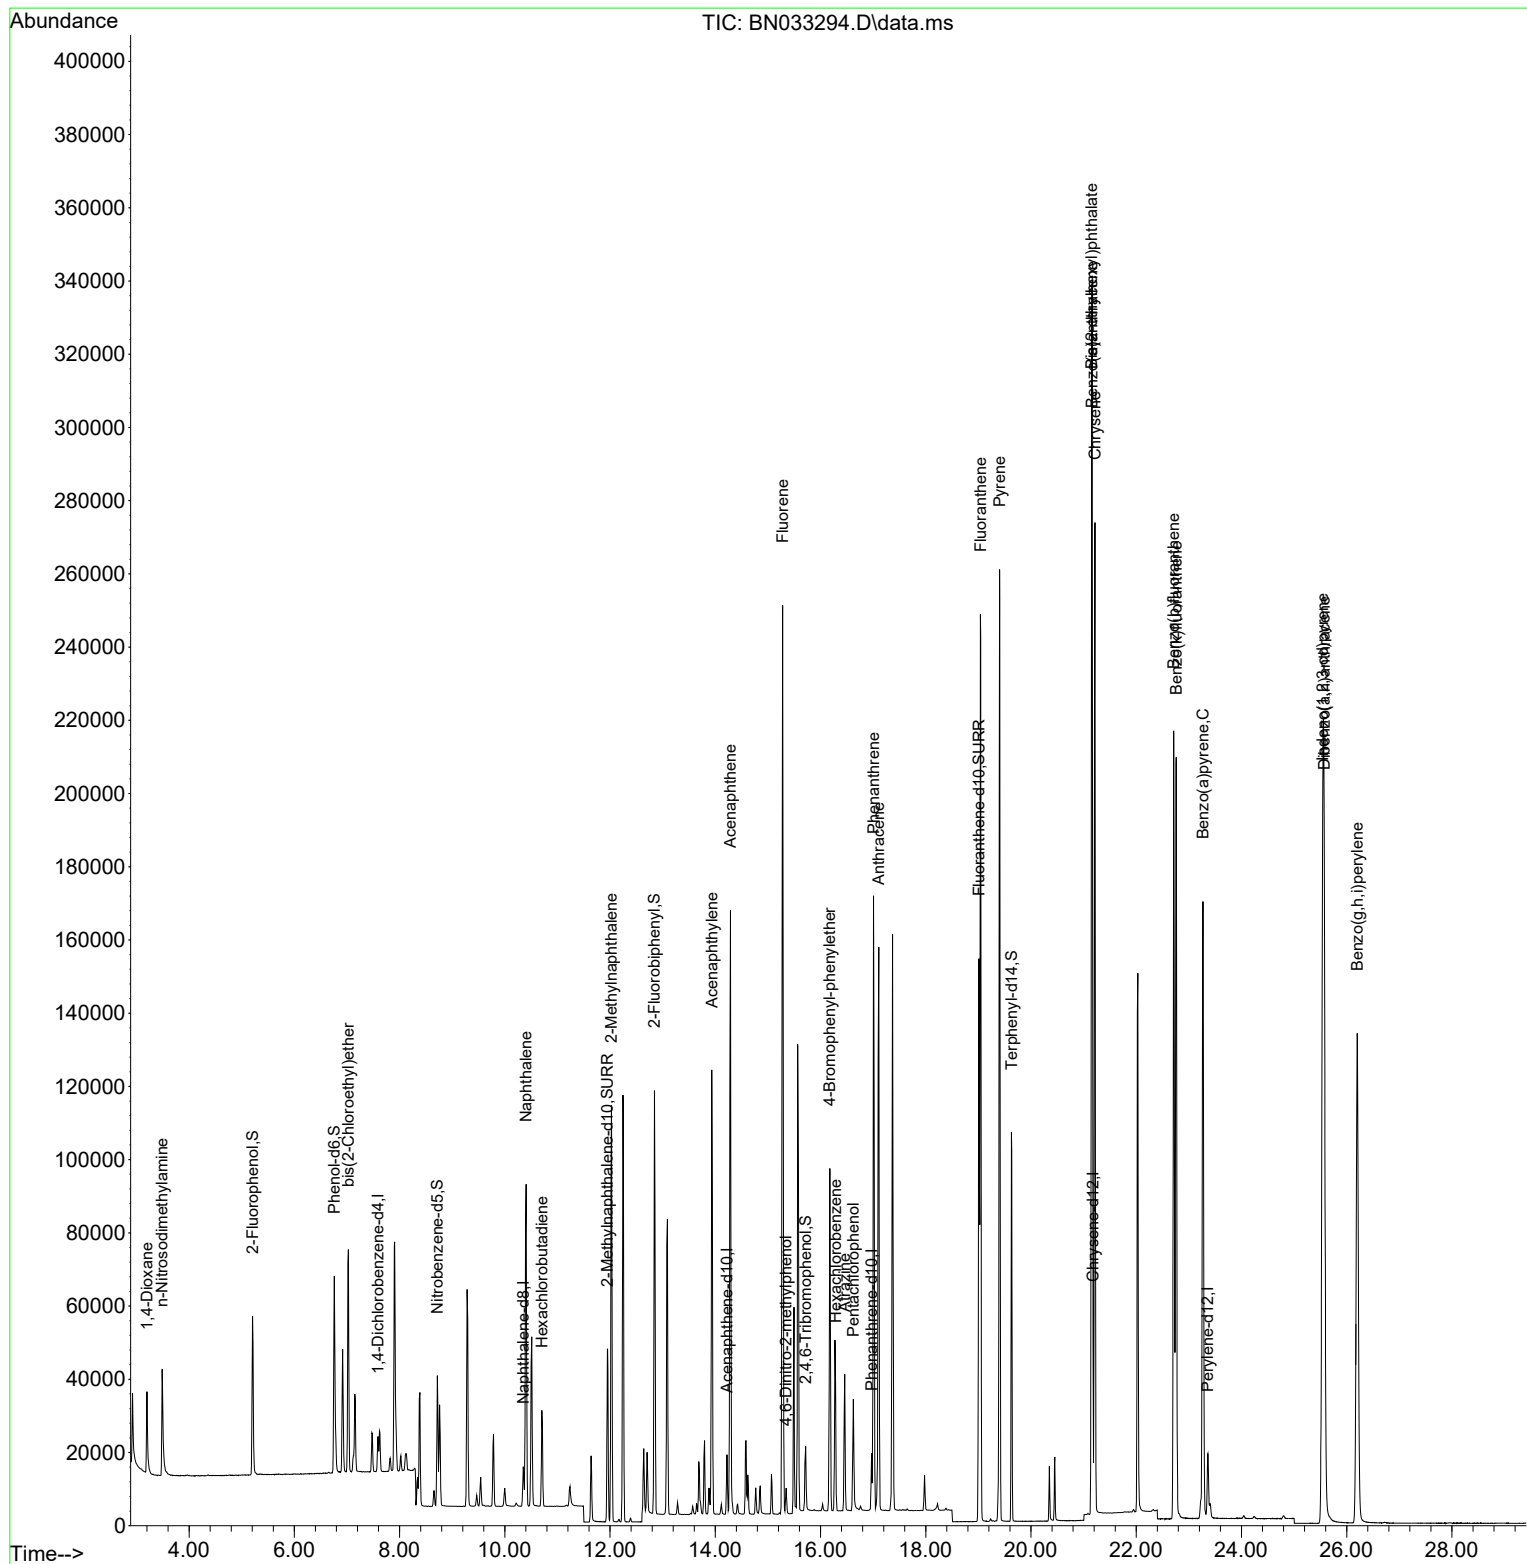




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.589 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN033294.D
 Acq: 07 Aug 2024 22:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:152 Resp: 4461
 Ion Ratio Lower Upper
 152 100
 150 150.2 120.7 181.1
 115 68.6 55.8 83.8

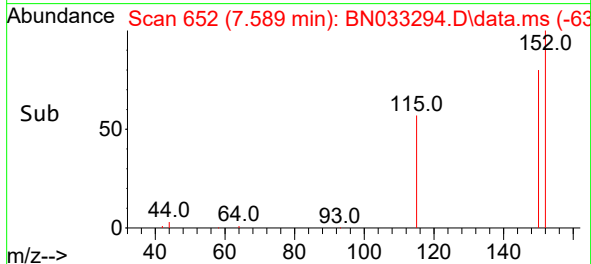

#2
 1,4-Dioxane
 Concen: 2.681 ng
 RT: 3.198 min Scan# 44
 Delta R.T. 0.000 min
 Lab File: BN033294.D
 Acq: 07 Aug 2024 22:24

Tgt Ion: 88 Resp: 14645
 Ion Ratio Lower Upper
 88 100
 43 32.6 37.0 55.6#
 58 81.6 65.1 97.7









#3
 n-Nitrosodimethylamine
 Concen: 3.725 ng
 RT: 3.487 min Scan# 84
 Delta R.T. -0.007 min
 Lab File: BN033294.D
 Acq: 07 Aug 2024 22:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion: 42 Resp: 19337
 Ion Ratio Lower Upper
 42 100
 74 116.4 94.9 142.3
 44 6.9 7.0 10.4#

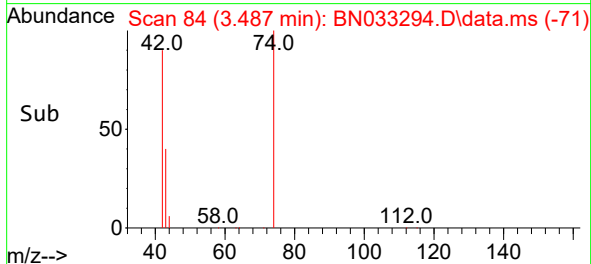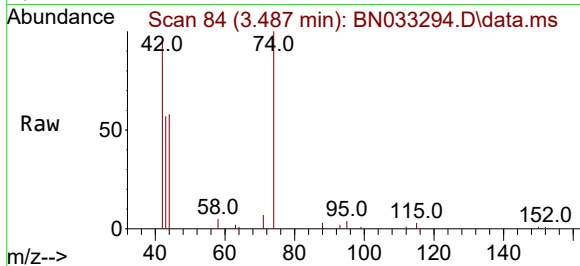

#4
 2-Fluorophenol
 Concen: 2.710 ng
 RT: 5.206 min Scan# 322
 Delta R.T. 0.000 min
 Lab File: BN033294.D
 Acq: 07 Aug 2024 22:24

Tgt Ion: 112 Resp: 34375
 Ion Ratio Lower Upper
 112 100
 64 60.5 48.7 73.1
 63 30.9 25.4 38.2




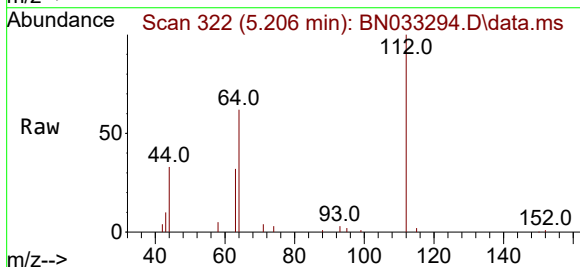




#5
Phenol-d6
Concen: 2.864 ng
RT: 6.759 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 47645
Ion Ratio Lower Upper
99 100
42 21.6 19.3 28.9
71 32.3 27.6 41.4

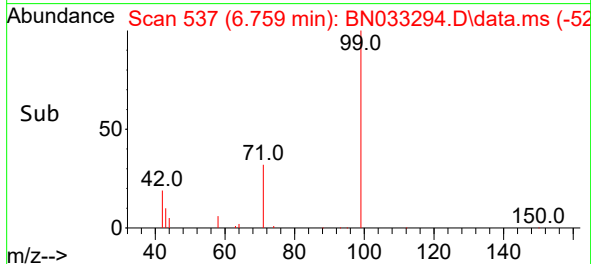

#6
bis(2-Chloroethyl)ether
Concen: 2.901 ng
RT: 7.026 min Scan# 574
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion: 93 Resp: 41546
Ion Ratio Lower Upper
93 100
63 80.8 64.5 96.7
95 32.5 26.6 39.8





#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.351 min Scan# 94

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2

Tgt Ion:136 Resp: 13219





Ion Ratio Lower Upper

136 100

137 12.0 9.9 14.9

54 13.8 11.4 17.2

68 11.2 9.5 14.3



#8

Nitrobenzene-d5

Concen: 2.290 ng

RT: 8.717 min Scan# 790

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24




Tgt Ion: 82 Resp: 25151


Ion Ratio Lower Upper

82 100

128 38.0 29.4 44.2

54 57.6 50.0 75.0


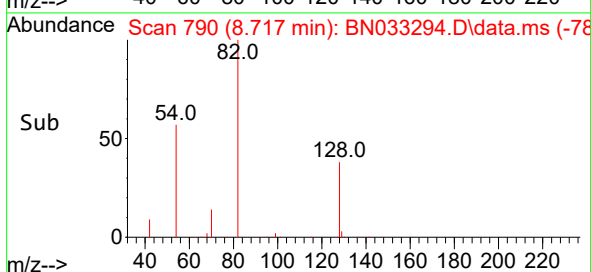






#9
Naphthalene
Concen: 3.211 ng
RT: 10.404 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:128 Resp: 114285
Ion Ratio Lower Upper
128 100
129 11.0 10.1 15.1
127 12.9 11.4 17.2

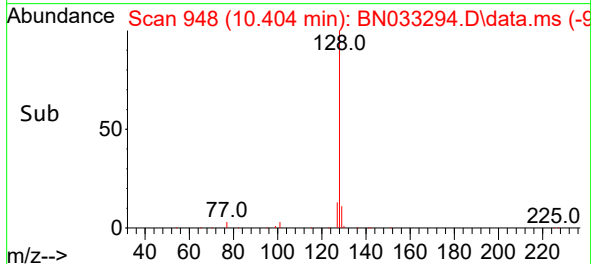

#10
Hexachlorobutadiene
Concen: 3.352 ng
RT: 10.703 min Scan# 976
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:225 Resp: 20850
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.6 51.8 77.6




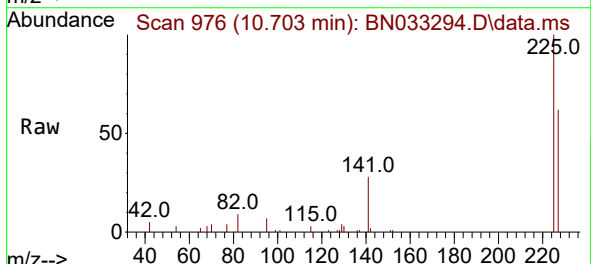




#11
2-Methylnaphthalene-d10
Concen: 2.995 ng
RT: 11.950 min Scan# 1170
Delta R.T. -0.004 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 63062
Ion Ratio Lower Upper
152 100
151 20.6 16.7 25.1

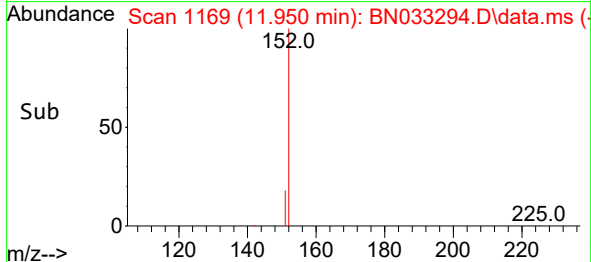

#12
2-Methylnaphthalene
Concen: 3.252 ng
RT: 12.026 min Scan# 1189
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:142 Resp: 79078
Ion Ratio Lower Upper
142 100
141 88.7 70.5 105.7
115 34.7 30.3 45.5




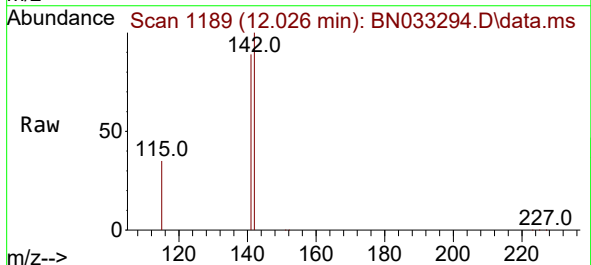


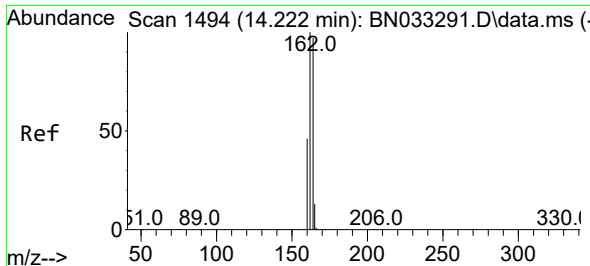

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.222 min Scan# 1494
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 8372
Ion Ratio Lower Upper
164 100
162 103.9 82.6 124.0
160 47.5 38.2 57.4

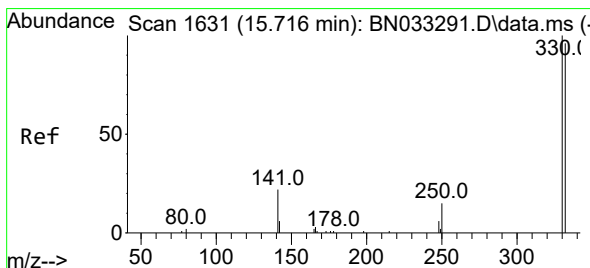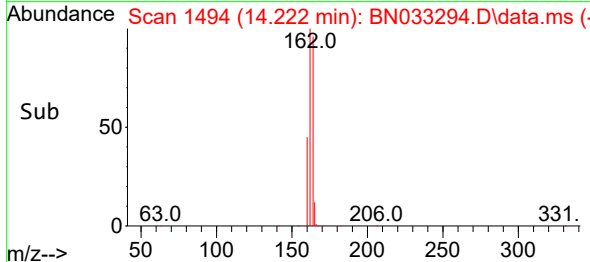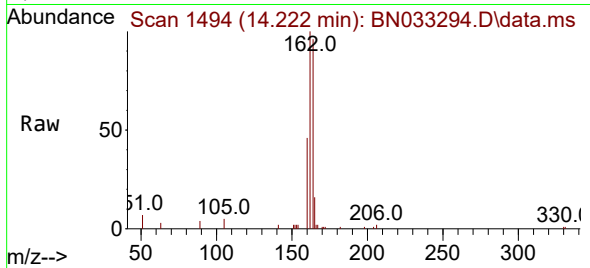

#14
2,4,6-Tribromophenol
Concen: 2.585 ng
RT: 15.716 min Scan# 1631
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:330 Resp: 10374
Ion Ratio Lower Upper
330 100
332 96.8 75.6 113.4
141 40.0 31.0 46.4

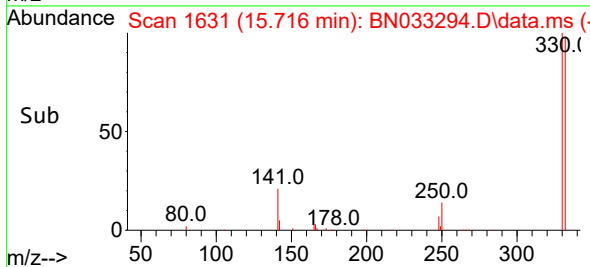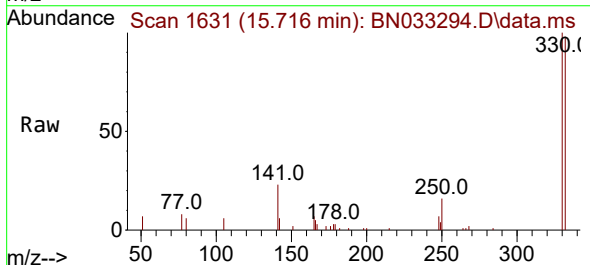



#15

2-Fluorobiphenyl

Concen: 3.079 ng

RT: 12.843 min Scan# 1365

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:172 Resp: 97795

Ion Ratio Lower Upper

172 100

171 35.1 28.3 42.5

170 23.9 19.4 29.2

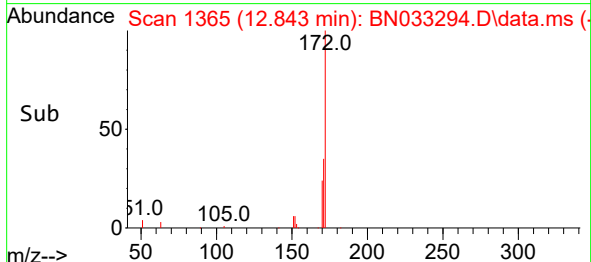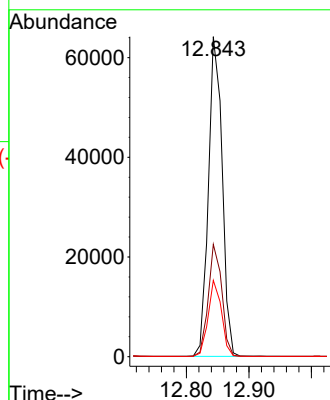

#16

Acenaphthylene

Concen: 3.288 ng

RT: 13.934 min Scan# 1467

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24




Tgt Ion:152 Resp: 126902


Ion Ratio Lower Upper

152 100

151 19.6 15.7 23.5

153 13.0 10.3 15.5



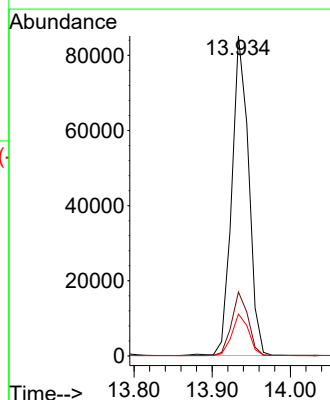





#17
Acenaphthene
Concen: 3.275 ng
RT: 14.286 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:154 Resp: 81352
Ion Ratio Lower Upper
154 100
153 110.4 89.5 134.3
152 53.6 43.6 65.4

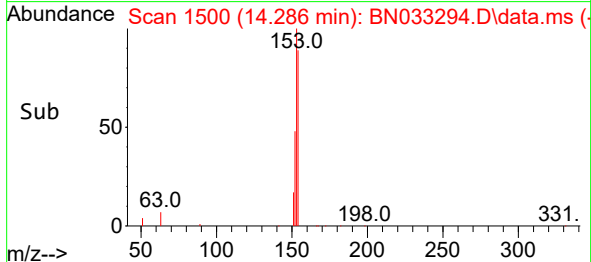

#18
Fluorene
Concen: 3.228 ng
RT: 15.281 min Scan# 1593
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:166 Resp: 107124
Ion Ratio Lower Upper
166 100
165 97.5 78.9 118.3
167 13.4 10.6 16.0

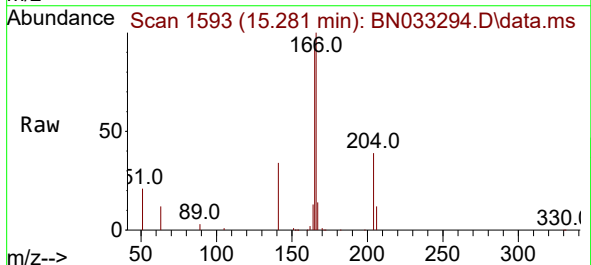



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.970 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:188 Resp: 18799

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 12.5 10.5 15.7

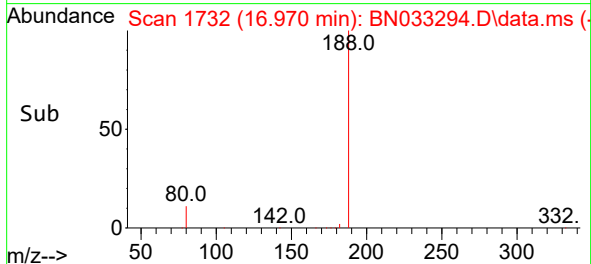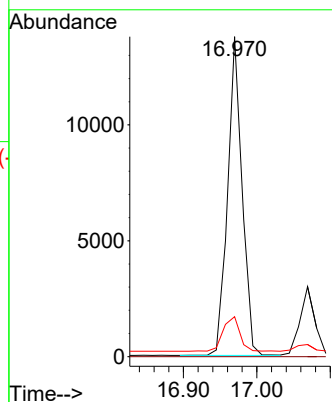

#20

4,6-Dinitro-2-methylphenol

Concen: 1.463 ng

RT: 15.345 min Scan# 1599

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24




Tgt Ion:198 Resp: 4744


Ion Ratio Lower Upper

198 100

51 59.8 127.9 191.9#

105 55.7 112.3 168.5#



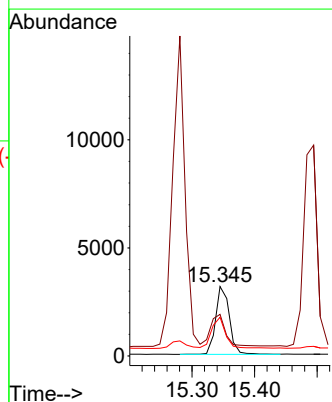



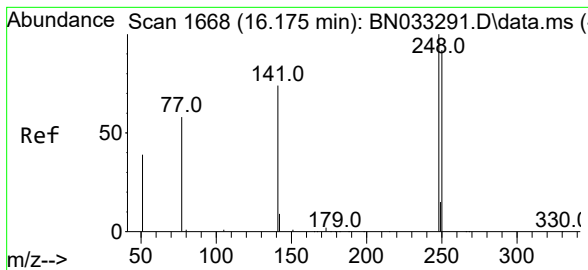

#21
4-Bromophenyl-phenylether
Concen: 3.284 ng
RT: 16.175 min Scan# 1668
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:248 Resp: 35018
Ion Ratio Lower Upper
248 100
250 92.8 74.6 112.0
141 71.8 62.2 93.2

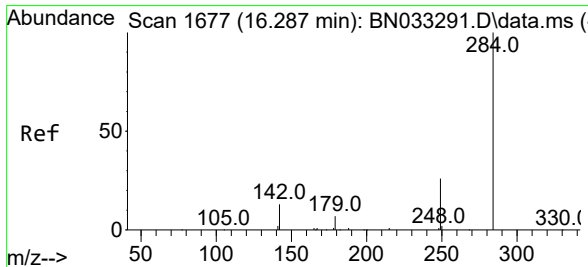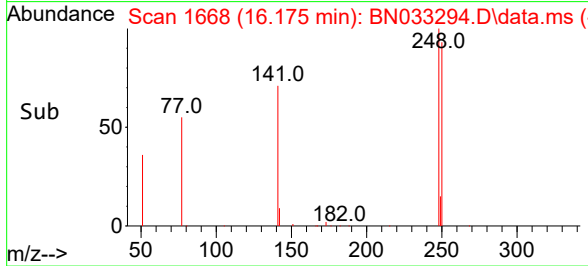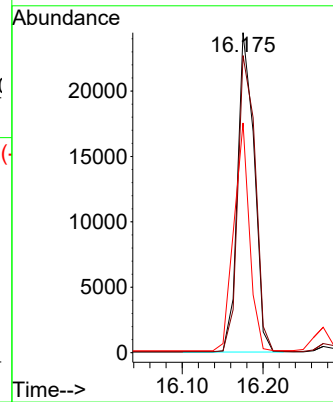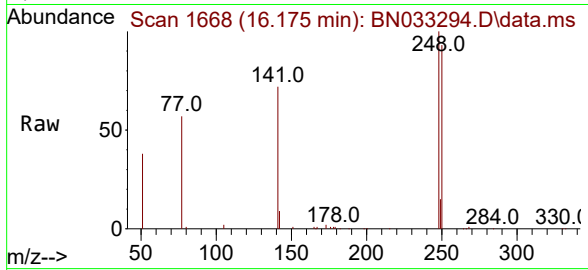

#22
Hexachlorobenzene
Concen: 3.342 ng
RT: 16.287 min Scan# 1677
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:284 Resp: 36939
Ion Ratio Lower Upper
284 100
142 38.2 30.6 45.8
249 31.3 24.6 36.8


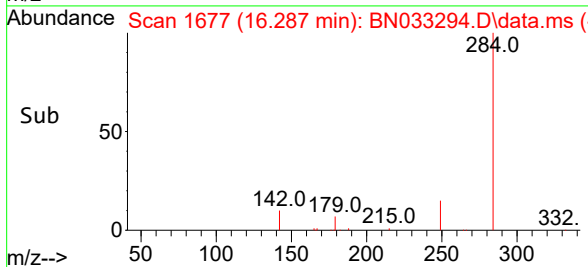
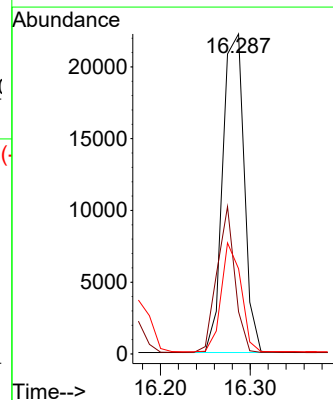
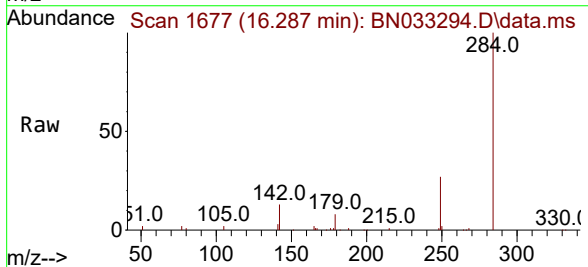


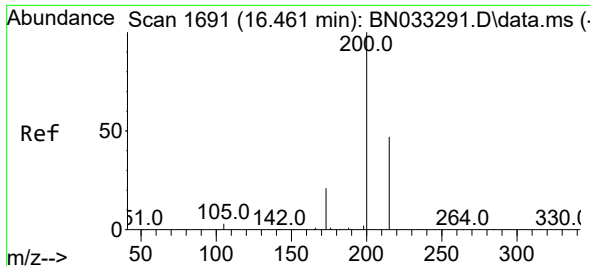

#23
Atrazine
Concen: 2.987 ng
RT: 16.461 min Scan# 1691
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:200 Resp: 29177
Ion Ratio Lower Upper
200 100
173 21.8 18.9 28.3
215 47.0 38.6 57.8

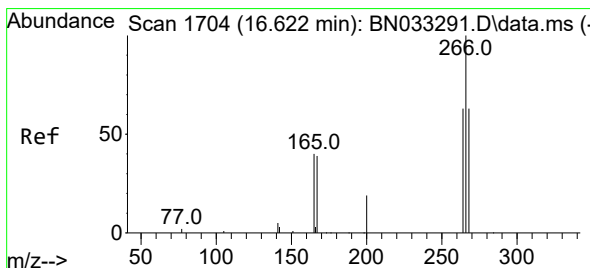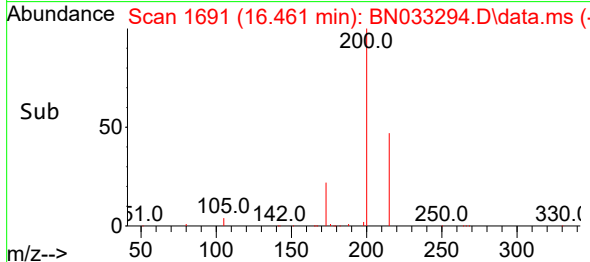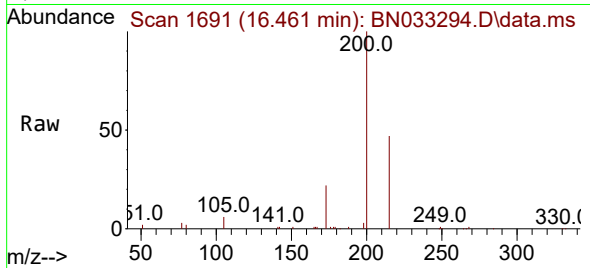

#24
Pentachlorophenol
Concen: 2.625 ng
RT: 16.622 min Scan# 1704
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:266 Resp: 14393
Ion Ratio Lower Upper
266 100
264 63.0 50.3 75.5
268 62.6 51.0 76.4

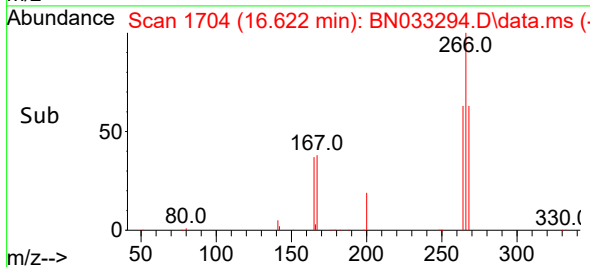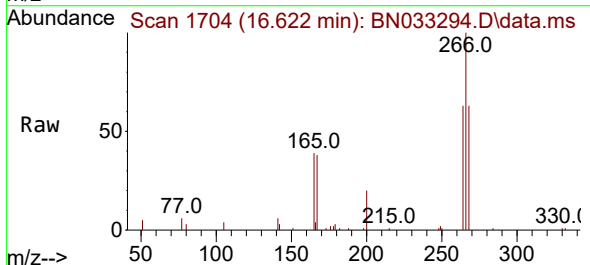



#25

Phenanthrene

Concen: 3.242 ng

RT: 17.007 min Scan# 1735

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:178 Resp: 169141

Ion Ratio Lower Upper

178 100

176 19.1 15.2 22.8

179 15.1 12.0 18.0

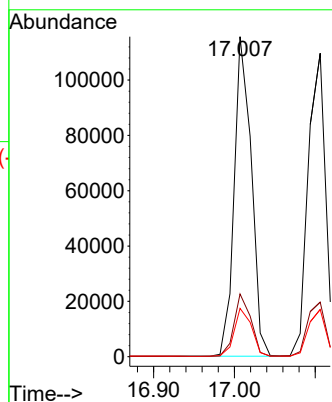

#26

Anthracene

Concen: 3.419 ng

RT: 17.106 min Scan# 1743

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24




Tgt Ion:178 Resp: 165514


Ion Ratio Lower Upper

178 100

176 18.4 14.8 22.2

179 15.2 12.2 18.4


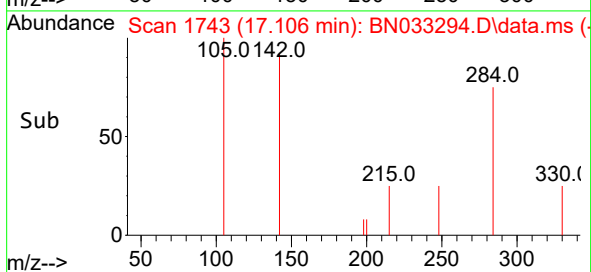
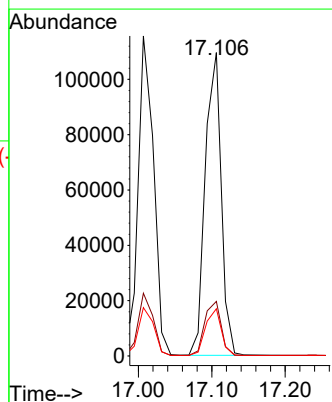





#27
Fluoranthene-d10
Concen: 3.155 ng
RT: 19.011 min Scan# 1964
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 161413
Ion Ratio Lower Upper
212 100
106 15.2 12.2 18.4
104 8.5 6.9 10.3

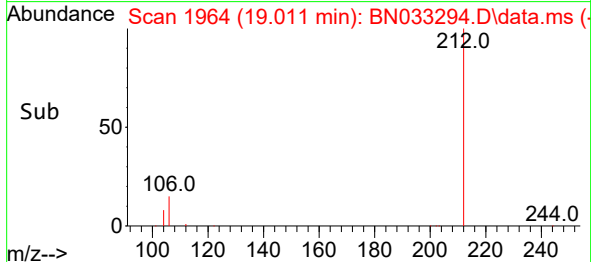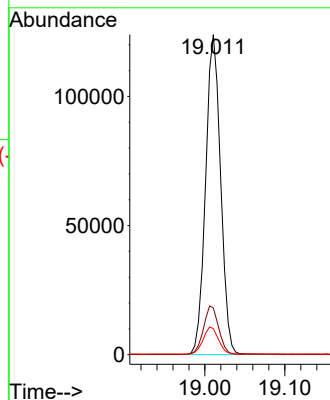

#28
Fluoranthene
Concen: 3.401 ng
RT: 19.038 min Scan# 1970
Delta R.T. -0.005 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:202 Resp: 215119
Ion Ratio Lower Upper
202 100
101 12.0 9.4 14.0
203 17.4 13.8 20.6

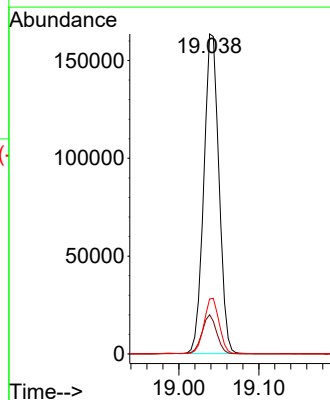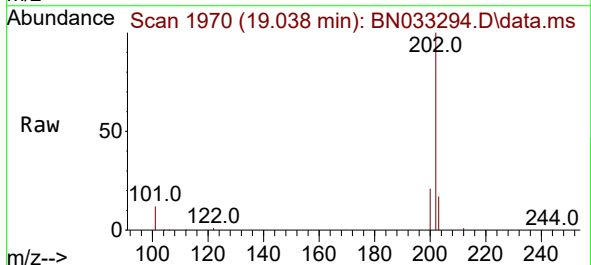

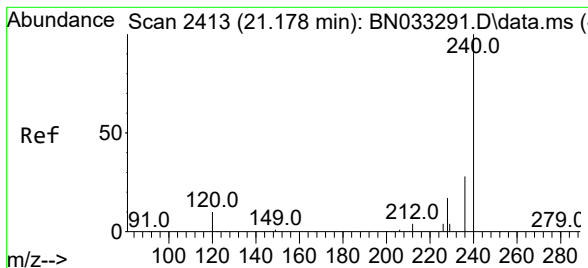

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.178 min Scan# 2413

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:240 Resp: 18827

Ion Ratio Lower Upper

240 100

120 10.5 9.0 13.6

236 27.5 22.4 33.6

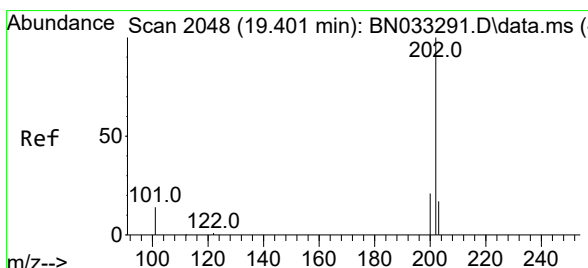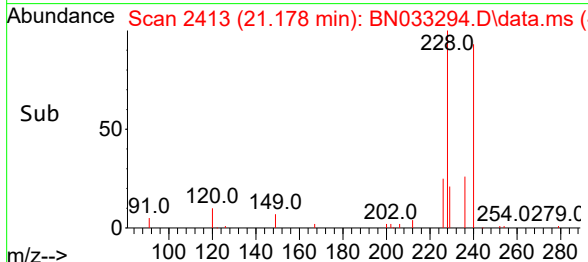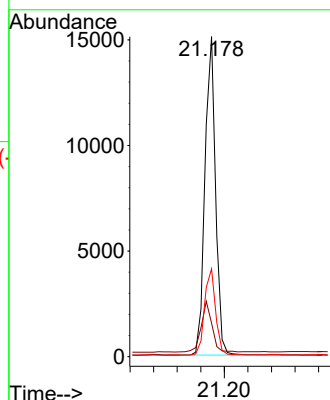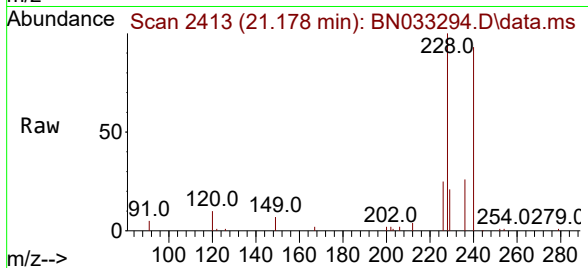

#30

Pyrene

Concen: 3.012 ng

RT: 19.401 min Scan# 2048

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24




Tgt Ion:202 Resp: 225330


Ion Ratio Lower Upper

202 100

200 20.9 16.7 25.1

203 17.8 14.2 21.4

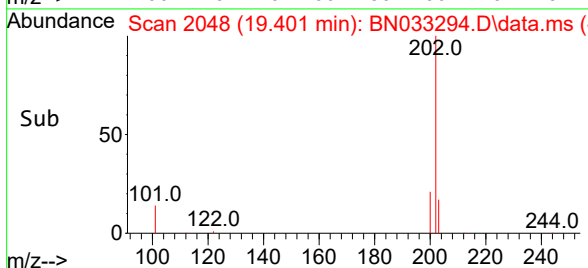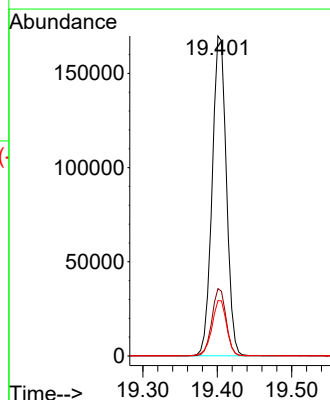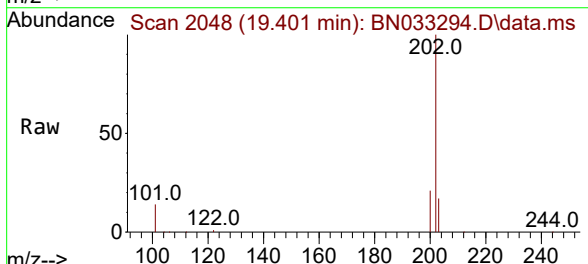



#31

Terphenyl-d14

Concen: 2.120 ng

RT: 19.628 min Scan# 2097

Delta R.T. -0.005 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:244 Resp: 97575

Ion Ratio Lower Upper

244 100

212 8.8 7.2 10.8

122 17.4 12.7 19.1

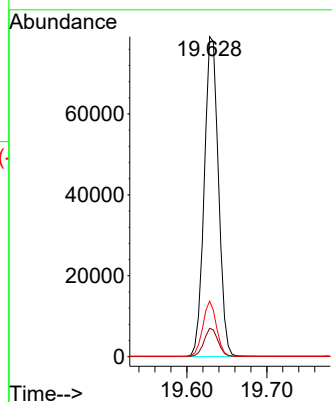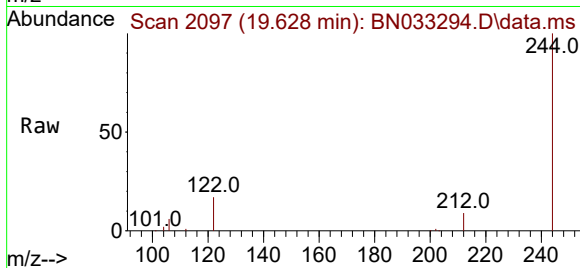

#32

Benzo(a)anthracene

Concen: 3.194 ng

RT: 21.160 min Scan# 2411

Delta R.T. 0.000 min

Lab File: BN033294.D

Acq: 07 Aug 2024 22:24




Tgt Ion:228 Resp: 226536


Ion Ratio Lower Upper

228 100

226 27.5 22.1 33.1

229 19.6 15.6 23.4




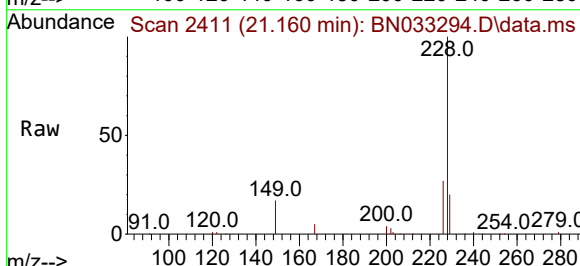


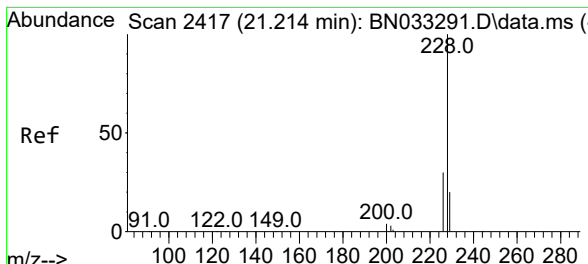

#33
 Chrysene
 Concen: 3.266 ng
 RT: 21.214 min Scan# 2417
 Delta R.T. 0.000 min
 Lab File: BN033294.D
 Acq: 07 Aug 2024 22:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:	228	Resp:	218946
Ion Ratio	Lower	Upper	
228	100		
226	30.0	23.8	35.8
229	19.5	15.8	23.8

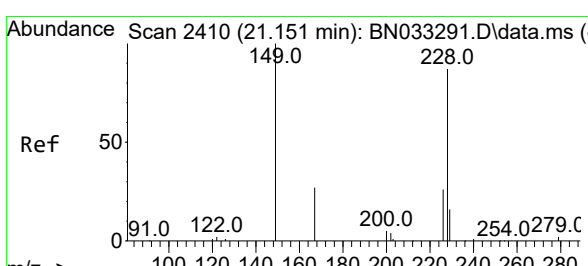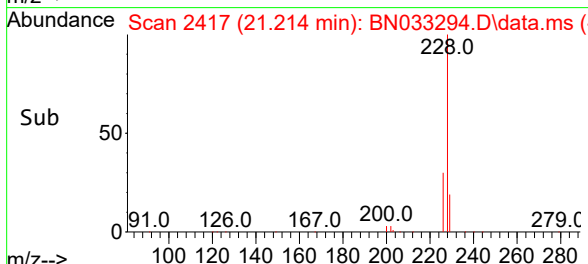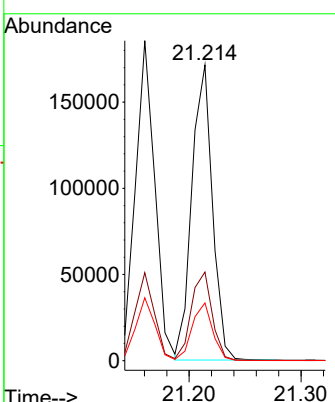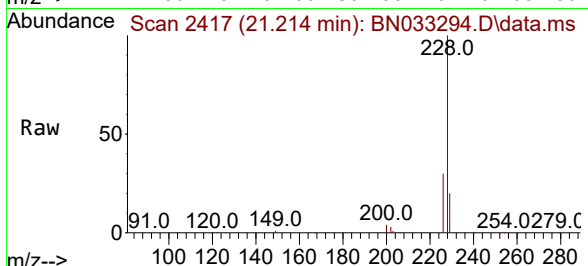

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 2.442 ng
 RT: 21.151 min Scan# 2410
 Delta R.T. 0.000 min
 Lab File: BN033294.D
 Acq: 07 Aug 2024 22:24

Tgt Ion:	149	Resp:	118211
Ion Ratio	Lower	Upper	
149	100		
167	27.2	21.6	32.4
279	3.0	2.6	4.0


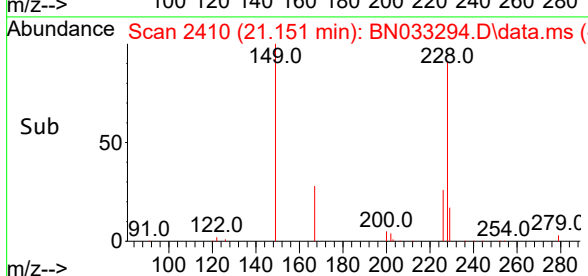
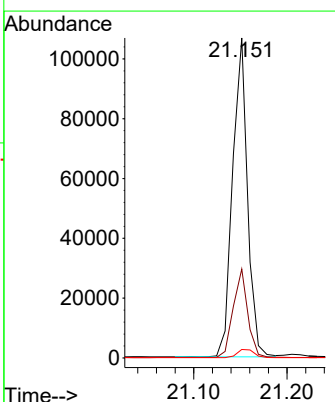
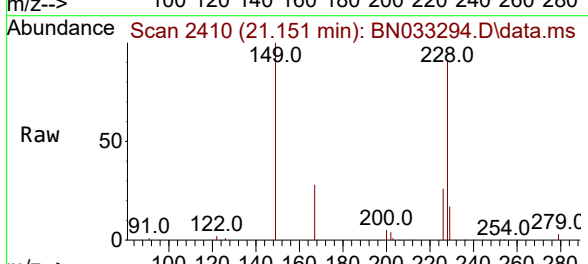




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.358 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:264 Resp: 21395
Ion Ratio Lower Upper
264 100
260 26.1 21.4 32.0
265 28.9 22.4 33.6

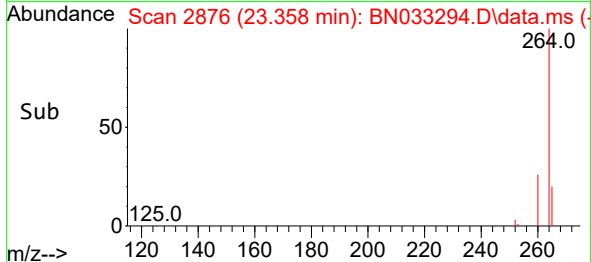

#36
Indeno(1,2,3-cd)pyrene
Concen: 3.787 ng
RT: 25.542 min Scan# 3623
Delta R.T. -0.003 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Tgt Ion:276 Resp: 302258
Ion Ratio Lower Upper
276 100
138 28.6 22.7 34.1
277 24.8 19.8 29.8


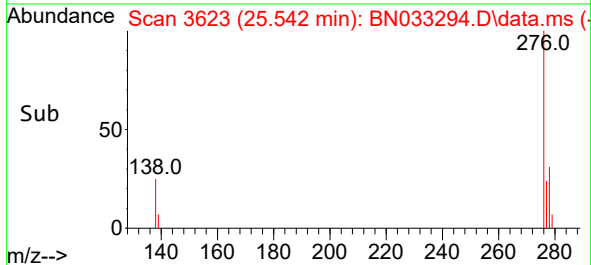






#37
Benzo(b)fluoranthene
Concen: 3.214 ng
RT: 22.712 min Scan# 2655
Delta R.T. -0.003 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 250636
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.6
125 11.3 10.0 15.0

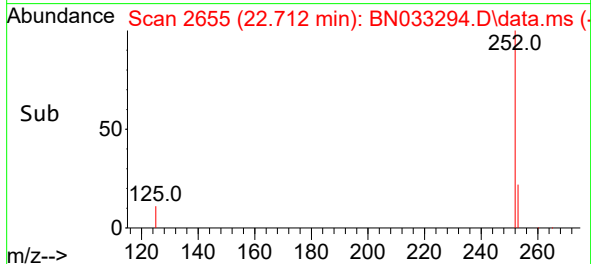

#38
Benzo(k)fluoranthene
Concen: 3.308 ng
RT: 22.759 min Scan# 2671
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24


Tgt Ion:252 Resp: 243911
Ion Ratio Lower Upper
252 100
253 21.8 18.3 27.5
125 11.3 10.2 15.4








#39
Benzo(a)pyrene
Concen: 3.326 ng
RT: 23.268 min Scan# 2845
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2







Tgt Ion:252 Resp: 223769
Ion Ratio Lower Upper
252 100
253 21.8 18.2 27.4
125 12.4 11.4 17.2

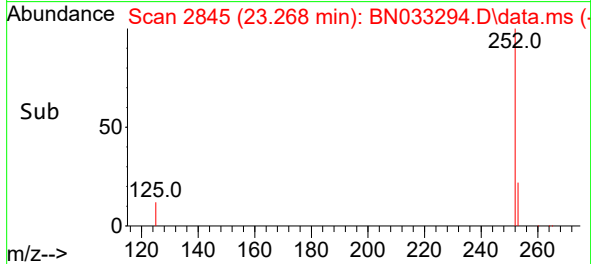

#40
Dibenzo(a,h)anthracene
Concen: 3.788 ng
RT: 25.572 min Scan# 3633
Delta R.T. 0.000 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24


Tgt Ion:278 Resp: 238179
Ion Ratio Lower Upper
278 100
139 18.7 16.3 24.5
279 23.3 19.4 29.2

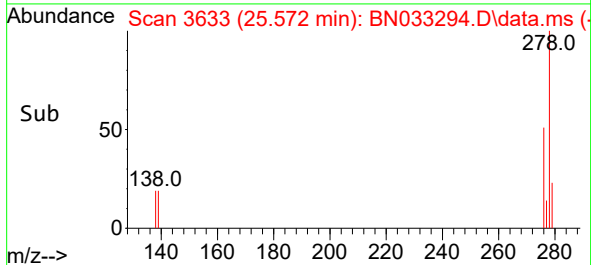

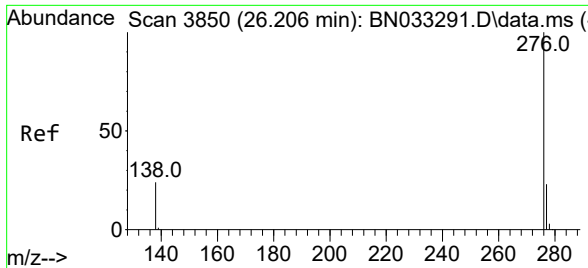

#41
Benzo(g,h,i)perylene
Concen: 3.828 ng
RT: 26.200 min Scan# 3848
Delta R.T. -0.006 min
Lab File: BN033294.D
Acq: 07 Aug 2024 22:24

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

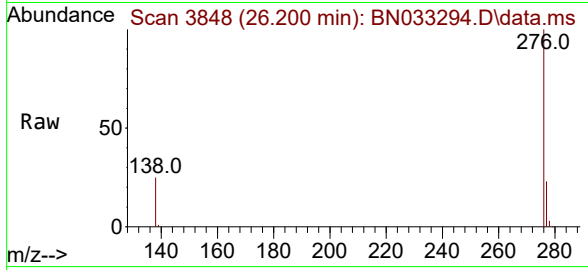

Tgt Ion:276 Resp: 258703
Ion Ratio Lower Upper
276 100
277 23.5 19.0 28.4
138 24.8 20.8 31.2

