
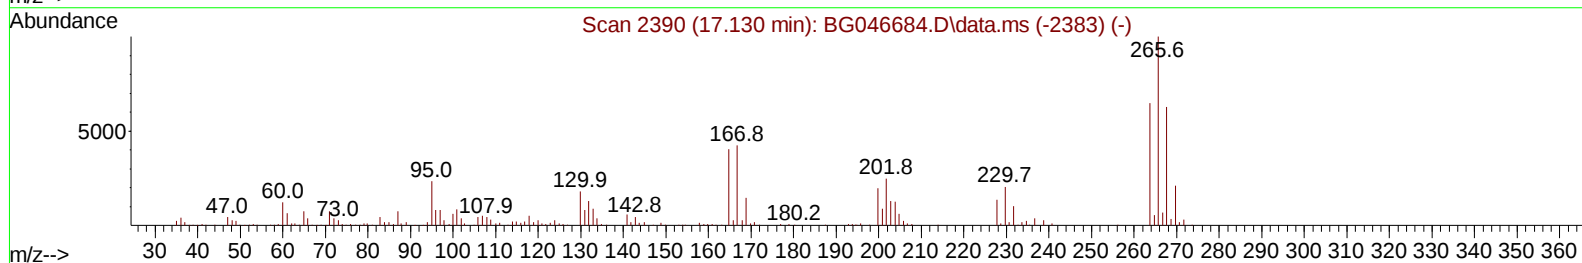
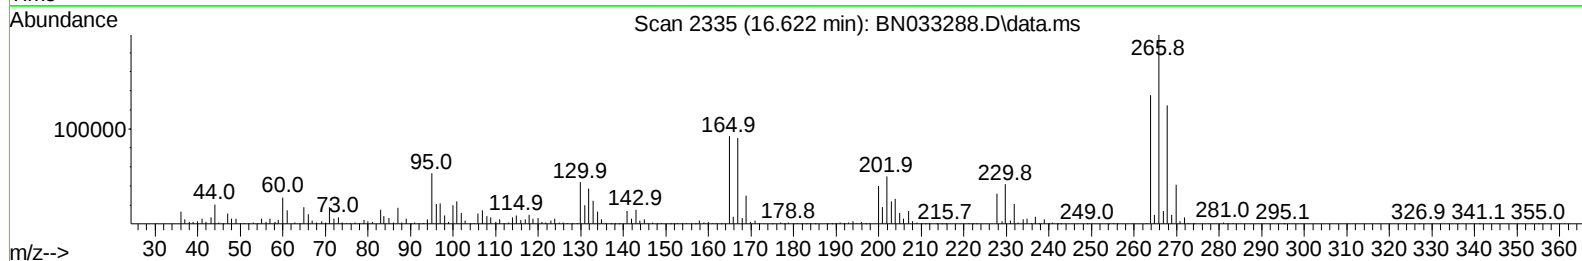


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033288.D
Acq On : 07 Aug 2024 18:05
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 05:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

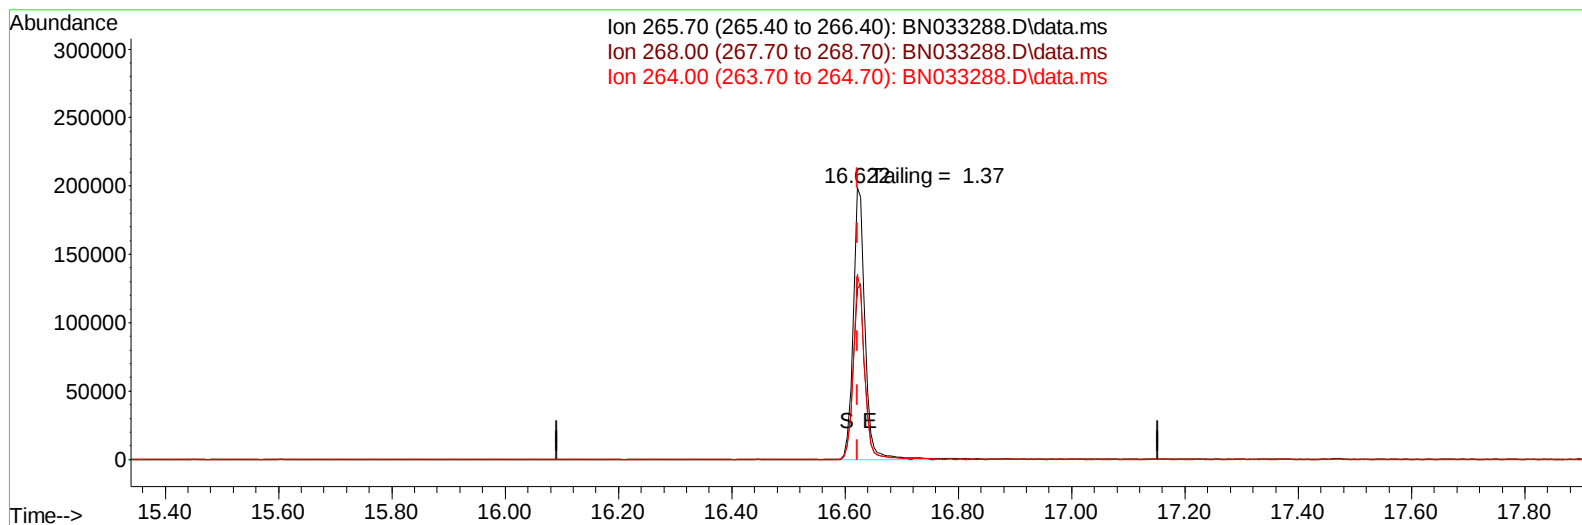

TIC: BN033288.D\data.ms

(70) Pentachlorophenol (C)




16.622min (+ 0.000) 19561.00 ng

response 288752

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	68.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033288.D
Acq On : 07 Aug 2024 18:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 05:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

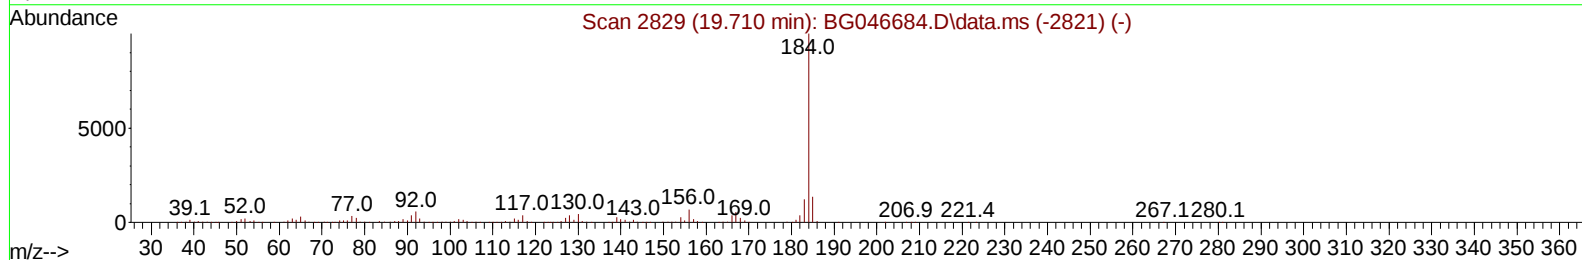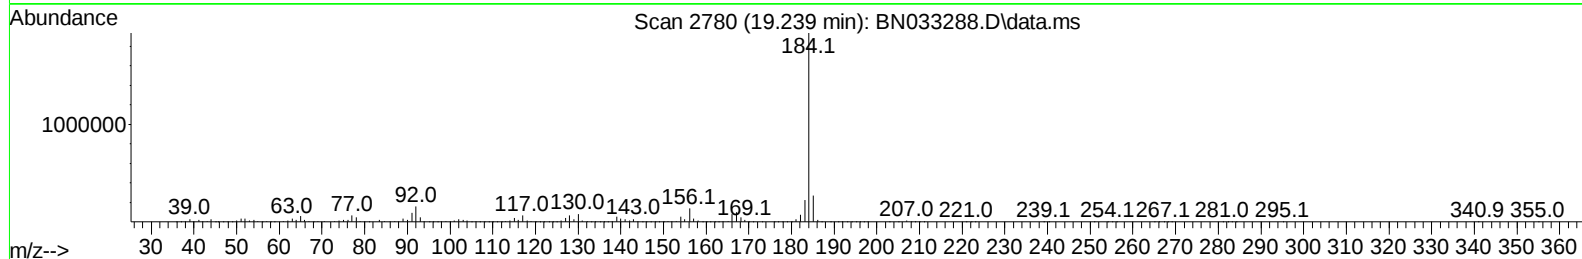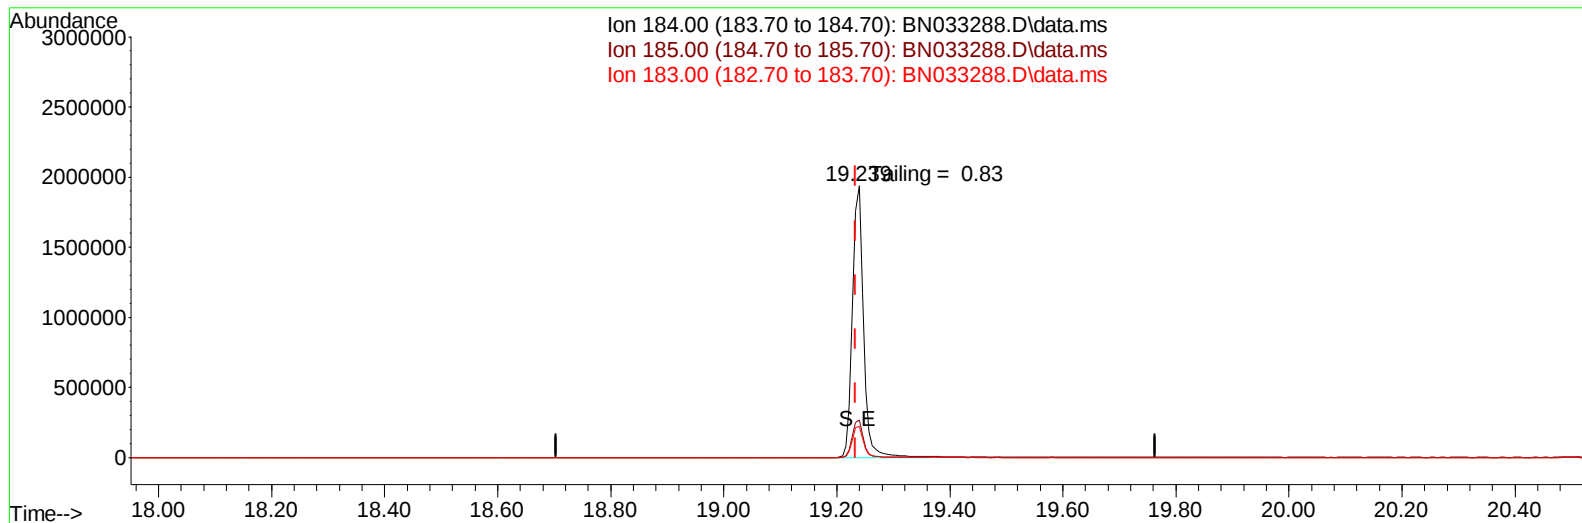

TIC: BN033288.D\data.ms

(77) Benzidine**19.239min (+ 0.006) 245325.72 ng****response 2654352**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.44
0.00	0.00	0.00