

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
 Data File : BN033289.D
 Acq On : 07 Aug 2024 19:24
 Operator : MA/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Aug 08 04:30:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 08 04:24:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	5380	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	15790	0.400	ng	0.00
13) Acenaphthene-d10	14.222	164	10323	0.400	ng	0.00
19) Phenanthrene-d10	16.970	188	23627	0.400	ng	0.00
29) Chrysene-d12	21.178	240	22752	0.400	ng	0.00
35) Perylene-d12	23.364	264	27062	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.213	112	1472	0.096	ng	0.00
5) Phenol-d6	6.759	99	1992	0.099	ng	0.00
8) Nitrobenzene-d5	8.717	82	991	0.076	ng	0.00
11) 2-Methylnaphthalene-d10	11.950	152	2517	0.100	ng	0.00
14) 2,4,6-Tribromophenol	15.716	330	442	0.089	ng	0.00
15) 2-Fluorobiphenyl	12.843	172	3876	0.099	ng	0.00
27) Fluoranthene-d10	19.011	212	6611	0.103	ng	0.00
31) Terphenyl-d14	19.633	244	4083	0.073	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.206	88	597	0.091	ng	# 83
3) n-Nitrosodimethylamine	3.502	42	722	0.115	ng	# 96
6) bis(2-Chloroethyl)ether	7.026	93	1672	0.097	ng	# 98
9) Naphthalene	10.404	128	4469	0.105	ng	# 88
10) Hexachlorobutadiene	10.703	225	834	0.112	ng	# 99
12) 2-Methylnaphthalene	12.026	142	3046	0.105	ng	# 89
16) Acenaphthylene	13.934	152	4958	0.104	ng	98
17) Acenaphthene	14.286	154	3126	0.102	ng	98
18) Fluorene	15.281	166	4337	0.106	ng	99
20) 4,6-Dinitro-2-methylph...	15.345	198	140	0.034	ng	# 1
21) 4-Bromophenyl-phenylether	16.175	248	1462	0.109	ng	90
22) Hexachlorobenzene	16.287	284	1508	0.109	ng	98
23) Atrazine	16.461	200	1191	0.097	ng	# 88
24) Pentachlorophenol	16.622	266	436	0.063	ng	94
25) Phenanthrene	17.007	178	6854	0.105	ng	100
26) Anthracene	17.106	178	6697	0.110	ng	99
28) Fluoranthene	19.038	202	8643	0.109	ng	99
30) Pyrene	19.401	202	9127	0.101	ng	100
32) Benzo(a)anthracene	21.160	228	9134	0.107	ng	99
33) Chrysene	21.214	228	8719	0.108	ng	98
34) Bis(2-ethylhexyl)phtha...	21.151	149	5002	0.085	ng	98
36) Indeno(1,2,3-cd)pyrene	25.545	276	11484	0.114	ng	99
37) Benzo(b)fluoranthene	22.712	252	9765	0.099	ng	# 91
38) Benzo(k)fluoranthene	22.759	252	9266	0.099	ng	# 91
39) Benzo(a)pyrene	23.268	252	8704	0.102	ng	# 89
40) Dibenzo(a,h)anthracene	25.572	278	9044	0.114	ng	# 90
41) Benzo(g,h,i)perylene	26.200	276	9880	0.116	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033289.D
Acq On : 07 Aug 2024 19:24
Operator : MA/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Aug 08 04:30:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 08 04:24:54 2024
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.589 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN033289.D
 Acq: 07 Aug 2024 19:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:152 Resp: 5380
 Ion Ratio Lower Upper
 152 100
 150 149.8 120.7 181.1
 115 70.9 55.8 83.8



#2
 1,4-Dioxane
 Concen: 0.091 ng
 RT: 3.206 min Scan# 45
 Delta R.T. 0.007 min
 Lab File: BN033289.D
 Acq: 07 Aug 2024 19:24

Tgt Ion: 88 Resp: 597
 Ion Ratio Lower Upper
 88 100
 43 71.4 37.0 55.6#
 58 77.2 65.1 97.7









#3
n-Nitrosodimethylamine
Concen: 0.115 ng
RT: 3.502 min Scan# 80
Delta R.T. 0.007 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 42 Resp: 722
Ion Ratio Lower Upper
42 100
74 120.8 94.9 142.3
44 21.7 7.0 10.4#



#4
2-Fluorophenol
Concen: 0.096 ng
RT: 5.213 min Scan# 323
Delta R.T. 0.007 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion: 112 Resp: 1472
Ion Ratio Lower Upper
112 100
64 65.8 48.7 73.1
63 32.3 25.4 38.2









#5
Phenol-d6
Concen: 0.099 ng
RT: 6.759 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	99	Resp:	1992
Ion	Ratio	Lower	Upper
99	100		
42	24.5	19.3	28.9
71	38.0	27.6	41.4



#6
bis(2-Chloroethyl)ether
Concen: 0.097 ng
RT: 7.026 min Scan# 574
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:	93	Resp:	1672
Ion	Ratio	Lower	Upper
93	100		
63	78.8	64.5	96.7
95	33.6	26.6	39.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.351 min Scan# 94
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	136	Resp:	15790
Ion	Ratio	Lower	Upper
136	100		
137	12.5	9.9	14.9
54	15.2	11.4	17.2
68	13.3	9.5	14.3



#8
Nitrobenzene-d5
Concen: 0.076 ng
RT: 8.717 min Scan# 790
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:	82	Resp:	991
Ion	Ratio	Lower	Upper
82	100		
128	34.1	29.4	44.2
54	68.1	50.0	75.0









#9
Naphthalene
Concen: 0.105 ng
RT: 10.404 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:128 Resp: 4469
Ion Ratio Lower Upper
128 100
129 18.3 10.1 15.1#
127 18.6 11.4 17.2#



#10
Hexachlorobutadiene
Concen: 0.112 ng
RT: 10.703 min Scan# 976
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:225 Resp: 834
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 51.8 77.6









#11
2-Methylnaphthalene-d10
Concen: 0.100 ng
RT: 11.950 min Scan# 1170
Delta R.T. -0.004 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 2517
Ion Ratio Lower Upper
152 100
151 21.0 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.105 ng
RT: 12.026 min Scan# 1189
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:142 Resp: 3046
Ion Ratio Lower Upper
142 100
141 92.5 70.5 105.7
115 54.0 30.3 45.5#









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.222 min Scan# 1494
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:164 Resp: 10323
Ion Ratio Lower Upper
164 100
162 104.1 82.6 124.0
160 47.5 38.2 57.4



#14
2,4,6-Tribromophenol
Concen: 0.089 ng
RT: 15.716 min Scan# 1631
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:330 Resp: 442
Ion Ratio Lower Upper
330 100
332 100.0 75.6 113.4
141 47.5 31.0 46.4#









#15
2-Fluorobiphenyl
Concen: 0.099 ng
RT: 12.843 min Scan# 1365
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	172	Resp:	3876
Ion	Ratio	Lower	Upper
172	100		
171	37.4	28.3	42.5
170	26.2	19.4	29.2



#16
Acenaphthylene
Concen: 0.104 ng
RT: 13.934 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:	152	Resp:	4958
Ion	Ratio	Lower	Upper
152	100		
151	20.6	15.7	23.5
153	13.8	10.3	15.5





#17

Acenaphthene

Concen: 0.102 ng

RT: 14.286 min Scan# 1500

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:154 Resp: 3126

Ion Ratio Lower Upper

154 100

153 114.3 89.5 134.3

152 54.4 43.6 65.4



#18

Fluorene

Concen: 0.106 ng

RT: 15.281 min Scan# 1593

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24




Tgt Ion:166 Resp: 4337


Ion Ratio Lower Upper

166 100

165 97.9 78.9 118.3

167 13.4 10.6 16.0





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.970 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:188 Resp: 23627

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 12.8 10.5 15.7



#20

4,6-Dinitro-2-methylphenol

Concen: 0.034 ng

RT: 15.345 min Scan# 1599

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24




Tgt Ion:198 Resp: 140


Ion Ratio Lower Upper

198 100

51 496.5 127.9 191.9#

105 397.9 112.3 168.5#









#21
4-Bromophenyl-phenylether
Concen: 0.109 ng
RT: 16.175 min Scan# 1668
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:248 Resp: 1462
Ion Ratio Lower Upper
248 100
250 97.0 74.6 112.0
141 92.3 62.2 93.2



#22
Hexachlorobenzene
Concen: 0.109 ng
RT: 16.287 min Scan# 1677
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:284 Resp: 1508
Ion Ratio Lower Upper
284 100
142 38.4 30.6 45.8
249 33.2 24.6 36.8





#23

Atrazine

Concen: 0.097 ng

RT: 16.461 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:200 Resp: 1191

Ion Ratio Lower Upper

200 100

173 29.1 18.9 28.3#

215 56.1 38.6 57.8



#24

Pentachlorophenol

Concen: 0.063 ng

RT: 16.622 min Scan# 1704

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24




Tgt Ion:266 Resp: 436


Ion Ratio Lower Upper

266 100

264 56.9 50.3 75.5

268 67.2 51.0 76.4









#25
 Phenanthrene
 Concen: 0.105 ng
 RT: 17.007 min Scan# 1735
 Delta R.T. 0.000 min
 Lab File: BN033289.D
 Acq: 07 Aug 2024 19:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:	178	Resp:	6854
Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.2	22.8
179	15.2	12.0	18.0



#26
 Anthracene
 Concen: 0.110 ng
 RT: 17.106 min Scan# 1743
 Delta R.T. 0.000 min
 Lab File: BN033289.D
 Acq: 07 Aug 2024 19:24

Tgt Ion:	178	Resp:	6697
Ion	Ratio	Lower	Upper
178	100		
176	19.0	14.8	22.2
179	15.6	12.2	18.4









#27
Fluoranthene-d10
Concen: 0.103 ng
RT: 19.011 min Scan# 1964
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:212 Resp: 6611
Ion Ratio Lower Upper
212 100
106 15.4 12.2 18.4
104 8.9 6.9 10.3



#28
Fluoranthene
Concen: 0.109 ng
RT: 19.038 min Scan# 1970
Delta R.T. -0.005 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:202 Resp: 8643
Ion Ratio Lower Upper
202 100
101 12.5 9.4 14.0
203 17.2 13.8 20.6









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.178 min Scan# 2413
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:240 Resp: 22752
Ion Ratio Lower Upper
240 100
120 11.4 9.0 13.6
236 28.4 22.4 33.6



#30
Pyrene
Concen: 0.101 ng
RT: 19.401 min Scan# 2048
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:202 Resp: 9127
Ion Ratio Lower Upper
202 100
200 20.8 16.7 25.1
203 18.1 14.2 21.4









#31
Terphenyl-d14
Concen: 0.073 ng
RT: 19.633 min Scan# 2098
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:244 Resp: 4083
Ion Ratio Lower Upper
244 100
212 10.6 7.2 10.8
122 19.6 12.7 19.1#



#32
Benzo(a)anthracene
Concen: 0.107 ng
RT: 21.160 min Scan# 2411
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Tgt Ion:228 Resp: 9134
Ion Ratio Lower Upper
228 100
226 27.7 22.1 33.1
229 20.1 15.6 23.4





#33

Chrysene

Concen: 0.108 ng

RT: 21.214 min Scan# 2417

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:228 Resp: 8719

Ion Ratio Lower Upper

228 100

226 30.8 23.8 35.8

229 20.4 15.8 23.8

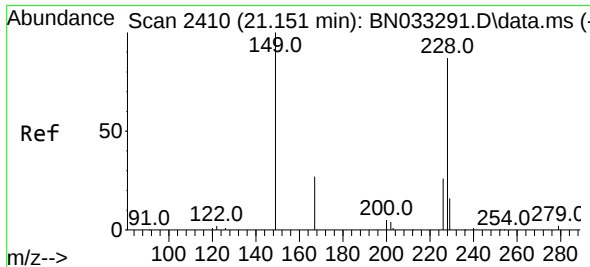

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.085 ng

RT: 21.151 min Scan# 2410

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24




Tgt Ion:149 Resp: 5002


Ion Ratio Lower Upper

149 100

167 28.2 21.6 32.4

279 3.0 2.6 4.0





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.364 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN033289.D


Acq: 07 Aug 2024 19:24

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:264 Resp: 27062

Ion Ratio Lower Upper

264 100

260 26.1 21.4 32.0

265 27.2 22.4 33.6



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.114 ng

RT: 25.545 min Scan# 3624

Delta R.T. 0.000 min

Lab File: BN033289.D

Acq: 07 Aug 2024 19:24




Tgt Ion:276 Resp: 11484


Ion Ratio Lower Upper

276 100

138 28.2 22.7 34.1


277 25.2 19.8 29.8








#37
Benzo(b)fluoranthene
Concen: 0.099 ng
RT: 22.712 min Scan# 2655
Delta R.T. -0.003 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1







Tgt Ion:252 Resp: 9765
Ion Ratio Lower Upper
252 100
253 25.5 17.8 26.6
125 17.6 10.0 15.0#



#38
Benzo(k)fluoranthene
Concen: 0.099 ng
RT: 22.759 min Scan# 2671
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24


Tgt Ion:252 Resp: 9266
Ion Ratio Lower Upper
252 100
253 26.0 18.3 27.5
125 17.8 10.2 15.4#








#39
Benzo(a)pyrene
Concen: 0.102 ng
RT: 23.268 min Scan# 2845
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1







Tgt Ion:252 Resp: 8704
Ion Ratio Lower Upper
252 100
253 26.5 18.2 27.4
125 20.9 11.4 17.2#



#40
Dibenzo(a,h)anthracene
Concen: 0.114 ng
RT: 25.572 min Scan# 3633
Delta R.T. 0.000 min
Lab File: BN033289.D
Acq: 07 Aug 2024 19:24


Tgt Ion:278 Resp: 9044
Ion Ratio Lower Upper
278 100
139 26.3 16.3 24.5#
279 28.2 19.4 29.2



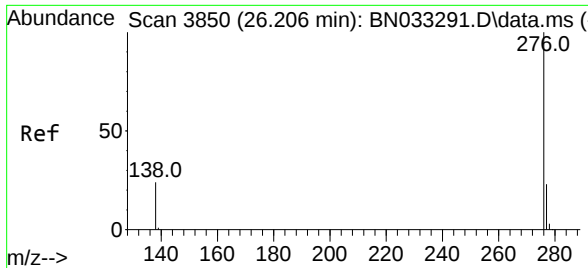

#41
 Benzo(g,h,i)perylene
 Concen: 0.116 ng
 RT: 26.200 min Scan# 3848
 Delta R.T. -0.006 min
 Lab File: BN033289.D
 Acq: 07 Aug 2024 19:24

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1



Tgt Ion:	276	Resp:	9880
Ion Ratio	Lower	Upper	
276	100		
277	25.7	19.0	28.4
138	32.4	20.8	31.2#

