

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
 Data File : BN033290.D
 Acq On : 07 Aug 2024 20:00
 Operator : MA/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Aug 08 04:31:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 08 04:24:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	4772	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	13956	0.400	ng	0.00
13) Acenaphthene-d10	14.222	164	9277	0.400	ng	0.00
19) Phenanthrene-d10	16.969	188	20862	0.400	ng	0.00
29) Chrysene-d12	21.178	240	19870	0.400	ng	0.00
35) Perylene-d12	23.367	264	23171	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.206	112	2557	0.188	ng	0.00
5) Phenol-d6	6.758	99	3399	0.191	ng	0.00
8) Nitrobenzene-d5	8.717	82	1609	0.139	ng	0.00
11) 2-Methylnaphthalene-d10	11.954	152	4234	0.190	ng	0.00
14) 2,4,6-Tribromophenol	15.716	330	730	0.164	ng	0.00
15) 2-Fluorobiphenyl	12.843	172	6612	0.188	ng	0.00
27) Fluoranthene-d10	19.010	212	11076	0.195	ng	0.00
31) Terphenyl-d14	19.633	244	6817	0.140	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.198	88	1099	0.188	ng	95
3) n-Nitrosodimethylamine	3.494	42	1329	0.239	ng	# 93
6) bis(2-Chloroethyl)ether	7.026	93	2843	0.186	ng	99
9) Naphthalene	10.404	128	7632	0.203	ng	95
10) Hexachlorobutadiene	10.703	225	1421	0.216	ng	# 98
12) 2-Methylnaphthalene	12.025	142	5250	0.204	ng	# 95
16) Acenaphthylene	13.933	152	8488	0.198	ng	99
17) Acenaphthene	14.286	154	5385	0.196	ng	100
18) Fluorene	15.280	166	7320	0.199	ng	99
20) 4,6-Dinitro-2-methylph...	15.355	198	251	0.070	ng	# 14
21) 4-Bromophenyl-phenylether	16.175	248	2463	0.208	ng	95
22) Hexachlorobenzene	16.287	284	2543	0.207	ng	99
23) Atrazine	16.460	200	2007	0.185	ng	94
24) Pentachlorophenol	16.622	266	821	0.135	ng	97
25) Phenanthrene	17.007	178	11597	0.200	ng	99
26) Anthracene	17.106	178	11220	0.209	ng	100
28) Fluoranthene	19.043	202	14522	0.207	ng	100
30) Pyrene	19.405	202	15275	0.193	ng	100
32) Benzo(a)anthracene	21.160	228	14819	0.198	ng	100
33) Chrysene	21.214	228	14588	0.206	ng	99
34) Bis(2-ethylhexyl)phtha...	21.151	149	7939	0.155	ng	99
36) Indeno(1,2,3-cd)pyrene	25.548	276	18661	0.216	ng	100
37) Benzo(b)fluoranthene	22.715	252	16302	0.193	ng	96
38) Benzo(k)fluoranthene	22.762	252	16033	0.201	ng	97
39) Benzo(a)pyrene	23.270	252	14433	0.198	ng	96
40) Dibenzo(a,h)anthracene	25.574	278	14703	0.216	ng	96
41) Benzo(g,h,i)perylene	26.203	276	16242	0.222	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
 Data File : BN033290.D
 Acq On : 07 Aug 2024 20:00
 Operator : MA/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Aug 08 04:31:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 08 04:24:54 2024
 Response via : Initial Calibration




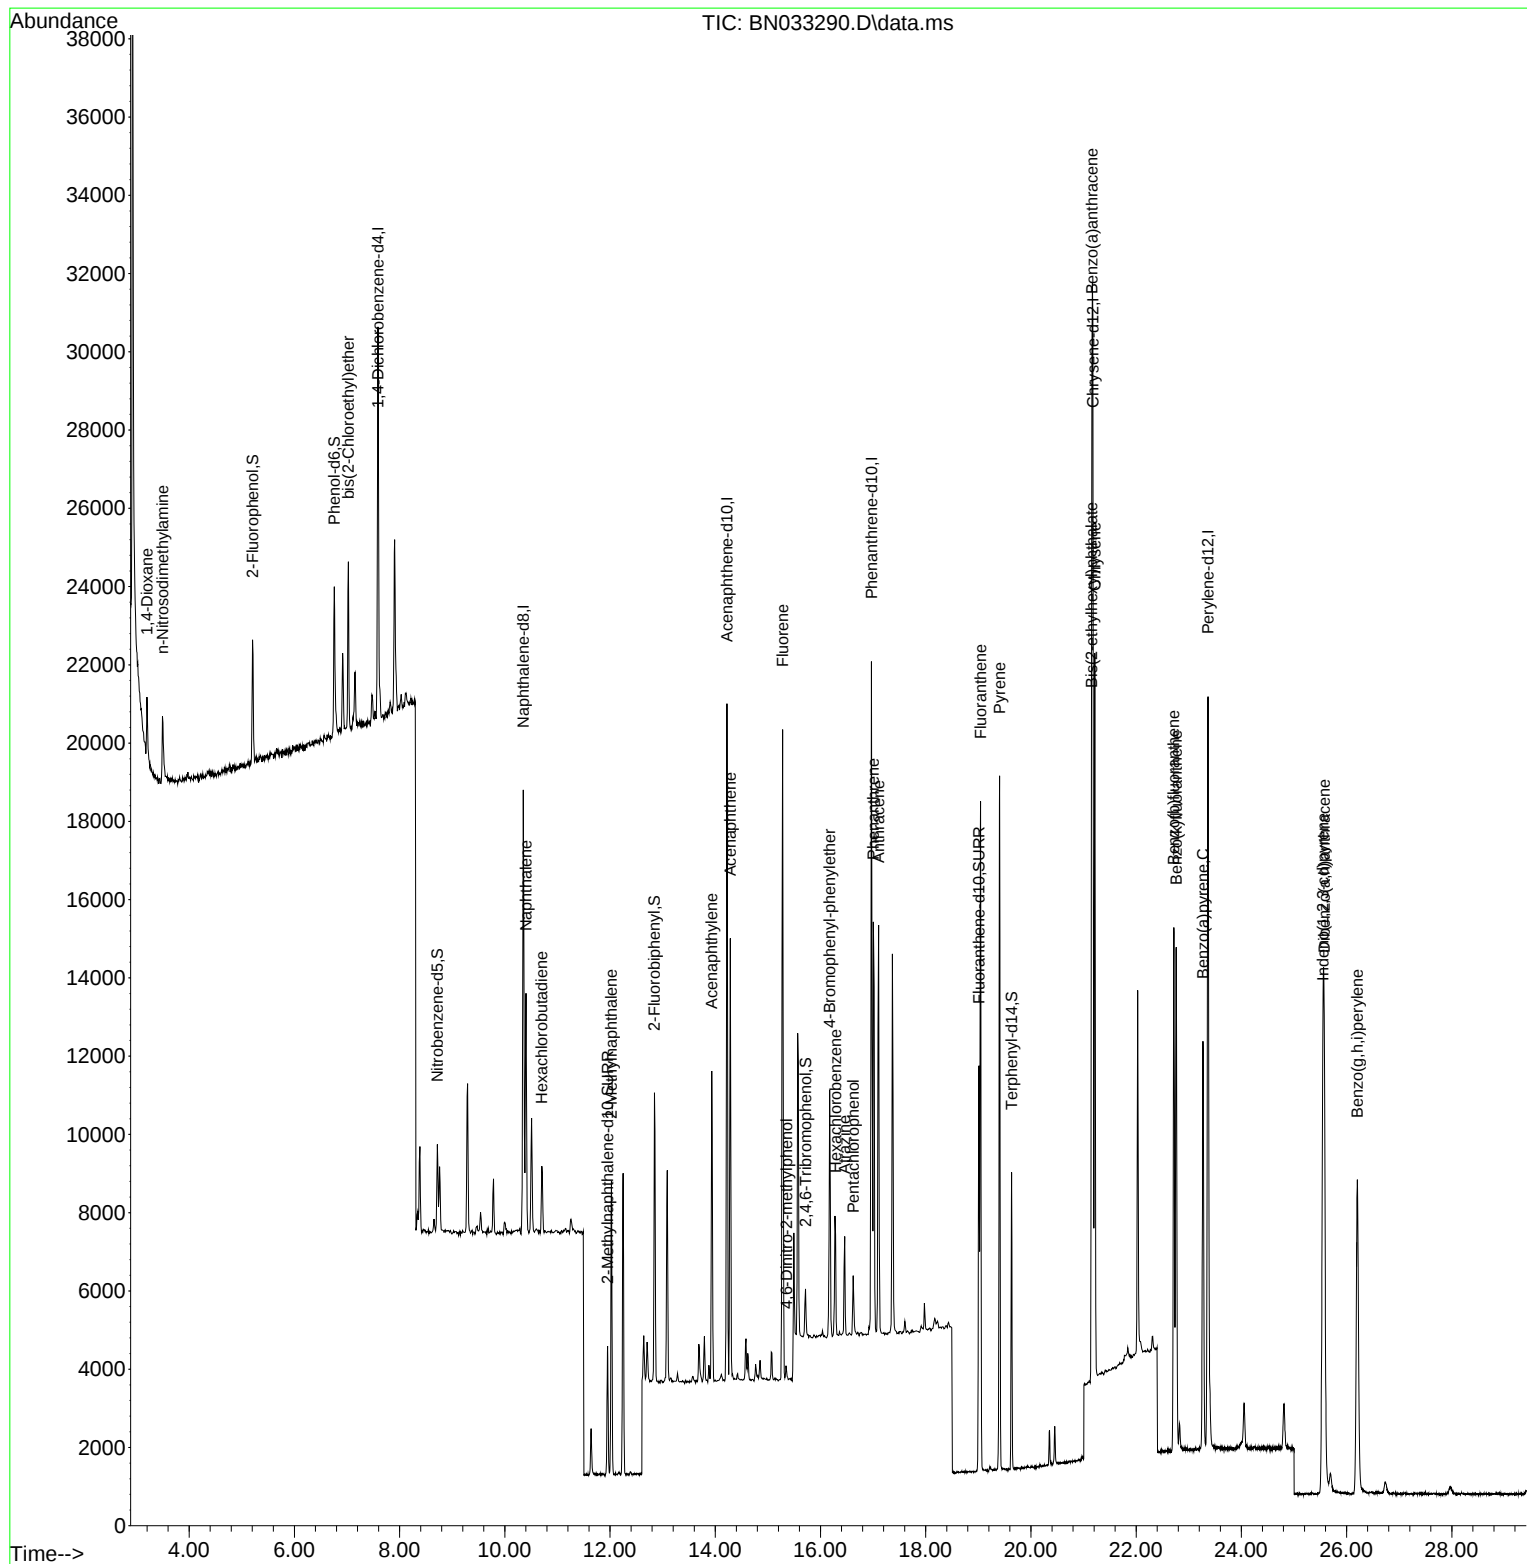




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.589 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN033290.D
 Acq: 07 Aug 2024 20:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:152 Resp: 4772
 Ion Ratio Lower Upper
 152 100
 150 149.3 120.7 181.1
 115 71.5 55.8 83.8

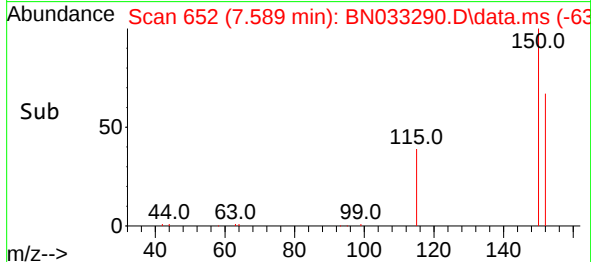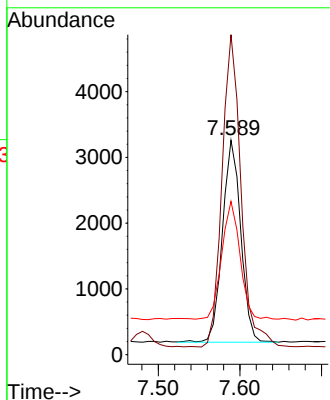

#2
 1,4-Dioxane
 Concen: 0.188 ng
 RT: 3.198 min Scan# 44
 Delta R.T. -0.000 min
 Lab File: BN033290.D
 Acq: 07 Aug 2024 20:00

Tgt Ion: 88 Resp: 1099
 Ion Ratio Lower Upper
 88 100
 43 53.7 37.0 55.6
 58 80.1 65.1 97.7


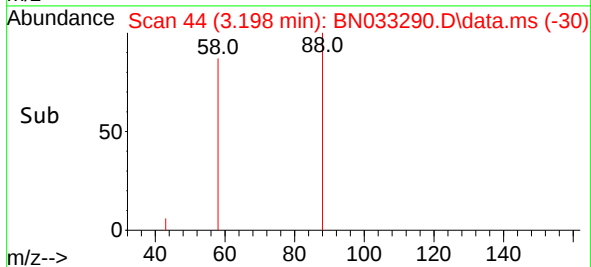
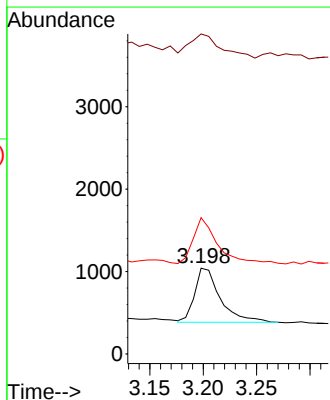
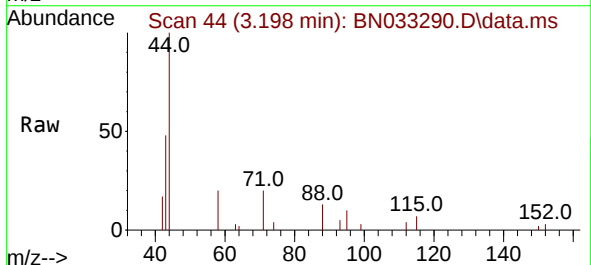


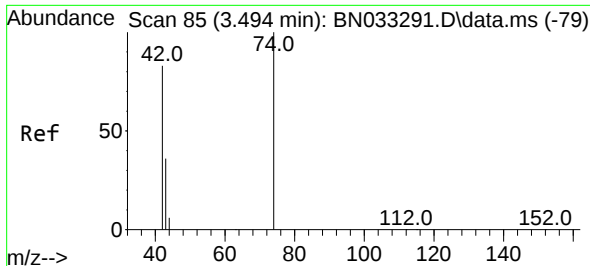

#3
n-Nitrosodimethylamine
Concen: 0.239 ng
RT: 3.494 min Scan# 85
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 42 Resp: 1329
Ion Ratio Lower Upper
42 100
74 112.6 94.9 142.3
44 0.0 7.0 10.4#

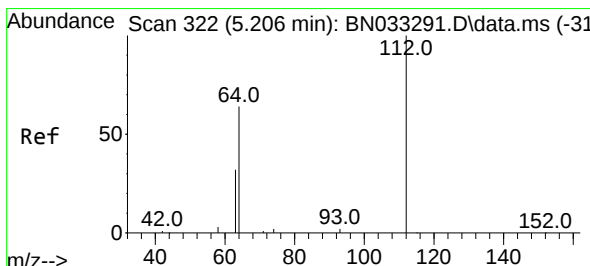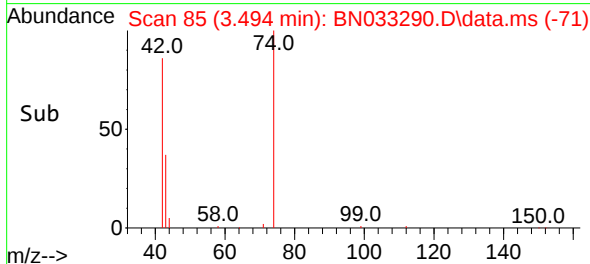

#4
2-Fluorophenol
Concen: 0.188 ng
RT: 5.206 min Scan# 322
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion: 112 Resp: 2557
Ion Ratio Lower Upper
112 100
64 59.8 48.7 73.1
63 30.8 25.4 38.2


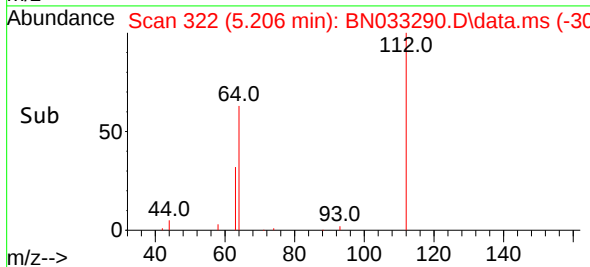

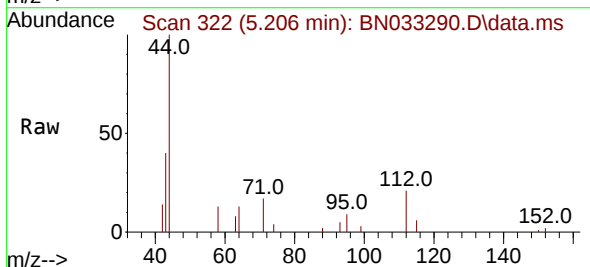




#5
Phenol-d6
Concen: 0.191 ng
RT: 6.758 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 99 Resp: 3399
Ion Ratio Lower Upper
99 100
42 24.2 19.3 28.9
71 35.1 27.6 41.4

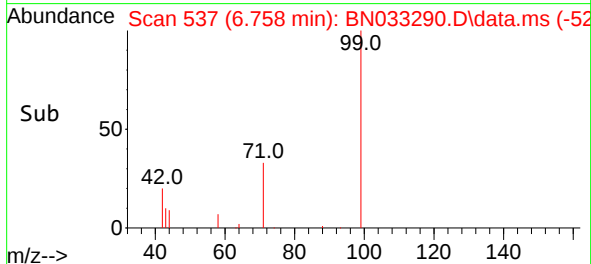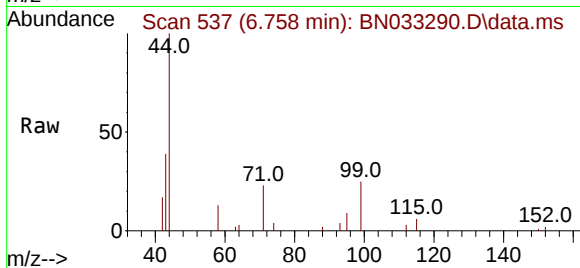

#6
bis(2-Chloroethyl)ether
Concen: 0.186 ng
RT: 7.026 min Scan# 574
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion: 93 Resp: 2843
Ion Ratio Lower Upper
93 100
63 82.1 64.5 96.7
95 33.3 26.6 39.8

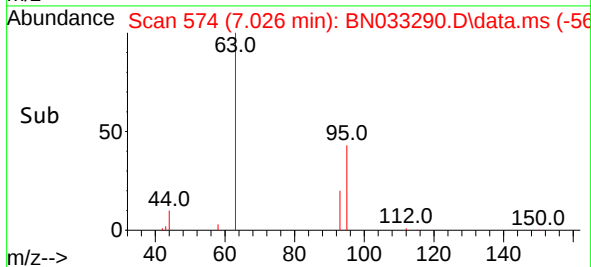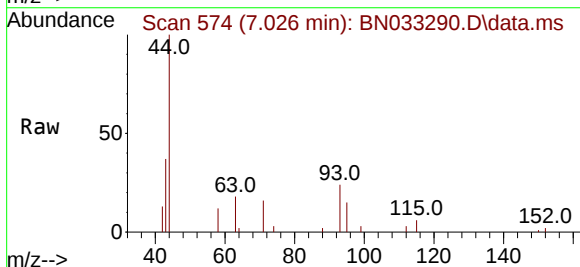



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.351 min Scan# 94

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

Tgt Ion:136 Resp: 13956





Ion Ratio Lower Upper

136 100

137 12.6 9.9 14.9

54 16.1 11.4 17.2

68 13.6 9.5 14.3

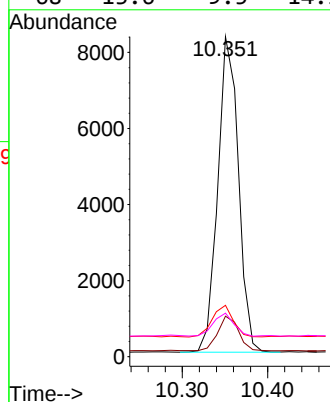

#8

Nitrobenzene-d5

Concen: 0.139 ng

RT: 8.717 min Scan# 790

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00




Tgt Ion: 82 Resp: 1609


Ion Ratio Lower Upper

82 100

128 34.7 29.4 44.2

54 65.0 50.0 75.0


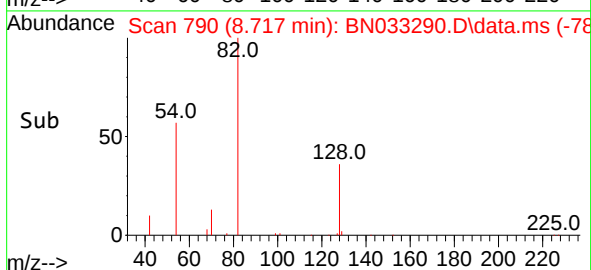
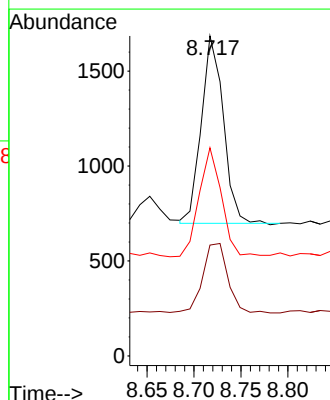





#9
Naphthalene
Concen: 0.203 ng
RT: 10.404 min Scan# 948
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	128	Resp:	7632
Ion	Ratio	Lower	Upper
128	100		
129	14.8	10.1	15.1
127	15.7	11.4	17.2

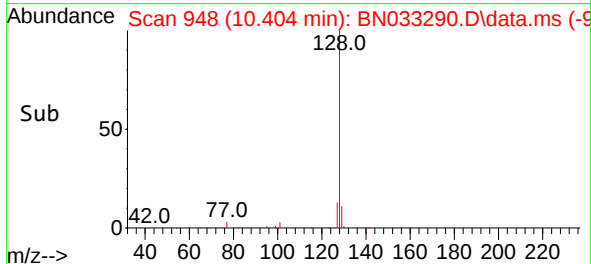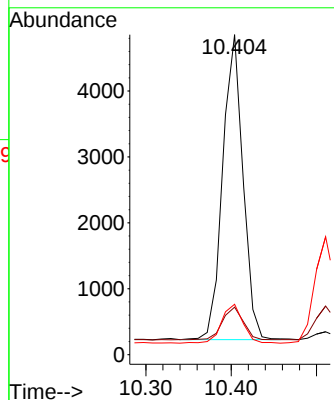

#10
Hexachlorobutadiene
Concen: 0.216 ng
RT: 10.703 min Scan# 976
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:	225	Resp:	1421
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	62.8	51.8	77.6


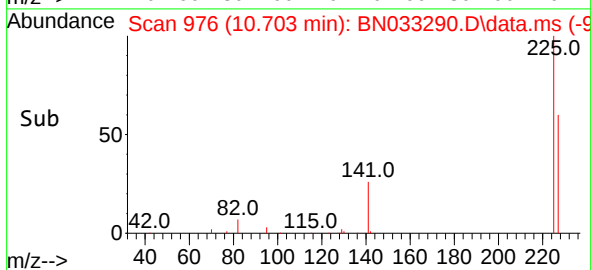
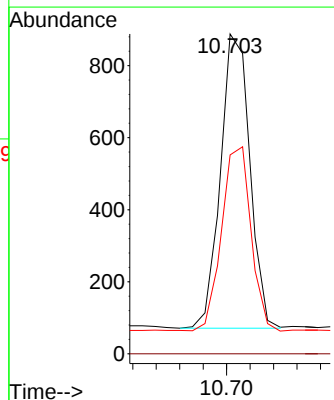
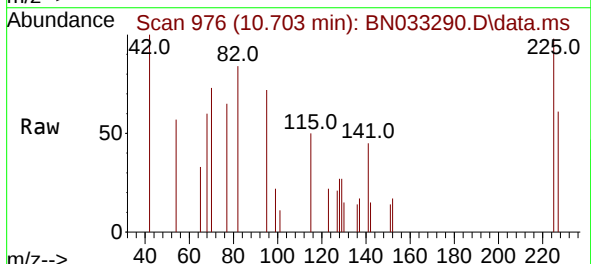


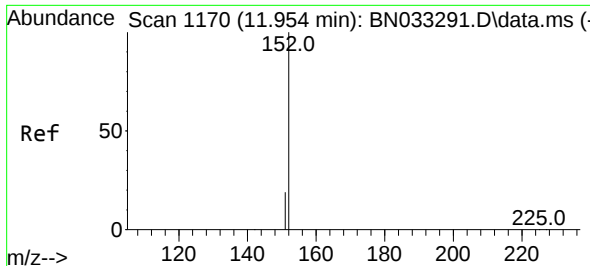

#11
2-Methylnaphthalene-d10
Concen: 0.190 ng
RT: 11.954 min Scan# 1170
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 4234
Ion Ratio Lower Upper
152 100
151 20.7 16.7 25.1

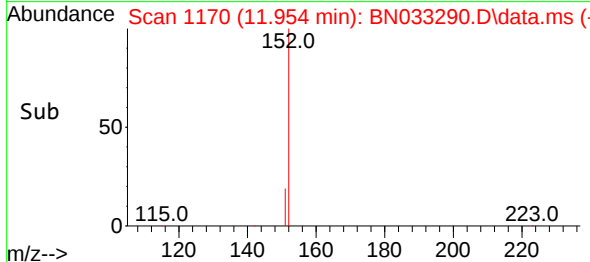

#12
2-Methylnaphthalene
Concen: 0.204 ng
RT: 12.025 min Scan# 1189
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:142 Resp: 5250
Ion Ratio Lower Upper
142 100
141 89.1 70.5 105.7
115 45.9 30.3 45.5#


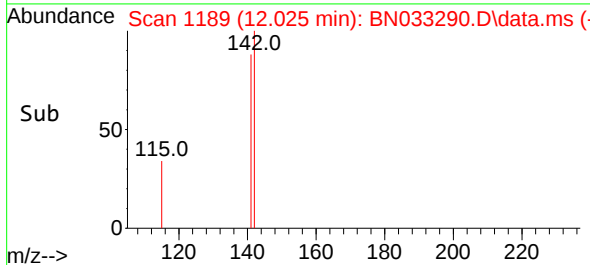

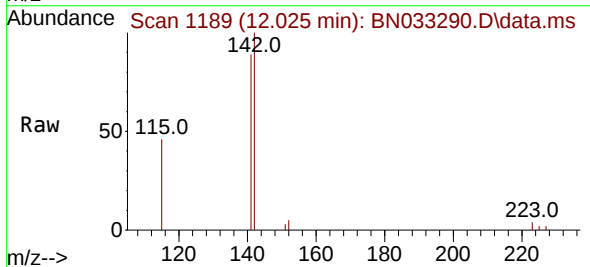


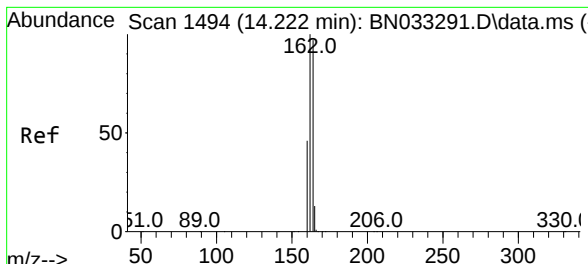

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.222 min Scan# 1494
 Delta R.T. -0.000 min
 Lab File: BN033290.D
 Acq: 07 Aug 2024 20:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:164 Resp: 9277
 Ion Ratio Lower Upper
 164 100
 162 103.6 82.6 124.0
 160 47.6 38.2 57.4

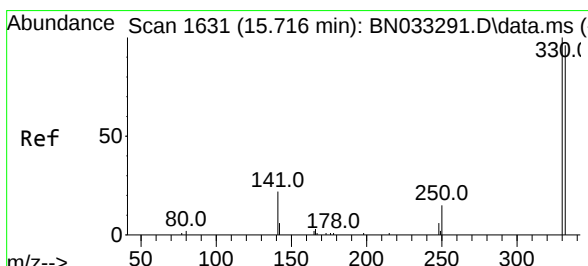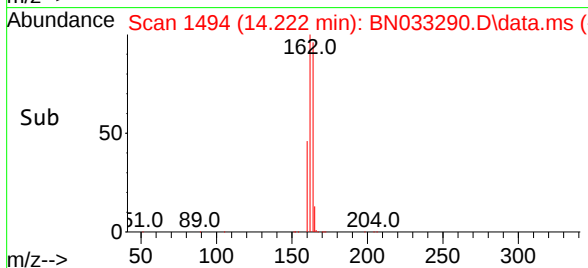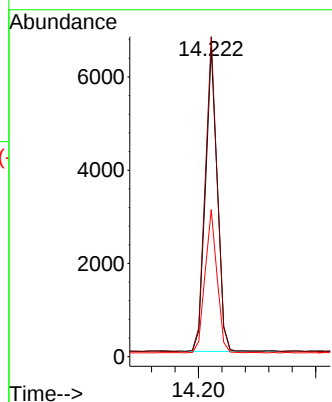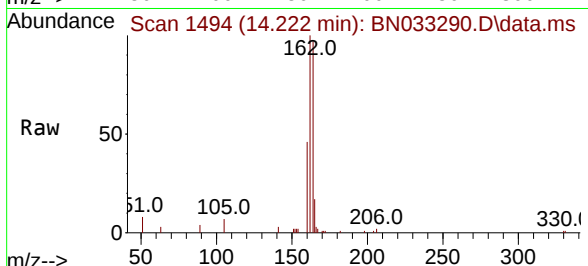

#14
 2,4,6-Tribromophenol
 Concen: 0.164 ng
 RT: 15.716 min Scan# 1631
 Delta R.T. -0.000 min
 Lab File: BN033290.D
 Acq: 07 Aug 2024 20:00

Tgt Ion:330 Resp: 730
 Ion Ratio Lower Upper
 330 100
 332 96.4 75.6 113.4
 141 42.7 31.0 46.4


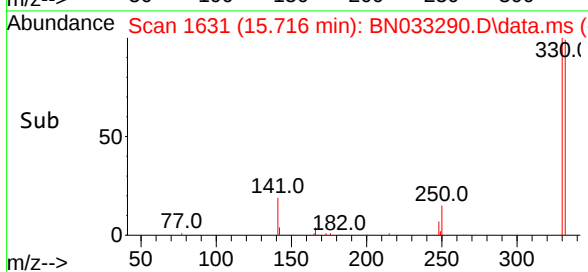
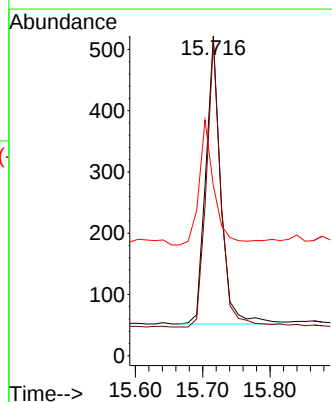
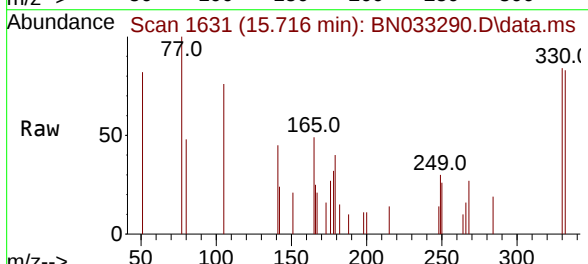




#15
2-Fluorobiphenyl
Concen: 0.188 ng
RT: 12.843 min Scan# 1365
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	172	Resp:	6612
Ion	Ratio	Lower	Upper
172	100		
171	37.0	28.3	42.5
170	25.3	19.4	29.2

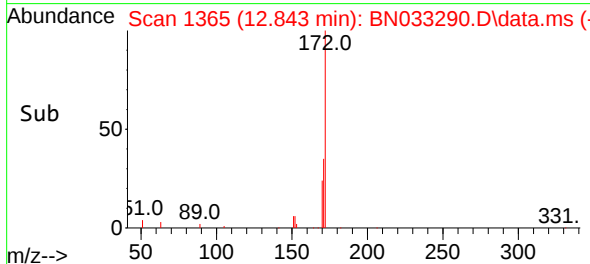

#16
Acenaphthylene
Concen: 0.198 ng
RT: 13.933 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:	152	Resp:	8488
Ion	Ratio	Lower	Upper
152	100		
151	20.0	15.7	23.5
153	13.5	10.3	15.5


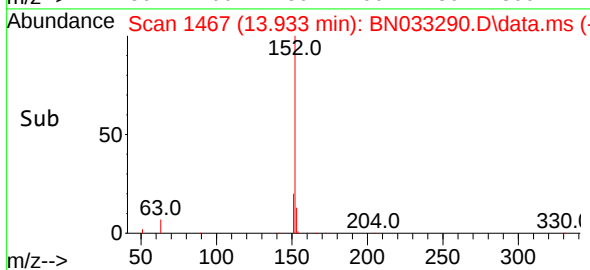

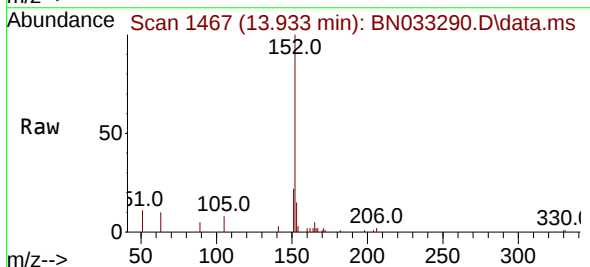




#17
Acenaphthene
Concen: 0.196 ng
RT: 14.286 min Scan# 1500
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:154 Resp: 5385
Ion Ratio Lower Upper
154 100
153 112.1 89.5 134.3
152 54.9 43.6 65.4

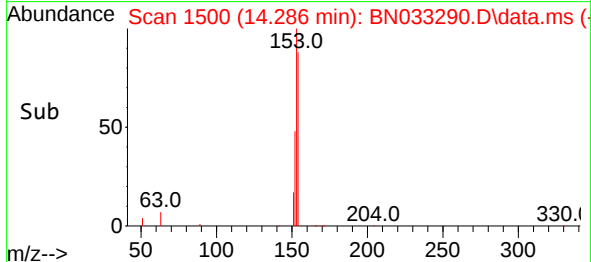

#18
Fluorene
Concen: 0.199 ng
RT: 15.280 min Scan# 1593
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:166 Resp: 7320
Ion Ratio Lower Upper
166 100
165 97.2 78.9 118.3
167 13.6 10.6 16.0


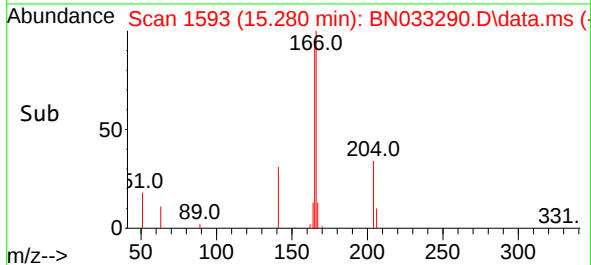

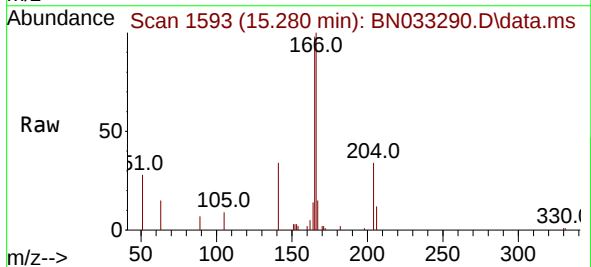


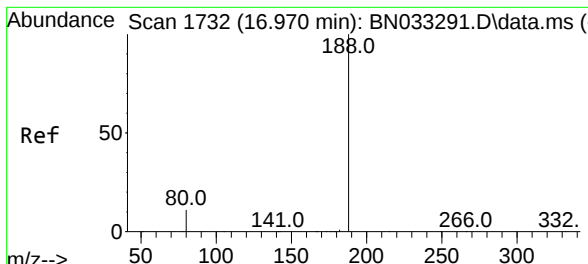

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 16.969 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BN033290.D
 Acq: 07 Aug 2024 20:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:	188	Resp:	20862
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	13.3	10.5	15.7

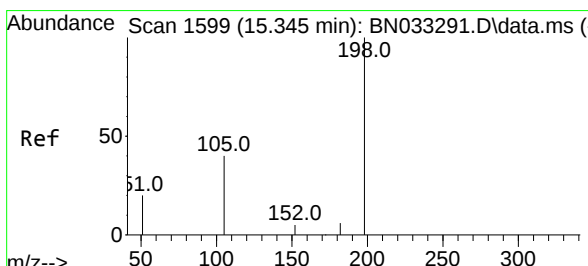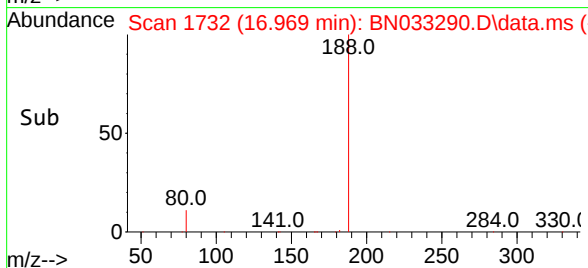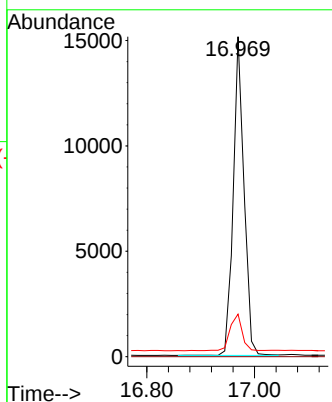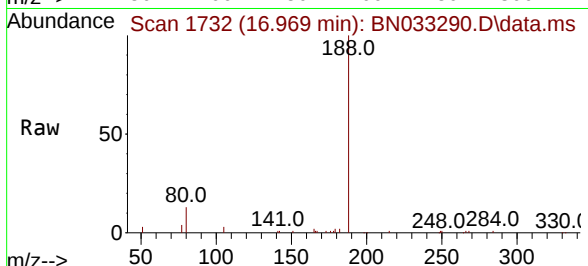

#20
 4,6-Dinitro-2-methylphenol
 Concen: 0.070 ng
 RT: 15.355 min Scan# 1600
 Delta R.T. 0.010 min
 Lab File: BN033290.D
 Acq: 07 Aug 2024 20:00

Tgt Ion:	198	Resp:	251
Ion Ratio	Lower	Upper	
198	100		
51	267.3	127.9	191.9#
105	252.0	112.3	168.5#


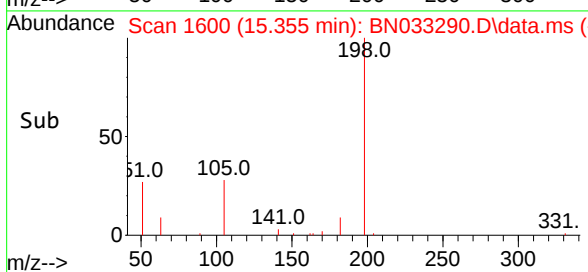
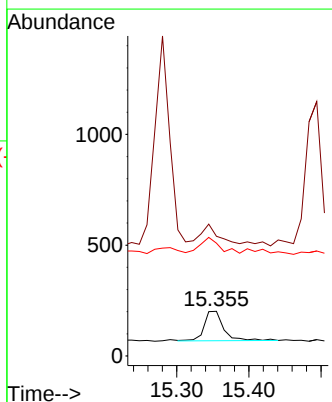
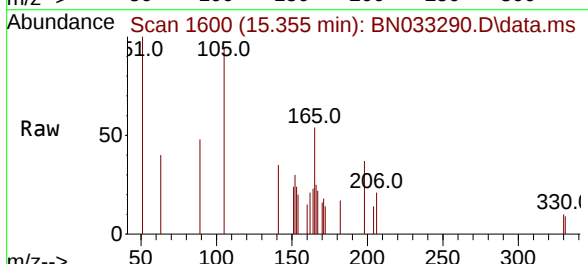


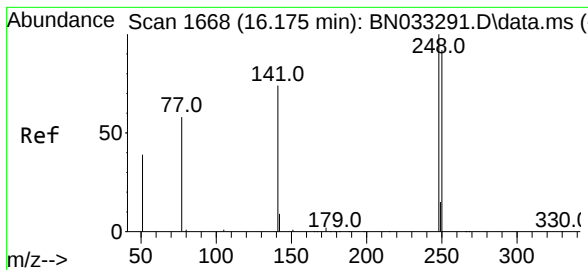

#21
4-Bromophenyl-phenylether
Concen: 0.208 ng
RT: 16.175 min Scan# 1668
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	248	Resp:	2463
Ion Ratio	Lower	Upper	
248	100		
250	95.6	74.6	112.0
141	85.3	62.2	93.2

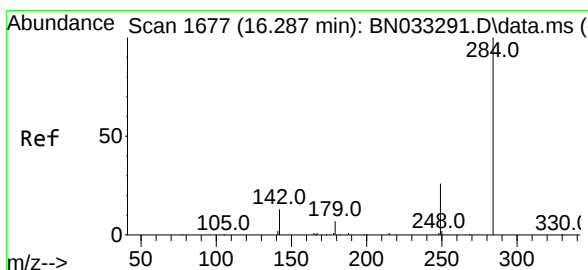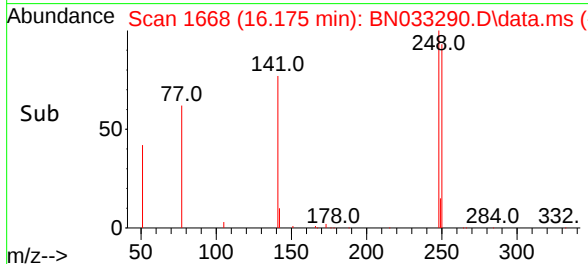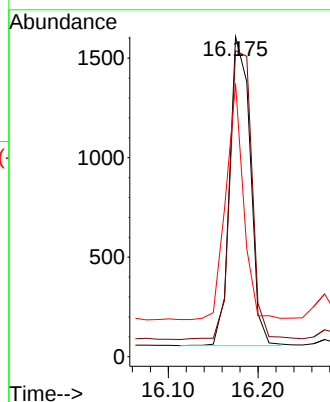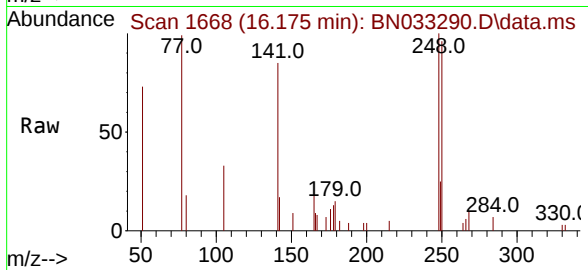

#22
Hexachlorobenzene
Concen: 0.207 ng
RT: 16.287 min Scan# 1677
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:	284	Resp:	2543
Ion Ratio	Lower	Upper	
284	100		
142	38.0	30.6	45.8
249	31.3	24.6	36.8


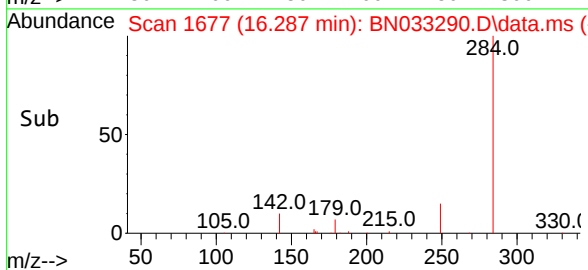
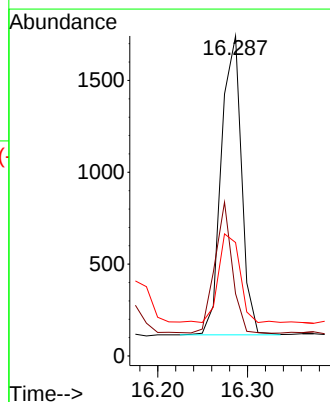
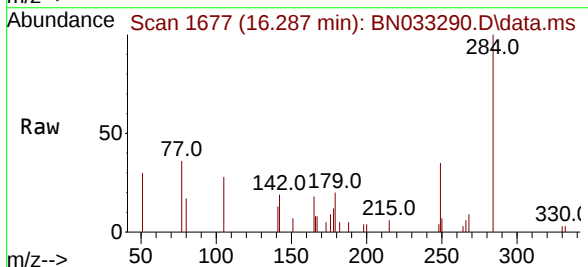


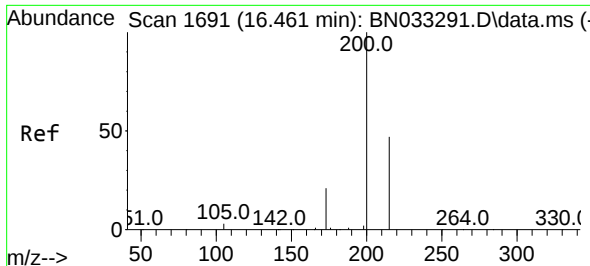

#23
Atrazine
Concen: 0.185 ng
RT: 16.460 min Scan# 1691
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:200 Resp: 2007
Ion Ratio Lower Upper
200 100
173 27.6 18.9 28.3
215 51.4 38.6 57.8

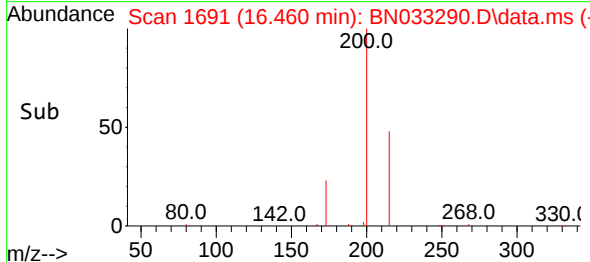

#24
Pentachlorophenol
Concen: 0.135 ng
RT: 16.622 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:266 Resp: 821
Ion Ratio Lower Upper
266 100
264 59.6 50.3 75.5
268 65.7 51.0 76.4

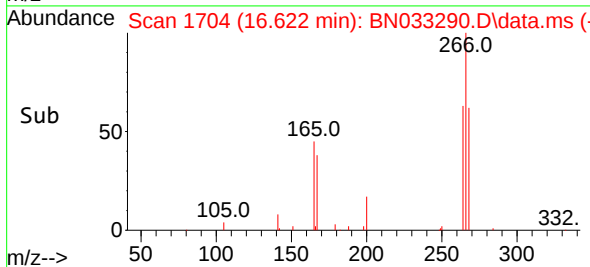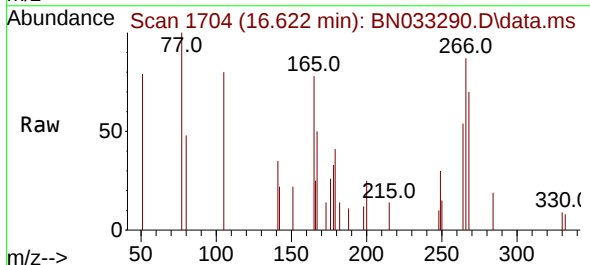



#25

Phenanthrene

Concen: 0.200 ng

RT: 17.007 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:178 Resp: 11597

Ion Ratio Lower Upper

178 100

176 19.4 15.2 22.8

179 15.5 12.0 18.0

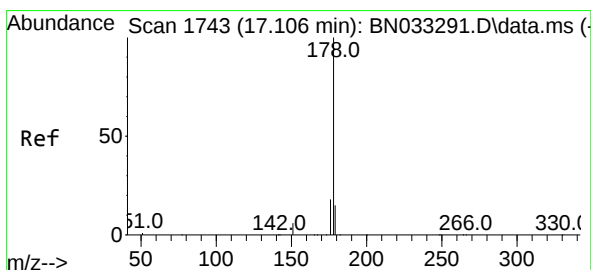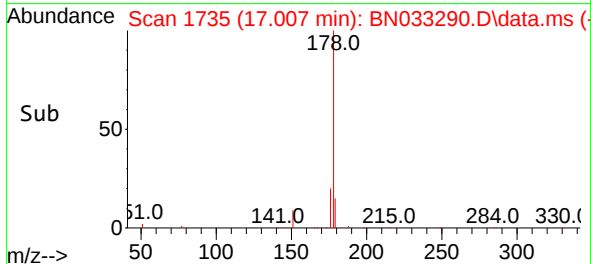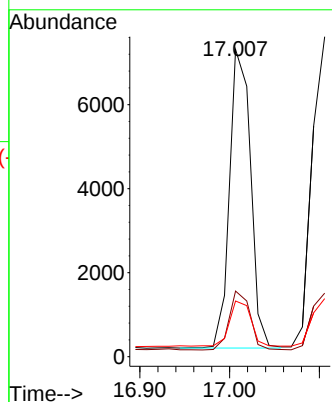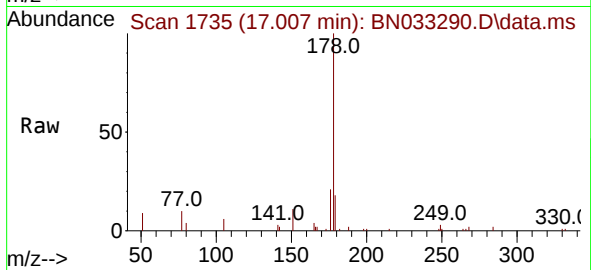

#26

Anthracene

Concen: 0.209 ng

RT: 17.106 min Scan# 1743

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00




Tgt Ion:178 Resp: 11220


Ion Ratio Lower Upper

178 100

176 18.7 14.8 22.2

179 15.5 12.2 18.4


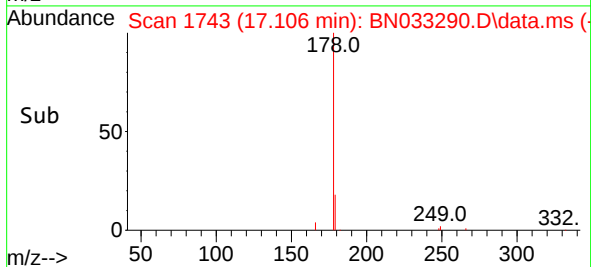
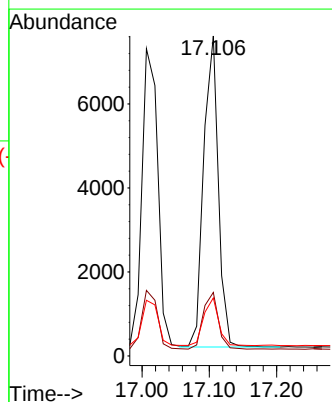
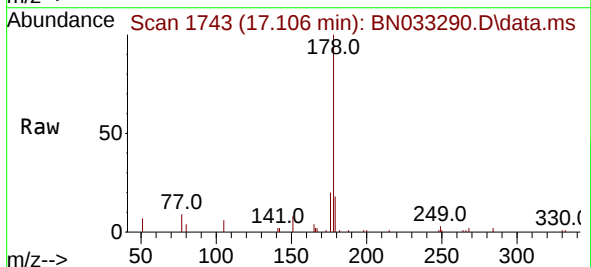


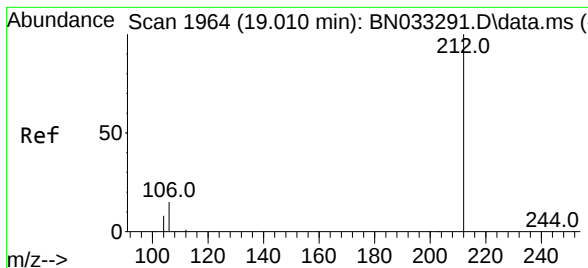

#27
Fluoranthene-d10
Concen: 0.195 ng
RT: 19.010 min Scan# 1964
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:212 Resp: 11076
Ion Ratio Lower Upper
212 100
106 15.6 12.2 18.4
104 8.8 6.9 10.3

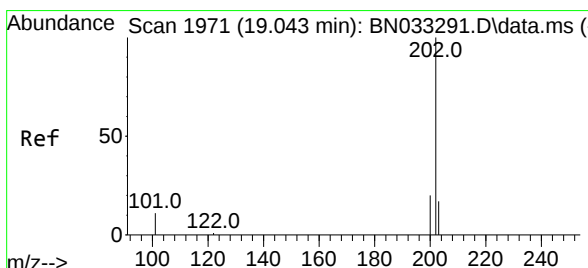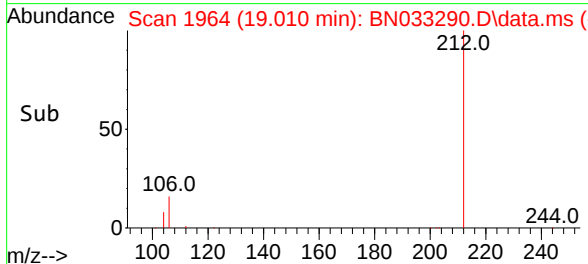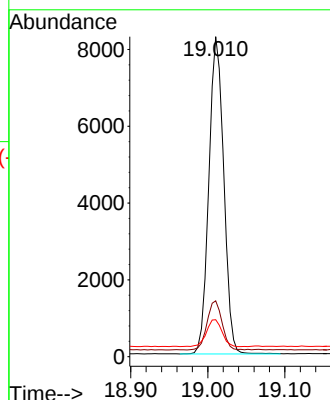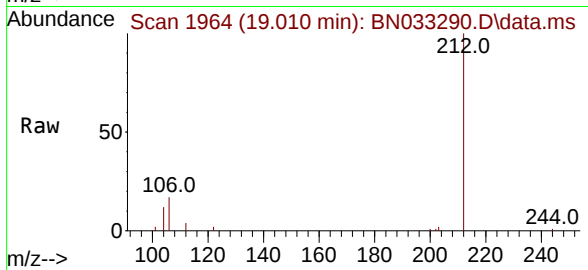

#28
Fluoranthene
Concen: 0.207 ng
RT: 19.043 min Scan# 1971
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:202 Resp: 14522
Ion Ratio Lower Upper
202 100
101 12.1 9.4 14.0
203 17.2 13.8 20.6


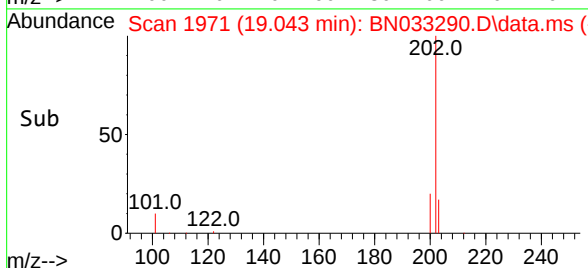
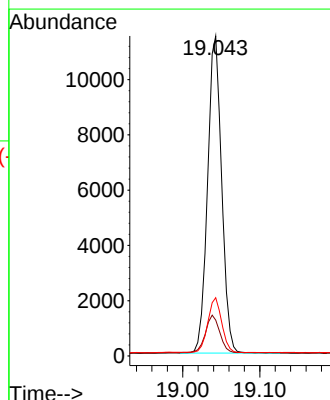
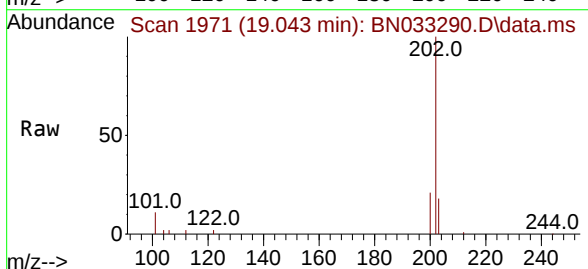


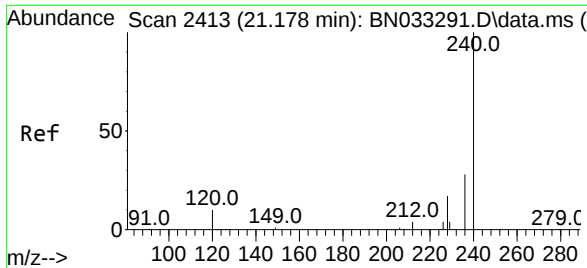

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.178 min Scan# 2413
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:240 Resp: 19870
Ion Ratio Lower Upper
240 100
120 12.2 9.0 13.6
236 27.9 22.4 33.6

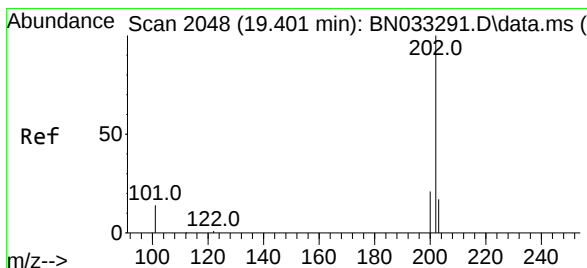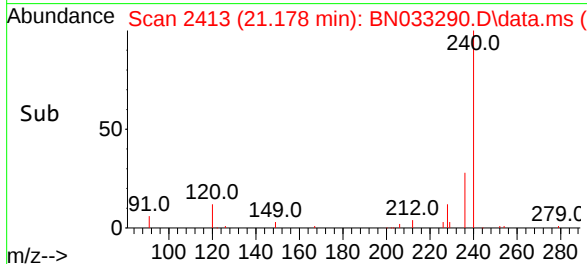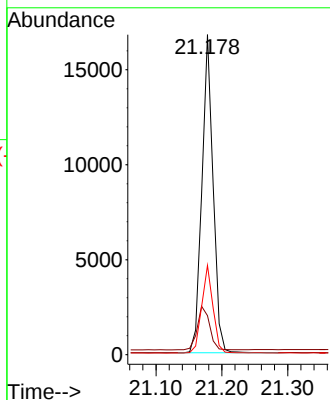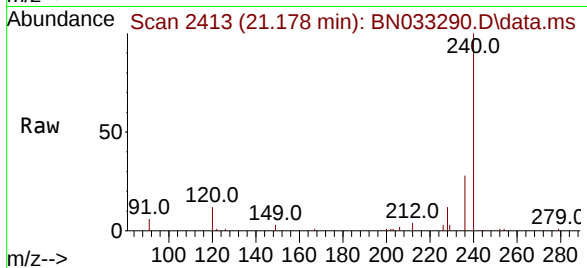

#30
Pyrene
Concen: 0.193 ng
RT: 19.405 min Scan# 2049
Delta R.T. 0.004 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Tgt Ion:202 Resp: 15275
Ion Ratio Lower Upper
202 100
200 20.9 16.7 25.1
203 18.0 14.2 21.4

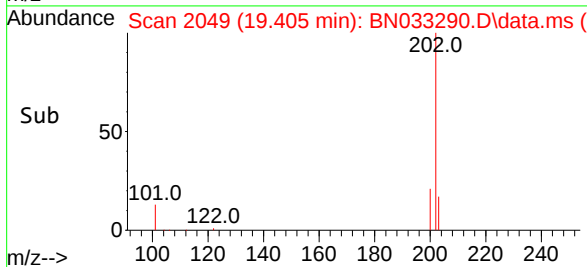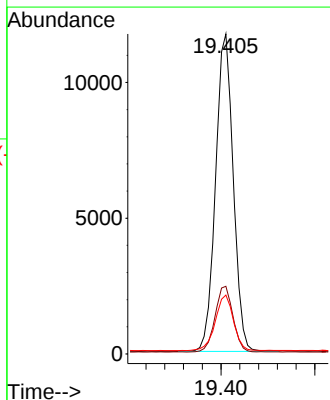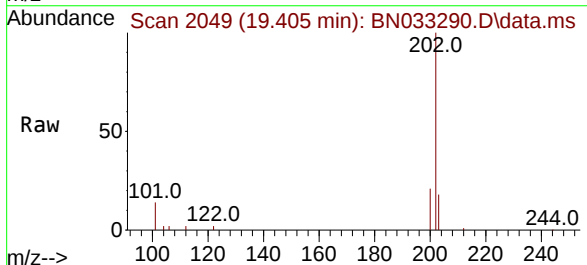



#31

Terphenyl-d14

Concen: 0.140 ng

RT: 19.633 min Scan# 2098

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:244 Resp: 6817

Ion Ratio Lower Upper

244 100

212 9.8 7.2 10.8

122 18.3 12.7 19.1

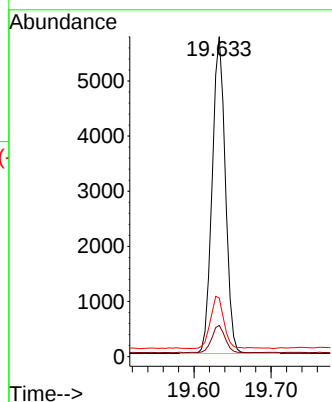

#32

Benzo(a)anthracene

Concen: 0.198 ng

RT: 21.160 min Scan# 2411

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00




Tgt Ion:228 Resp: 14819


Ion Ratio Lower Upper

228 100

226 27.8 22.1 33.1

229 19.7 15.6 23.4

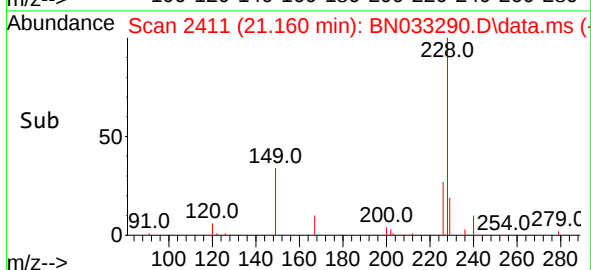



#33

Chrysene

Concen: 0.206 ng

RT: 21.214 min Scan# 2417

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:228 Resp: 14588

Ion Ratio Lower Upper

228 100

226 30.2 23.8 35.8

229 19.7 15.8 23.8

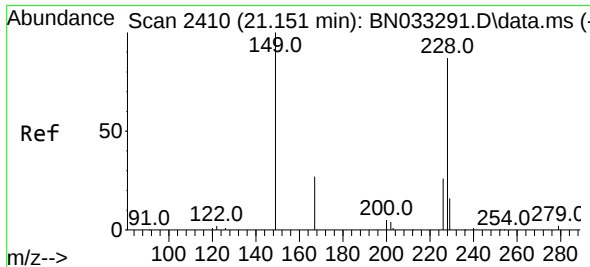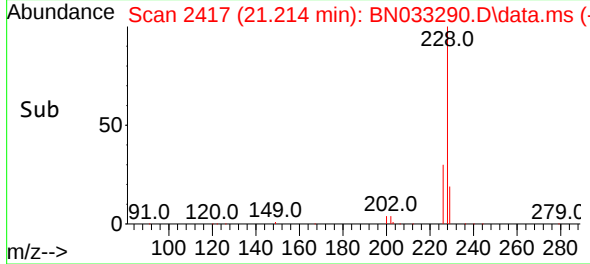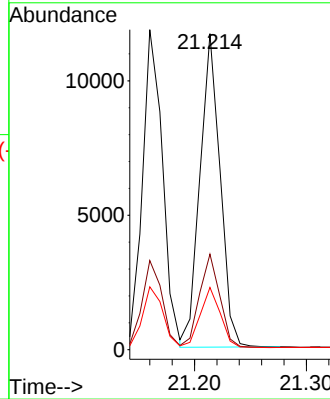

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.155 ng

RT: 21.151 min Scan# 2410

Delta R.T. -0.000 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00




Tgt Ion:149 Resp: 7939


Ion Ratio Lower Upper

149 100

167 27.7 21.6 32.4

279 3.1 2.6 4.0


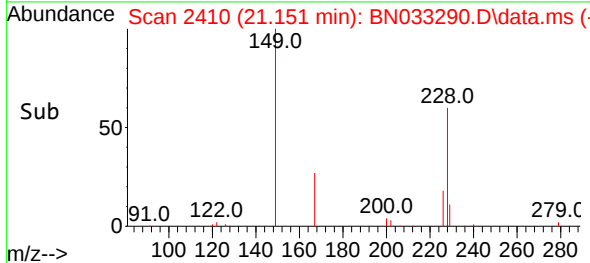
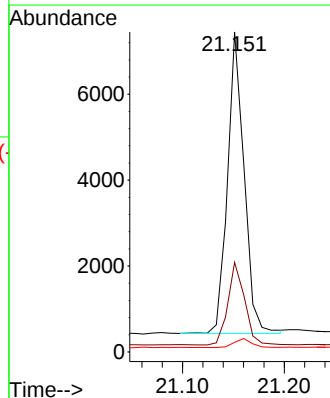
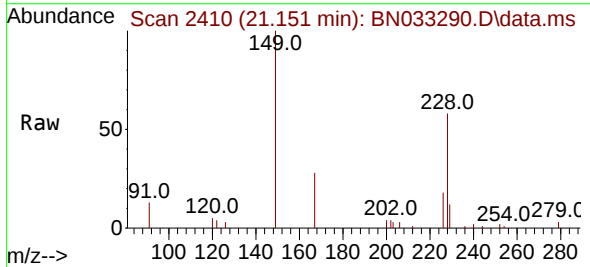




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.367 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:264 Resp: 23171
Ion Ratio Lower Upper
264 100
260 26.1 21.4 32.0
265 28.0 22.4 33.6

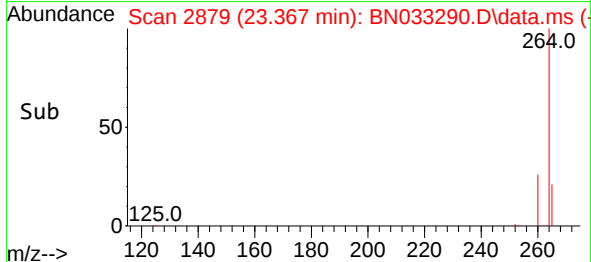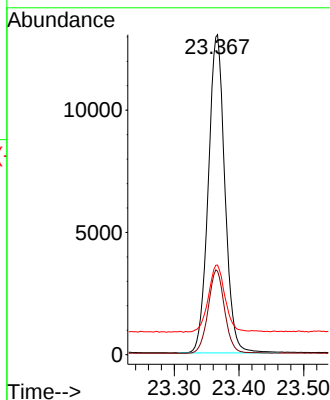

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.216 ng
RT: 25.548 min Scan# 3625
Delta R.T. 0.003 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00


Tgt Ion:276 Resp: 18661
Ion Ratio Lower Upper
276 100
138 28.3 22.7 34.1
277 25.0 19.8 29.8

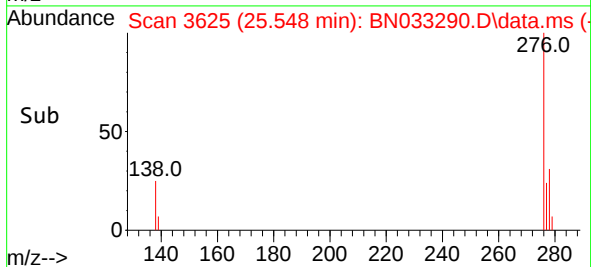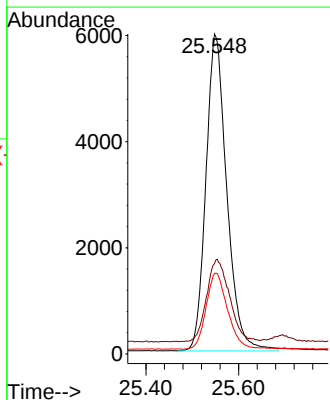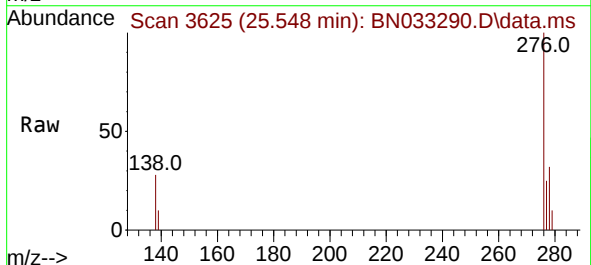






#37
Benzo(b)fluoranthene
Concen: 0.193 ng
RT: 22.715 min Scan# 2656
Delta R.T. -0.000 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2





Tgt Ion:252 Resp: 16302
Ion Ratio Lower Upper
252 100
253 23.5 17.8 26.6
125 14.9 10.0 15.0

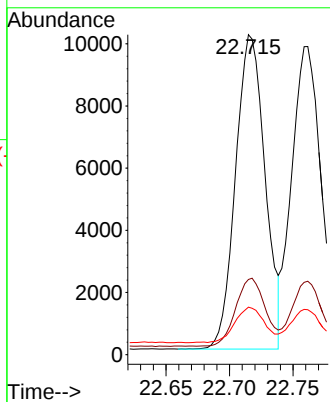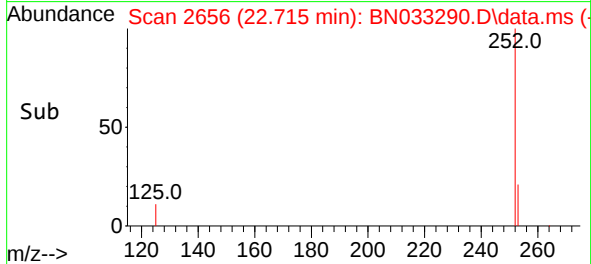


#38
Benzo(k)fluoranthene
Concen: 0.201 ng
RT: 22.762 min Scan# 2672
Delta R.T. 0.003 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

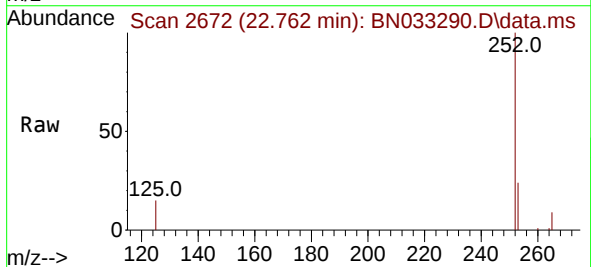

Tgt Ion:252 Resp: 16033
Ion Ratio Lower Upper
252 100
253 23.8 18.3 27.5
125 14.6 10.2 15.4

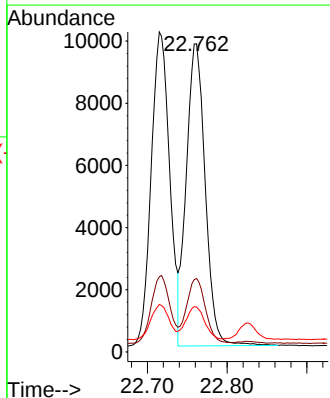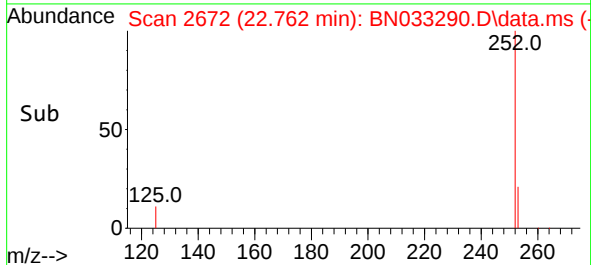



#39

Benzo(a)pyrene

Concen: 0.198 ng

RT: 23.270 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN033290.D


Acq: 07 Aug 2024 20:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

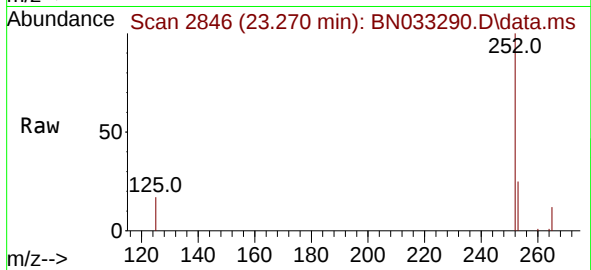




Tgt Ion:252 Resp: 14433

Ion	Ratio	Lower	Upper
-----	-------	-------	-------

252	100		
-----	-----	--	--

253	24.5	18.2	27.4
-----	------	------	------

125	16.6	11.4	17.2
-----	------	------	------

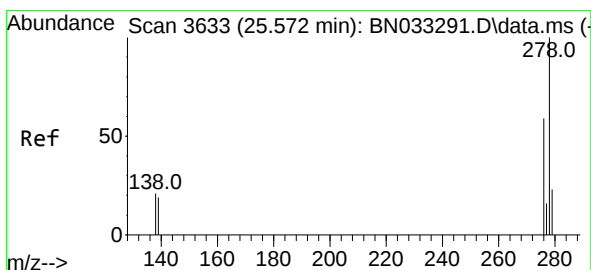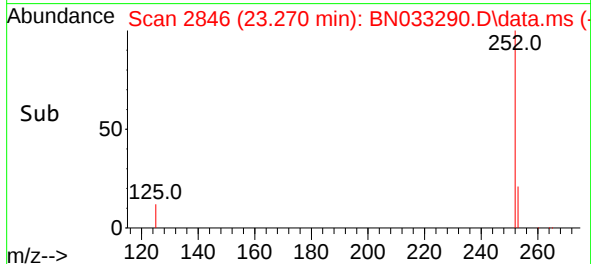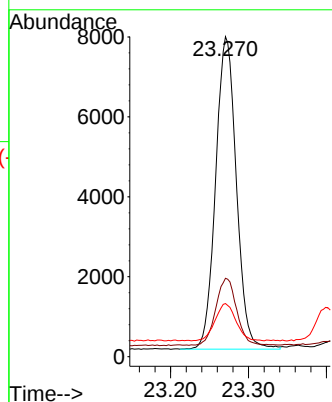

#40

Dibenzo(a,h)anthracene

Concen: 0.216 ng

RT: 25.574 min Scan# 3634

Delta R.T. 0.003 min

Lab File: BN033290.D

Acq: 07 Aug 2024 20:00




Tgt Ion:278 Resp: 14703


Ion	Ratio	Lower	Upper
-----	-------	-------	-------

278	100		
-----	-----	--	--

139	22.7	16.3	24.5
-----	------	------	------

279	25.8	19.4	29.2
-----	------	------	------

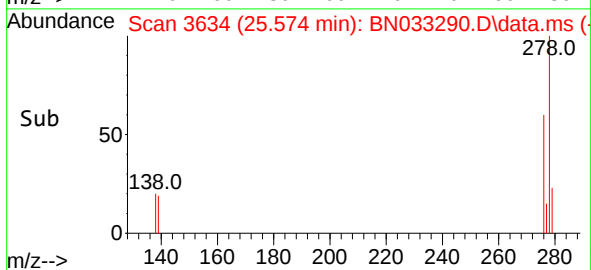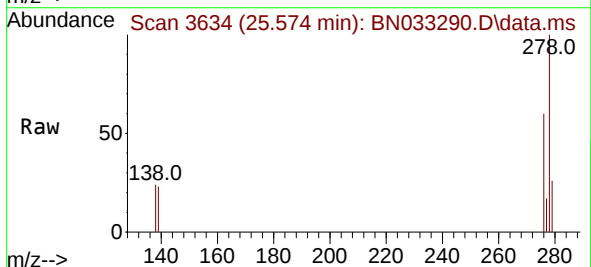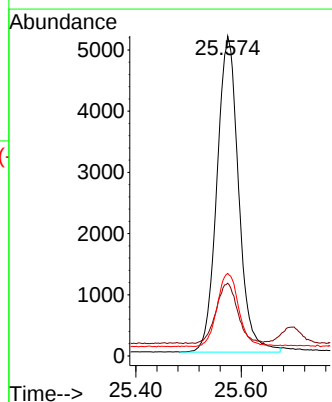

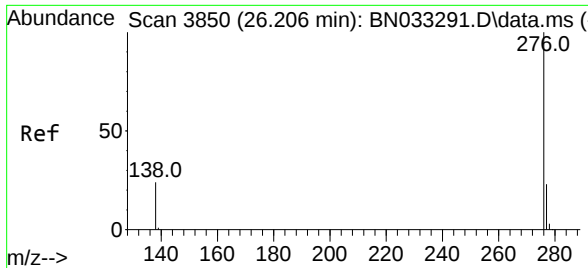

#41
Benzo(g,h,i)perylene
Concen: 0.222 ng
RT: 26.203 min Scan# 3849
Delta R.T. -0.003 min
Lab File: BN033290.D
Acq: 07 Aug 2024 20:00

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:276 Resp: 16242
Ion Ratio Lower Upper
276 100
277 25.0 19.0 28.4
138 28.6 20.8 31.2

