


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033288.D
Acq On : 07 Aug 2024 18:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 08 04:39:01 2024

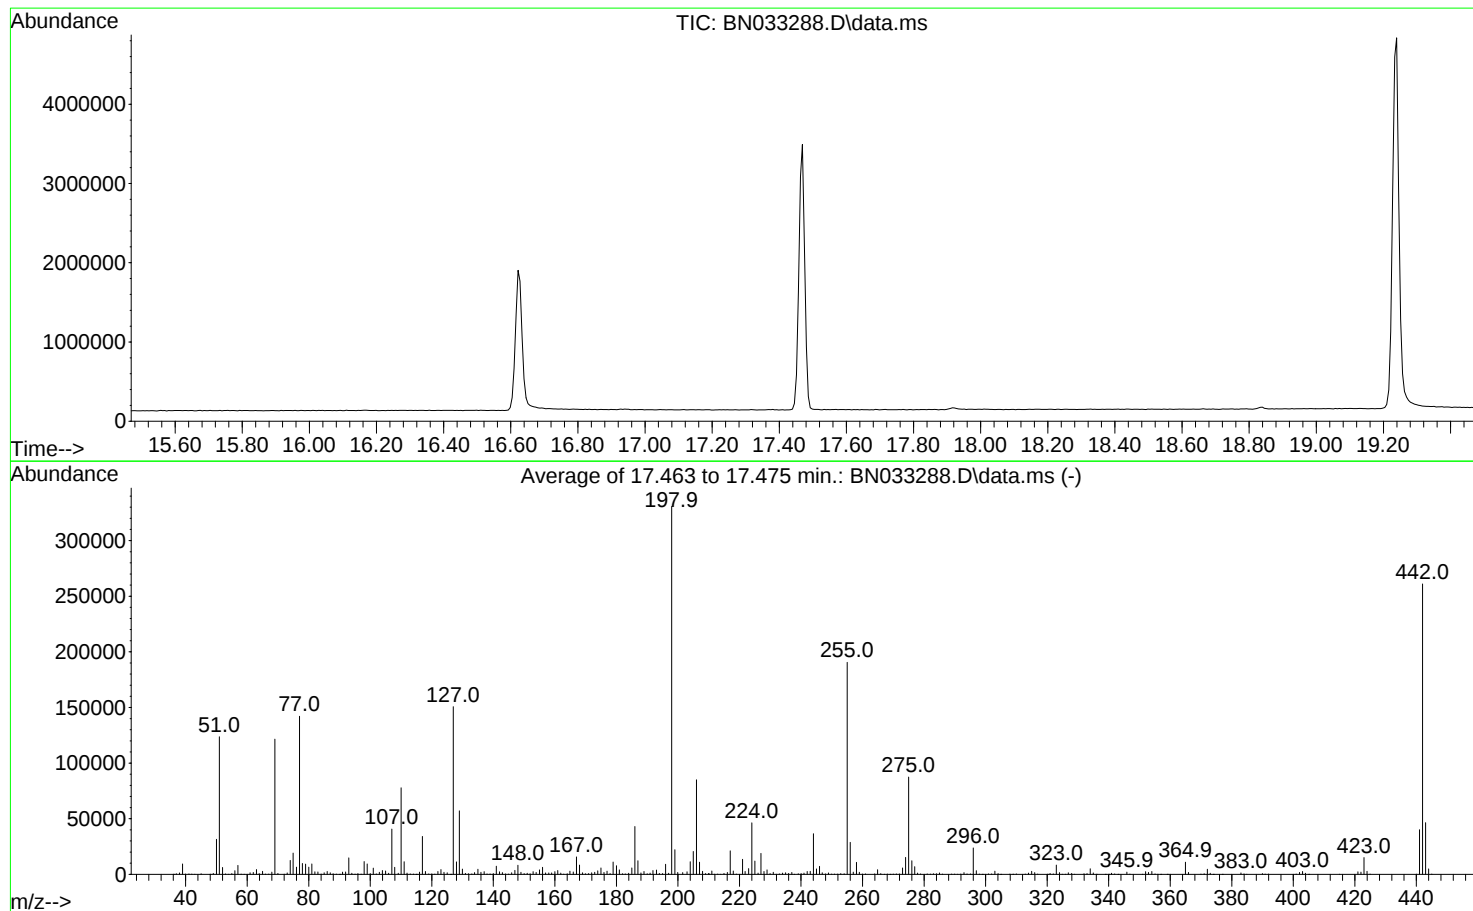

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	123696	PASS
68	69	0.00	2	1.6	1997	PASS
69	198	0.00	100	36.8	121580	PASS
70	69	0.00	2	0.7	868	PASS
127	198	10	80	45.6	150669	PASS
197	198	0.00	2	0.3	1056	PASS
198	198	100	100	100.0	330645	PASS
199	198	5	9	6.7	22125	PASS
275	198	10	60	26.4	87389	PASS
365	198	1	100	3.3	10872	PASS
441	198	0.01	100	12.1	40101	PASS
442	442	50	100	100.0	260992	PASS
443	442	15	24	17.8	46437	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/7/2024	BNA_N	<u>BN033288.D</u>
Compound Name	Response	Retention Time
DDT	993251	20.498
DDD	21317	20.051
DDE	351	19.545
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21668	1014919	2.13

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033288.D
Acq On : 07 Aug 2024 18:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 05:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

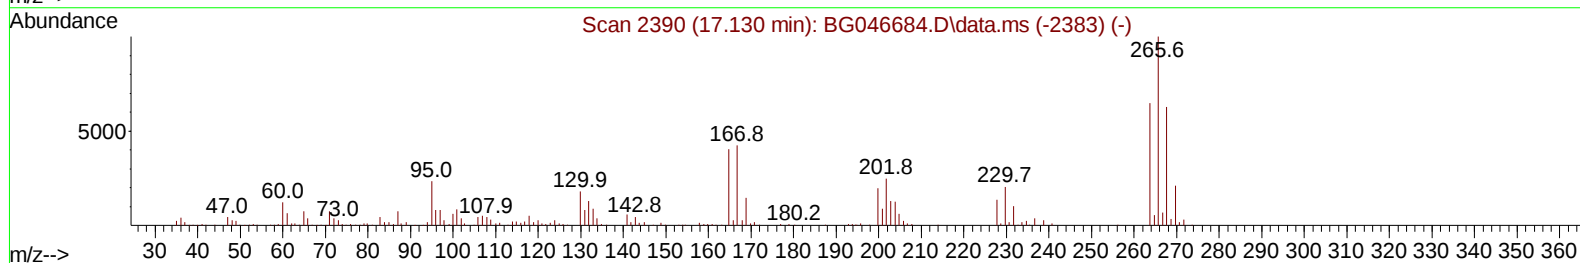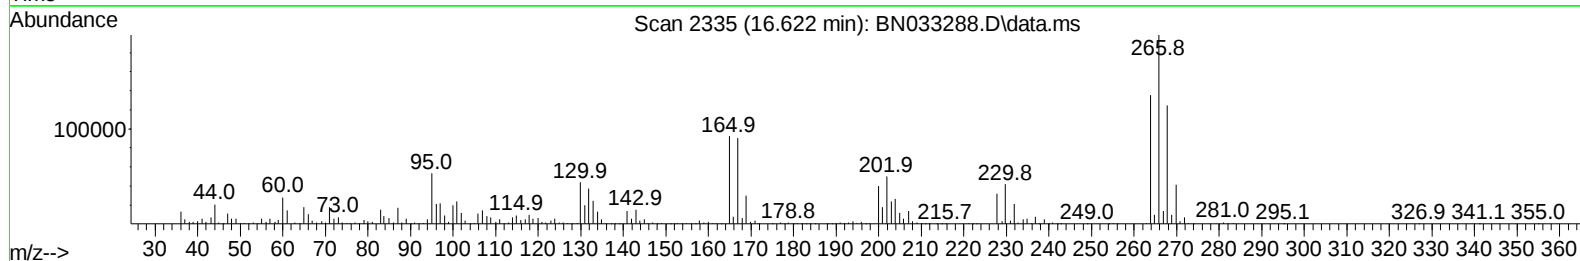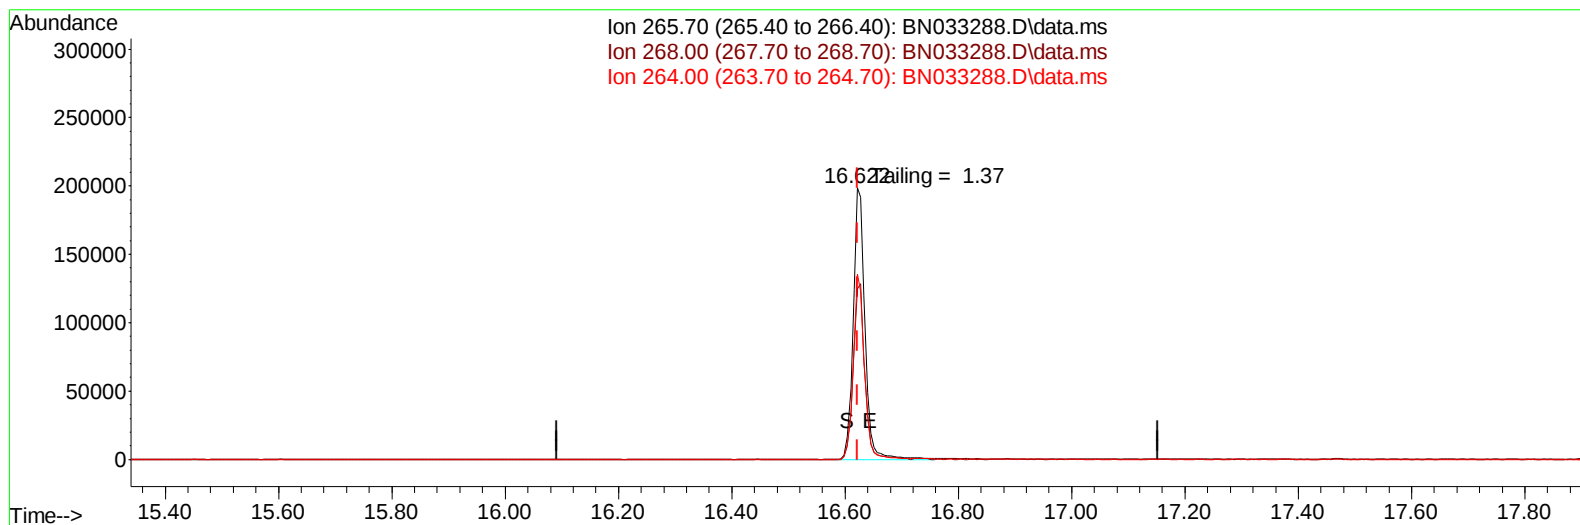

TIC: BN033288.D\data.ms

(70) Pentachlorophenol (C)

16.622min (+ 0.000) 19561.00 ng




response 288752

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	68.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080724\
Data File : BN033288.D
Acq On : 07 Aug 2024 18:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 05:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 05:52:05 2024
Response via : Initial Calibration

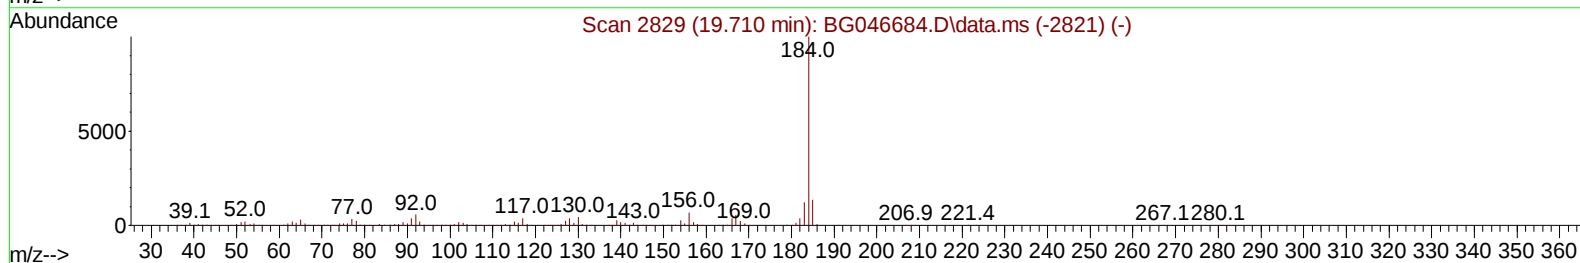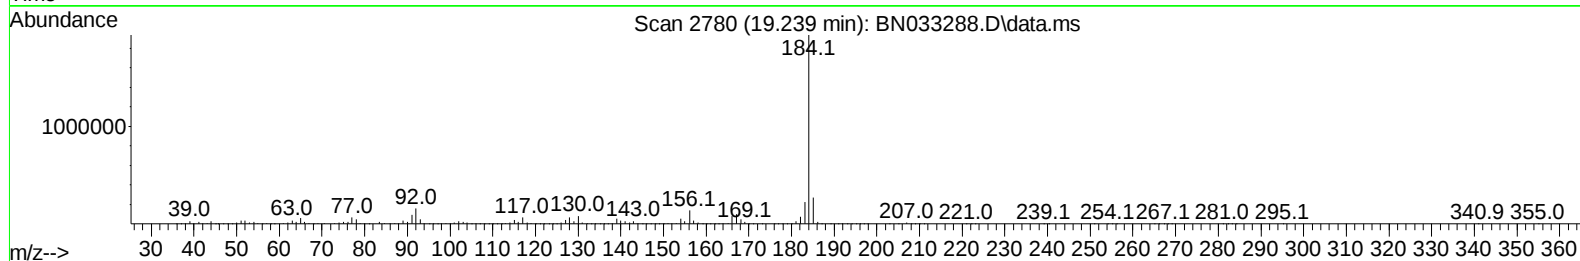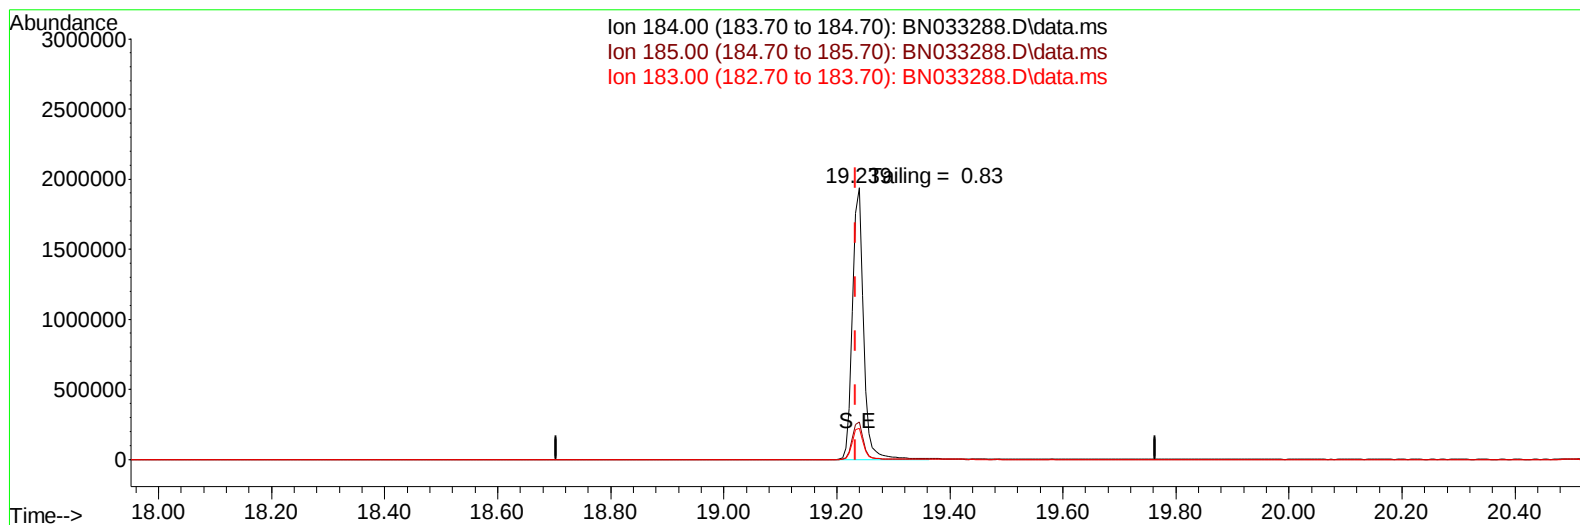

TIC: BN033288.D\data.ms

(77) Benzidine

19.239min (+ 0.006) 245325.72 ng

response 2654352

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.44
0.00	0.00	0.00