

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080818\
 Data File : BN002253.D
 Acq On : 08 Aug 2018 15:58
 Operator : JU/SJ
 Sample : J4268-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA1

Quant Time: Aug 09 02:18:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 09 02:16:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	238405	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	998530	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	491609	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	915037	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	797746	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	845407	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	16779	3.18	ng/uL	0.00
5) Phenol-d5	6.87	99	337774	15.04	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.03	67	238816	17.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	294393	16.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	284143	15.71	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	147579	17.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	158210	16.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	266107	15.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	363779	18.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	765610	18.37	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	980928	18.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	47632	5.98	ng/ul	0.00
57) Fluorene-d10	15.32	176	627806	17.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	46012	7.72	ng/ul	0.00
70) Anthracene-d10	17.16	188	854458	19.15	ng/ul	0.00
78) Pyrene-d10	19.46	212	848482	20.46	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	849295	18.60	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.89	94	30192	1.339	ng/ul#	85
44) Dimethylphthalate	13.77	163	224684	5.505	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080818\
Data File : BN002253.D
Acq On : 08 Aug 2018 15:58
Operator : JU/SJ
Sample : J4268-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA1

Quant Time: Aug 09 02:18:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 09 02:16:22 2018
Response via : Initial Calibration

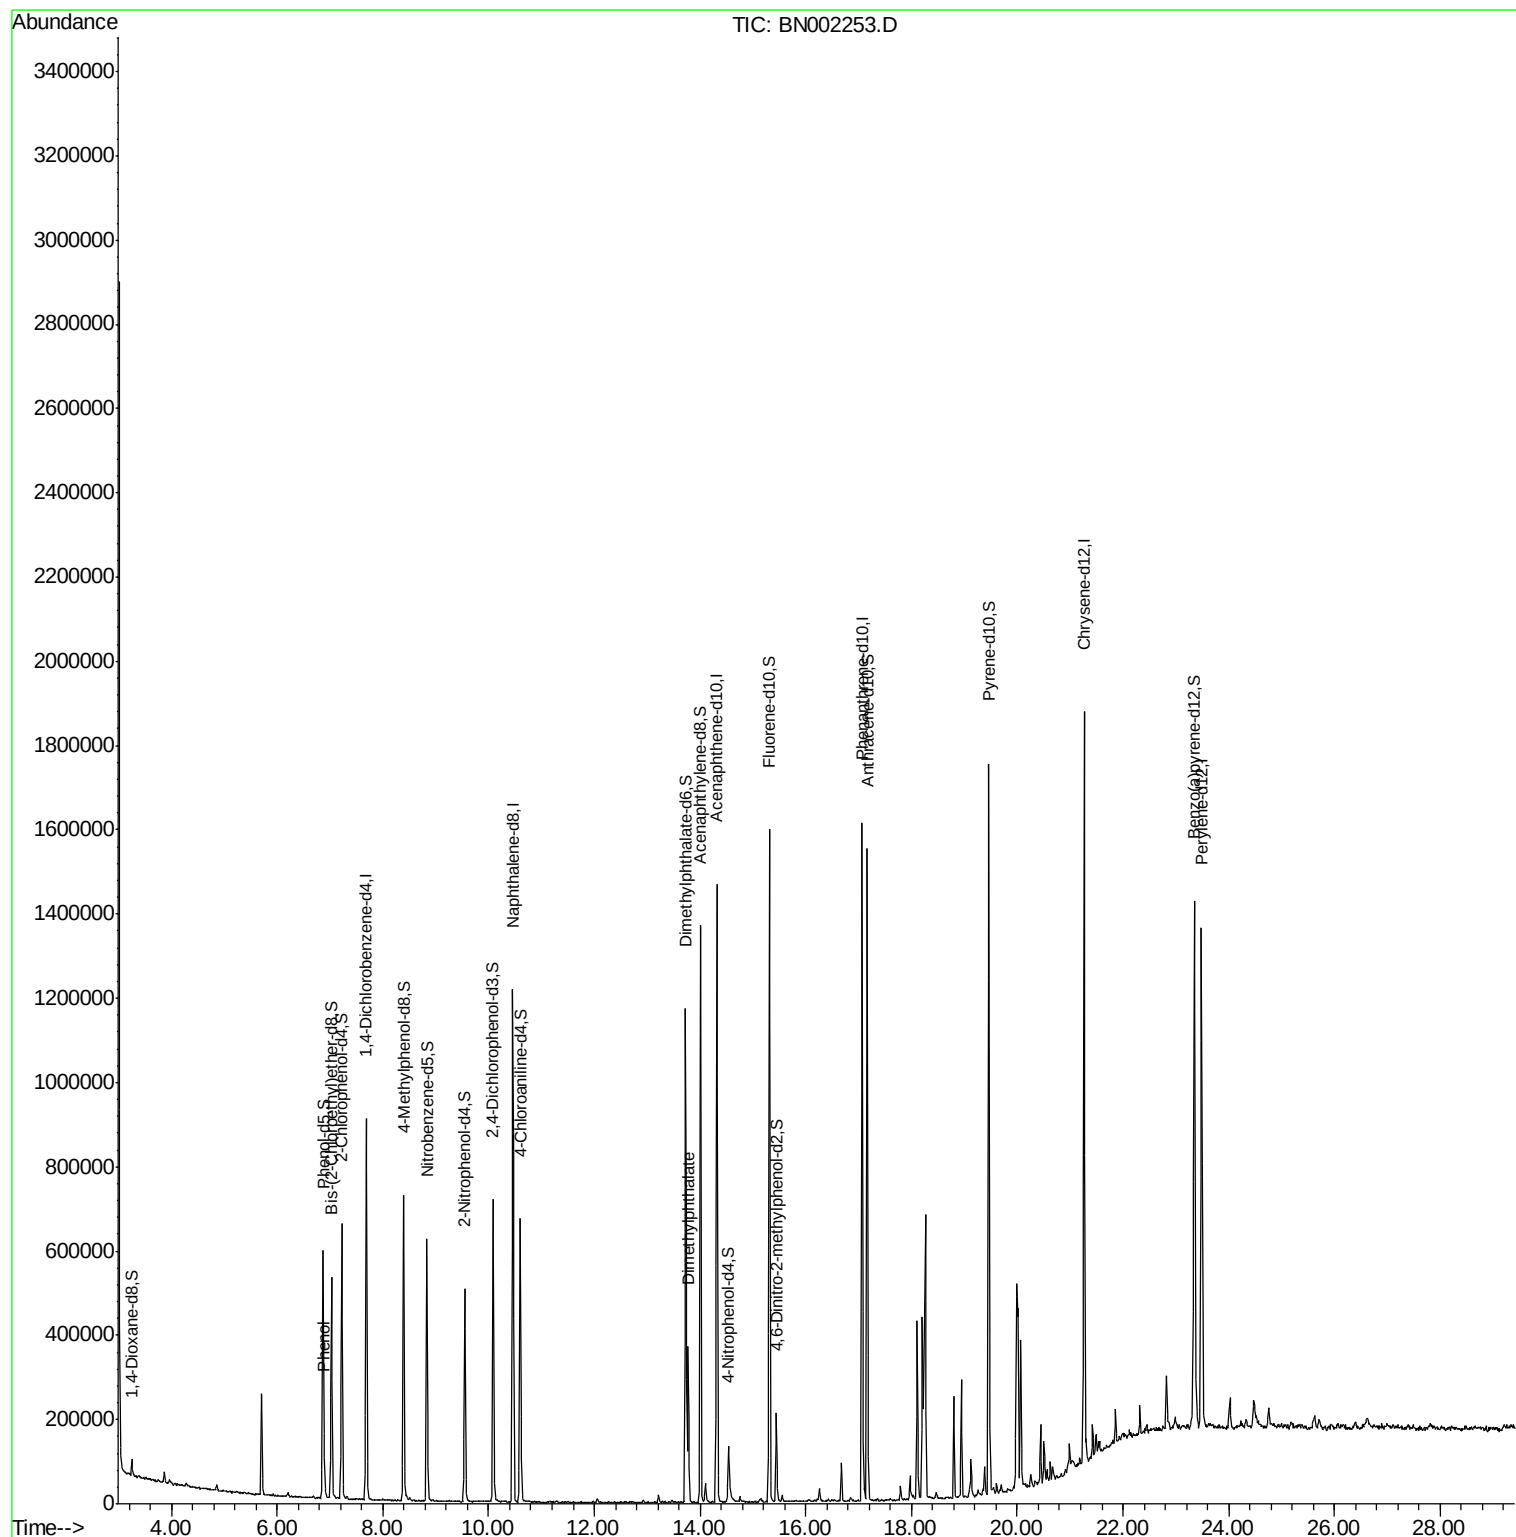

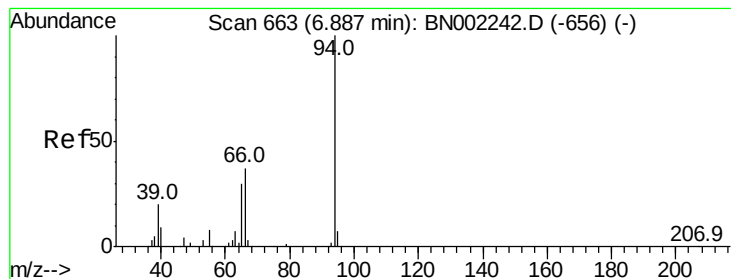

#6

Phenol

Concen: 1.339 ng/ul

RT: 6.89 min Scan# 664

Delta R.T. 0.01 min

Lab File: BN002253.D

Acq: 08 Aug 2018 15:58

Instrument :

BNA_N

ClientSampleId :

C0AA1


Tot Ion: 94 Resp: 30192

Ion Ratio Lower Upper




94 100

65 31.9 21.0 31.6#

66 47.3 29.3 43.9#

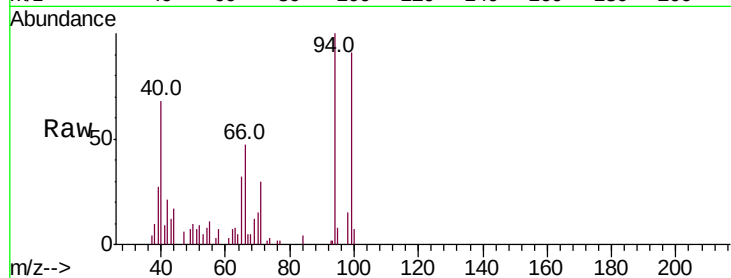

Abundance Ion 94.00 (93.70 to 94.70): BN0
Ion 65.00 (64.70 to 65.70): BN0
Ion 66.00 (65.70 to 66.70): BN0

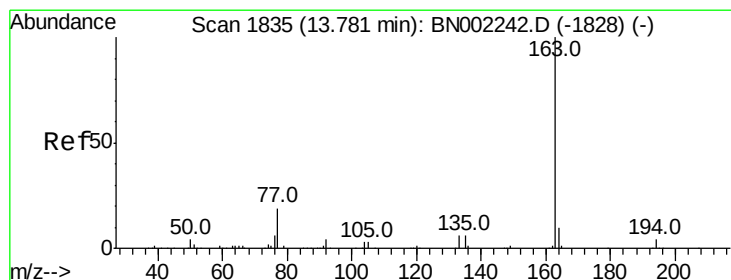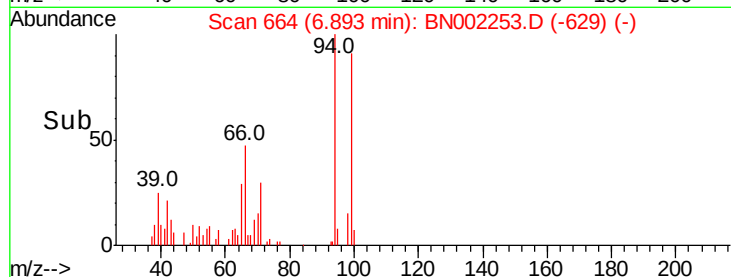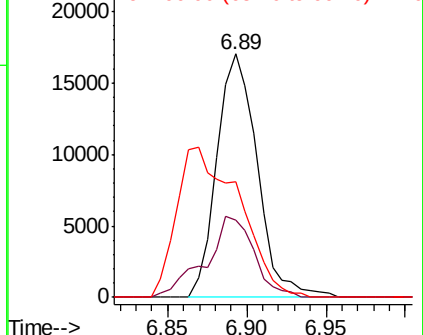

#44

Dimethylphthalate

Concen: 5.505 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BN002253.D

Acq: 08 Aug 2018 15:58


Tgt Ion:163 Resp: 224684

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.5 7.8 11.8

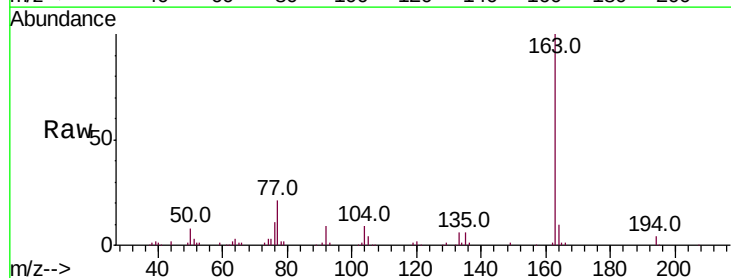

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

