

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080818\
 Data File : BN002255.D
 Acq On : 08 Aug 2018 17:09
 Operator : JU/SJ
 Sample : J4268-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:40:45 PM

Quant Time: Aug 09 03:58:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 09 02:16:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	254939	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1060149	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	526001	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	999702	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	920729	20.00	ng/ul	0.00
85) Perylene-d12	23.51	264	981634	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	14234	2.52	ng/uL	0.00
5) Phenol-d5	6.86	99	300979	12.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	204666	13.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	255567	13.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	239015	12.36	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	127819	14.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	131283	13.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	221635	12.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	302966	14.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	645081	14.47	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	822930	14.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	48811m	5.73	ng/ul	0.00
57) Fluorene-d10	15.32	176	536213	13.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	42353	6.50	ng/ul	0.00
70) Anthracene-d10	17.16	188	753382	15.46	ng/ul	0.00
78) Pyrene-d10	19.46	212	788830	16.48	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.37	264	815390	15.38	ng/ul	0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	161038	3.687	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080818\
Data File : BN002255.D
Acq On : 08 Aug 2018 17:09
Operator : JU/SJ
Sample : J4268-04
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AA6

Quant Time: Aug 09 03:58:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 09 02:16:22 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/9/2018 4:40:45 PM

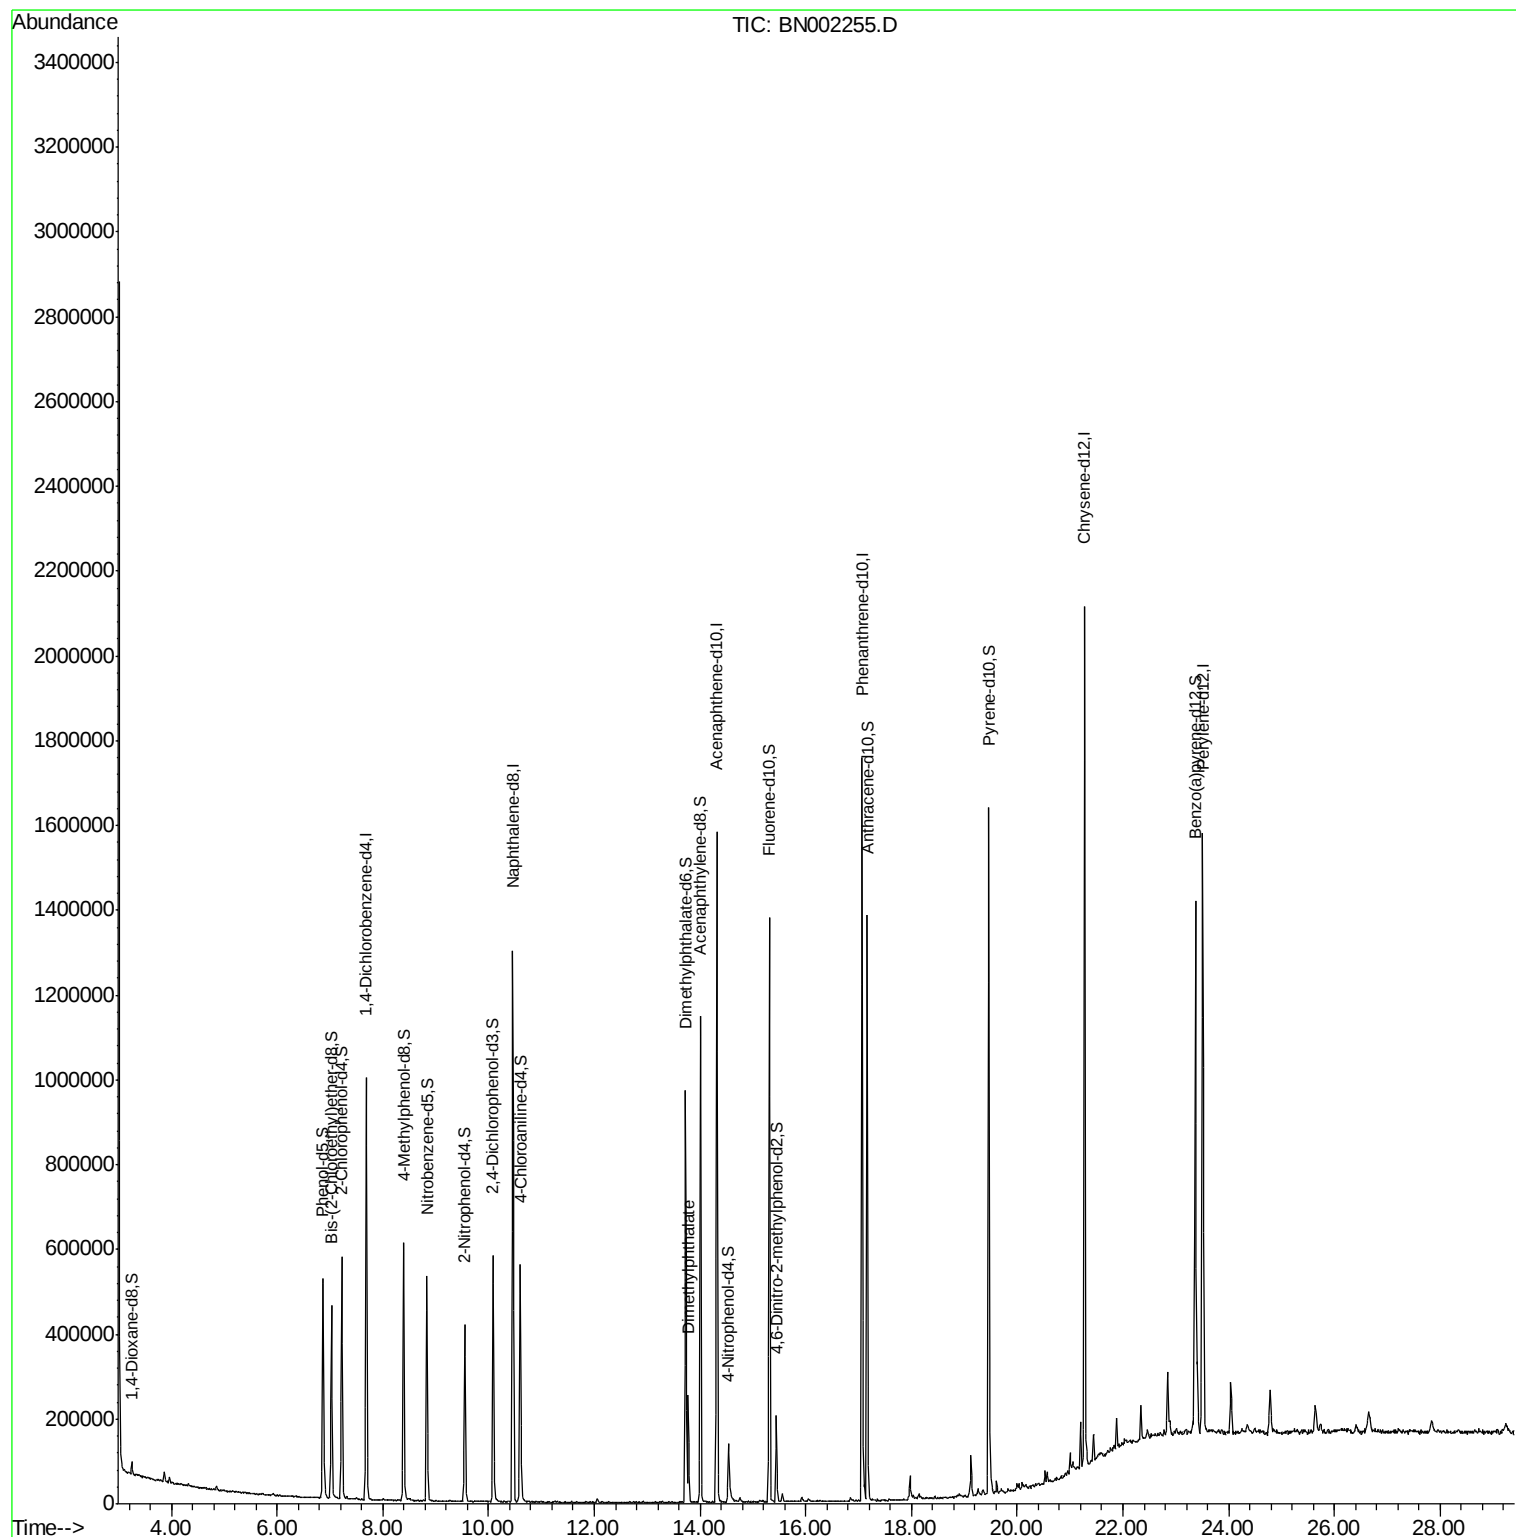

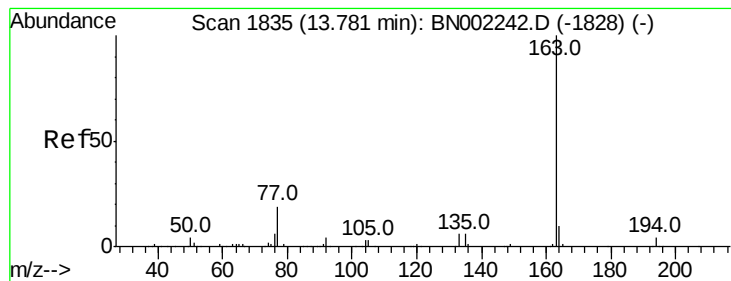

#44

Dimethylphthalate

Concen: 3.687 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BN002255.D

Acq: 08 Aug 2018 17:09

Instrument :

BNA_N

ClientSampleId :

C0AA6

Tot Ion	Ratio	Resp	Lower	Upper
163	100	161038		
194	3.7		3.2	4.8
164	9.9		7.8	11.8

Manual Integrations
APPROVED

Sohil
8/9/2018 4:40:45 PM

