

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080823\
 Data File : BN026840.D
 Acq On : 08 Aug 2023 09:19
 Operator : MA/JU
 Sample : PB154648BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 09 00:52:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 03:46:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	12077	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	37882	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.740	164	22476	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.485	188	48973	0.400	ng/ul	0.00
17) Chrysene-d12	21.665	240	37444	0.400	ng/ul	0.00
23) Perylene-d12	24.223	264	42481	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	57663	4.022	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	13177	0.236	ng/ul	0.00
18) Fluoranthene-d10	19.501	212	33797	0.286	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.873	202	4755	0.029	ng/ul#	1
26) Benzo(a)pyrene	24.062	252	10827	0.075	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080823\
Data File : BN026840.D
Acq On : 08 Aug 2023 09:19
Operator : MA/JU
Sample : PB154648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 09 00:52:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 03:46:36 2023
Response via : Initial Calibration

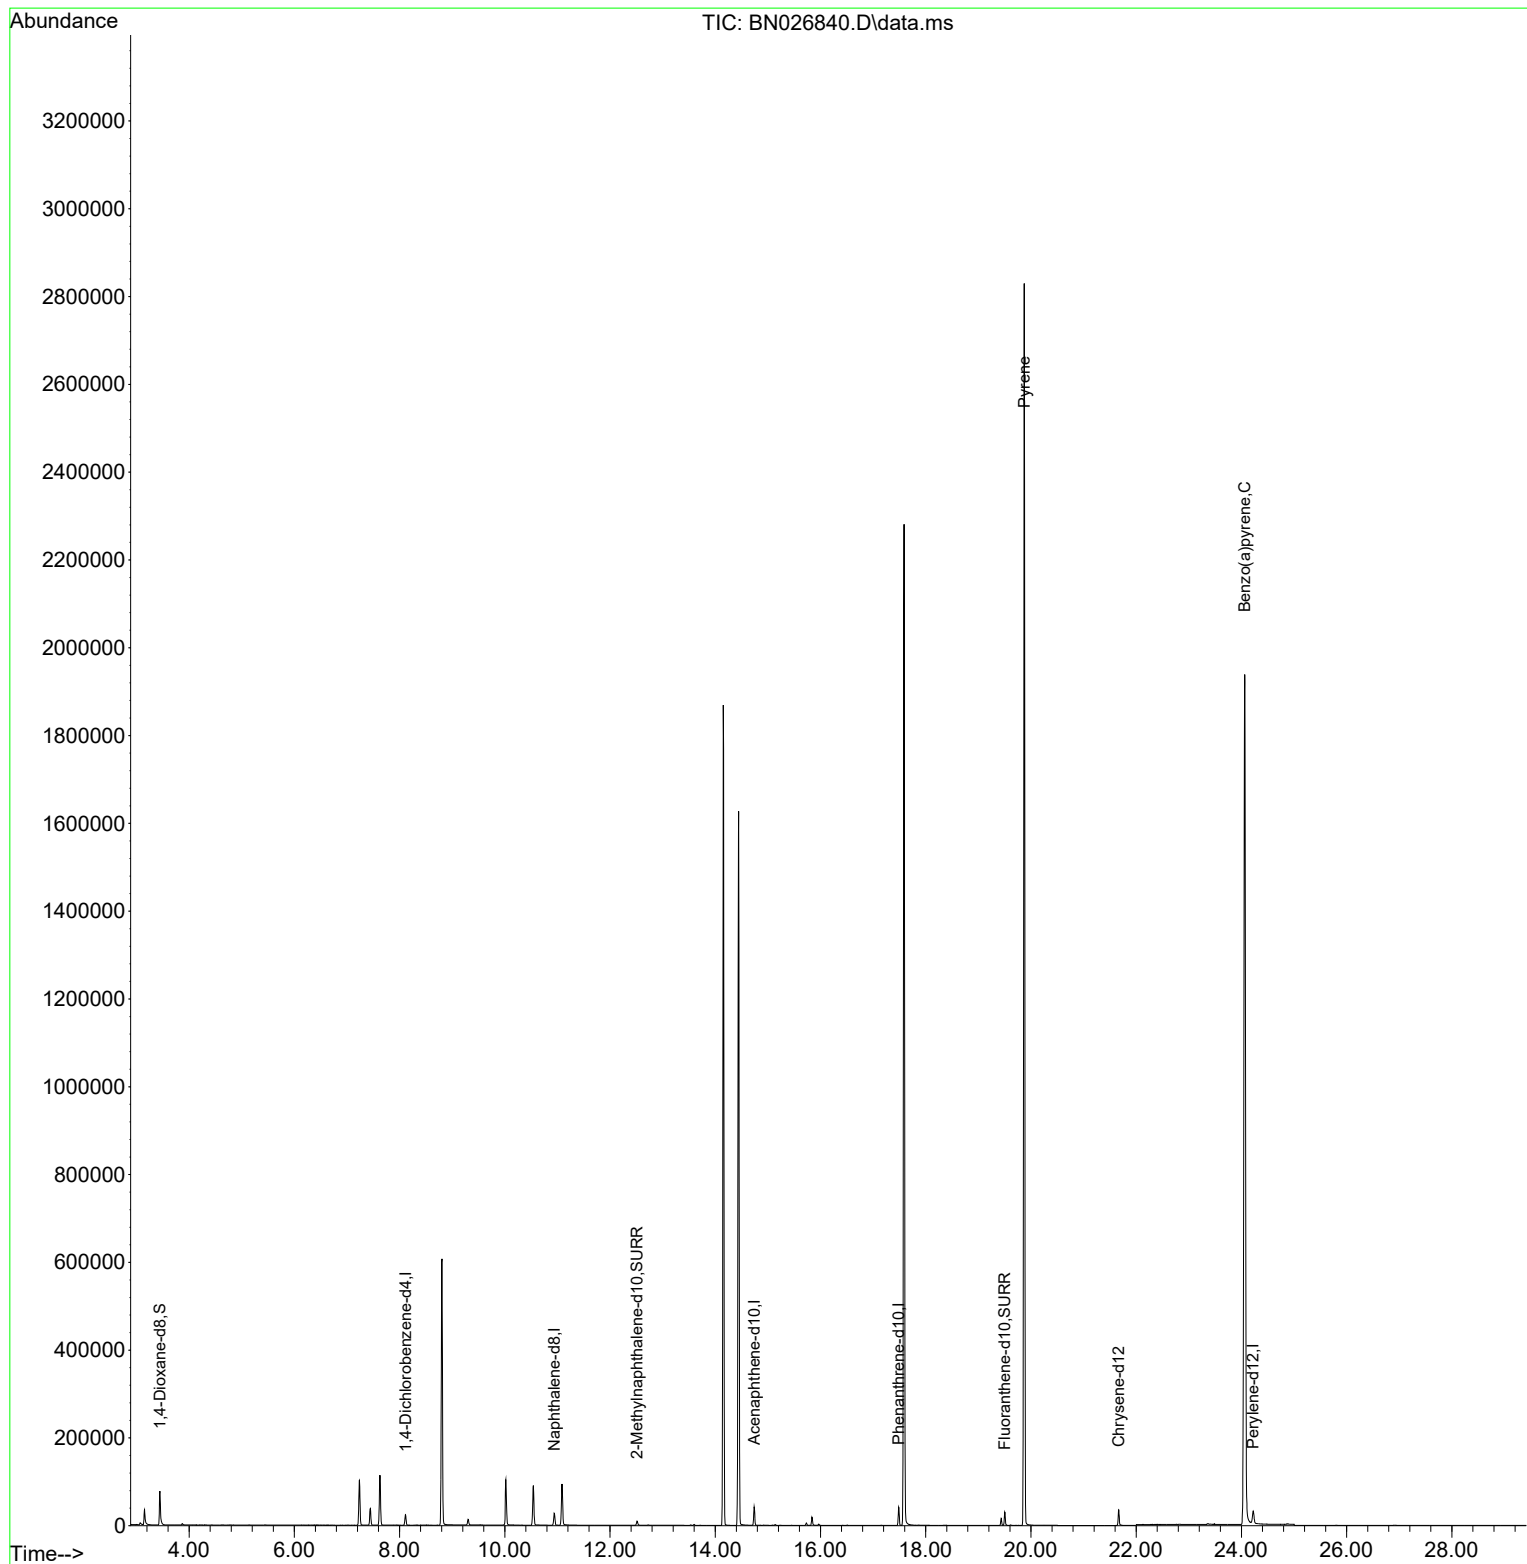

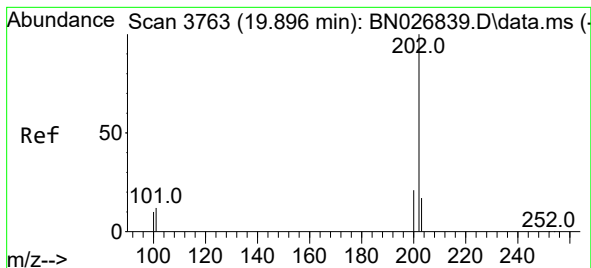

#20

Pyrene

Concen: 0.029 ng/ul

RT: 19.873 min Scan# 31

Delta R.T. -0.028 min

Lab File: BN026840.D

Acq: 08 Aug 2023 09:19





Instrument :

BNA_N

ClientSampleId :

Tgt Ion:202 Resp: 4755

Ion	Ratio	Lower	Upper
202	100		
101	151.2	10.7	16.1#
100	1106.5	8.5	12.7#

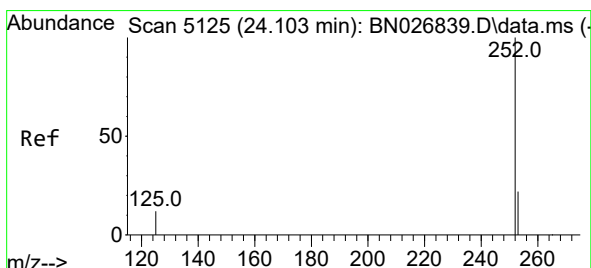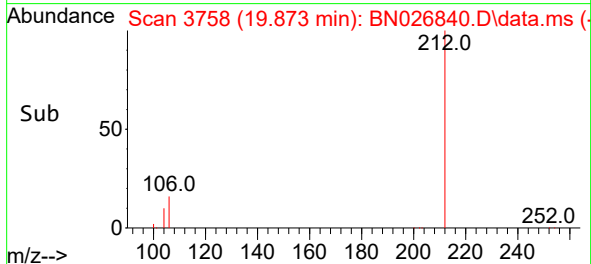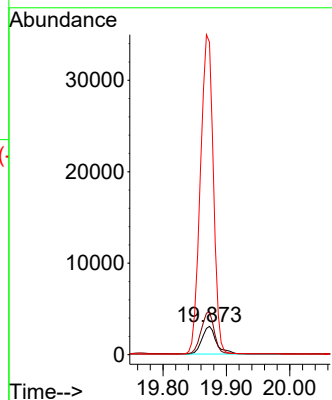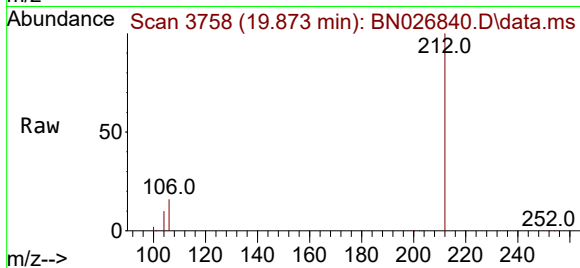

#26

Benzo(a)pyrene

Concen: 0.075 ng/ul

RT: 24.062 min Scan# 5111

Delta R.T. -0.050 min

Lab File: BN026840.D

Acq: 08 Aug 2023 09:19

Tgt Ion:252 Resp: 10827

Ion	Ratio	Lower	Upper
252	100		
253	34.9	19.0	28.6#
125	30.8	11.4	17.0#

