

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080823\
 Data File : BN026843.D
 Acq On : 08 Aug 2023 11:10
 Operator : MA/JU
 Sample : 03901-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 09 00:52:58 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 03:46:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	7215	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	22829	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.740	164	13620	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.489	188	29679	0.400	ng/ul	0.00
17) Chrysene-d12	21.662	240	22717	0.400	ng/ul	0.00
23) Perylene-d12	24.220	264	26364	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.443	96	31757	3.707	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	13898	0.414	ng/ul	0.00
18) Fluoranthene-d10	19.501	212	35358	0.493	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.481	88	7438	0.851	ng/ul	95
20) Pyrene	19.873	202	4882	0.048	ng/ul#	1
26) Benzo(a)pyrene	24.056	252	11147	0.124	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080823\
Data File : BN026843.D
Acq On : 08 Aug 2023 11:10
Operator : MA/JU
Sample : 03901-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 09 00:52:58 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 03:46:36 2023
Response via : Initial Calibration

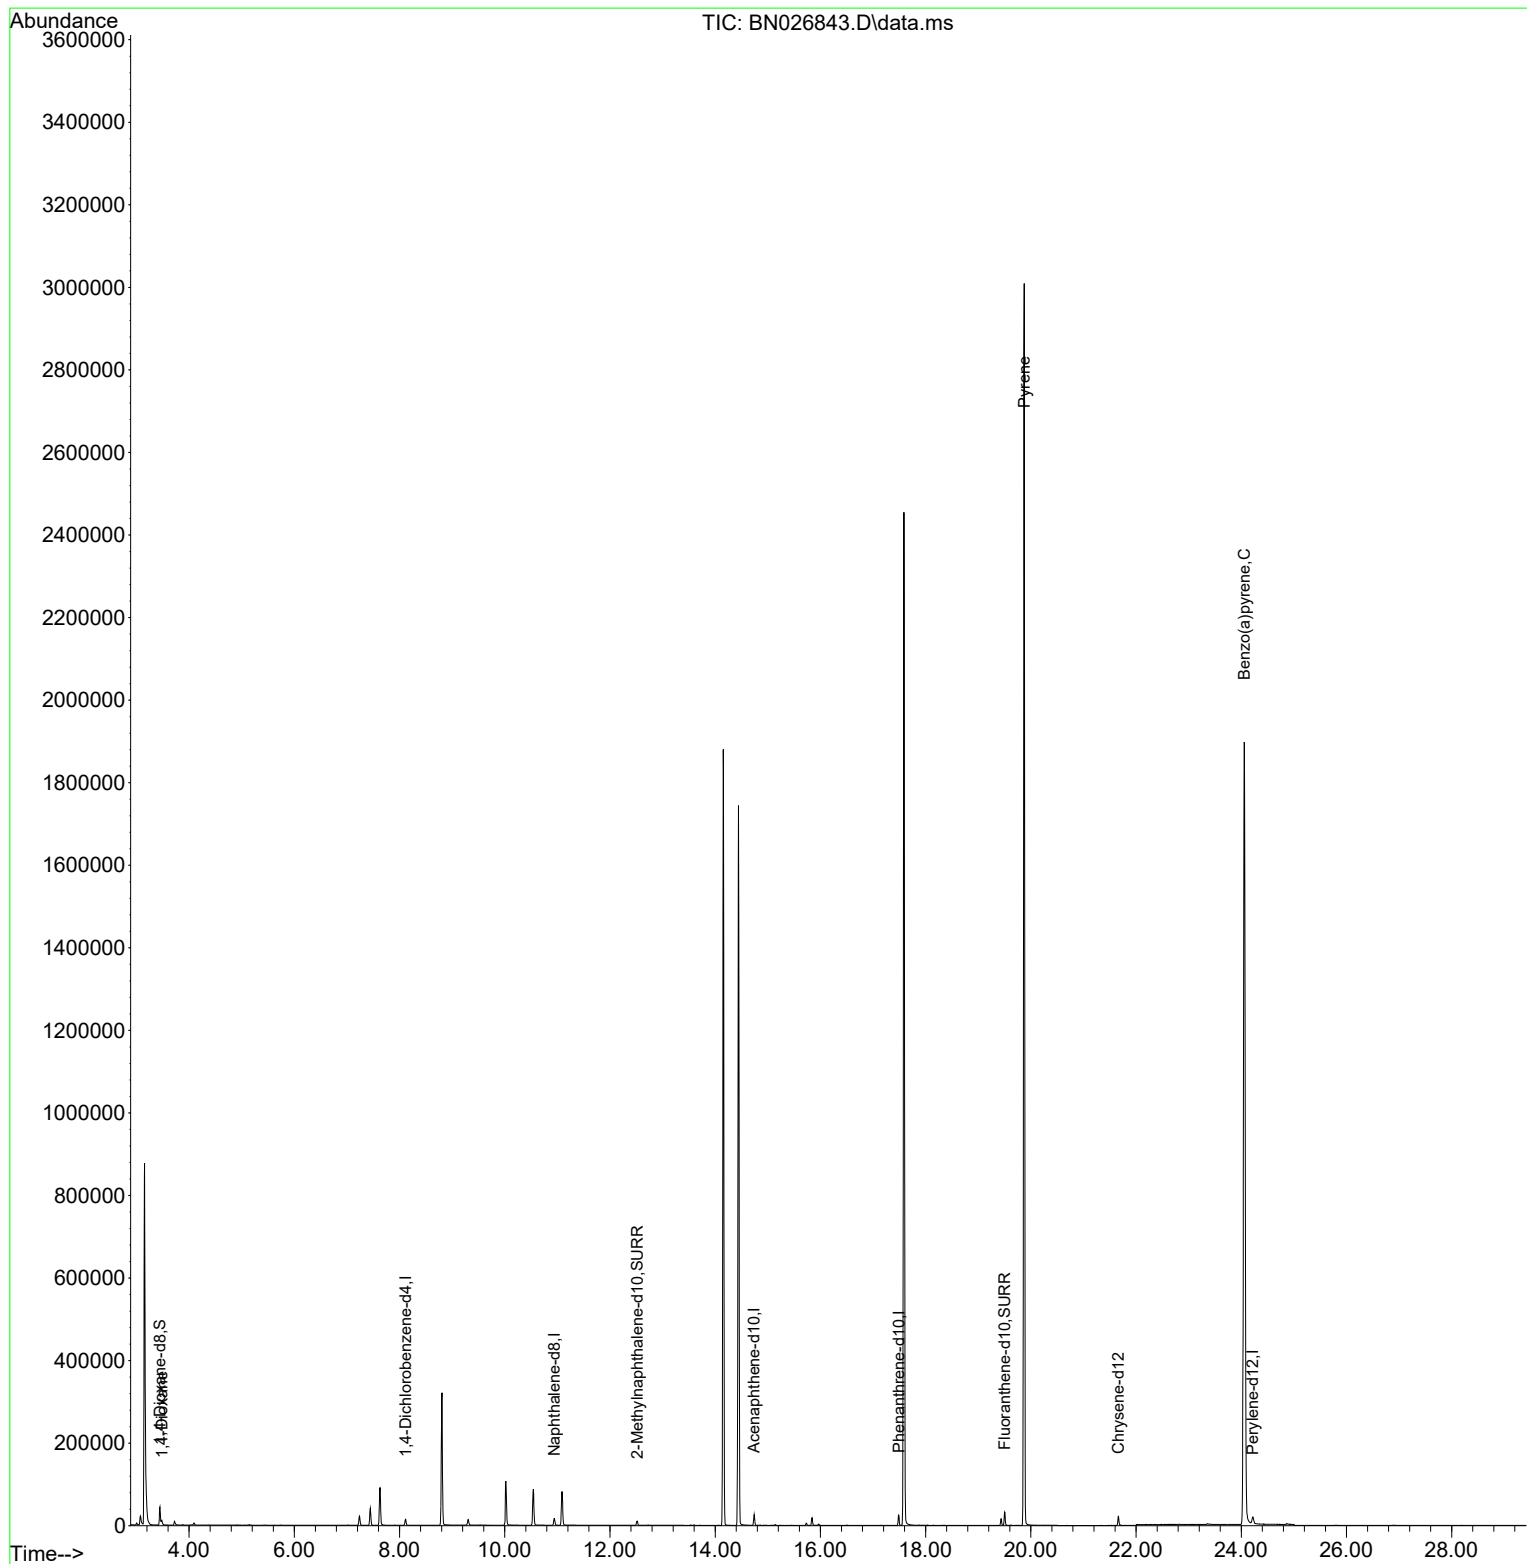



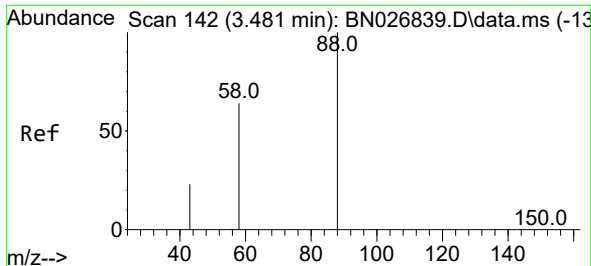


#2
1,4-Dioxane
Concen: 0.851 ng/ul
RT: 3.481 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN026843.D
Acq: 08 Aug 2023 11:10


Instrument :
BNA_N
ClientSampleId :

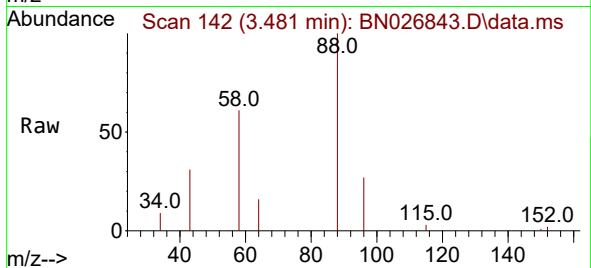



Tgt Ion: 88 Resp: 7438
Ion Ratio Lower Upper
88 100
43 30.8 28.0 42.0
58 60.7 46.0 69.0

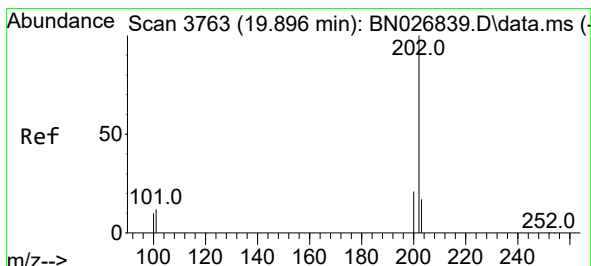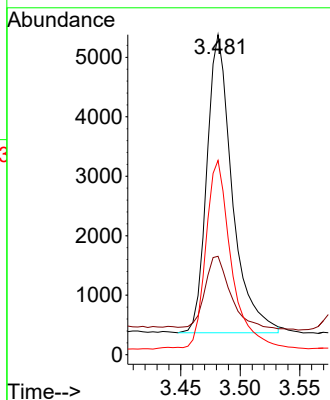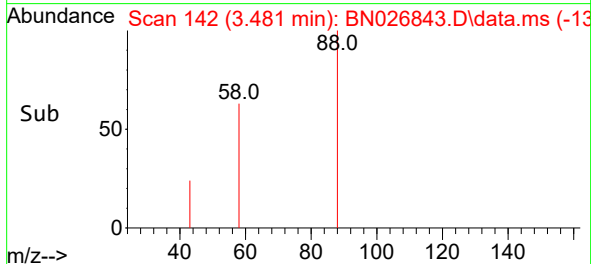


#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.873 min Scan# 3758
Delta R.T. -0.028 min
Lab File: BN026843.D
Acq: 08 Aug 2023 11:10

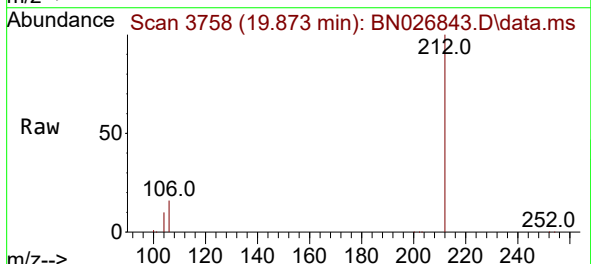


Tgt Ion: 202 Resp: 4882
Ion Ratio Lower Upper
202 100
101 143.1 10.7 16.1#
100 1053.1 8.5 12.7#

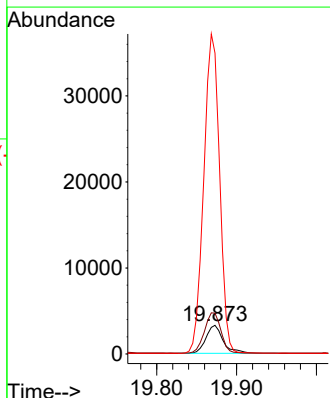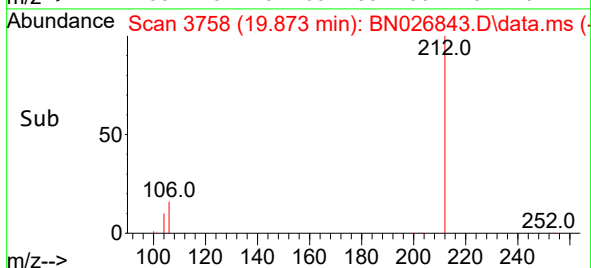

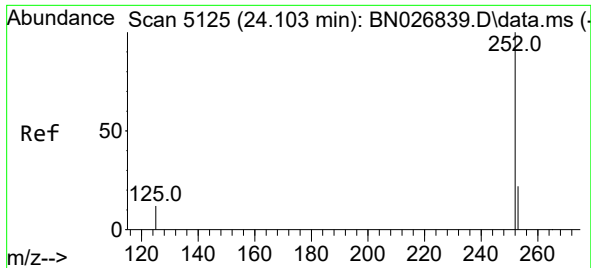

#26
Benzo(a)pyrene
Concen: 0.124 ng/ul
RT: 24.056 min Scan# 51
Delta R.T. -0.056 min
Lab File: BN026843.D
Acq: 08 Aug 2023 11:10

Instrument :
BNA_N
ClientSampleId :

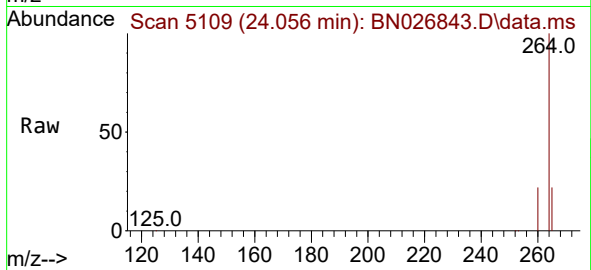

Tgt Ion:252 Resp: 11147
Ion Ratio Lower Upper
252 100
253 34.9 19.0 28.6#
125 32.2 11.4 17.0#

