

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
 Data File : BN002264.D
 Acq On : 09 Aug 2018 15:48
 Operator : JU/SJ
 Sample : J4301-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 10 01:06:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 10 01:04:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	306606	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1332700	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	715001	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1328559	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	992271	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1041051	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	24530	3.61	ng/uL	0.00
5) Phenol-d5	6.86	99	557162	19.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	374169	21.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	457630	20.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	459003	19.74	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	242364	21.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	256988	20.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	435944	19.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	524197	20.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1282783	21.16	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1686200	22.36	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	157809	13.63	ng/ul	0.00
57) Fluorene-d10	15.32	176	1078110	20.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	142737	16.50	ng/ul	0.00
70) Anthracene-d10	17.16	188	1449734	22.38	ng/ul	0.00
78) Pyrene-d10	19.46	212	1299185	25.19	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	1174672	20.90	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	604955	10.190	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
Data File : BN002264.D
Acq On : 09 Aug 2018 15:48
Operator : JU/SJ
Sample : J4301-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 10 01:06:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 10 01:04:23 2018
Response via : Initial Calibration

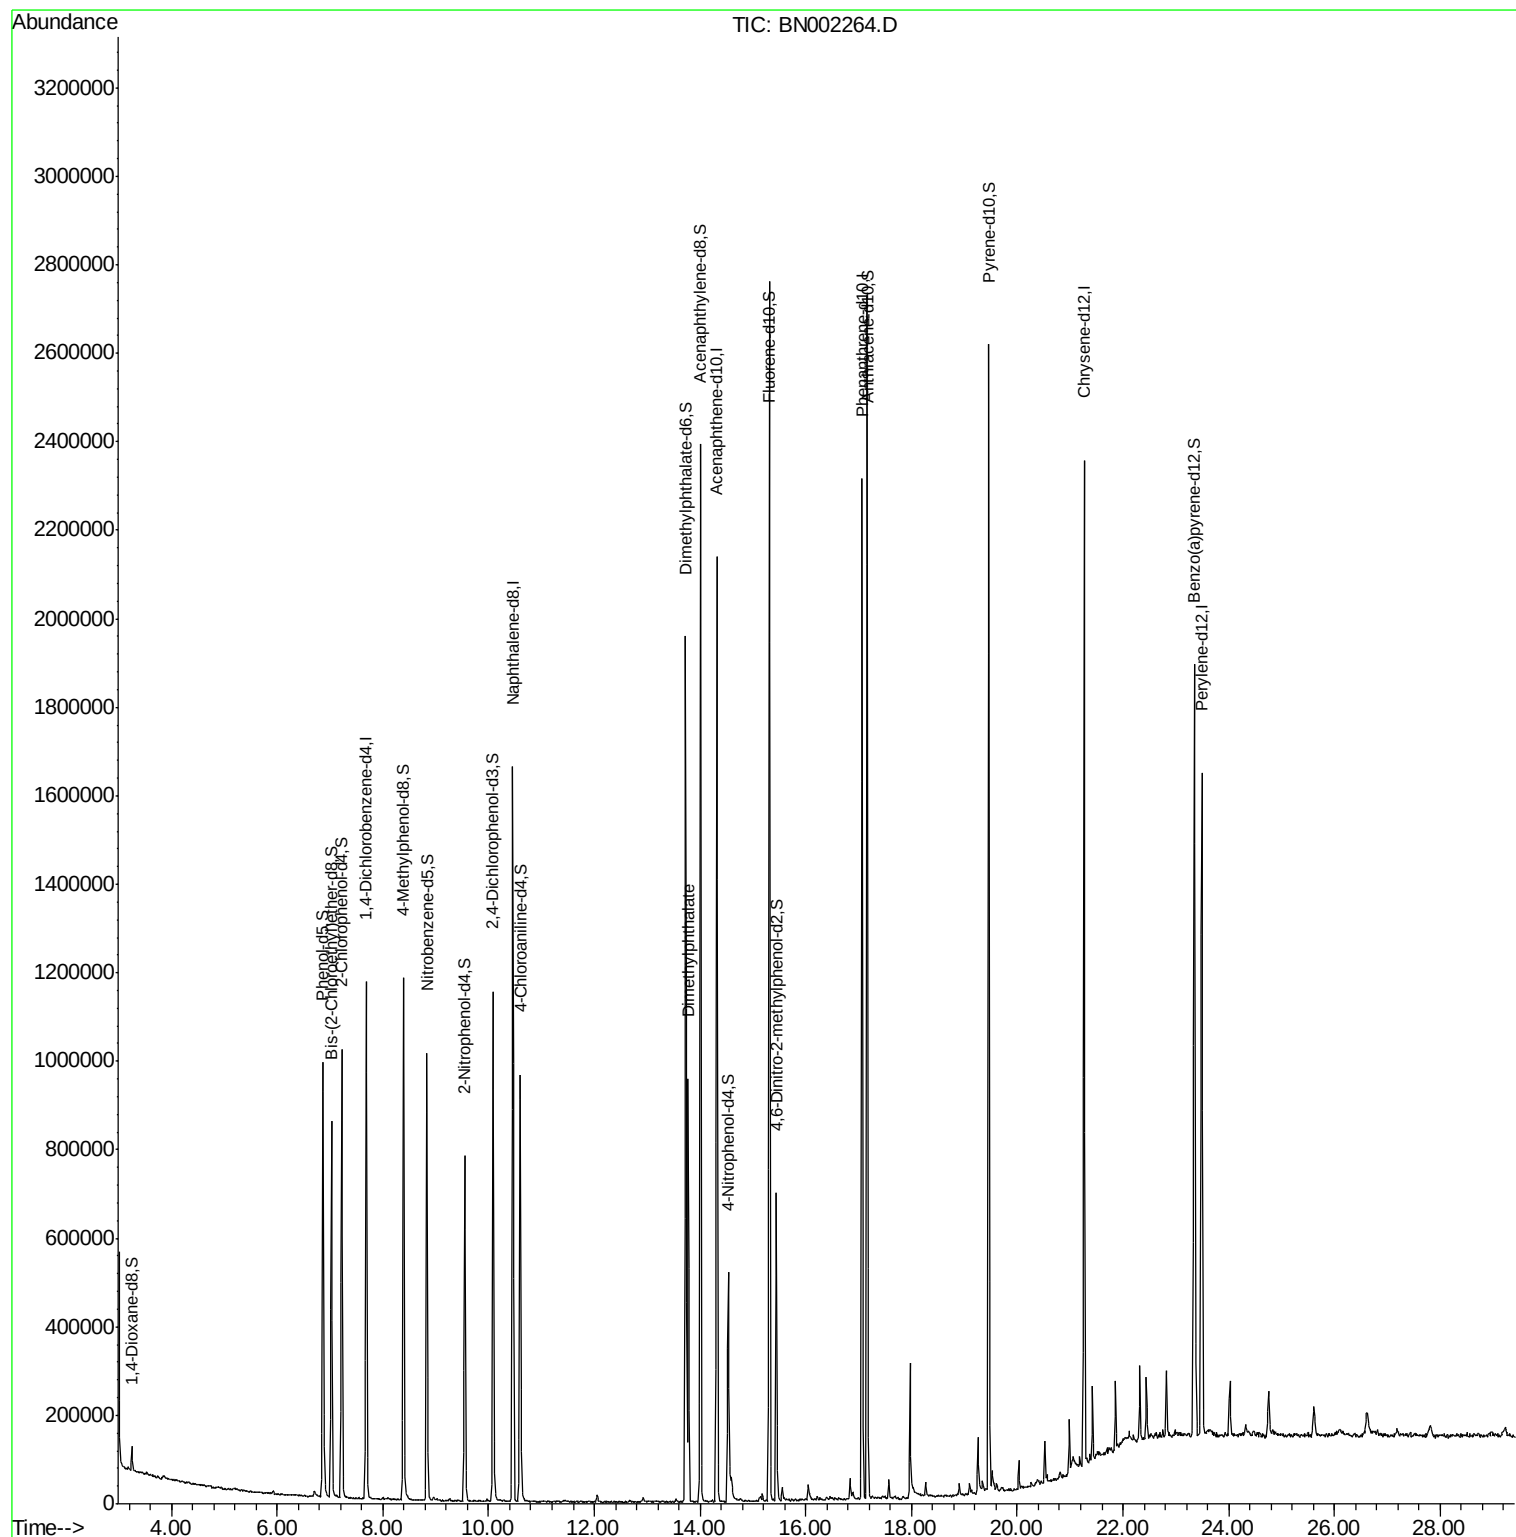

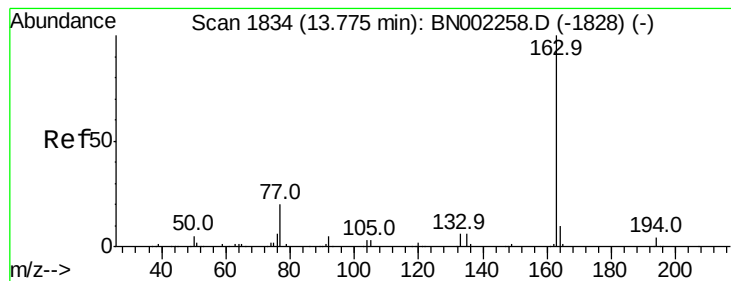

#44

Dimethylphthalate

Concen: 10.190 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.00 min

Lab File: BN002264.D

Acq: 09 Aug 2018 15:48

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 604955

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.3 7.8 11.8

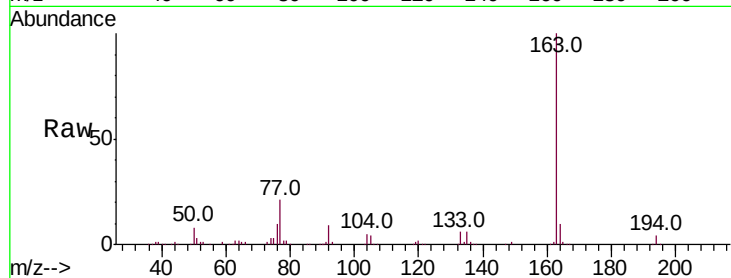

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

