

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
 Data File : BN002261.D
 Acq On : 09 Aug 2018 14:02
 Operator : JU/SJ
 Sample : J4301-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE3

Quant Time: Aug 10 01:06:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 10 01:04:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	279131	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1242802	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	681024	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1304912	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	937892	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	942574	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	21386	3.46	ng/uL	0.00
5) Phenol-d5	6.86	99	503526	19.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	339766	21.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	411724	19.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	406756	19.21	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	222852	21.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	235609	20.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	401251	19.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	75556	3.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1264513	21.90	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1615313	22.49	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	156005	14.15	ng/ul	0.00
57) Fluorene-d10	15.32	176	1060483	21.36	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	141258	16.62	ng/ul	0.00
70) Anthracene-d10	17.16	188	1444778	22.71	ng/ul	0.00
78) Pyrene-d10	19.46	212	1285781	26.37	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	1081042	21.24	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	672628	11.896	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
Data File : BN002261.D
Acq On : 09 Aug 2018 14:02
Operator : JU/SJ
Sample : J4301-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Time: Aug 10 01:06:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 10 01:04:23 2018
Response via : Initial Calibration

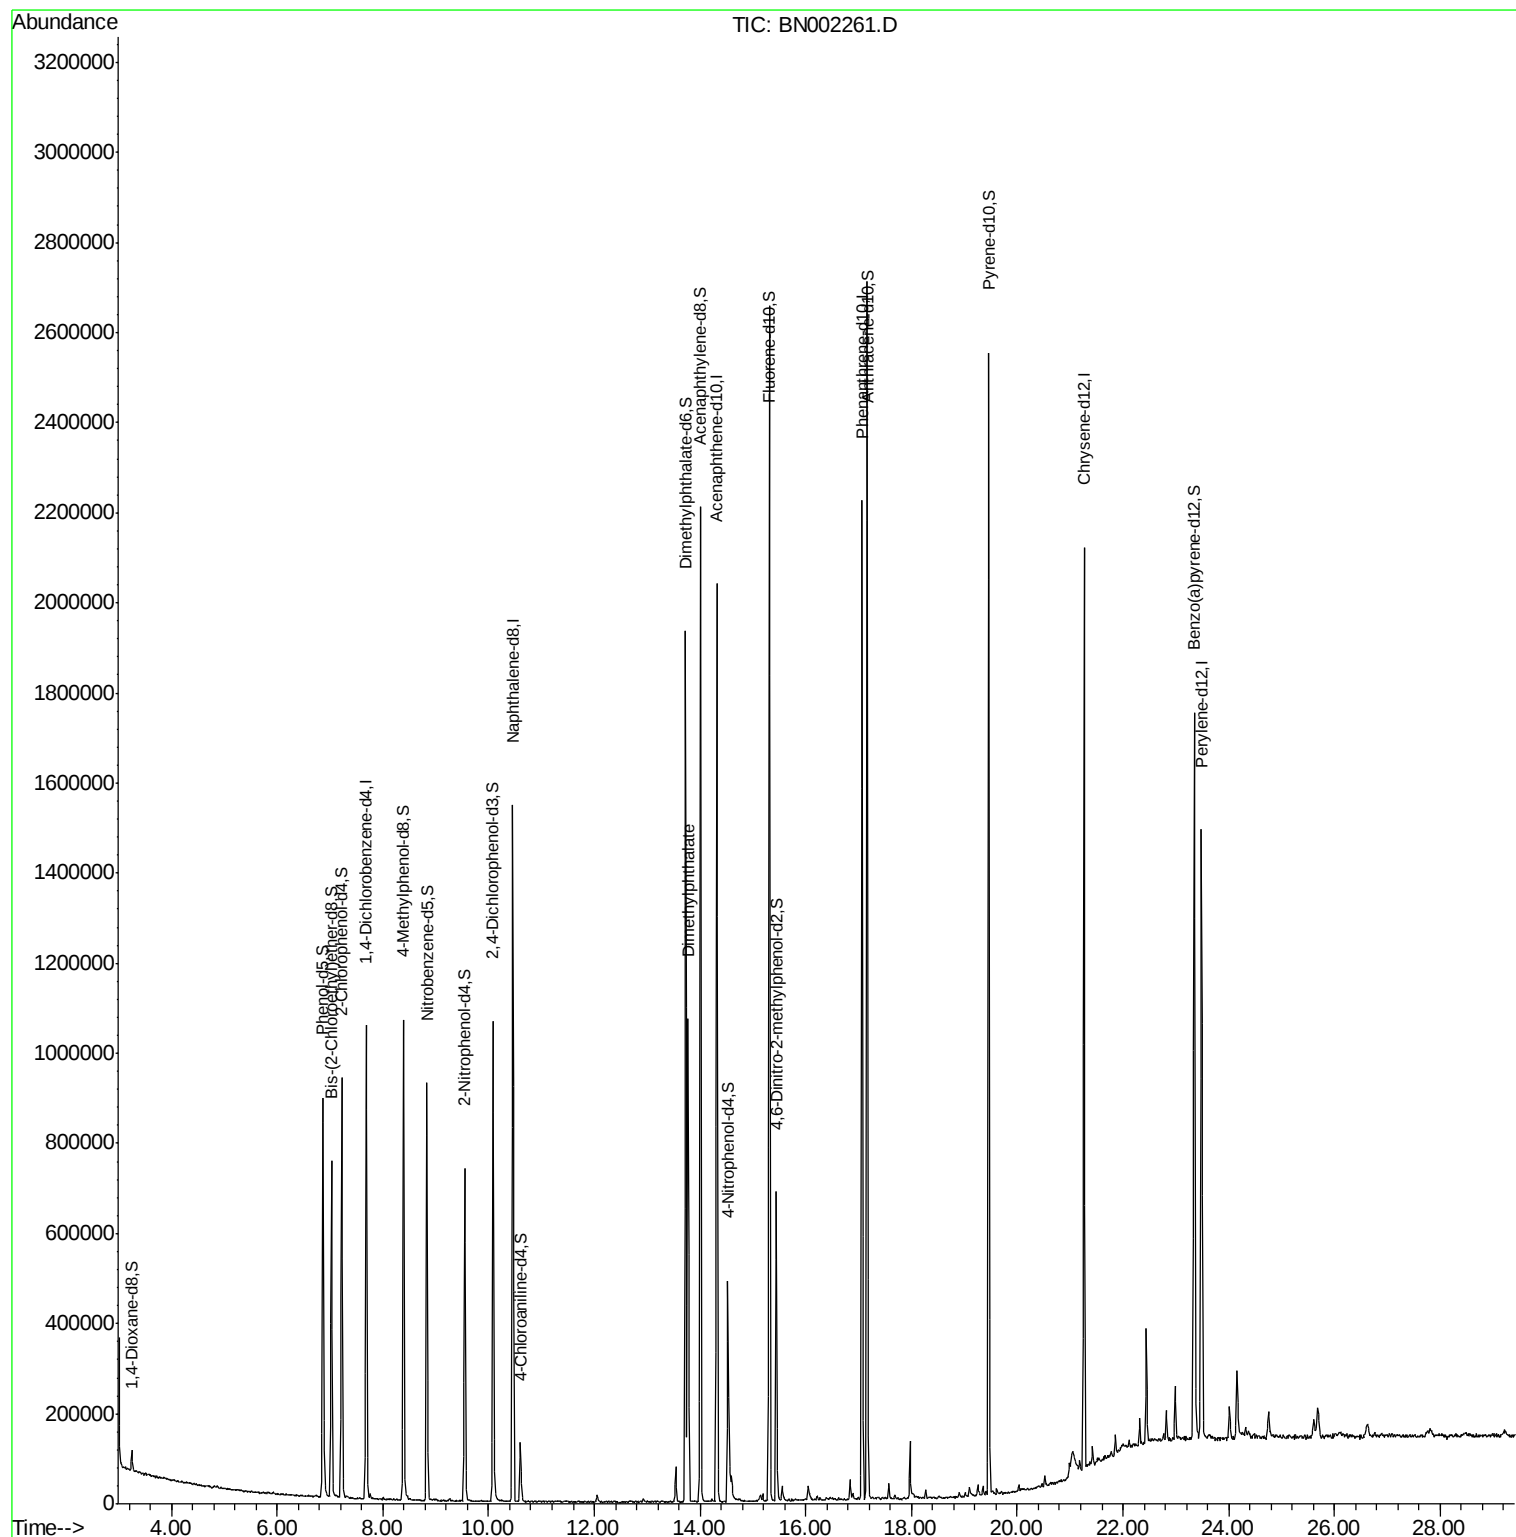

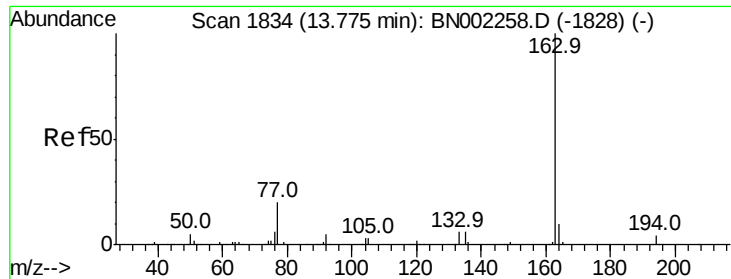

#44

Dimethylphthalate

Concen: 11.896 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. 0.00 min

Lab File: BN002261.D

Acq: 09 Aug 2018 14:02

Instrument :

BNA_N

ClientSampleId :

C0AE3



Tot Ion:163 Resp: 672628

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.3 7.8 11.8

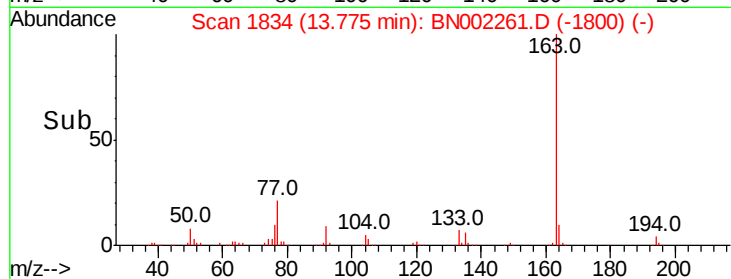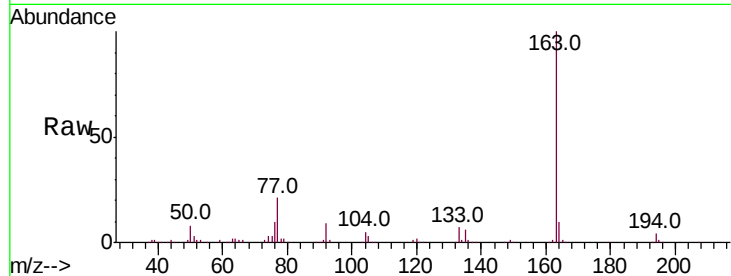

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

