

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
 Data File : BN002267.D
 Acq On : 09 Aug 2018 17:34
 Operator : JU/SJ
 Sample : J4301-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Manual Integrations
 APPROVED

Sohil
 8/10/2018 4:26:32 PM

Quant Time: Aug 10 02:08:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 10 02:01:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	308337	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1363529	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	751668	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1491136	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1068636	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1041561	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	15407	2.25	ng/uL	0.00
5) Phenol-d5	6.86	99	354971	12.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	236476	13.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	290342	12.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	296054	12.66	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	155298	13.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	165455	12.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	285886	12.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	335920	12.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	922907	14.48	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	1151761	14.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	115782m	9.51	ng/ul	0.00
57) Fluorene-d10	15.32	176	770255	14.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	99812	10.28	ng/ul	0.00
70) Anthracene-d10	17.16	188	1087095	14.95	ng/ul	0.00
78) Pyrene-d10	19.46	212	987196	17.77	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	790151	14.05	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	13.77	163	437502	7.010	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080918\
Data File : BN002267.D
Acq On : 09 Aug 2018 17:34
Operator : JU/SJ
Sample : J4301-08
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AE7

Quant Time: Aug 10 02:08:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 10 02:01:28 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/10/2018 4:26:32 PM

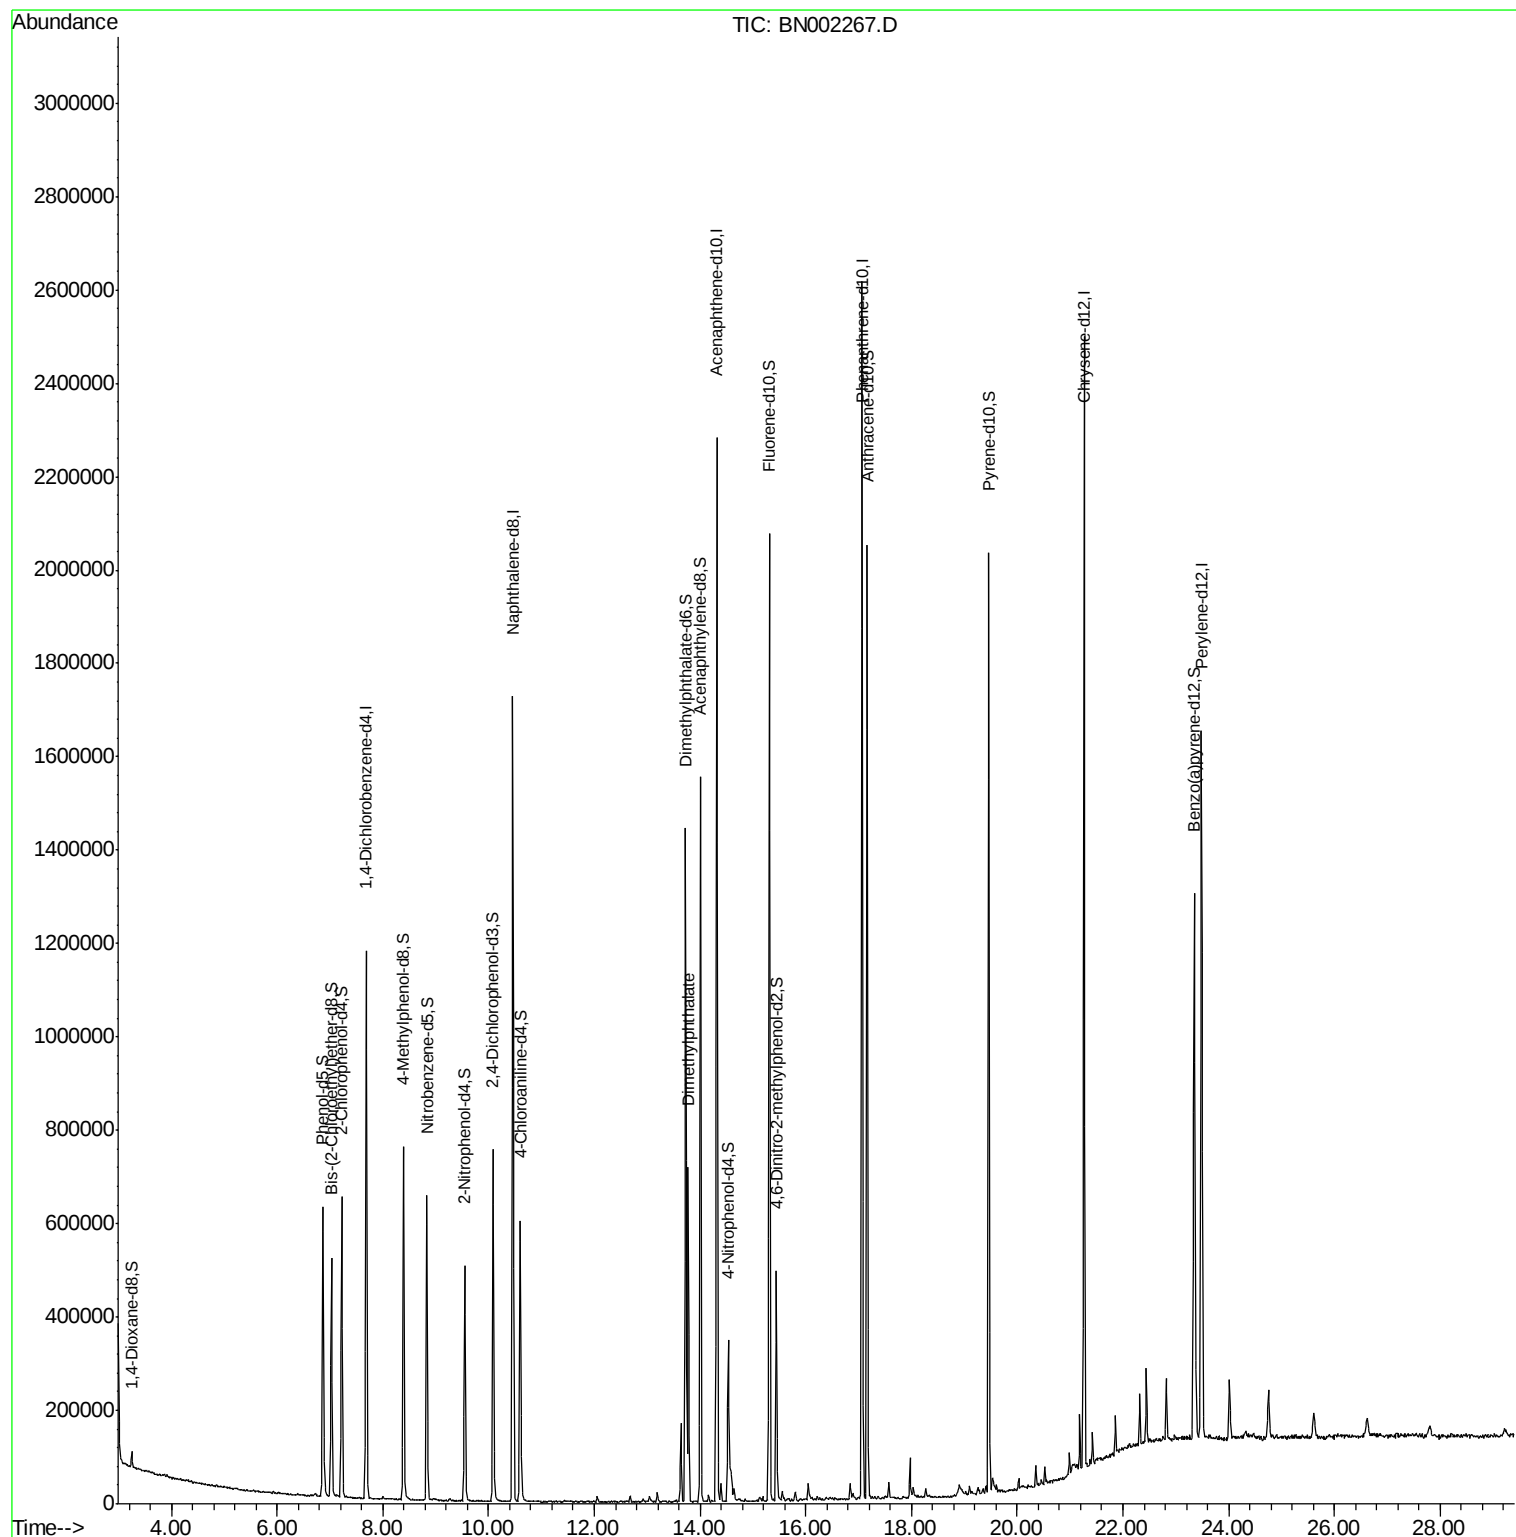

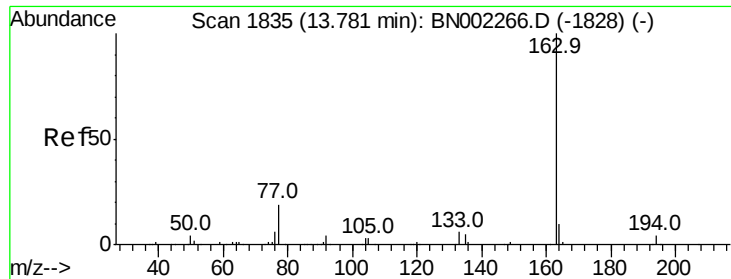

#44
 Dimethylphthalate
 Concen: 7.010 ng/ul
 RT: 13.77 min Scan# 1834
 Delta R.T. -0.01 min
 Lab File: BN002267.D
 Acq: 09 Aug 2018 17:34

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Tot Ion	Ratio	Resp	Lower	Upper
163	100	437502		
194	4.2		3.2	4.8
164	10.6		7.8	11.8

Manual Integrations
 APPROVED

Sohil
 8/10/2018 4:26:32 PM

