

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
Data File : BN002282.D
Acq On : 10 Aug 2018 09:36
Operator : JU/SJ
Sample : PB111761BL
Misc : for PCB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	41	rVB	847921	925094	28.17%	5.667%
2	7.681	791	798	805	rBV	1069666	1695792	51.64%	10.388%
3	10.452	1262	1269	1286	rBV	1395884	2376110	72.36%	14.556%
4	14.316	1919	1926	1935	rBV2	1936263	2989164	91.02%	18.312%
5	17.063	2386	2393	2404	rBV	2323639	3283897	100.00%	20.117%
6	21.263	3101	3107	3116	rBV	1958136	2689579	81.90%	16.476%
7	23.486	3477	3485	3492	rBV	1235014	2364221	71.99%	14.483%


Sum of corrected areas: 16323857

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080918\
Data File : BN002282.D
Acq On : 10 Aug 2018 09:36
Operator : JU/SJ
Sample : PB111761BL
Misc : for PCB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

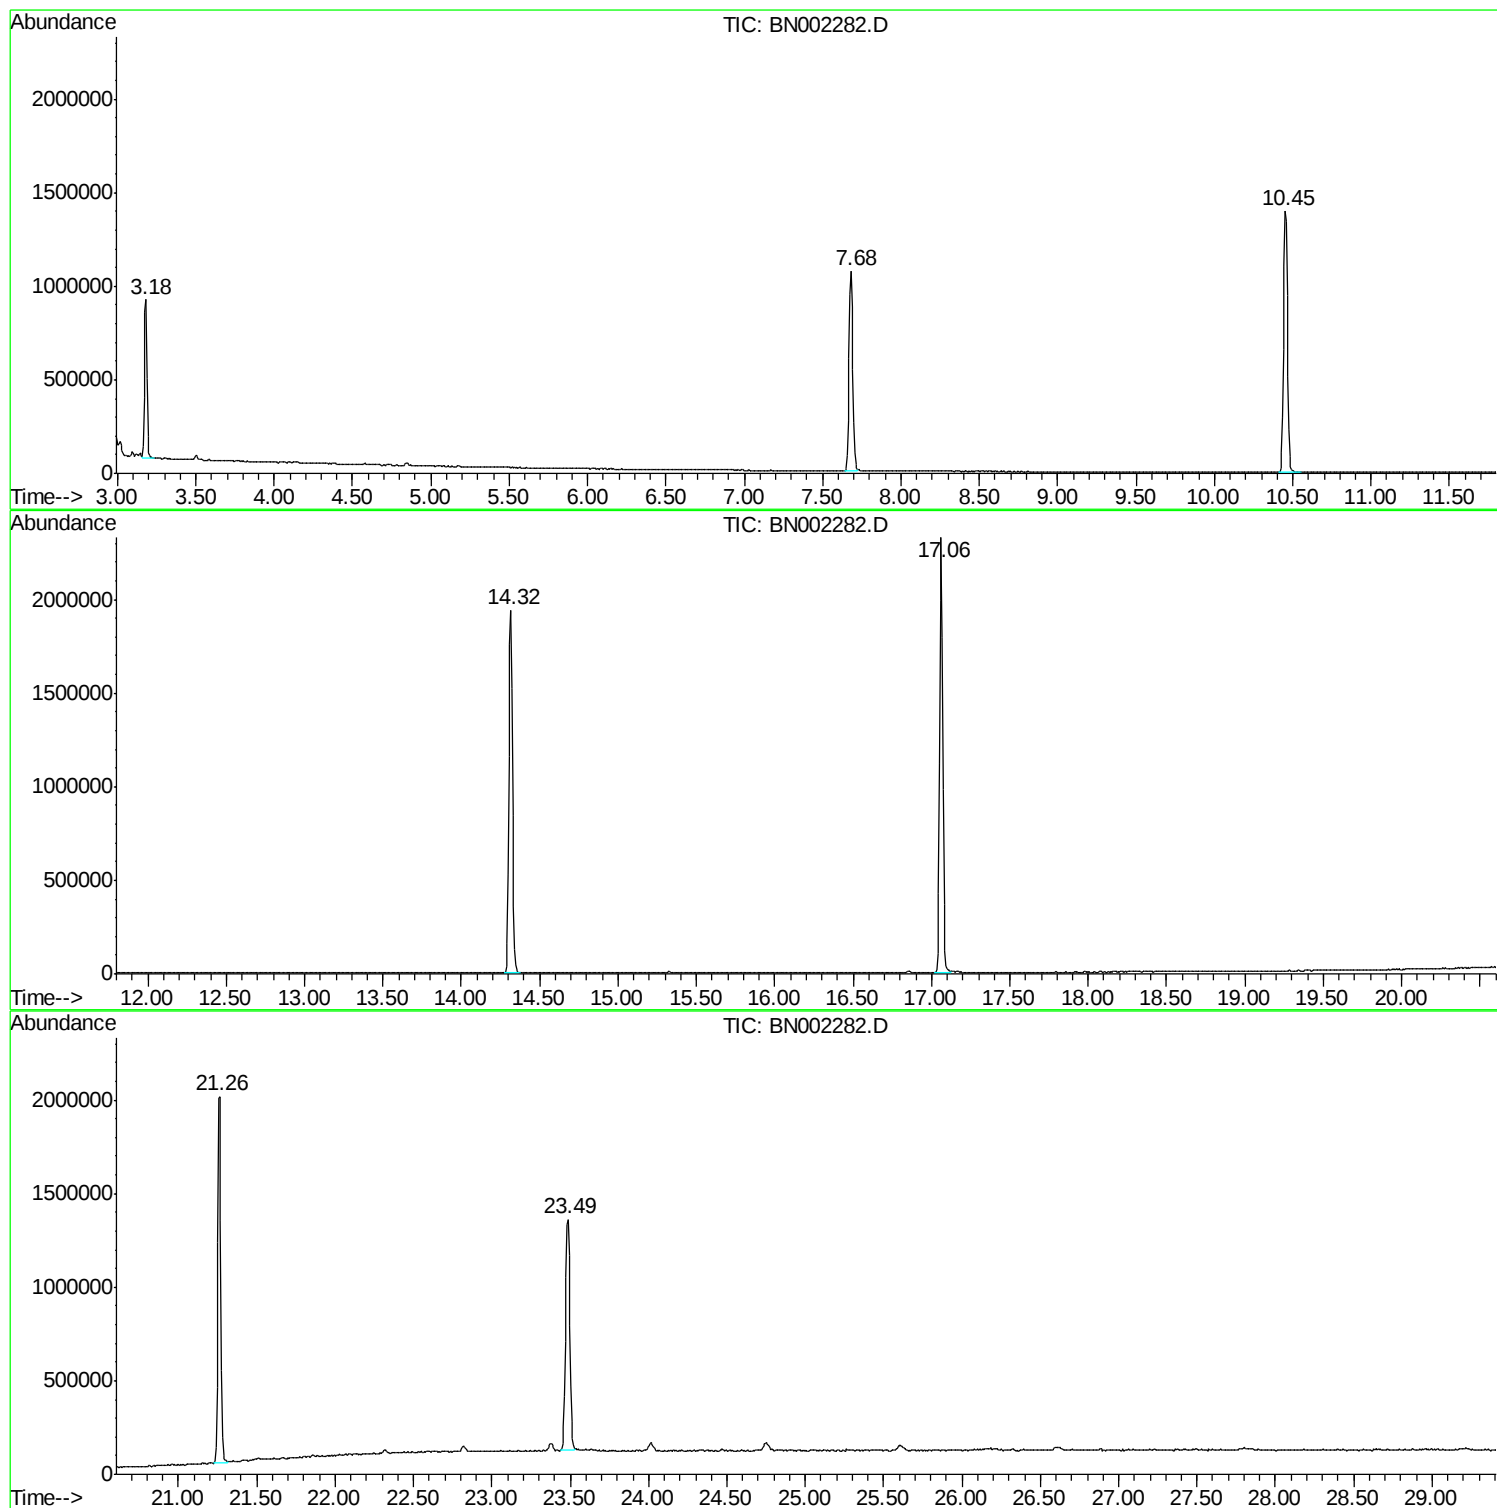

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN080918\
Data File : BN002282.D
Acq On : 10 Aug 2018 09:36
Operator : JU/SJ
Sample : PB111761BL
Misc : for PCB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK61










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.18	10.91 ng/ul	925094	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	94
2		Heptane	100	C7H16	000142-82-5	94
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	87
5		Oxalic acid, isobutyl pentyl ester	216	C11H20O4	1000309-37-0	59

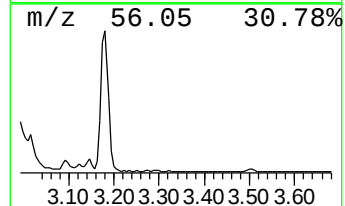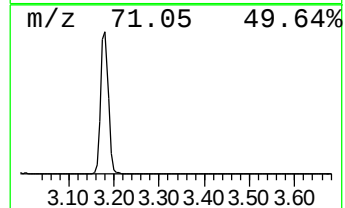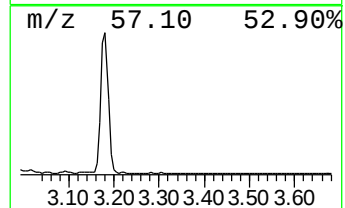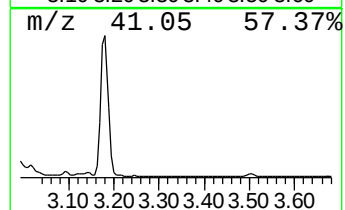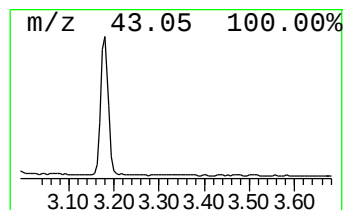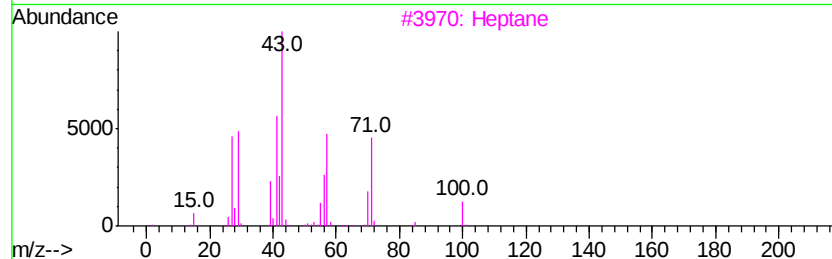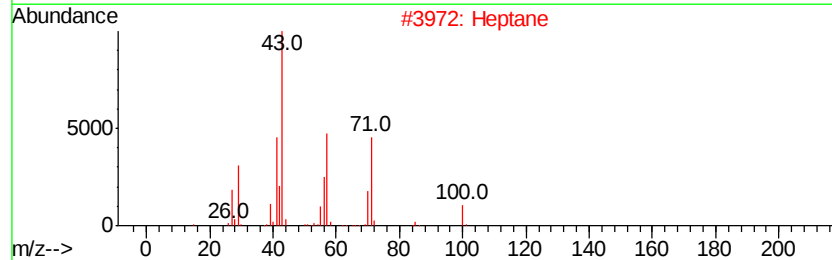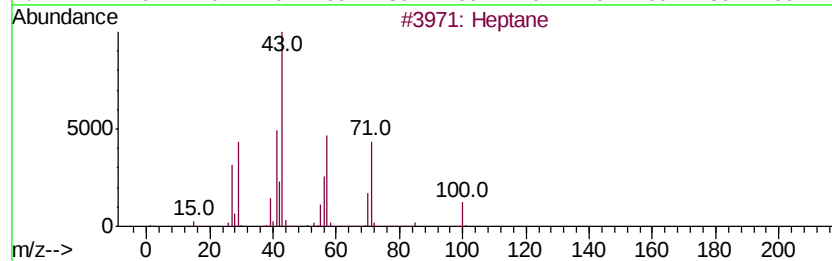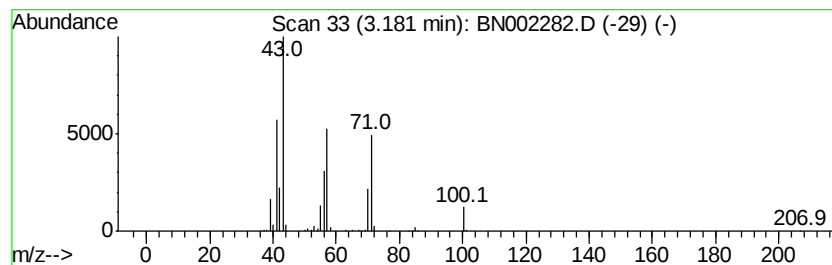

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN080918\
Data File : BN002282.D
Acq On : 10 Aug 2018 09:36
Operator : JU/SJ
Sample : PB111761BL
Misc : for PCB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.18	10.9	ng/ul	925094	1	7.68	1695790	20.0