

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
 Data File : BN015823.D
 Acq On : 09 Aug 2021 14:59
 Operator : CG/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Aug 09 17:25:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 16:46:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	8614	0.400	ng	0.00
7) Naphthalene-d8	10.724	136	41158	0.400	ng	0.00
13) Acenaphthene-d10	14.561	164	22987	0.400	ng	0.00
19) Phenanthrene-d10	17.310	188	45569	0.400	ng	0.00
29) Chrysene-d12	21.493	240	45961	0.400	ng	0.00
35) Perylene-d12	23.926	264	44069	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.485	112	2655	0.105	ng	0.00
5) Phenol-d6	7.080	99	3643	0.104	ng	0.00
8) Nitrobenzene-d5	9.076	82	3339	0.108	ng	0.00
11) 2-Methylnaphthalene-d10	12.314	152	6579	0.104	ng	0.00
14) 2,4,6-Tribromophenol	16.044	330	1028	0.086	ng	0.00
15) 2-Fluorobiphenyl	13.190	172	11173	0.130	ng	0.00
27) Fluoranthene-d10	19.336	212	13225	0.104	ng	0.00
31) Terphenyl-d14	19.937	244	15793	0.111	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.410	88	332	0.096	ng	89
3) n-Nitrosodimethylamine	3.788	42	775	0.095	ng	# 94
6) bis(2-Chloroethyl)ether	7.347	93	2629	0.106	ng	100
9) Naphthalene	10.774	128	11859	0.110	ng	98
10) Hexachlorobutadiene	11.066	225	2926	0.149	ng	# 97
12) 2-Methylnaphthalene	12.390	142	7922	0.108	ng	99
16) Acenaphthylene	14.282	152	9931	0.093	ng	100
17) Acenaphthene	14.624	154	6917	0.103	ng	98
18) Fluorene	15.601	166	8713	0.107	ng	99
20) 4,6-Dinitro-2-methylph...	15.690	198	222	0.062	ng	# 29
21) 4-Bromophenyl-phenylether	16.494	248	2615	0.107	ng	100
22) Hexachlorobenzene	16.616	284	3461	0.115	ng	# 87
23) Atrazine	16.762	200	2023	0.081	ng	98
24) Pentachlorophenol	16.957	266	1147	0.101	ng	97
25) Phenanthrene	17.346	178	14059	0.108	ng	99
26) Anthracene	17.431	178	12063	0.096	ng	99
28) Fluoranthene	19.371	202	16212	0.111	ng	100
30) Pyrene	19.728	202	16390	0.101	ng	100
32) Benzo(a)anthracene	21.482	228	15865	0.101	ng	99
33) Chrysene	21.536	228	16765	0.113	ng	100
34) Bis(2-ethylhexyl)phtha...	21.408	149	6963	0.060	ng	98
36) Indeno(1,2,3-cd)pyrene	26.442	276	15108	0.091	ng	# 96
37) Benzo(b)fluoranthene	23.183	252	16811	0.109	ng	# 92
38) Benzo(k)fluoranthene	23.231	252	15410	0.106	ng	# 93
39) Benzo(a)pyrene	23.817	252	14192	0.104	ng	# 90
40) Dibenzo(a,h)anthracene	26.466	278	11904	0.087	ng	# 82
41) Benzo(g,h,i)perylene	27.216	276	14120	0.098	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
Data File : BN015823.D
Acq On : 09 Aug 2021 14:59
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Aug 09 17:25:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 16:46:20 2021
Response via : Initial Calibration









1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.928 min Scan# 526
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion: 152 Resp: 8614




Ion	Ratio	Lower	Upper
152	100		
150	152.8	123.0	184.4
115	64.7	52.2	78.2




1,4-Dioxane
 Concen: 0.096 ng
 RT: 3.410 min Scan# 36
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59

Tgt Ion: 88 Resp: 332

Ion	Ratio	Lower	Upper
88	100		
43	40.4	27.4	41.2
58	90.1	64.3	96.5









n-Nitrosodimethylamine
Concen: 0.095 ng
RT: 3.788 min Scan# 77
Delta R.T. 0.019 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion: 42 Resp: 775




Ion	Ratio	Lower	Upper
42	100		
74	98.6	83.4	125.2
44	4.0	0.0	0.0#




2-Fluorophenol
Concen: 0.105 ng
RT: 5.485 min Scan# 261
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Tgt Ion: 112 Resp: 2655

Ion	Ratio	Lower	Upper
112	100		
64	69.5	53.4	80.0
63	36.9	28.6	43.0









Phenol-d6
 Concen: 0.104 ng
 RT: 7.080 min Scan# 434
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion:	99	Resp:	3643
Ion	Ratio	Lower	Upper
99	100		
42	24.6	19.0	28.4
71	38.5	31.2	46.8



bis(2-Chloroethyl)ether
 Concen: 0.106 ng
 RT: 7.347 min Scan# 463
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59

Tgt Ion:	93	Resp:	2629
Ion	Ratio	Lower	Upper
93	100		
63	80.4	64.3	96.5
95	32.9	25.6	38.4



Abundance Scan 758 (10.724 min): BN015825.D\data.ms (-752) (-)

Naphthalene-d8

Concen: 0.400 ng

RT: 10.724 min Scan# 758

Delta R.T. 0.000 min

Lab File: BN015823.D


Acq: 09 Aug 2021 14:59

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1



Tgt Ion: 136 Resp: 41158




Ion Ratio Lower Upper

136 100

137 11.2 8.8 13.2

54 8.8 7.1 10.7

68 5.9 4.9 7.3



Abundance Scan 628 (9.076 min): BN015825.D\data.ms (-625) (-)

Nitrobenzene-d5

Concen: 0.108 ng

RT: 9.076 min Scan# 628

Delta R.T. 0.000 min

Lab File: BN015823.D

Acq: 09 Aug 2021 14:59




Tgt Ion: 82 Resp: 3339


Ion Ratio Lower Upper

82 100

128 35.5 26.2 39.2

54 59.0 45.4 68.0









Naphthalene
 Concen: 0.110 ng
 RT: 10.774 min Scan# 762
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion:	128	Resp:	11859
Ion	Ratio	Lower	Upper
128	100		
129	11.8	8.9	13.3
127	14.1	10.8	16.2




Hexachlorobutadiene
 Concen: 0.149 ng
 RT: 11.066 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59

Tgt Ion:	225	Resp:	2926
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	62.8	51.8	77.8





Abundance Scan 1001 (12.314 min): BN015825.D\data.ms (-971) (-)




2-Methylnaphthalene-d10
Concen: 0.104 ng
RT: 12.314 min Scan# 1001
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 6579
Ion Ratio Lower Upper
152 100
151 20.6 16.4 24.6



Abundance Scan 1001 (12.314 min): BN015823.D\data.ms (-956) (-)





Abundance Scan 1018 (12.390 min): BN015825.D\data.ms (-1012) (-)




2-Methylnaphthalene
Concen: 0.108 ng
RT: 12.390 min Scan# 1018
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion:142 Resp: 7922
Ion Ratio Lower Upper
142 100
141 87.7 70.6 106.0
115 37.7 29.1 43.7



Abundance Scan 1018 (12.390 min): BN015823.D\data.ms (-995) (-)





Abundance Scan 1206 (14.561 min): BN015825.D\data.ms (-1190) (-)




Acenaphthene-d10
Concen: 0.400 ng
RT: 14.561 min Scan# 1206
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	164	Resp:	22987
Ion	Ratio	Lower	Upper
164	100		
162	101.0	81.2	121.8
160	43.6	35.0	52.4



Abundance Scan 1206 (14.561 min): BN015823.D\data.ms (-1190) (-)





Abundance Scan 1323 (16.044 min): BN015825.D\data.ms (-1315) (-)




2,4,6-Tribromophenol
Concen: 0.086 ng
RT: 16.044 min Scan# 1323
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion:	330	Resp:	1028
Ion	Ratio	Lower	Upper
330	100		
332	133.2	86.2	129.2#
141	32.3	25.0	37.6



Abundance Scan 1323 (16.044 min): BN015823.D\data.ms (-1315) (-)






Abundance Scan 1098 (13.190 min): BN015825.D\data.ms (-1098) (-)




2-Fluorobiphenyl
Concen: 0.130 ng
RT: 13.190 min Scan# 1098
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:	172	Resp:	11173
Ion	Ratio	Lower	Upper
172	100		
171	35.2	26.9	40.3
170	22.3	17.3	25.9






Abundance Scan 1184 (14.281 min): BN015825.D\data.ms (-1184) (-)



Acenaphthylene
Concen: 0.093 ng
RT: 14.282 min Scan# 1184
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion:	152	Resp:	9931
Ion	Ratio	Lower	Upper
152	100		
151	19.7	15.6	23.4
153	13.1	10.5	15.7





Abundance Scan 1211 (14.624 min): BN015825.D\data.ms (-1205) (-)

Acenaphthene
Concen: 0.103 ng
RT: 14.624 min Scan# 1211
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1



Tgt Ion:	154	Resp:	6917
Ion	Ratio	Lower	Upper
154	100		
153	114.9	90.1	135.1
152	55.1	42.7	64.1




Abundance Scan 1211 (14.624 min): BN015823.D\data.ms (-1203) (-)





Abundance Scan 1288 (15.601 min): BN015825.D\data.ms (-1214) (-)


Fluorene
Concen: 0.107 ng
RT: 15.601 min Scan# 1288
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59




Tgt Ion:	166	Resp:	8713
Ion	Ratio	Lower	Upper
166	100		
165	97.8	78.8	118.2
167	14.0	10.9	16.3



Abundance Scan 1288 (15.601 min): BN015823.D\data.ms (-1272) (-)






Abundance Scan 1427 (17.310 min): BN015825.D\data.ms (-1411) (-)




Phenanthrene-d10
Concen: 0.400 ng
RT: 17.310 min Scan# 1427
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:	188	Resp:	45569
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	5.9	4.7	7.1






Abundance Scan 1294 (15.677 min): BN015825.D\data.ms (-1220) (-)



4,6-Dinitro-2-methylphenol
Concen: 0.062 ng
RT: 15.690 min Scan# 1295
Delta R.T. 0.013 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion:	198	Resp:	222
Ion	Ratio	Lower	Upper
198	100		
182	42.0	10.8	16.2#
77	0.0	0.0	0.0





Abundance Scan 1360 (16.494 min): BN015825.D\data.ms (-1352) (-)

4-Bromophenyl-phenylether
Concen: 0.107 ng
RT: 16.494 min Scan# 1360
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1



Tgt Ion	Ratio	Lower	Upper
248	100		
250	92.8	74.8	112.2
141	75.4	60.5	90.7






Abundance Scan 1360 (16.494 min): BN015823.D\data.ms (-1352) (-)




Abundance Scan 1370 (16.616 min): BN015825.D\data.ms (-1362) (-)

Hexachlorobenzene
Concen: 0.115 ng
RT: 16.616 min Scan# 1370
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Tgt Ion	Ratio	Lower	Upper
284	100		
142	43.0	23.0	34.4#
249	31.8	25.3	37.9




Abundance Scan 1370 (16.616 min): BN015823.D\data.ms (-1362) (-)





Abundance Scan 1382 (16.762 min): BN015825.D\data.ms (-1323) (-)

Atrazine
Concen: 0.081 ng
RT: 16.762 min Scan# 1382
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1



Tgt Ion	Ratio	Lower	Upper
200	100		
173	25.4	19.4	29.2
215	50.3	39.4	59.2






Abundance Scan 1382 (16.762 min): BN015823.D\data.ms (-1341) (-)




Abundance Scan 1398 (16.957 min): BN015825.D\data.ms (-1324) (-)

Pentachlorophenol
Concen: 0.101 ng
RT: 16.957 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion	Ratio	Lower	Upper
266	100		
264	64.9	51.0	76.6
268	67.9	51.8	77.6



Abundance Scan 1398 (16.957 min): BN015823.D\data.ms (-1390) (-)






Abundance Scan 1430 (17.346 min): BN015825.D\data.ms (-1425) (-)




Phenanthrene
Concen: 0.108 ng
RT: 17.346 min Scan# 1430
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:	178	Resp:	14059
Ion Ratio	Lower	Upper	
178	100		
176	18.7	14.6	22.0
179	16.0	12.7	19.1






Abundance Scan 1437 (17.431 min): BN015825.D\data.ms (-1426) (-)




Anthracene
Concen: 0.096 ng
RT: 17.431 min Scan# 1437
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Tgt Ion:	178	Resp:	12063
Ion Ratio	Lower	Upper	
178	100		
176	18.3	14.3	21.5
179	15.3	12.3	18.5





Abundance Scan 1752 (19.341 min): BN015825.D\data.ms (-1732) (-)




Fluoranthene-d10
Concen: 0.104 ng
RT: 19.336 min Scan# 1751
Delta R.T. -0.005 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	212	Resp:	13225
Ion Ratio	Lower	Upper	
212	100		
106	10.0	7.8	11.8
104	6.0	4.6	6.8



Abundance Scan 1751 (19.336 min): BN015823.D\data.ms (-1732) (-)





Abundance Scan 1758 (19.371 min): BN015825.D\data.ms (-1732) (-)




Fluoranthene
Concen: 0.111 ng
RT: 19.371 min Scan# 1758
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Tgt Ion:	202	Resp:	16212
Ion Ratio	Lower	Upper	
202	100		
101	9.0	7.0	10.6
203	17.2	13.8	20.8




Abundance Scan 1758 (19.371 min): BN015823.D\data.ms (-1718) (-)






Abundance Scan 2026 (21.493 min): BN015825.D\data.ms (-2029) (-)

Chrysene-d12
Concen: 0.400 ng
RT: 21.493 min Scan# 2026
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1




Tgt Ion	Ratio	Lower	Upper
240	100		
120	8.8	7.8	11.8
236	26.3	21.1	31.7






Abundance Scan 1831 (19.733 min): BN015825.D\data.ms (-1830) (-)

Pyrene
Concen: 0.101 ng
RT: 19.728 min Scan# 1830
Delta R.T. -0.005 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59




Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.2	16.2	24.2
203	17.9	14.1	21.1






Abundance Scan 1872 (19.937 min): BN015825.D\data.ms (-1842) (-)

Terphenyl-d14
Concen: 0.111 ng
RT: 19.937 min Scan# 1872
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1







Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.0	6.1	9.1
122	9.1	7.0	10.4




Abundance Scan 2025 (21.482 min): BN015825.D\data.ms (-2006) (-)

Benzo(a)anthracene
Concen: 0.101 ng
RT: 21.482 min Scan# 2025
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.5	20.6	31.0
229	20.4	15.8	23.6








Chrysene
 Concen: 0.113 ng
 RT: 21.536 min Scan# 2030
 Delta R.T. 0.000 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1





Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.4	22.7	34.1
229	20.1	15.8	23.8



Bis(2-ethylhexyl)phthalate
 Concen: 0.060 ng
 RT: 21.408 min Scan# 2018
 Delta R.T. -0.010 min
 Lab File: BN015823.D
 Acq: 09 Aug 2021 14:59




Tgt Ion	Ratio	Lower	Upper
149	100		
167	27.4	22.7	34.1
279	5.0	4.2	6.4





Abundance Scan 2556 (23.926 min): BN015825.D\data.ms (-2535) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.926 min Scan# 2556
Delta R.T. 0.000 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

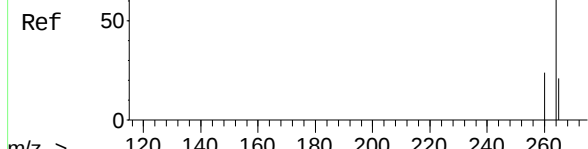

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.6	29.4
265	27.6	21.7	32.5






Abundance Scan 2556 (23.926 min): BN015823.D\data.ms (-2512) (-)




Abundance Scan 3292 (26.445 min): BN015825.D\data.ms (-3236) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.091 ng
RT: 26.442 min Scan# 3291
Delta R.T. -0.003 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59


Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.5	14.5	21.7#
277	25.4	20.2	30.4



Abundance Scan 3291 (26.442 min): BN015823.D\data.ms (-3263) (-)





Abundance Scan 2340 (23.187 min): BN015825.D\data.ms (-2340) (-)




Benzo(b)fluoranthene
Concen: 0.109 ng
RT: 23.183 min Scan# 2339
Delta R.T. -0.003 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion	Ratio	Lower	Upper
252	100		
253	26.1	18.2	27.2
125	11.3	6.3	9.5#



Abundance Scan 2339 (23.183 min): BN015823.D\data.ms (-2282) (-)





Abundance Scan 2354 (23.235 min): BN015825.D\data.ms (-2348) (-)




Benzo(k)fluoranthene
Concen: 0.106 ng
RT: 23.231 min Scan# 2353
Delta R.T. -0.003 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.9	18.1	27.1
125	10.7	6.2	9.4#




Abundance Scan 2353 (23.231 min): BN015823.D\data.ms (-2339) (-)






Abundance Scan 2525 (23.820 min): BN015825.D\data.ms (-2509) (-)

Benzo(a)pyrene
Concen: 0.104 ng
RT: 23.817 min Scan# 2524
Delta R.T. -0.003 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1




Tgt Ion	Ratio	Lower	Upper
252	100		
253	27.3	18.5	27.7
125	13.4	7.0	10.6#






Abundance Scan 3297 (26.462 min): BN015825.D\data.ms (-3274) (-)


Dibenzo(a,h)anthracene
Concen: 0.087 ng
RT: 26.466 min Scan# 3298
Delta R.T. 0.004 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59



Tgt Ion	Ratio	Lower	Upper
278	100		
139	28.3	10.5	15.7#
279	28.0	19.5	29.3



Abundance Scan 3516 (27.212 min): BN015825.D\data.ms (-3454) (-)





Benzo(g,h,i)perylene
Concen: 0.098 ng
RT: 27.216 min Scan# 3517
Delta R.T. 0.004 min
Lab File: BN015823.D
Acq: 09 Aug 2021 14:59

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:276 Resp: 14120
Ion Ratio Lower Upper

276	100		
277	25.3	19.0	28.6
138	17.8	12.2	18.4



Abundance Scan 3517 (27.216 min): BN015823.D\data.ms (-3458) (-)

