
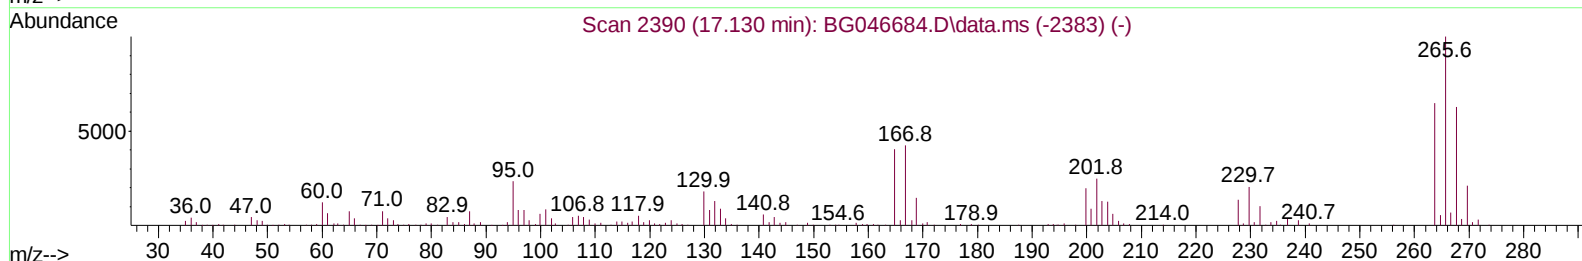
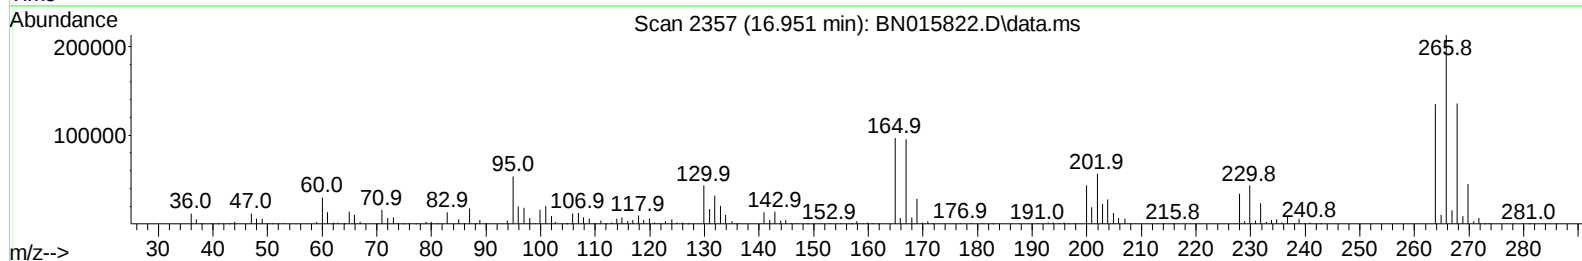


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
Data File : BN015822.D
Acq On : 09 Aug 2021 14:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 15:33:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 15:33:12 2021
Response via : Initial Calibration

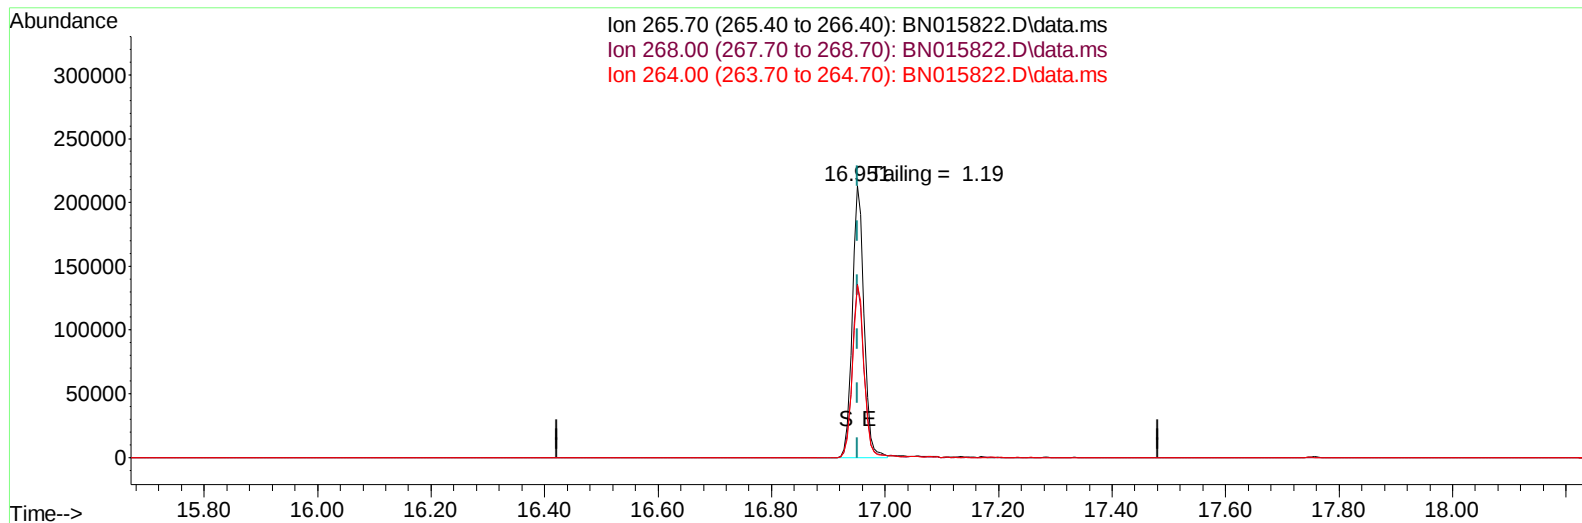




TIC: BN015822.D\data.ms

(70) Pentachlorophenol (C)**16.951min (0.000) 22108.50 ng****response 311436**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.72
264.00	61.60	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
Data File : BN015822.D
Acq On : 09 Aug 2021 14:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 15:33:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 15:33:12 2021
Response via : Initial Calibration

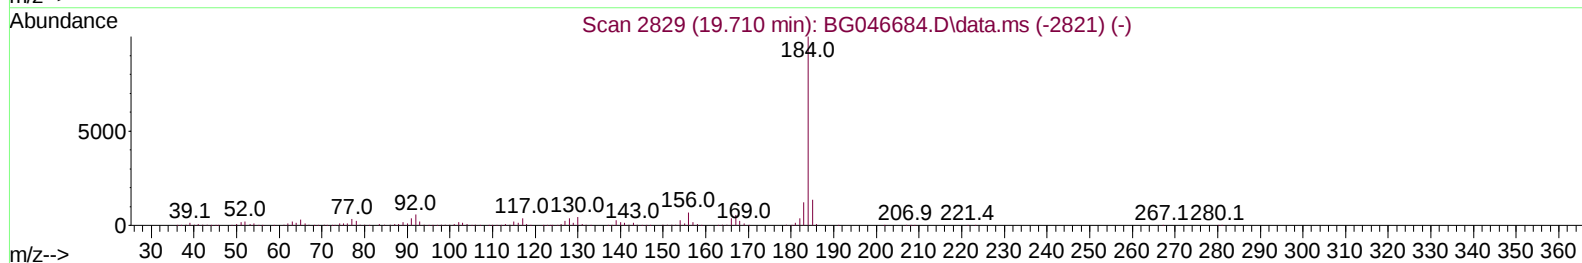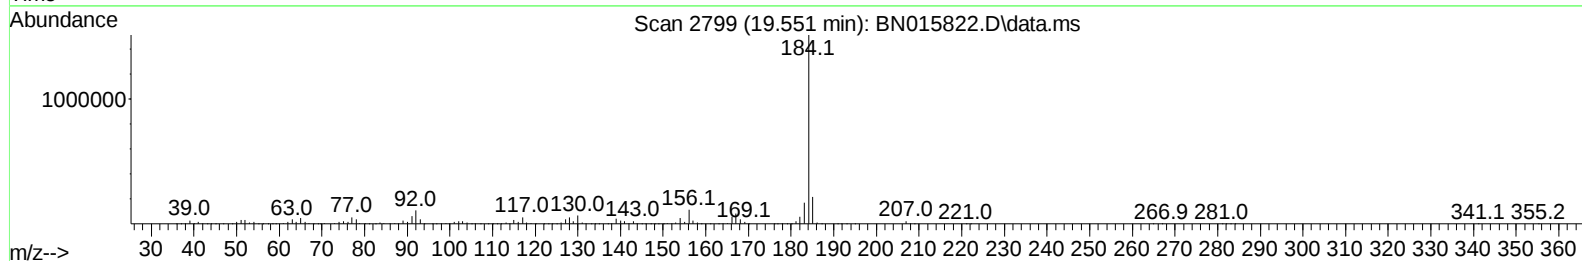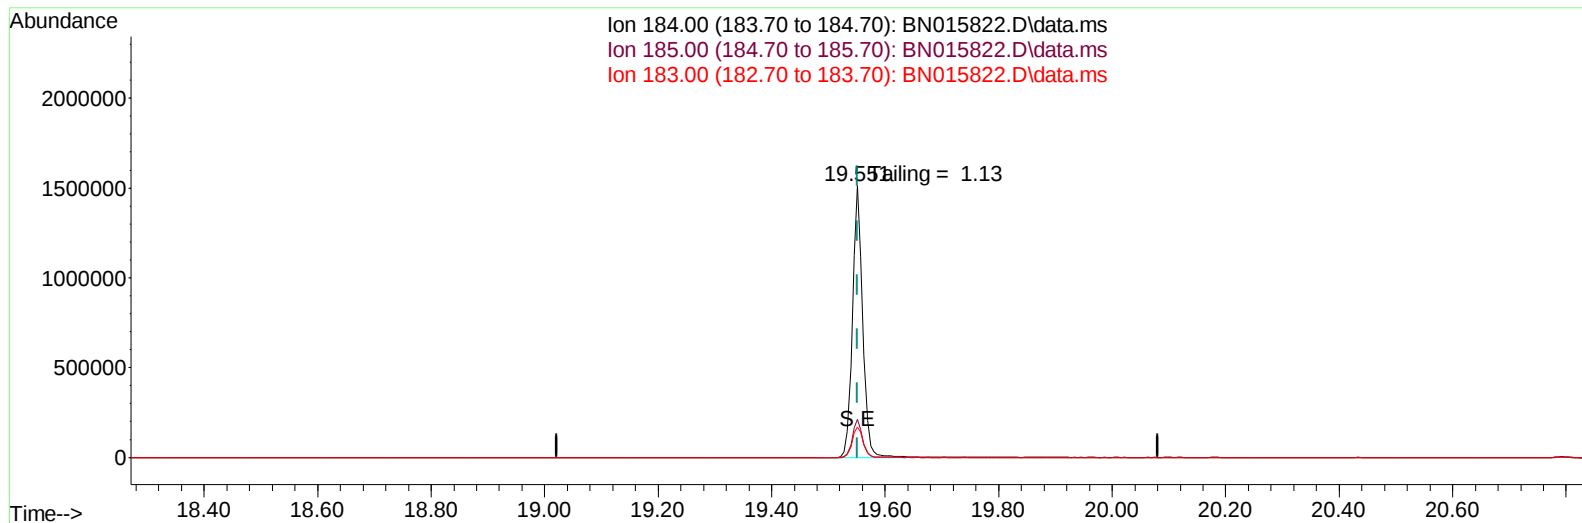

TIC: BN015822.D\data.ms

(77) Benzidine**19.551min (0.000) 0.00 ng****response 1914341**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.24
0.00	0.00	0.00