
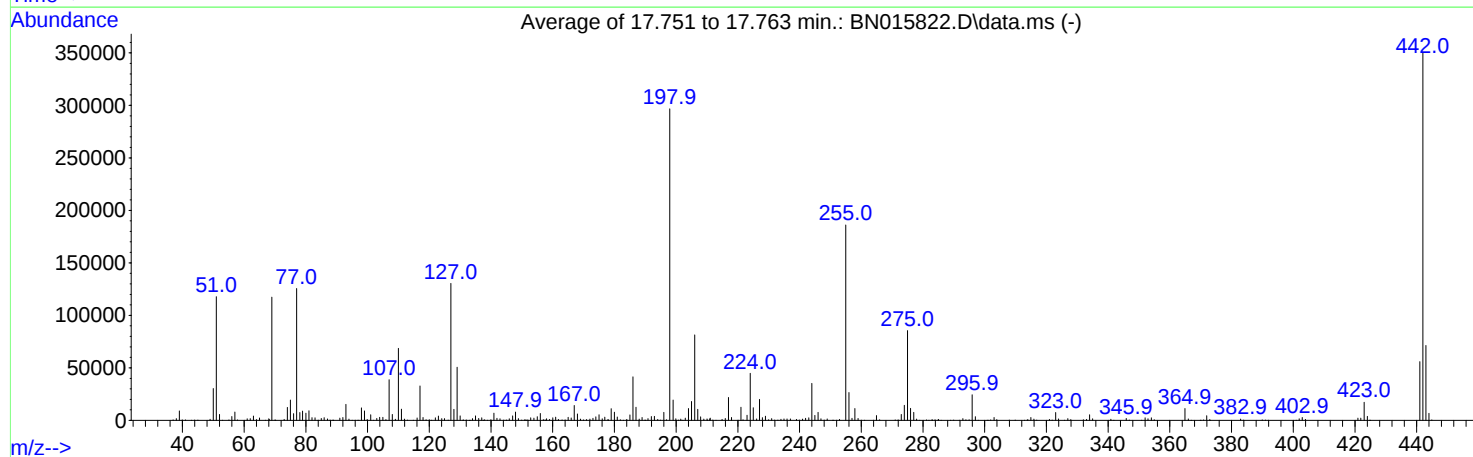


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
 Data File : BN015822.D
 Acq On : 09 Aug 2021 14:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 09 19:13:08 2021

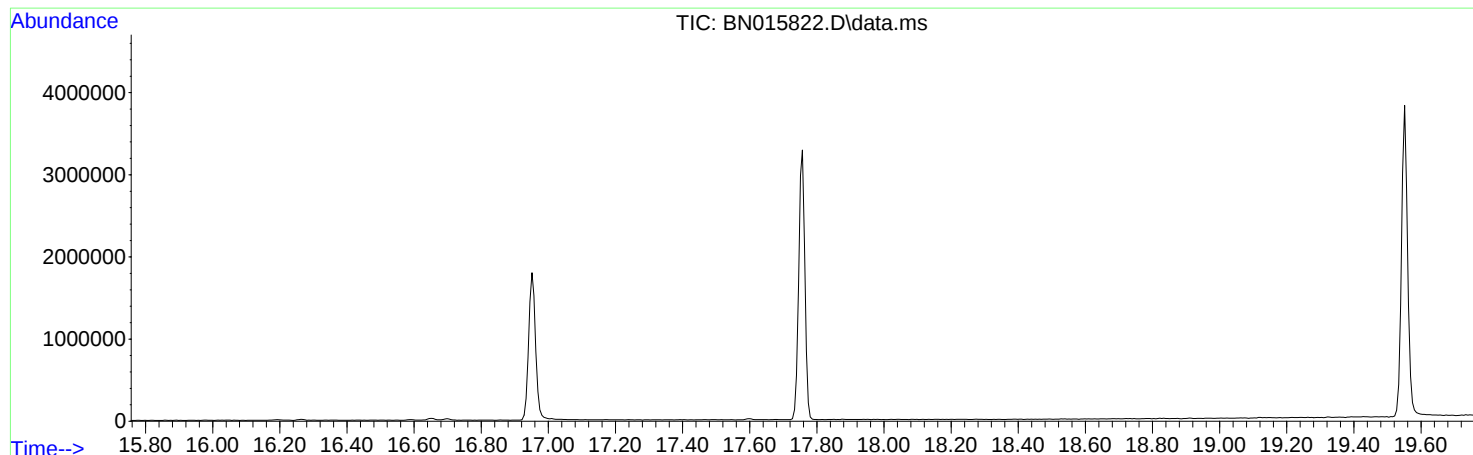




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	117880	PASS
68	69	0.00	2	1.3	1546	PASS
69	198	0.00	100	39.6	117365	PASS
70	69	0.00	2	0.4	421	PASS
127	198	10	80	44.0	130408	PASS
197	198	0.00	2	0.2	676	PASS
198	198	100	100	100.0	296661	PASS
199	198	5	9	6.5	19345	PASS
275	198	10	60	28.8	85437	PASS
365	198	1	100	3.8	11291	PASS
441	198	0.01	100	18.9	55949	PASS
442	442	50	100	100.0	350357	PASS
443	442	15	24	20.4	71333	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
Data File : BN015822.D
Acq On : 09 Aug 2021 14:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 15:33:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 15:33:12 2021
Response via : Initial Calibration

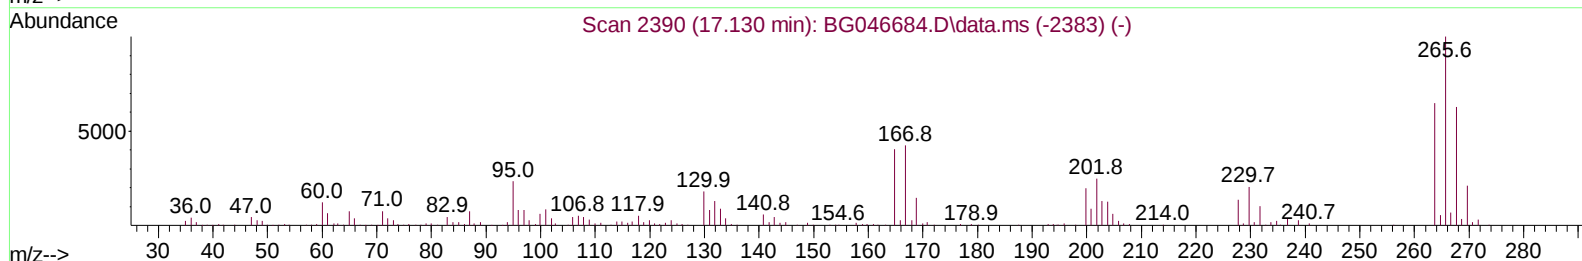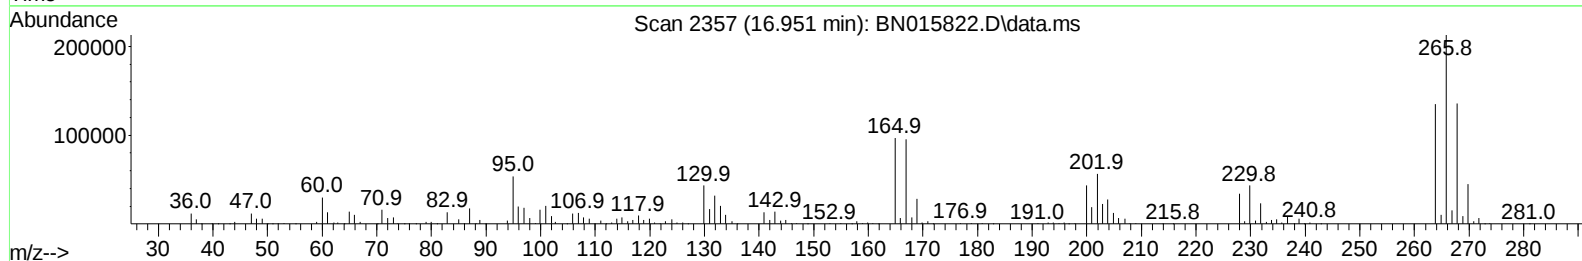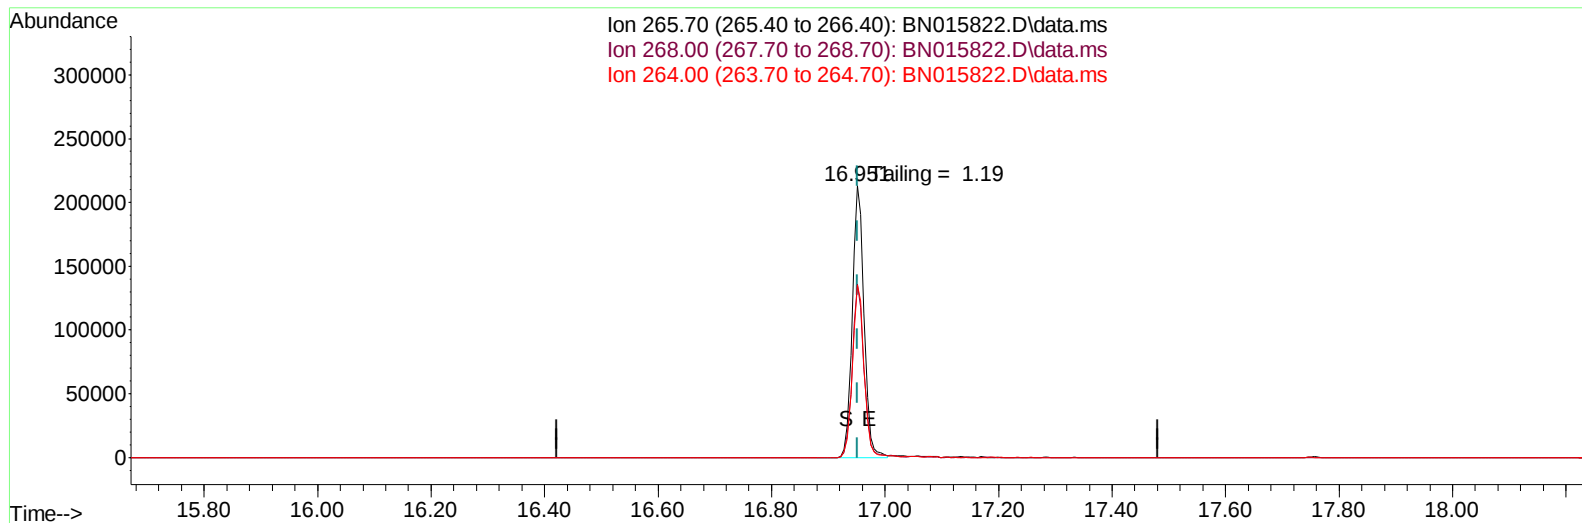

TIC: BN015822.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 22108.50 ng




response 311436

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.72
264.00	61.60	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080921\
Data File : BN015822.D
Acq On : 09 Aug 2021 14:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 15:33:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 15:33:12 2021
Response via : Initial Calibration

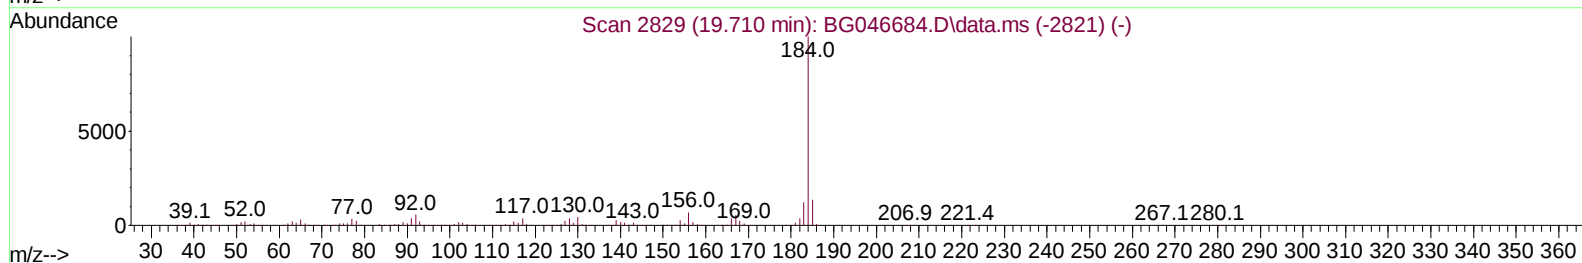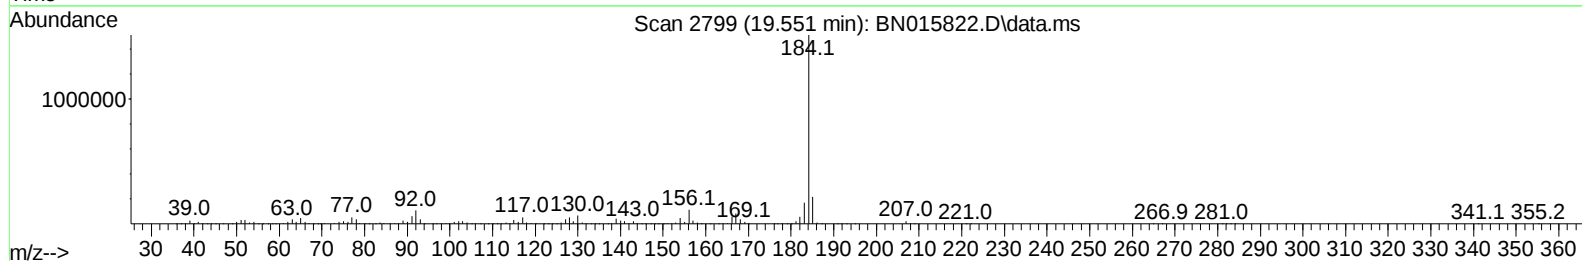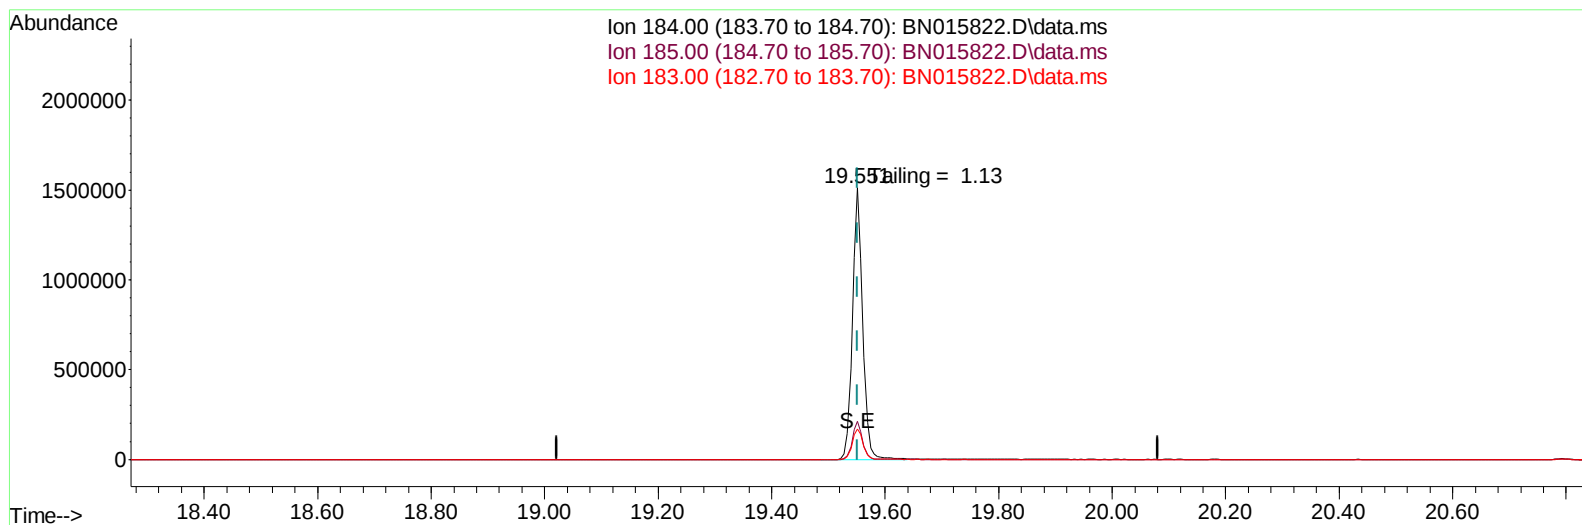

TIC: BN015822.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 1914341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2021	BNA_N	<u>BN015822.D</u>
Compound Name	Response	Retention Time
DDT	980002	20.792
DDD	3652	20.35
DDE	1101	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4753	984755	0.48

Instrument :
BNA_N
ClientSampleId :
DFTPP