
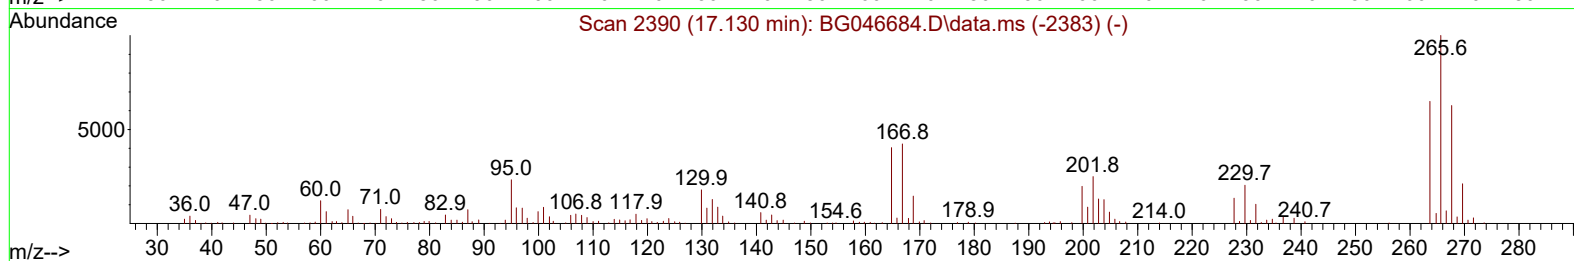
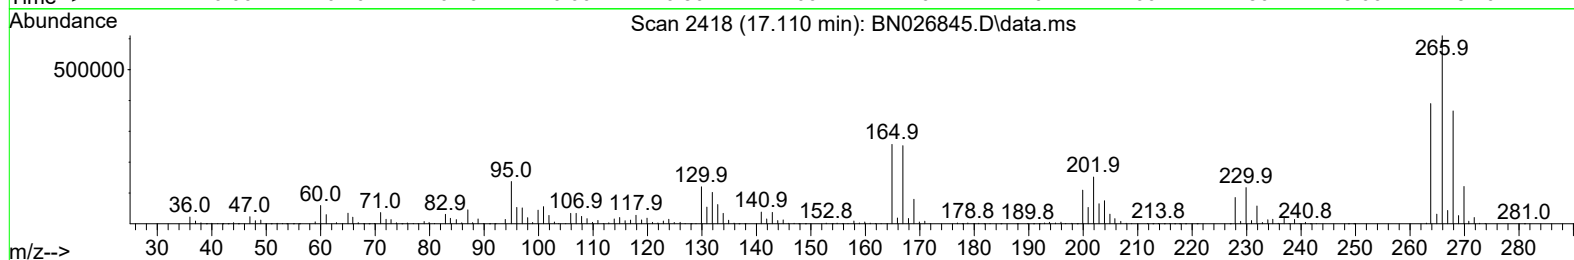


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080923\
Data File : BN026845.D
Acq On : 08 Aug 2023 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 02:05:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 02:05:22 2023
Response via : Initial Calibration

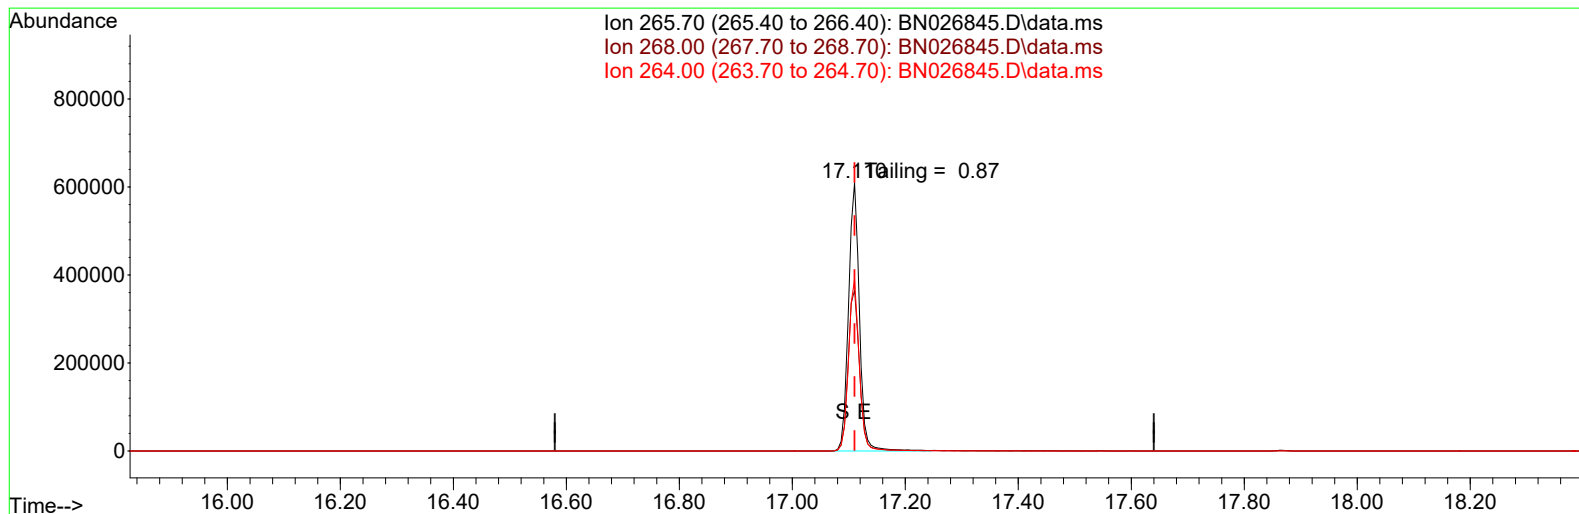

TIC: BN026845.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 24969.01 ng

response 823384

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.99
264.00	61.60	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080923\
Data File : BN026845.D
Acq On : 08 Aug 2023 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 02:05:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 02:05:22 2023
Response via : Initial Calibration

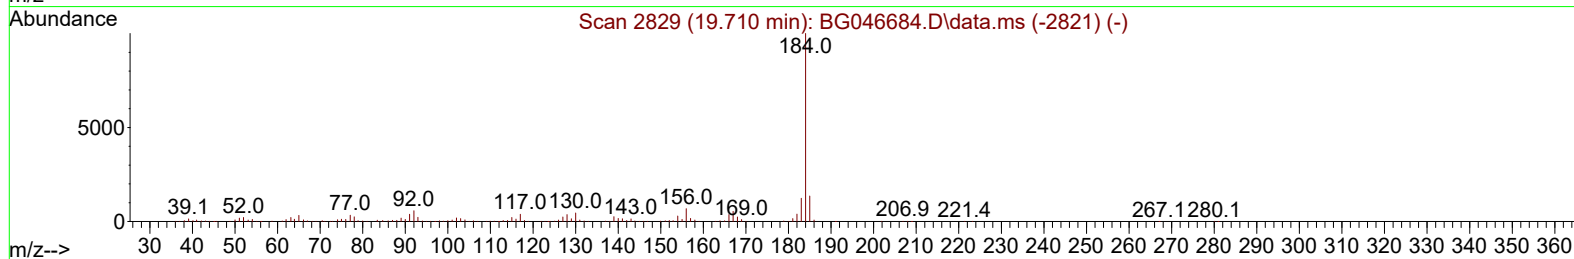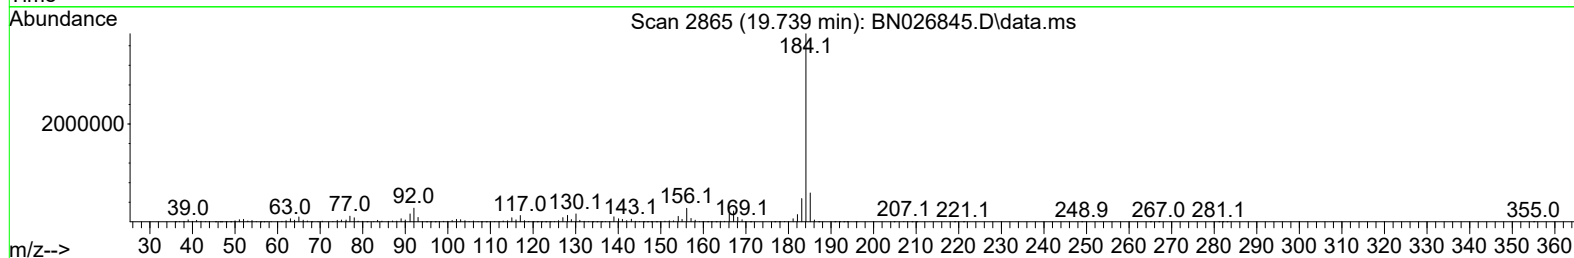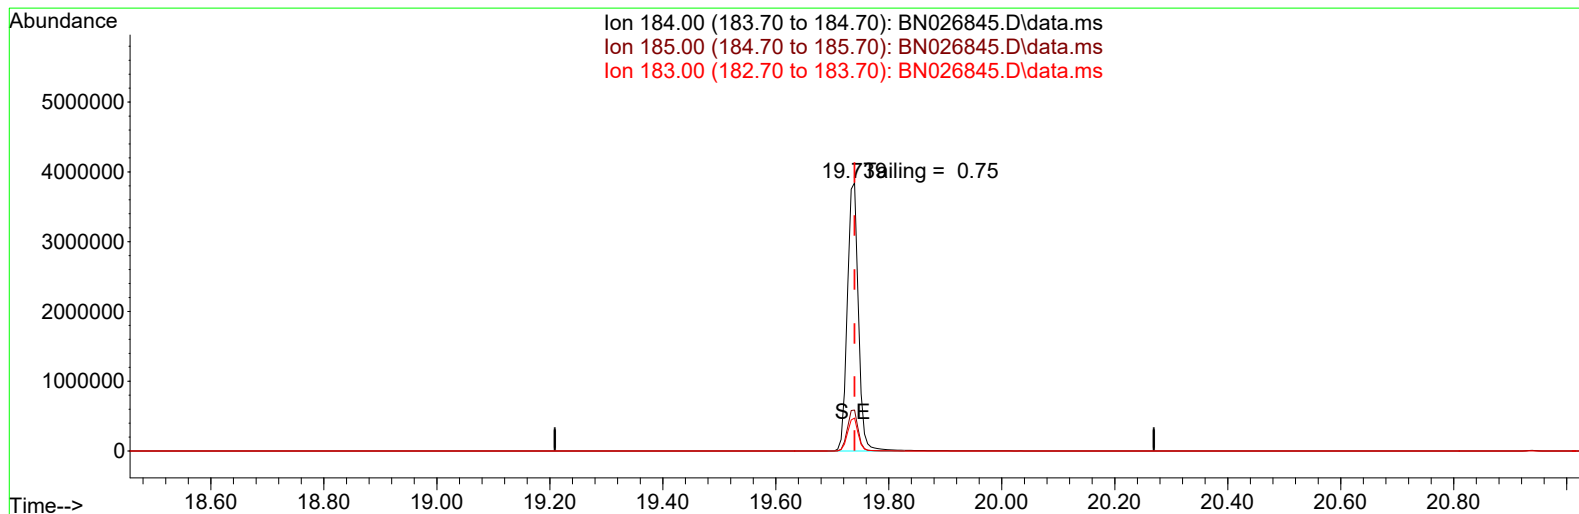

TIC: BN026845.D\data.ms

(77) Benzidine

19.739min (0.000) 0.00 ng

response 5263696

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.29
183.00	13.20	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2023	BNA_N	<u>BN026845.D</u>
Compound Name	Response	Retention Time
DDT	2348027	20.939
DDD	24219	20.545
DDE	590	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24809	2372836	1.05