
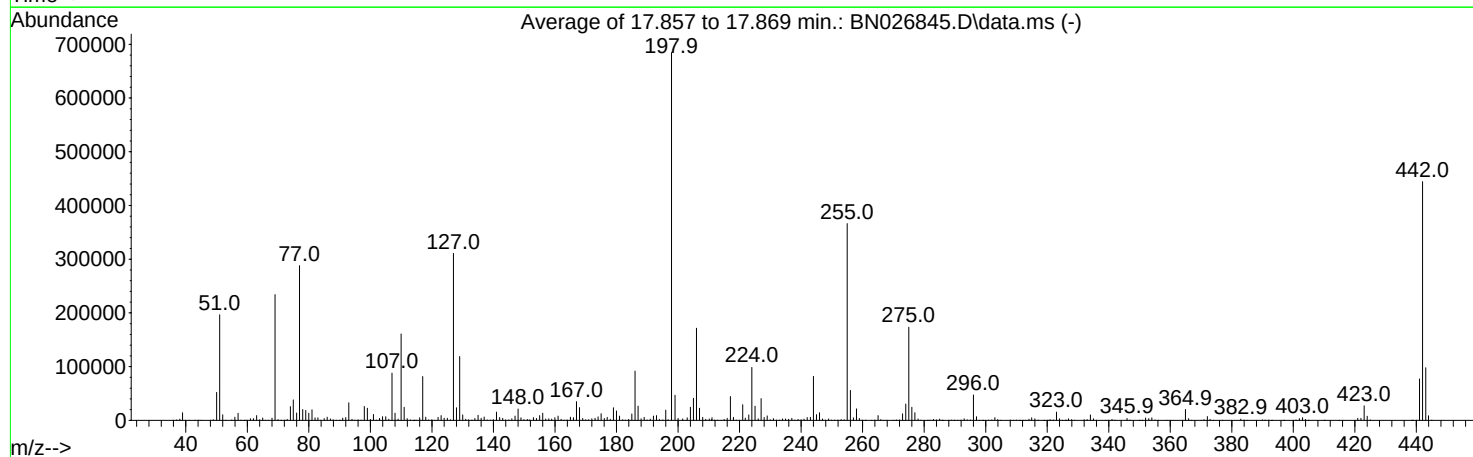


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080923\
 Data File : BN026845.D
 Acq On : 08 Aug 2023 12:24
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 09 01:06:23 2023

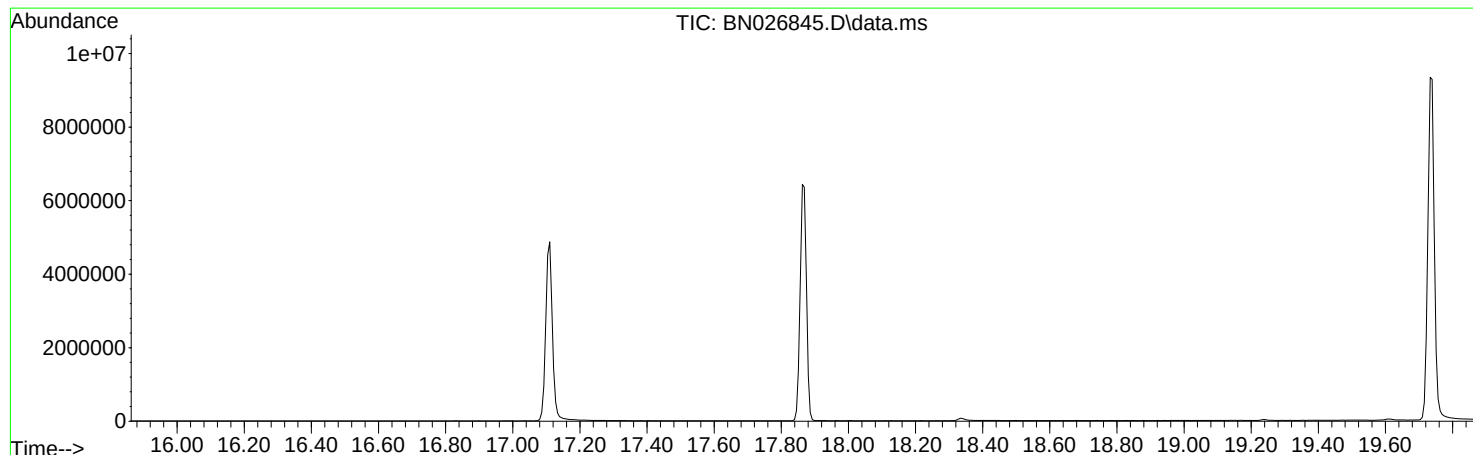




Spectrum Information: Average of 17.857 to 17.869 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	196630	PASS
68	69	0.00	2	1.7	4069	PASS
69	198	0.00	100	34.2	234112	PASS
70	69	0.00	2	0.6	1377	PASS
127	198	10	80	45.4	310827	PASS
197	198	0.00	2	0.2	1284	PASS
198	198	100	100	100.0	684736	PASS
199	198	5	9	6.8	46701	PASS
275	198	10	60	25.3	173344	PASS
365	198	1	100	3.0	20203	PASS
441	198	0.01	100	11.3	77093	PASS
442	442	50	100	100.0	444245	PASS
443	442	15	24	22.1	98080	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080923\
Data File : BN026845.D
Acq On : 08 Aug 2023 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 02:05:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 02:05:22 2023
Response via : Initial Calibration

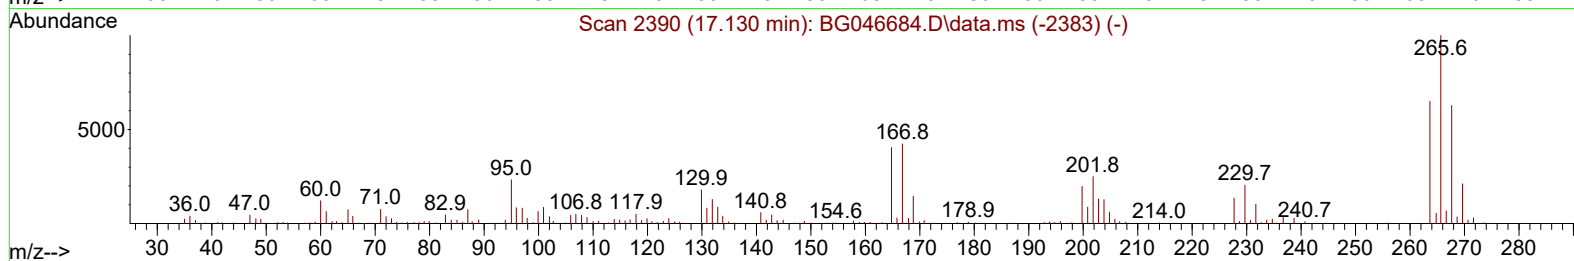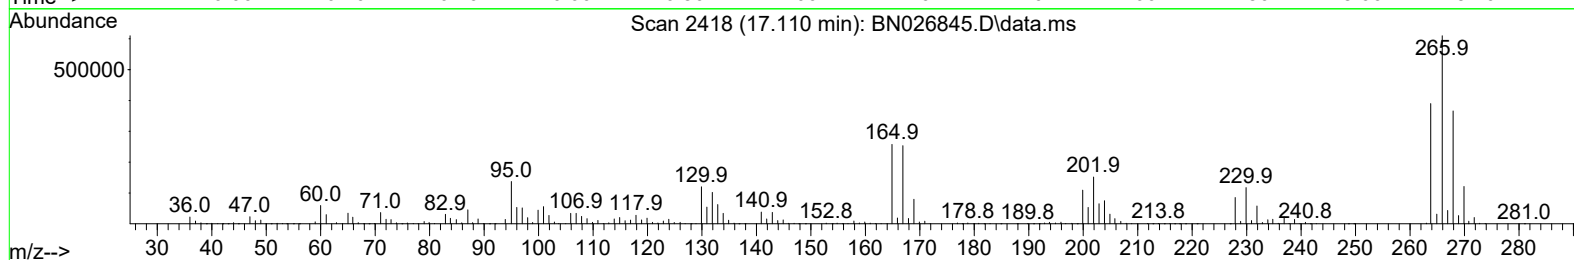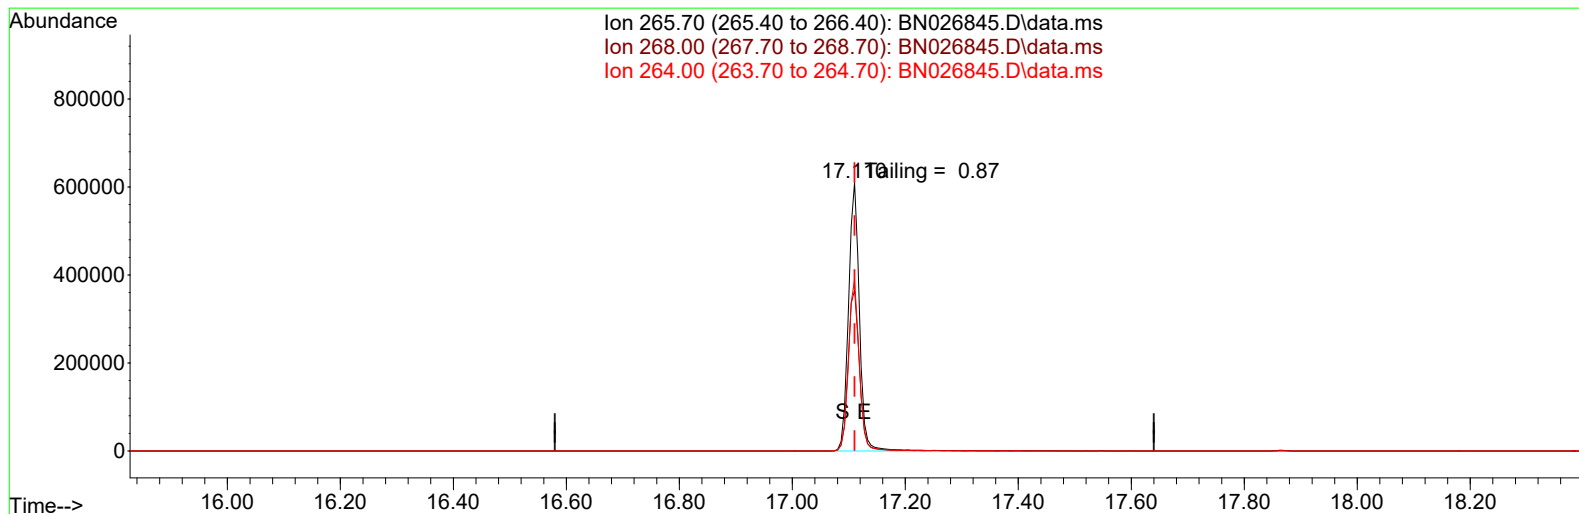

TIC: BN026845.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 24969.01 ng




response 823384

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.99
264.00	61.60	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080923\
Data File : BN026845.D
Acq On : 08 Aug 2023 12:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 02:05:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 02:05:22 2023
Response via : Initial Calibration

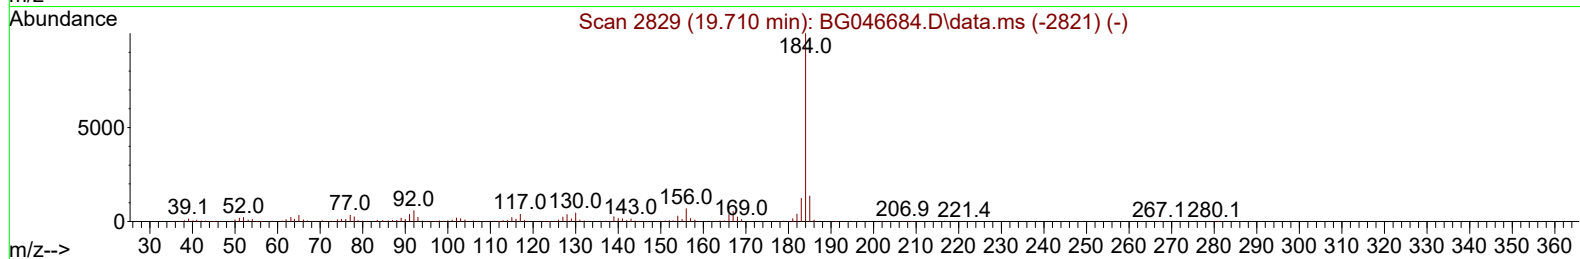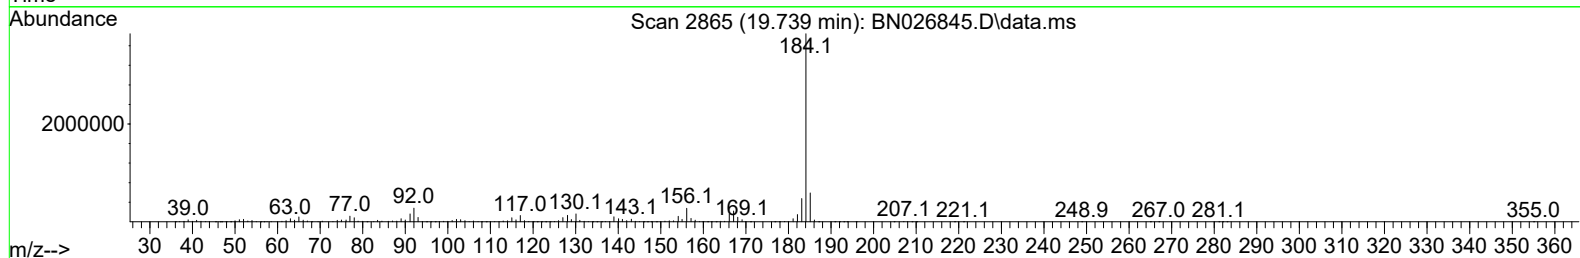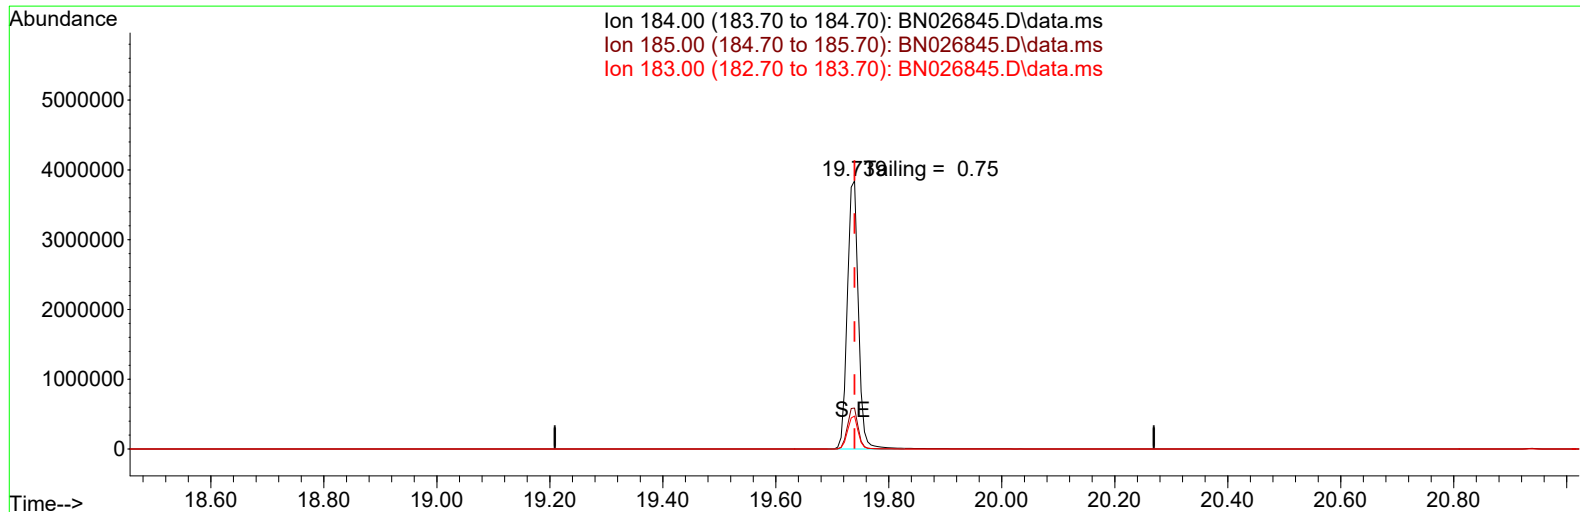

TIC: BN026845.D\data.ms

(77) Benzidine

19.739min (0.000) 0.00 ng

response 5263696

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.29
183.00	13.20	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2023	BNA_N	<u>BN026845.D</u>
Compound Name	Response	Retention Time
DDT	2348027	20.939
DDD	24219	20.545
DDE	590	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24809	2372836	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP