

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
 Data File : BN007045.D
 Acq On : 10 Aug 2019 11:54
 Operator : HP/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:55:57 AM

Quant Time: Aug 10 21:39:52 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Aug 10 21:17:06 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	6023	0.40	ng	0.00
6) Naphthalene-d8	10.19	136	21593	0.40	ng	0.00
12) Acenaphthene-d10	14.08	164	12333	0.40	ng	0.00
18) Phenanthrene-d10	16.82	188	32128	0.40	ng	0.00
26) Chrysene-d12	21.06	240	34159	0.40	ng	0.00
32) Perylene-d12	23.17	264	35053	0.40	ng	0.00

System Monitoring Compounds

3) 2-Fluorophenol	5.06	112	2937	0.19	ng	0.00
4) Phenol-d6	6.61	99	3533	0.19	ng	0.00
7) Nitrobenzene-d5	8.56	82	3323	0.20	ng	0.00
10) 2-Methylnaphthalene-d10	11.79	152	7754	0.19	ng	0.00
13) 2,4,6-Tribromophenol	15.57	330	1063	0.18	ng	0.00
14) 2-Fluorobiphenyl	12.71	172	4384	0.21	ng	0.00
24) Fluoranthene-d10	18.87	212	24109	0.20	ng	0.00
28) Terphenyl-d14	19.49	244	20165	0.20	ng	0.00

Target Compounds

						Qvalue
2) n-Nitrosodimethylamine	3.37	42	614	0.178	ng	# 93
5) bis(2-Chloroethyl)ether	6.87	93	3214	0.189	ng	98
8) Naphthalene	10.24	128	11899	0.187	ng	100
9) Hexachlorobutadiene	10.55	225	2567	0.188	ng	# 100
11) 2-Methylnaphthalene	11.87	142	8207	0.185	ng	97
15) Acenaphthylene	13.79	152	12721	0.196	ng	100
16) Acenaphthene	14.14	154	8122	0.194	ng	98
17) Fluorene	15.13	166	11184	0.184	ng	100
19) 4-Bromophenyl-phenylether	16.04	248	4431	0.207	ng	99
20) Hexachlorobenzene	16.14	284	4083	0.204	ng	99
21) Pentachlorophenol	16.48	266	1399	0.201	ng	98
22) Phenanthrene	16.87	178	20703	0.205	ng	100
23) Anthracene	16.96	178	17920	0.204	ng	100
25) Fluoranthene	18.90	202	26188	0.202	ng	99
27) Pyrene	19.27	202	26746	0.207	ng	100
29) Benzo(a)anthracene	21.03	228	26246	0.203	ng	99
30) Chrysene	21.09	228	26433	0.207	ng	100
31) Indeno(1,2,3-cd)pyrene	25.25	276	27366	0.200	ng	99
33) Benzo(b)fluoranthene	22.55	252	25438	0.208	ng	98
34) Benzo(k)fluoranthene	22.59	252	24661m	0.202	ng	
35) Benzo(a)pyrene	23.08	252	22600	0.205	ng	97
36) Dibenzo(a,h)anthracene	25.27	278	21913	0.200	ng	97
37) Benzo(g,h,i)perylene	25.88	276	23249	0.203	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
Data File : BN007045.D
Acq On : 10 Aug 2019 11:54
Operator : HP/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM

Quant Time: Aug 10 21:39:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 10 21:17:06 2019
Response via : Initial Calibration

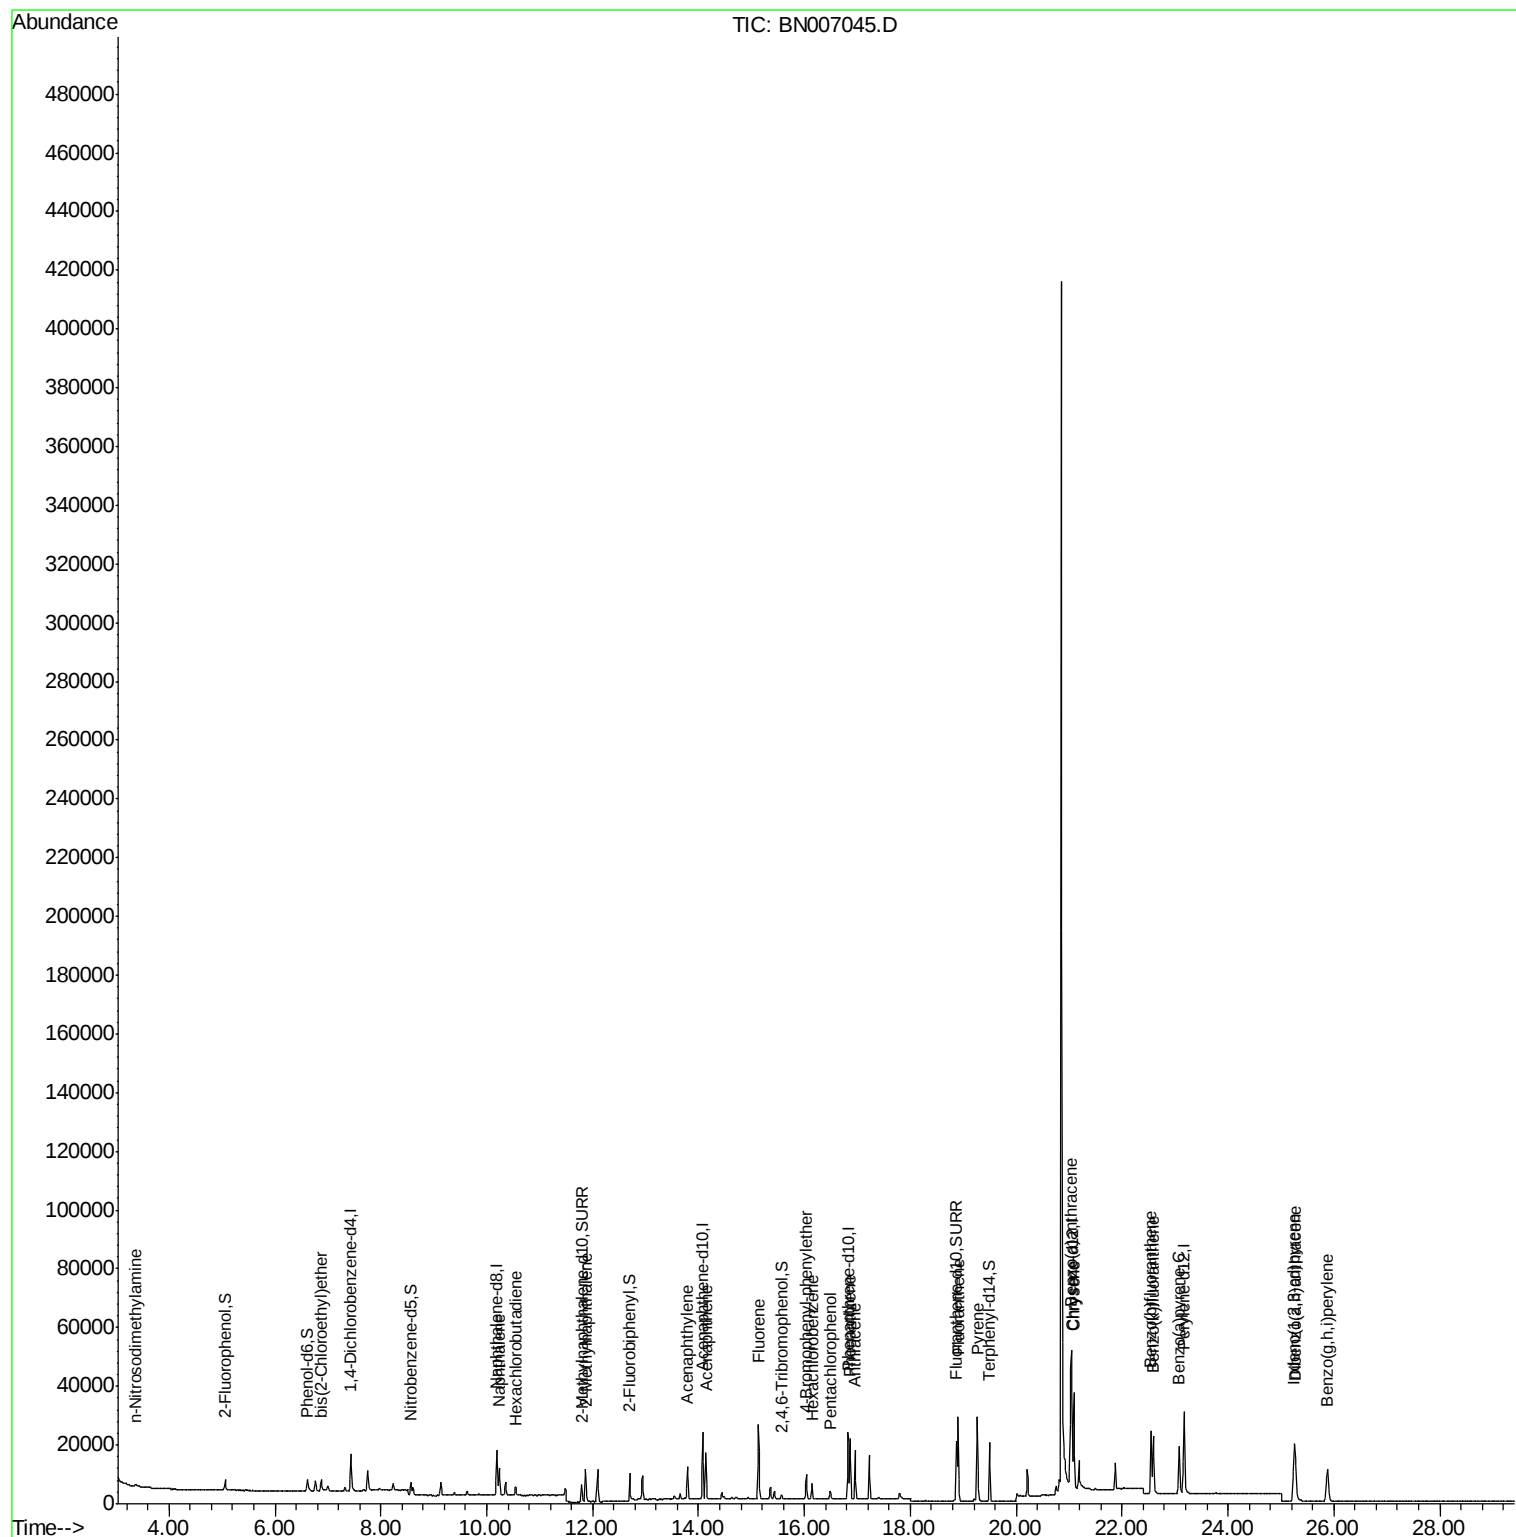



#1





1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 547
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
152	100		
150	154.4	121.7	182.5
115	58.1	46.2	69.4

Manual Integrations
APPROVED




mohammad
8/14/2019 2:55:57 AM




#2

n-Nitrosodimethylamine
Concen: 0.178 ng
RT: 3.37 min Scan# 42
Delta R.T. 0.01 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
42	100		
74	146.3	110.6	166.0
44	0.0	0.0	0.0



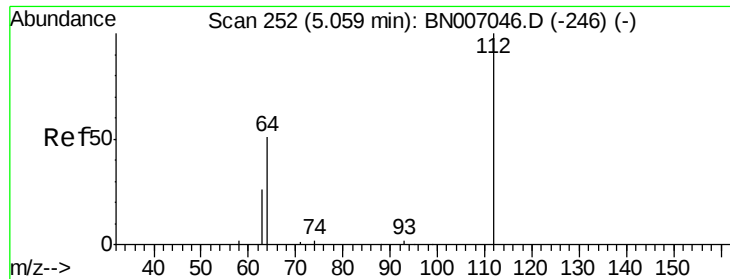

#3

2-Fluorophenol

Concen: 0.188 ng

RT: 5.06 min Scan# 252

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N





ClientSampled :

SSTDICC0.2

Tgt Ion:	112	Resp:	2937
Ion Ratio	Lower	Upper	
112	100		
64	52.7	42.6	63.8
63	29.1	22.2	33.2

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM

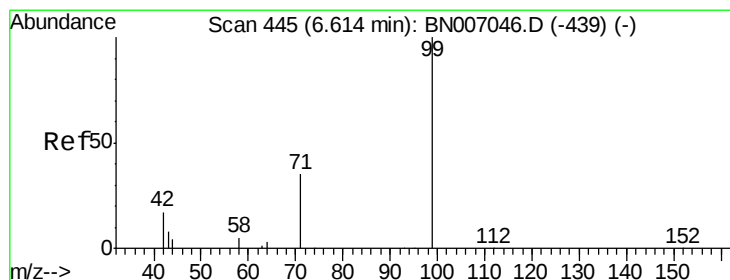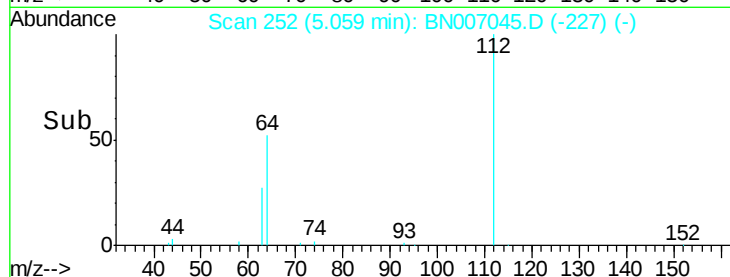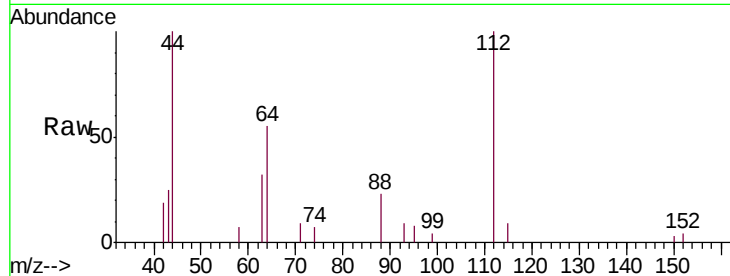

#4

Phenol-d6

Concen: 0.186 ng




RT: 6.61 min Scan# 445




Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion:	99	Resp:	3533
Ion Ratio	Lower	Upper	
99	100		
42	18.6	15.8	23.6
71	33.9	27.0	40.4

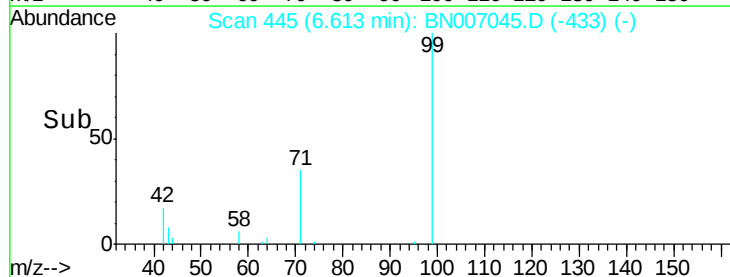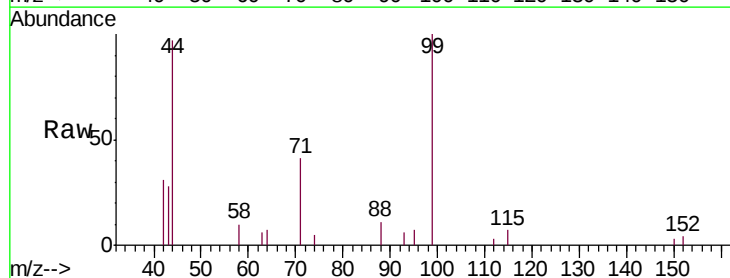



#5

bis(2-Chloroethyl)ether

Concen: 0.189 ng

RT: 6.87 min Scan# 477

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion:	93	Resp:	3214
Ion	Ratio	Lower	Upper
93	100		
63	71.1	55.6	83.4
95	32.8	26.7	40.1

Instrument :





BNA_N

ClientSampleId :

SSTDICC0.2

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM



#6

Naphthalene-d8

Concen: 0.400 ng


RT: 10.19 min Scan# 813


Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion:	136	Resp:	21593
Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.4	14.0
54	9.0	6.6	9.8
68	7.5	6.0	9.0

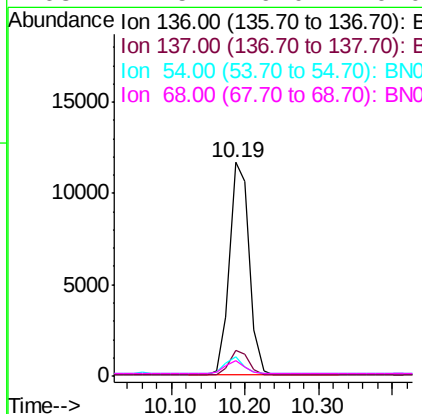



#7

Nitrobenzene-d5

Concen: 0.197 ng

RT: 8.56 min Scan# 685

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N





ClientSampleId :

SSTDIC0.2

Tgt Ion:	82	Resp:	3323
Ion	Ratio	Lower	Upper
82	100		
128	43.4	34.6	51.8
54	48.2	36.2	54.4

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM



#8

Naphthalene

Concen: 0.187 ng




RT: 10.24 min Scan# 817


Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion:	128	Resp:	11899
Ion	Ratio	Lower	Upper
128	100		
129	11.8	9.4	14.2
127	14.0	11.0	16.6



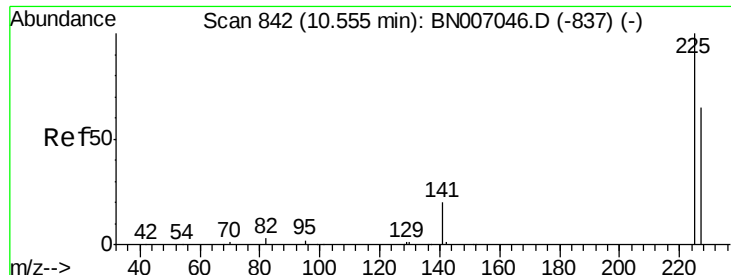

#9

Hexachlorobutadiene

Concen: 0.188 ng

RT: 10.55 min Scan# 842

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N


ClientSampleId :

SSTDIC0.2




Tgt Ion:	225	Resp:	2567
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.6	51.1	76.7

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM



Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E

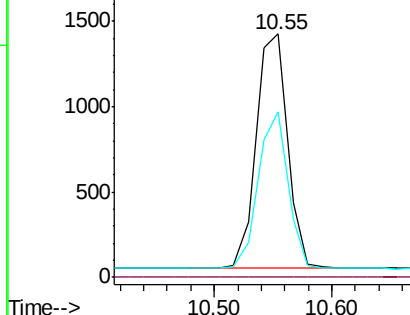

#10

2-Methylnaphthalene-d10

Concen: 0.187 ng


RT: 11.79 min Scan# 982

Delta R.T. -0.00 min



Lab File: BN007045.D


Acq: 10 Aug 2019 11:54

Tgt Ion:	152	Resp:	7754
Ion Ratio	Lower	Upper	
152	100		
151	19.4	15.5	23.3



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E

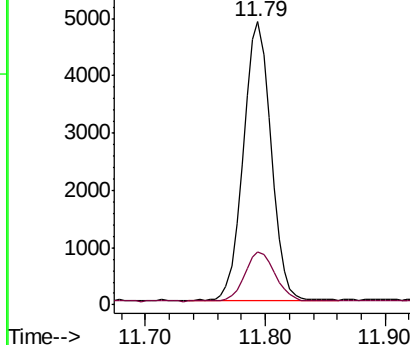







#11
2-Methylnaphthalene
Concen: 0.185 ng
RT: 11.87 min Scan# 999
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.4	69.0	103.6
115	35.8	27.1	40.7




Manual Integrations
APPROVED


mohammad
8/14/2019 2:55:57 AM

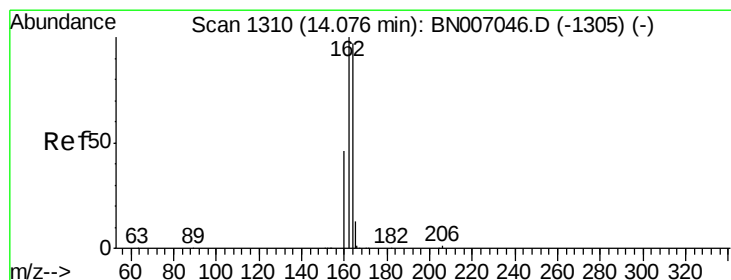

#12
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.08 min Scan# 1310
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.6	82.2	123.4
160	49.5	38.3	57.5






#13
 2,4,6-Tribromophenol
 Concen: 0.183 ng
 RT: 15.57 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2




Tgt Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	46.7	33.6	50.4

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:55:57 AM




Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


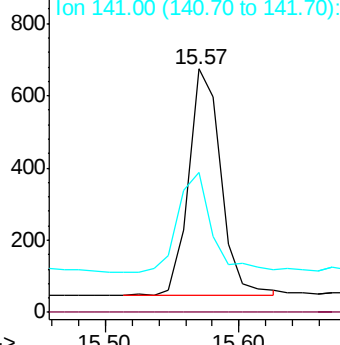



#14
 2-Fluorobiphenyl
 Concen: 0.214 ng
 RT: 12.71 min Scan# 1187
 Delta R.T. -0.00 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.6	26.3	39.5
170	21.7	17.0	25.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

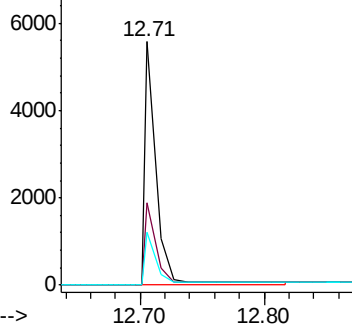







#15
Acenaphthylene
Concen: 0.196 ng
RT: 13.79 min Scan# 1284
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampled :
SSTDICC0.2

Tgt Ion:	152	Resp:	12721
Ion Ratio	Lower	Upper	
152	100		
151	19.6	15.8	23.6
153	13.3	10.4	15.6




Manual Integrations
APPROVED


mohammad
8/14/2019 2:55:57 AM

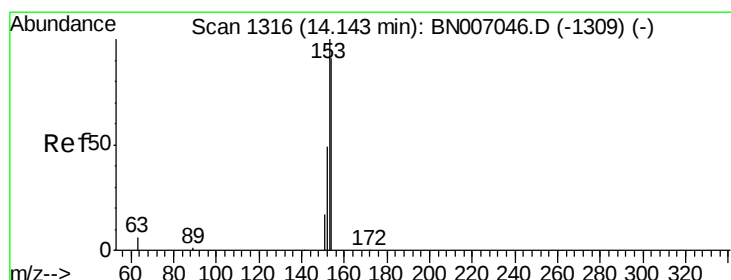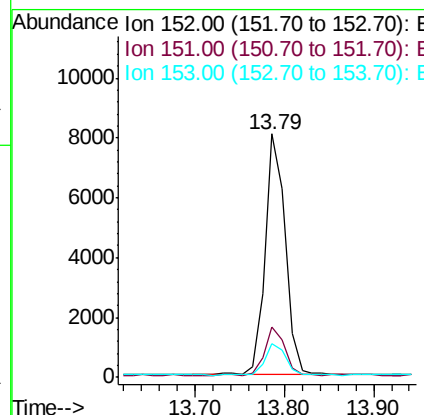

#16
Acenaphthene
Concen: 0.194 ng
RT: 14.14 min Scan# 1316
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion:	154	Resp:	8122
Ion Ratio	Lower	Upper	
154	100		
153	114.1	89.5	134.3
152	57.1	44.8	67.2

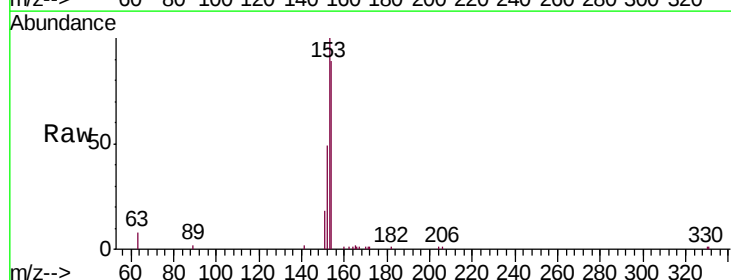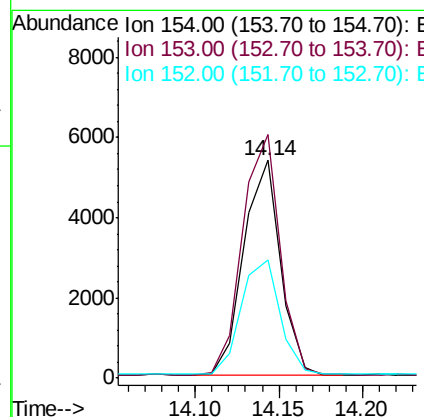



#17

Fluorene

Concen: 0.184 ng

RT: 15.13 min Scan# 1405

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N





ClientSampleId :

SSTDIC0.2

Tgt Ion	Ratio	Lower	Upper
166	100		
165	97.5	77.9	116.9
167	13.9	10.9	16.3

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM

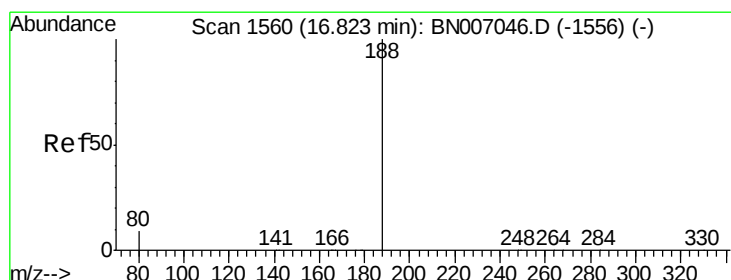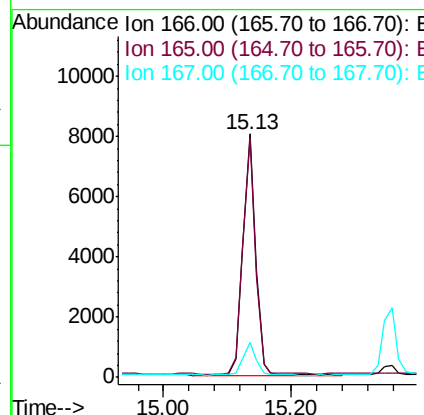

#18

Phenanthrene-d10

Concen: 0.400 ng




RT: 16.82 min Scan# 1560


Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	9.9	7.8	11.6

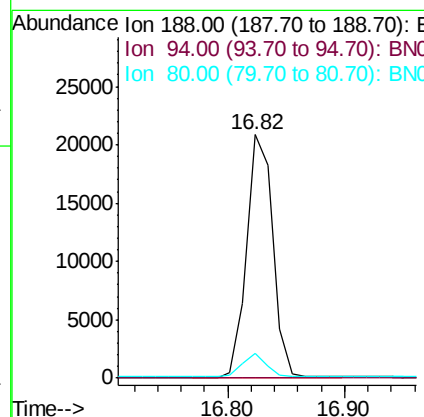







#19
4-Bromophenyl-phenylether
Concen: 0.207 ng
RT: 16.04 min Scan# 1486
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampled :
SSTDIC0.2

Tgt Ion	Ratio	Lower	Upper
248	100		
250	98.2	78.9	118.3
141	52.9	43.3	64.9




Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM

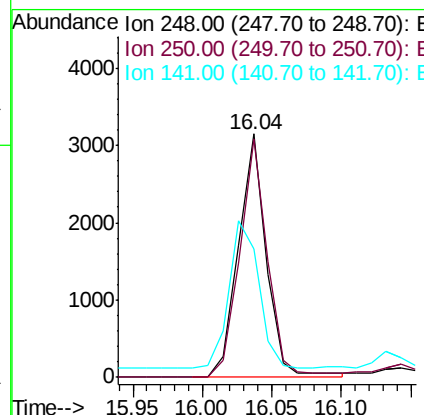

#20
Hexachlorobenzene
Concen: 0.204 ng
RT: 16.14 min Scan# 1496
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
284	100		
142	37.1	30.5	45.7
249	33.1	26.7	40.1

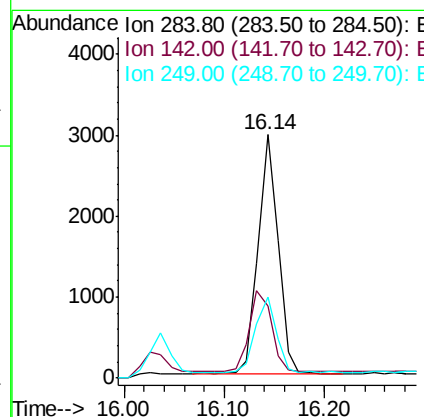







#21
 Pentachlorophenol
 Concen: 0.201 ng
 RT: 16.48 min Scan# 1528
 Delta R.T. -0.00 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	266	Resp:	1399
Ion Ratio	Lower	Upper	
266	100		
264	63.8	52.3	78.5
268	65.4	51.5	77.3




Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:55:57 AM

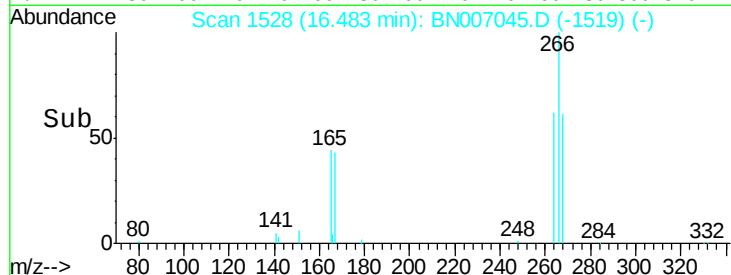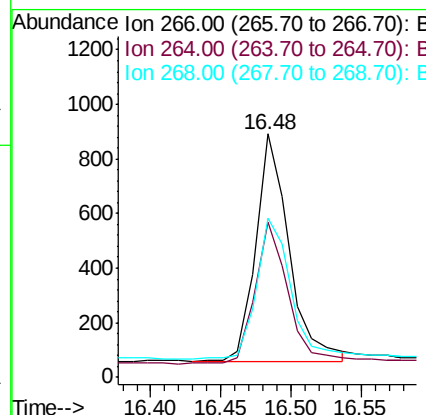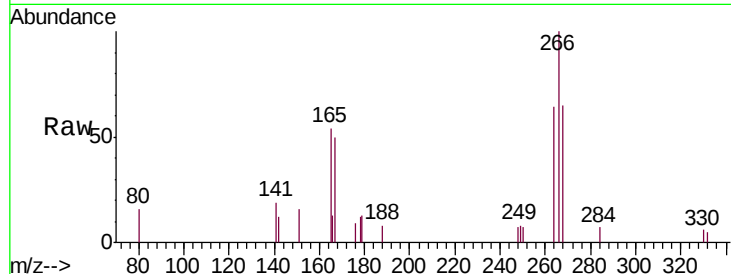

#22
 Phenanthrene
 Concen: 0.205 ng
 RT: 16.87 min Scan# 1564
 Delta R.T. -0.00 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Tgt Ion:	178	Resp:	20703
Ion Ratio	Lower	Upper	
178	100		
176	19.1	15.2	22.8
179	15.4	12.3	18.5

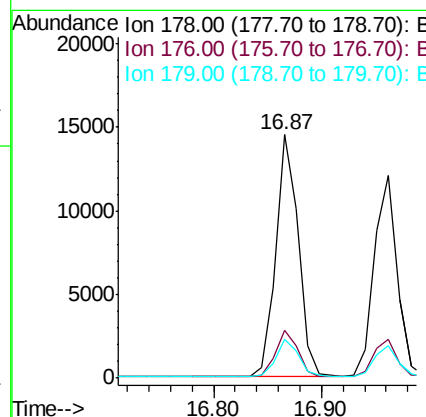



#23

Anthracene

Concen: 0.204 ng

RT: 16.96 min Scan# 1573

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N





ClientSampleId :

SSTDIC0.2

Tgt Ion:	178	Resp:	17920
Ion Ratio	Lower	Upper	
178	100		
176	18.3	14.6	21.8
179	15.5	12.5	18.7

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM



#24

Fluoranthene-d10

Concen: 0.203 ng




RT: 18.87 min Scan# 1845


Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion:	212	Resp:	24109
Ion Ratio	Lower	Upper	
212	100		
106	10.3	8.2	12.2
104	6.0	4.5	6.7





#25

Fluoranthene

Concen: 0.202 ng

RT: 18.90 min Scan# 1851

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N





ClientSampleId :

SSTDICC0.2

Tgt Ion:	202	Resp:	26188
Ion Ratio	Lower	Upper	
202	100		
101	8.9	7.0	10.4
203	17.6	13.8	20.8

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM

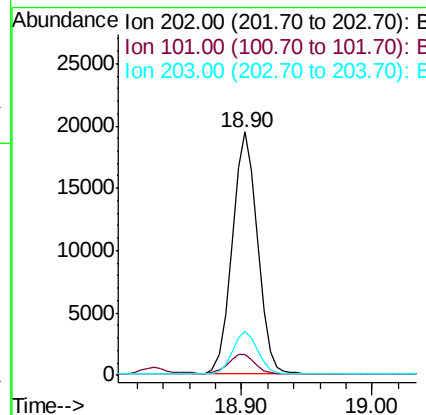

#26

Chrysene-d12

Concen: 0.400 ng




RT: 21.06 min Scan# 2172


Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Tgt Ion:	240	Resp:	34159
Ion Ratio	Lower	Upper	
240	100		
120	5.0	4.0	6.0
236	26.3	21.3	31.9

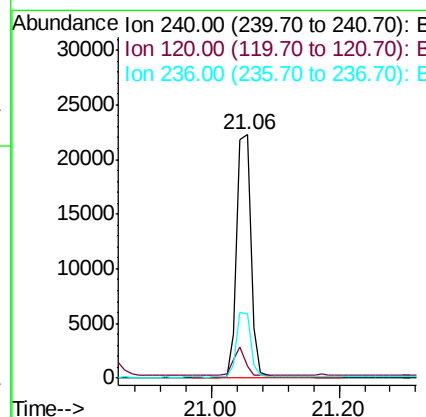







#27
 Pyrene
 Concen: 0.207 ng
 RT: 19.27 min Scan# 1925
 Delta R.T. -0.00 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.8	16.6	24.8
203	17.4	14.0	21.0




Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:55:57 AM

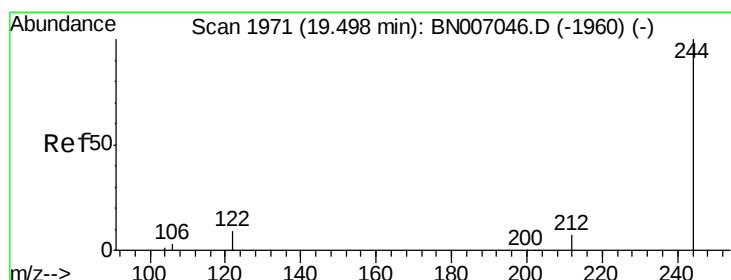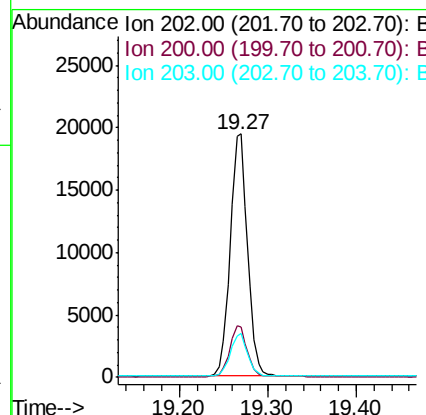

#28
 Terphenyl-d14
 Concen: 0.204 ng
 RT: 19.49 min Scan# 1970
 Delta R.T. -0.01 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.1	6.2	9.2
122	10.9	7.4	11.2

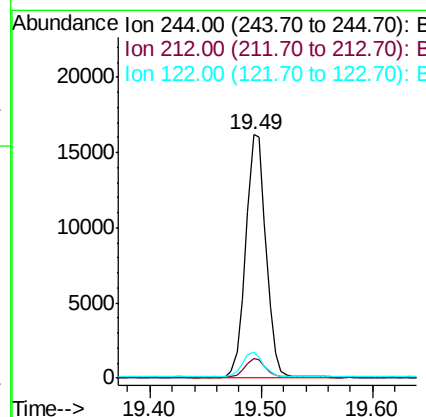







#29
Benzo(a)anthracene
Concen: 0.203 ng
RT: 21.03 min Scan# 2170
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.9	21.8	32.6
229	19.9	15.6	23.4




Manual Integrations
APPROVED


mohammad
8/14/2019 2:55:57 AM

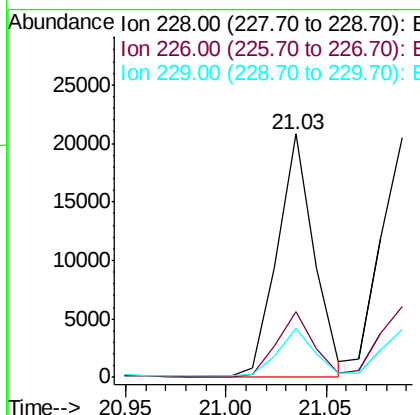

#30
Chrysene
Concen: 0.207 ng
RT: 21.09 min Scan# 2175
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.5	23.8	35.6
229	19.8	15.7	23.5

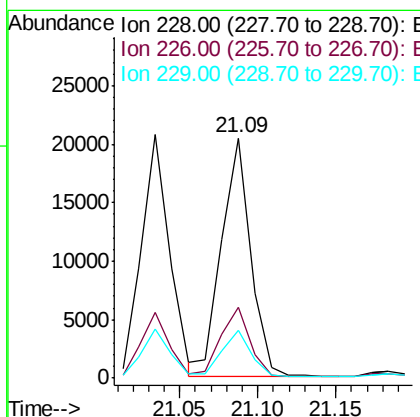







#31
Indeno(1,2,3-cd)pyrene
Concen: 0.200 ng
RT: 25.25 min Scan# 3130
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion	Ratio	Lower	Upper
276	100		
138	20.5	16.0	24.0
277	24.6	19.9	29.9




Manual Integrations
APPROVED


mohammad
8/14/2019 2:55:57 AM



#32
Perylene-d12
Concen: 0.400 ng
RT: 23.17 min Scan# 2523
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.8
265	32.5	26.2	39.4



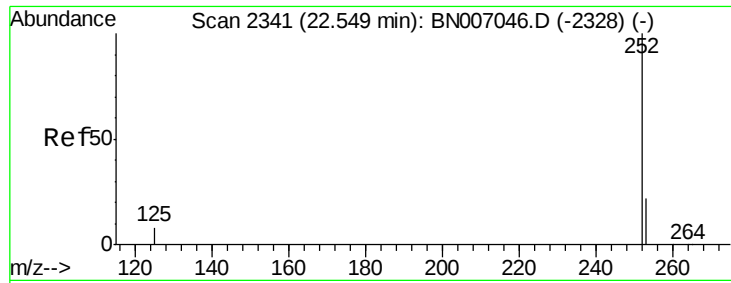





#33
Benzo(b)fluoranthene
Concen: 0.208 ng
RT: 22.55 min Scan# 2341
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	18.2	27.2
125	10.9	7.4	11.0




Manual Integrations
APPROVED


mohammad
8/14/2019 2:55:57 AM

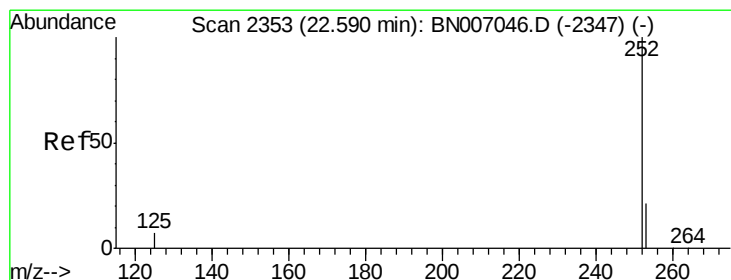

#34
Benzo(k)fluoranthene
Concen: 0.202 ng m
RT: 22.59 min Scan# 2353
Delta R.T. -0.00 min
Lab File: BN007045.D
Acq: 10 Aug 2019 11:54

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.8	18.1	27.1
125	11.2	7.4	11.0

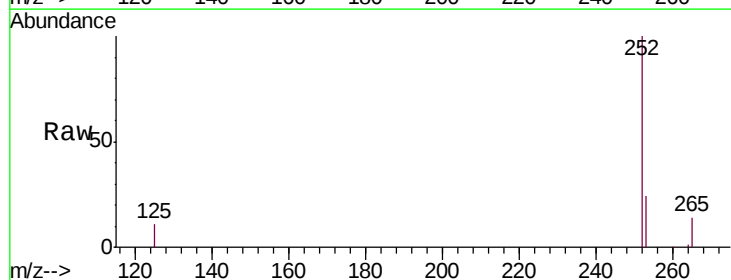



#35

Benzo(a)pyrene

Concen: 0.205 ng

RT: 23.08 min Scan# 2496

Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54

Instrument :

BNA_N





ClientSampleId :

SSTDIC0.2

Tgt Ion:	252	Resp:	22600
Ion Ratio	Lower	Upper	
252	100		
253	23.9	18.5	27.7
125	12.3	8.2	12.4

Manual Integrations
APPROVED

mohammad
8/14/2019 2:55:57 AM



#36

Dibenzo(a,h)anthracene

Concen: 0.200 ng




RT: 25.27 min Scan# 3136


Delta R.T. -0.00 min

Lab File: BN007045.D

Acq: 10 Aug 2019 11:54


Tgt Ion:	278	Resp:	21913
Ion Ratio	Lower	Upper	
278	100		
139	15.5	11.3	16.9
279	25.5	19.3	28.9





#37
 Benzo(g,h,i)perylene
 Concen: 0.203 ng
 RT: 25.88 min Scan# 3314
 Delta R.T. -0.00 min
 Lab File: BN007045.D
 Acq: 10 Aug 2019 11:54

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2



Tgt Ion:	276	Resp:	23249
Ion Ratio		Lower	Upper
276	100		
277	25.9	19.8	29.8
138	18.9	14.6	22.0

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:55:57 AM

