

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
 Data File : BN007084.D
 Acq On : 11 Aug 2019 13:26
 Operator : HP/JU
 Sample : K4143-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXT-004-SW072-073019

Quant Time: Aug 12 07:26:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 10 21:44:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	9972	0.40	ng	0.00
6) Naphthalene-d8	10.19	136	38198	0.40	ng	0.00
12) Acenaphthene-d10	14.08	164	21851	0.40	ng	0.00
18) Phenanthrene-d10	16.82	188	53669	0.40	ng	0.00
26) Chrysene-d12	21.05	240	54625	0.40	ng	-0.01
32) Perylene-d12	23.16	264	58870	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2-Fluorophenol	5.06	112	5527	0.23	ng	0.00
4) Phenol-d6	6.61	99	7573	0.26	ng	0.00
7) Nitrobenzene-d5	8.56	82	5896	0.19	ng	0.00
10) 2-Methylnaphthalene-d10	11.79	152	14133	0.20	ng	0.00
13) 2,4,6-Tribromophenol	15.57	330	1236	0.11	ng	0.00
14) 2-Fluorobiphenyl	12.71	172	4275	0.13	ng	0.00
24) Fluoranthene-d10	18.87	212	34843	0.18	ng	0.00
28) Terphenyl-d14	19.49	244	25381	0.17	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
Data File : BN007084.D
Acq On : 11 Aug 2019 13:26
Operator : HP/JU
Sample : K4143-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXT-004-SW072-073019

Quant Time: Aug 12 07:26:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 10 21:44:50 2019
Response via : Initial Calibration

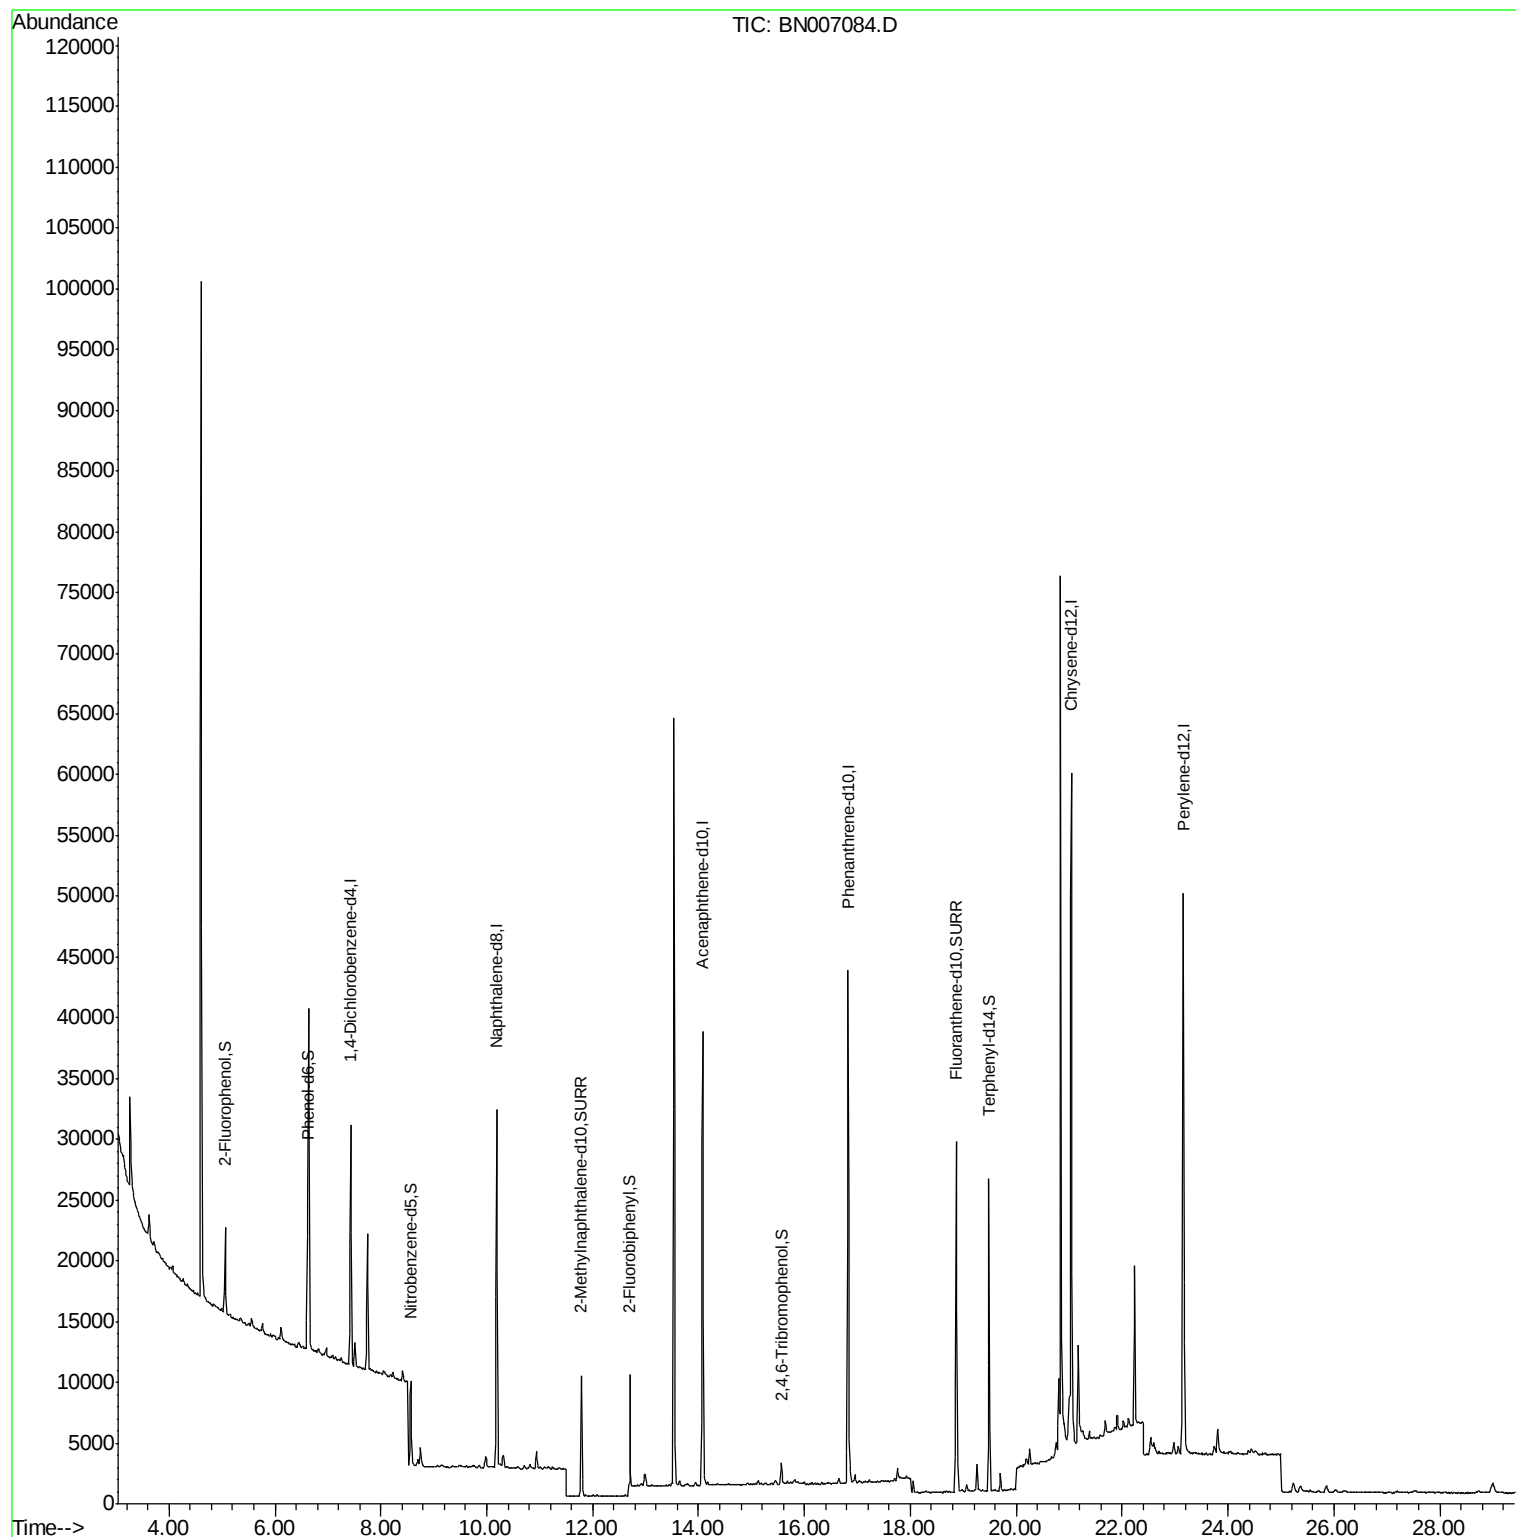

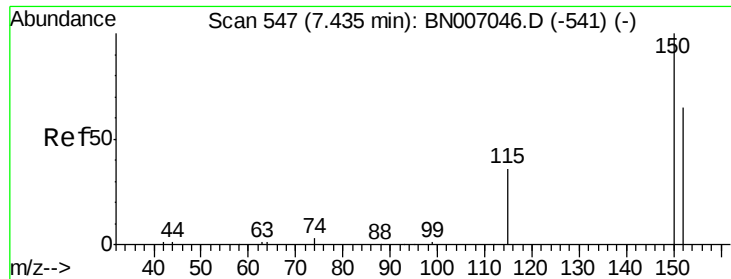


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 547
Delta R.T. -0.00 min
Lab File: BN007084.D
Acq: 11 Aug 2019 13:26

Instrument :
BNA_N
ClientSampleId :
EXT-004-SW072-073019

Tgt Ion:152 Resp: 9972
Ion Ratio Lower Upper
152 100
150 150.4 121.7 182.5
115 55.4 46.2 69.4

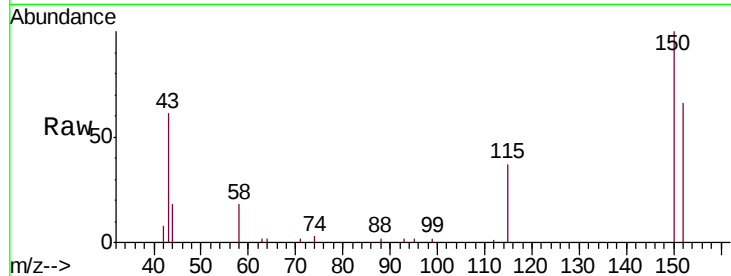


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

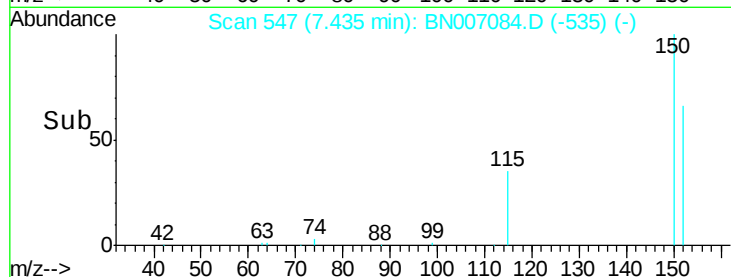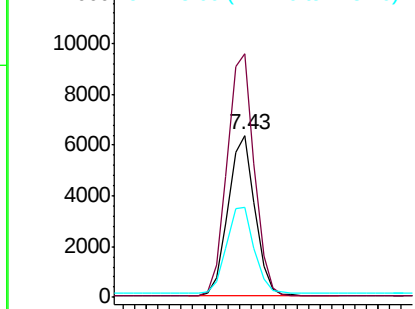



#3


2-Fluorophenol
Concen: 0.231 ng
RT: 5.06 min Scan# 252
Delta R.T. -0.00 min
Lab File: BN007084.D
Acq: 11 Aug 2019 13:26

Tgt Ion:112 Resp: 5527
Ion Ratio Lower Upper
112 100
64 54.1 42.6 63.8
63 28.5 22.2 33.2



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

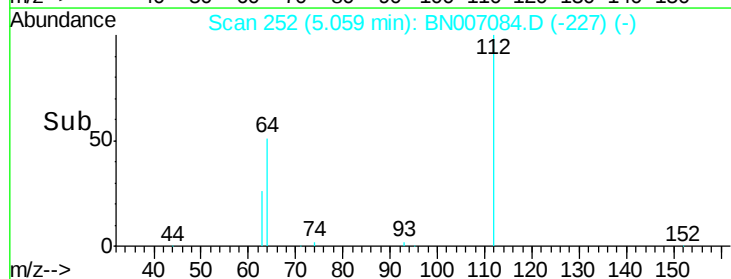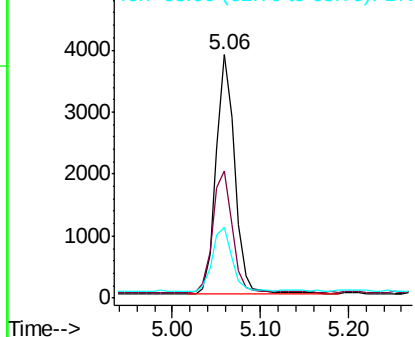

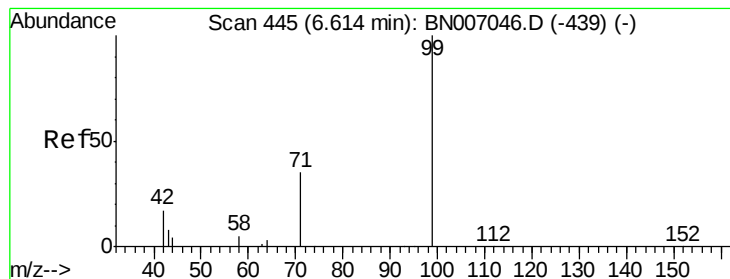

#4

Phenol-d6

Concen: 0.255 ng

RT: 6.61 min Scan# 445

Delta R.T. -0.00 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26

Instrument :

BNA_N

ClientSampleId :

EXT-004-SW072-073019


Tgt Ion: 99 Resp: 7573

Ion Ratio Lower Upper

99 100

42 0.0 15.8 23.6#




71 34.4 27.0 40.4

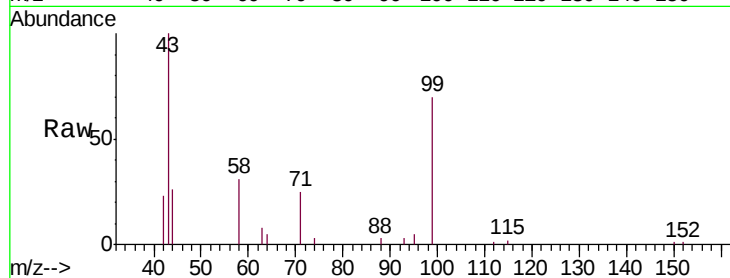

Abundance Ion 99.00 (98.70 to 99.70): BN007046.D (-439) (-)

Ion 42.00 (41.70 to 42.70): BN007046.D (-439) (-)

Ion 71.00 (70.70 to 71.70): BN007046.D (-439) (-)

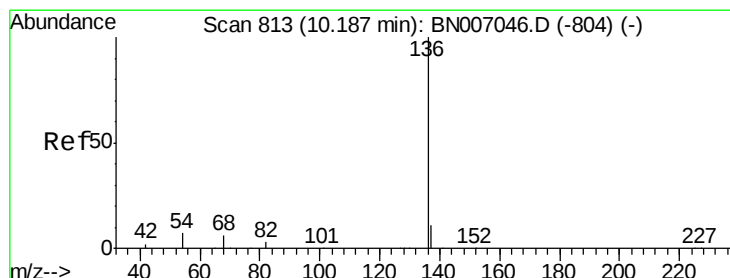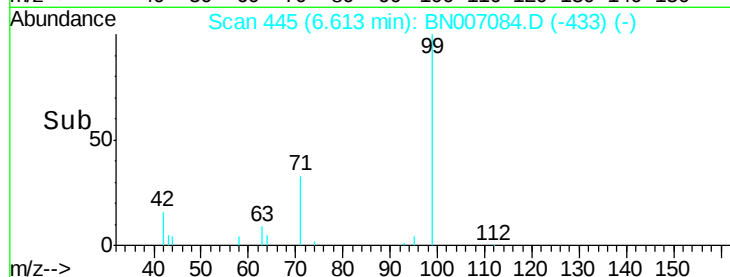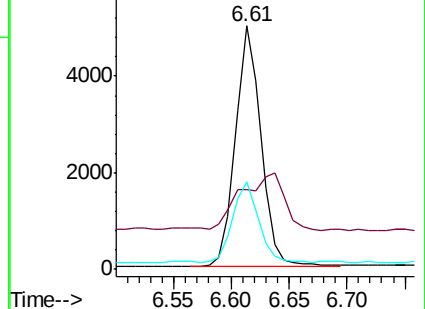

#6

Naphthalene-d8

Concen: 0.400 ng

RT: 10.19 min Scan# 813

Delta R.T. -0.00 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26

Tgt Ion: 136 Resp: 38198


Ion Ratio Lower Upper

136 100

137 11.2 9.4 14.0

54 6.3 6.6 9.8#

68 5.8 6.0 9.0#


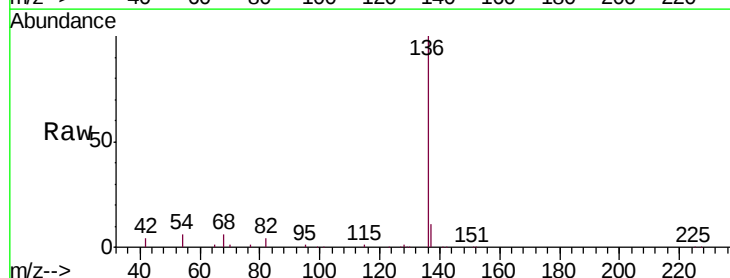



Abundance Ion 136.00 (135.70 to 136.70): BN007046.D (-804) (-)

Ion 137.00 (136.70 to 137.70): BN007046.D (-804) (-)

Ion 54.00 (53.70 to 54.70): BN007046.D (-804) (-)

Ion 68.00 (67.70 to 68.70): BN007046.D (-804) (-)

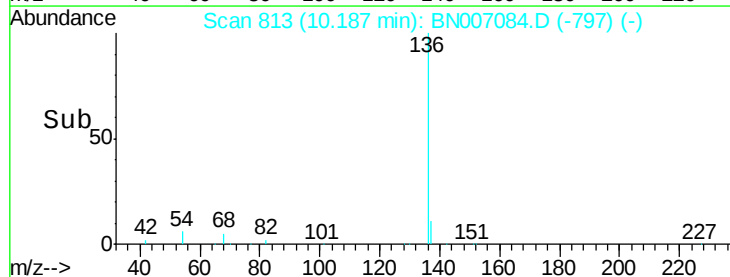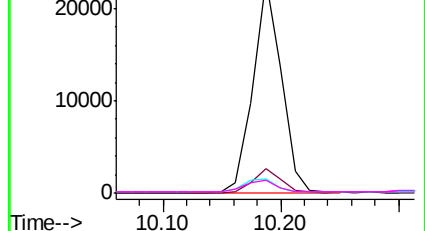

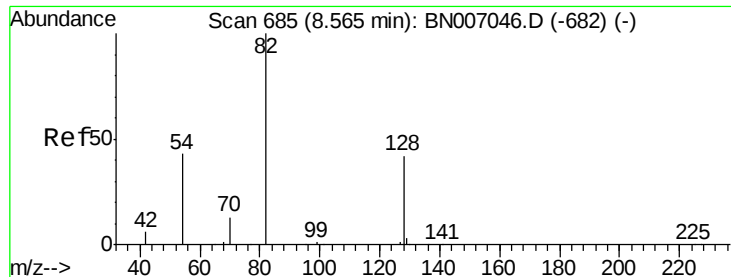

#7

Nitrobenzene-d5

Concen: 0.191 ng

RT: 8.56 min Scan# 685

Delta R.T. -0.00 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26

Instrument :

BNA_N

ClientSampleId :

EXT-004-SW072-073019


Tgt Ion: 82 Resp: 5896

Ion Ratio Lower Upper

82 100

128 48.2 34.6 51.8




54 43.1 36.2 54.4



Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): BNC

Ion 54.00 (53.70 to 54.70): BNC

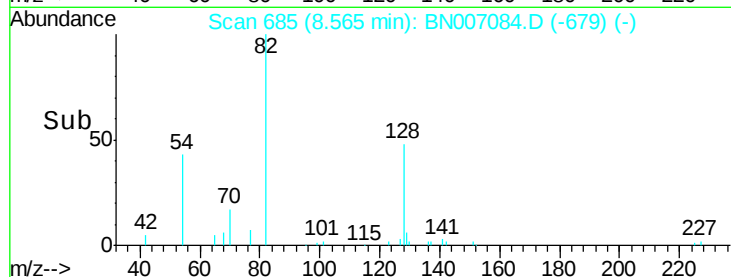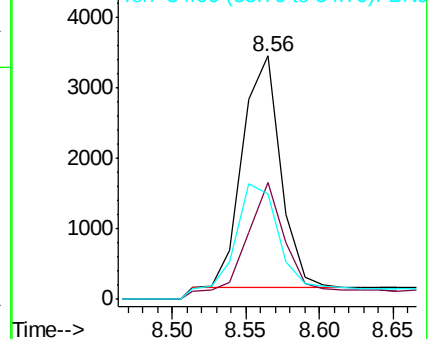

#10

2-Methylnaphthalene-d10

Concen: 0.198 ng

RT: 11.79 min Scan# 981

Delta R.T. -0.00 min

Lab File: BN007084.D


Acq: 11 Aug 2019 13:26

Tgt Ion: 152 Resp: 14133

Ion Ratio Lower Upper



152 100


151 19.3 15.5 23.3



Abundance Ion 152.00 (151.70 to 152.70): BNC

Ion 151.00 (150.70 to 151.70): BNC

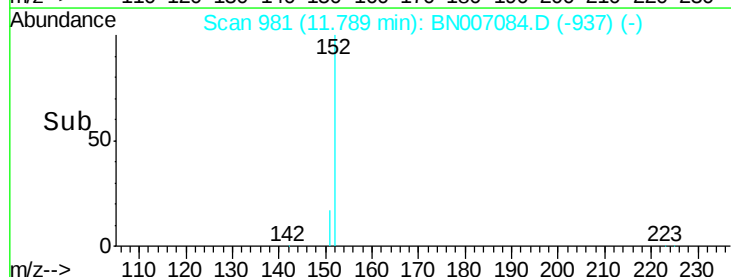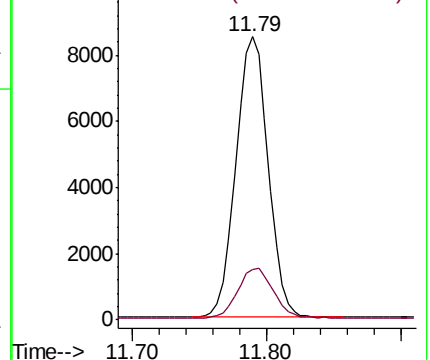

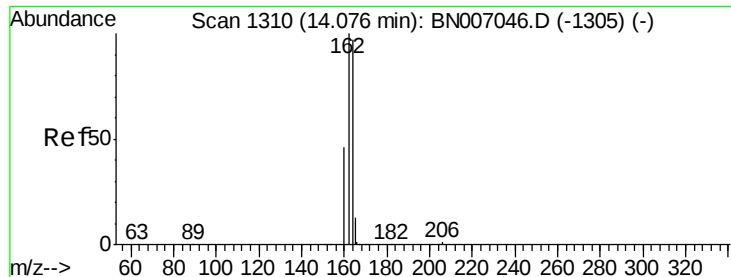

#12

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.08 min Scan# 1310

Delta R.T. -0.00 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26

Instrument :

BNA_N

ClientSampleId :

EXT-004-SW072-073019


Tgt Ion:164 Resp: 21851

Ion Ratio Lower Upper

164 100

162 99.5 82.2 123.4

160 45.4 38.3 57.5



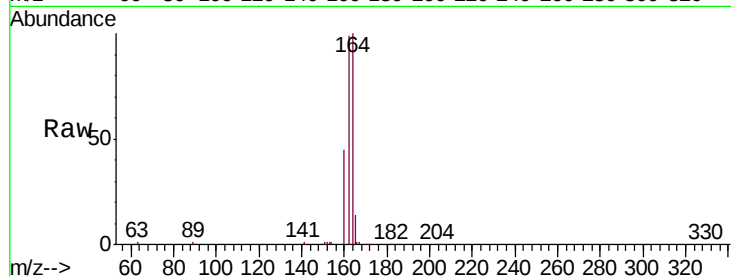


Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

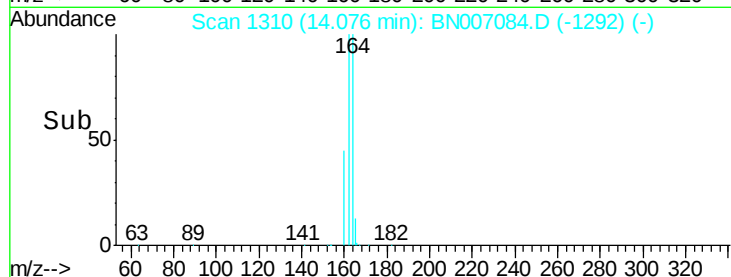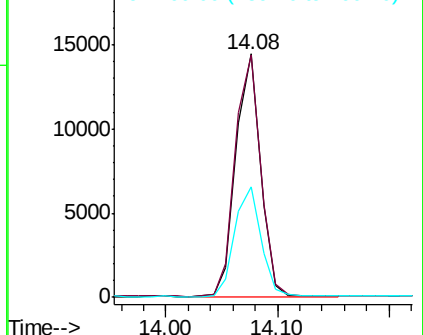

#13

2,4,6-Tribromophenol

Concen: 0.105 ng

RT: 15.57 min Scan# 1444

Delta R.T. -0.00 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26


Tgt Ion:330 Resp: 1236

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 42.7 33.6 50.4






Abundance

Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



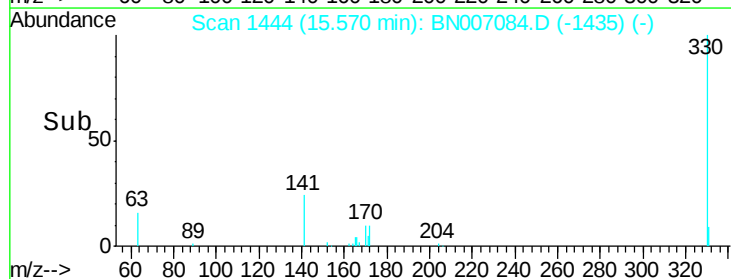
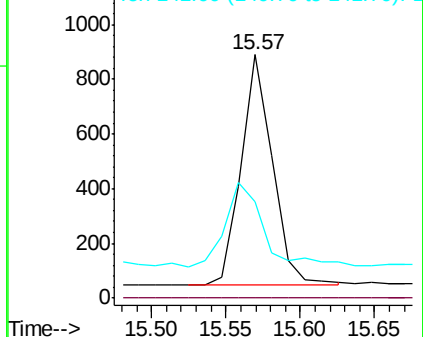


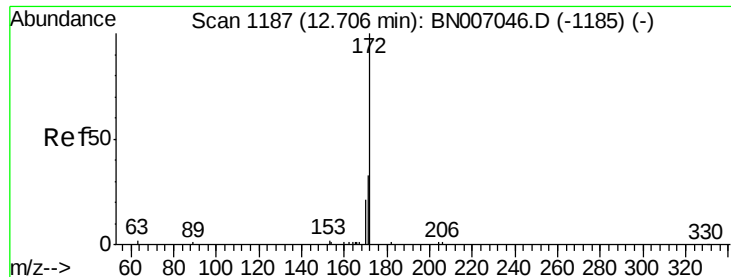

#14
2-Fluorobiphenyl
Concen: 0.135 ng
RT: 12.71 min Scan# 1187
Delta R.T. -0.00 min
Lab File: BN007084.D
Acq: 11 Aug 2019 13:26




Instrument :
BNA_N
ClientSampleId :
EXT-004-SW072-073019


Tgt Ion:172 Resp: 4275
Ion Ratio Lower Upper
172 100
171 33.2 26.3 39.5
170 20.7 17.0 25.4

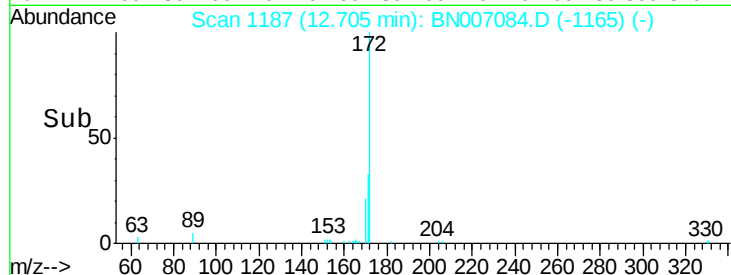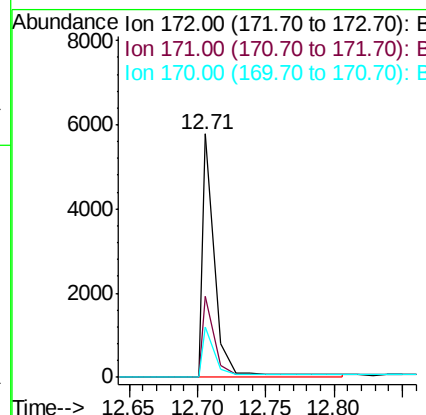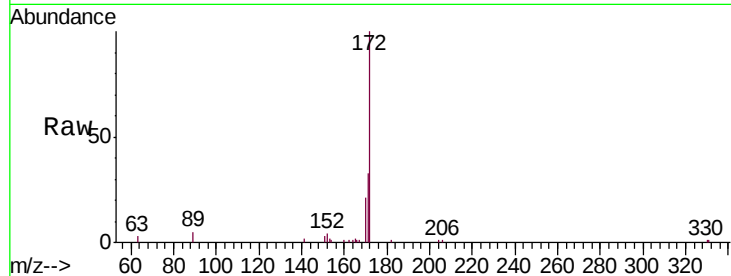

#18
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.82 min Scan# 1560
Delta R.T. -0.00 min
Lab File: BN007084.D
Acq: 11 Aug 2019 13:26

Tgt Ion:188 Resp: 53669
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.7 7.8 11.6#

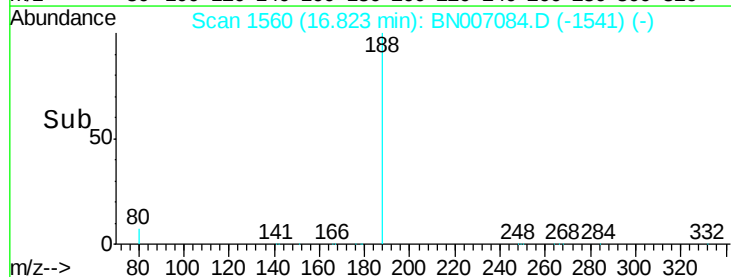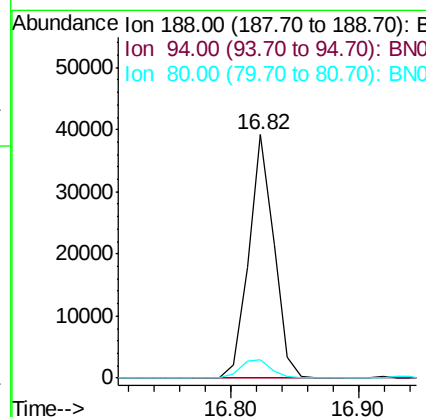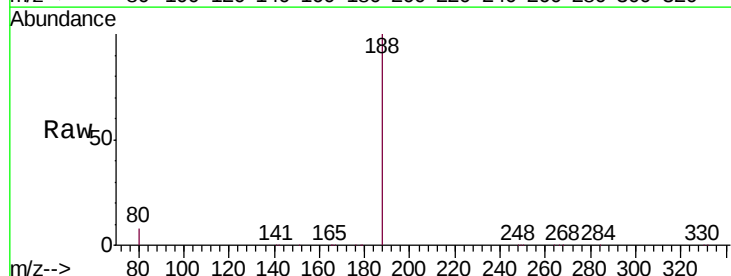

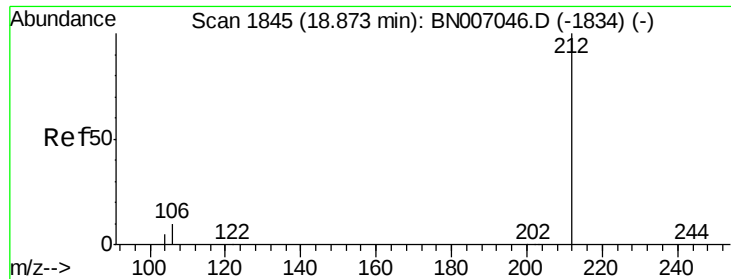

#24

Fluoranthene-d10

Concen: 0.183 ng

RT: 18.87 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26

Instrument :

BNA_N

ClientSampleId :

EXT-004-SW072-073019


Tgt Ion:212 Resp: 34843

Ion Ratio Lower Upper

212 100

106 10.3 8.2 12.2




104 5.7 4.5 6.7

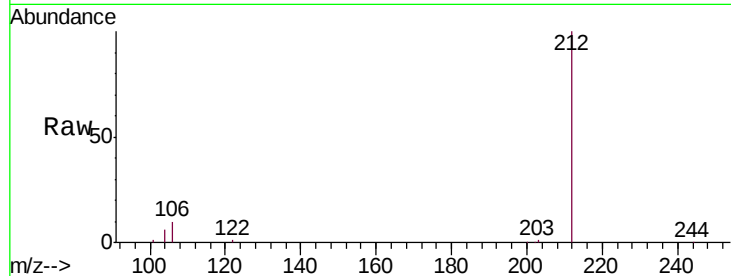

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

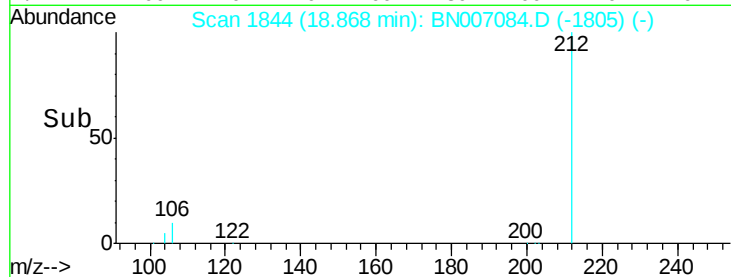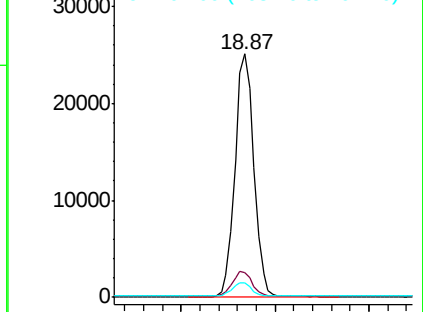

#26

Chrysene-d12

Concen: 0.400 ng

RT: 21.05 min Scan# 2171

Delta R.T. -0.01 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26


Tgt Ion:240 Resp: 54625

Ion Ratio Lower Upper

240 100

120 5.1 4.0 6.0



236 26.5 21.3 31.9




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

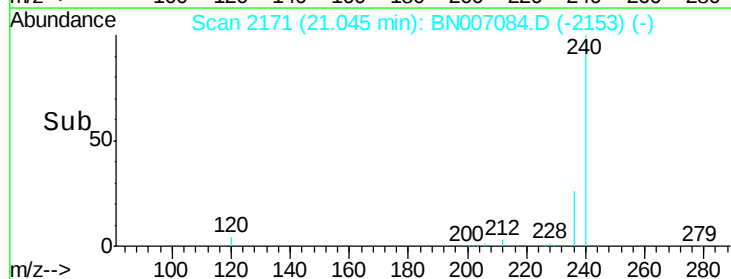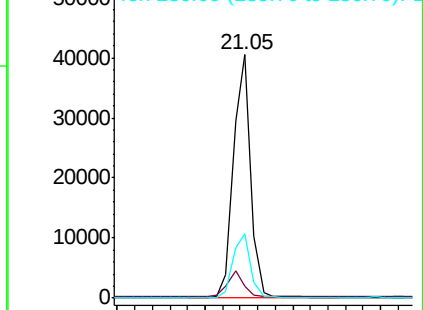

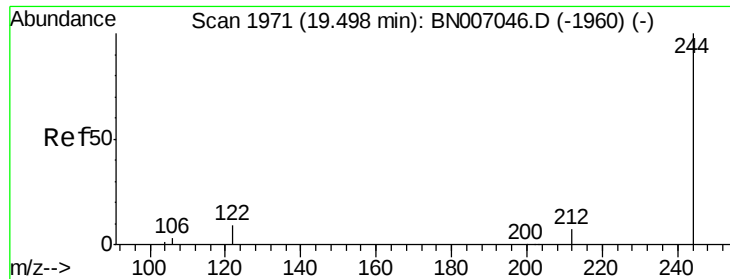

#28

Terphenyl-d14

Concen: 0.170 ng

RT: 19.49 min Scan# 1969

Delta R.T. -0.01 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26

Instrument :

BNA_N

ClientSampleId :

EXT-004-SW072-073019


Tgt Ion:244 Resp: 25381

Ion Ratio Lower Upper

244 100

212 7.8 6.2 9.2




122 10.6 7.4 11.2

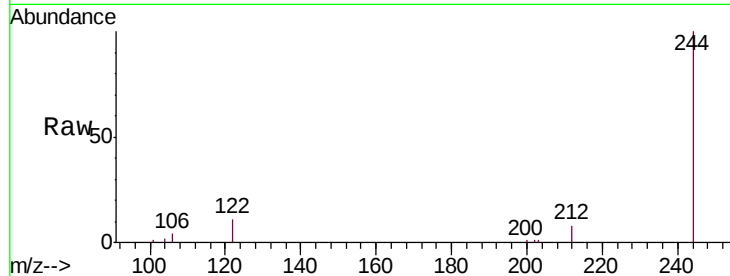

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

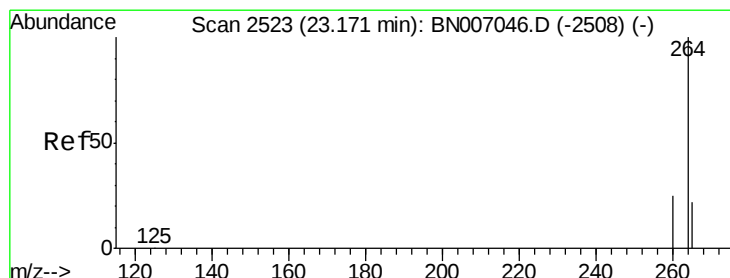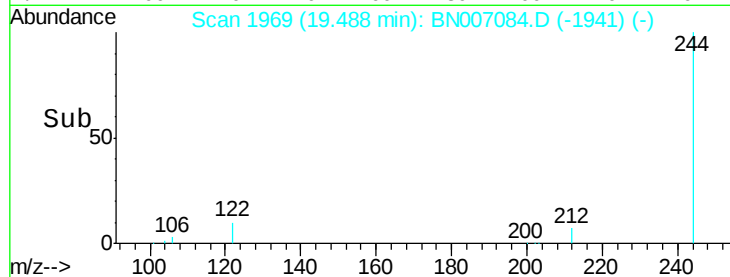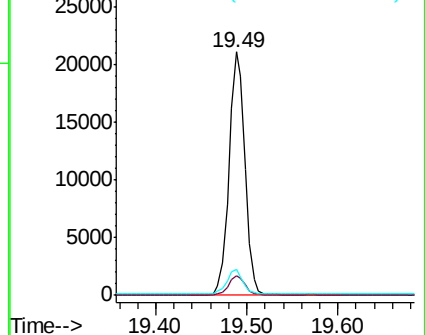

#32

Perylene-d12

Concen: 0.400 ng

RT: 23.16 min Scan# 2519

Delta R.T. -0.01 min

Lab File: BN007084.D

Acq: 11 Aug 2019 13:26


Tgt Ion:264 Resp: 58870

Ion Ratio Lower Upper

264 100

260 24.6 19.8 29.8

265 28.5 26.2 39.4

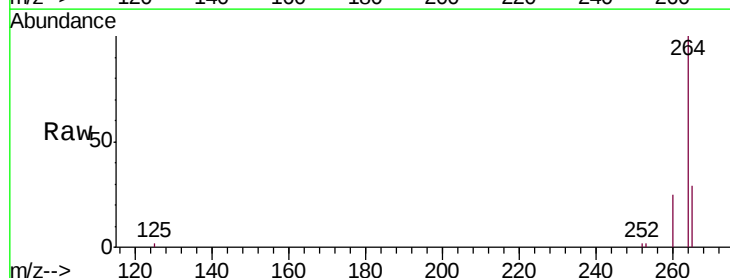

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

