


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
Data File : BN007043.D
Acq On : 10 Aug 2019 08:10
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 10 21:44:50 2019

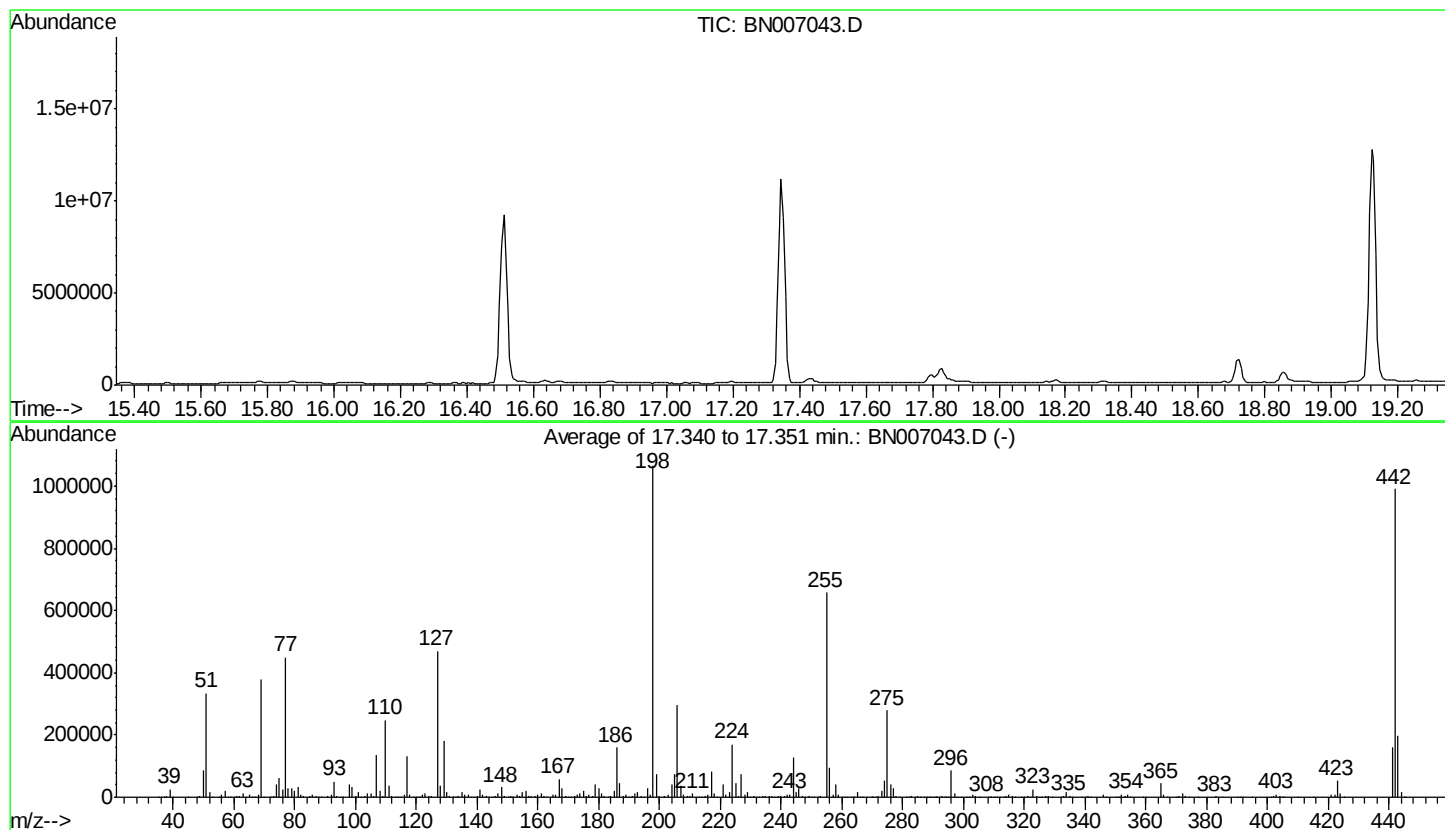

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	333498	PASS
68	69	0.00	2	1.9	7200	PASS
69	198	0.00	100	35.3	376613	PASS
70	69	0.00	2	0.2	767	PASS
127	198	10	80	44.2	470649	PASS
197	198	0.00	2	0.6	6427	PASS
198	198	100	100	100.0	1065685	PASS
199	198	5	9	6.9	73632	PASS
275	198	10	60	26.2	279488	PASS
365	198	1	100	4.1	43466	PASS
441	198	0.01	100	15.1	160861	PASS
442	198	50	100	92.9	989866	PASS
443	442	15	24	19.9	196589	PASS