


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
 Data File : BN007053.D
 Acq On : 10 Aug 2019 18:11
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 10 21:44:50 2019

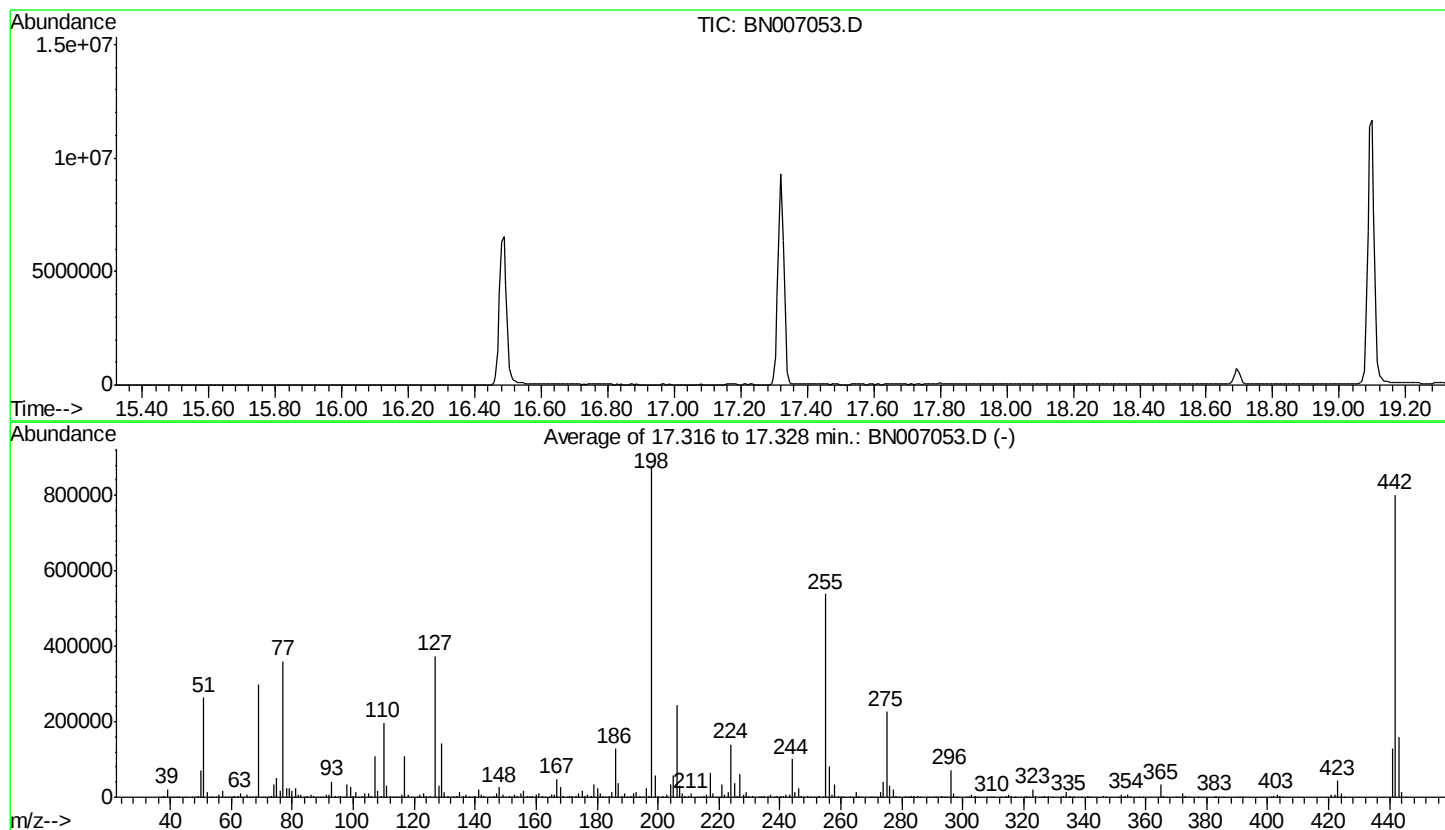

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2429

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	264573	PASS
68	69	0.00	2	1.7	5164	PASS
69	198	0.00	100	34.1	299851	PASS
70	69	0.00	2	0.4	1261	PASS
127	198	10	80	42.5	373696	PASS
197	198	0.00	2	0.5	4228	PASS
198	198	100	100	100.0	879082	PASS
199	198	5	9	6.8	59362	PASS
275	198	10	60	25.8	226922	PASS
365	198	1	100	3.8	33722	PASS
441	198	0.01	100	14.6	127962	PASS
442	198	50	100	91.3	802218	PASS
443	442	15	24	19.7	158093	PASS