


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081019\
 Data File : BN007072.D
 Acq On : 11 Aug 2019 05:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 10 21:44:50 2019

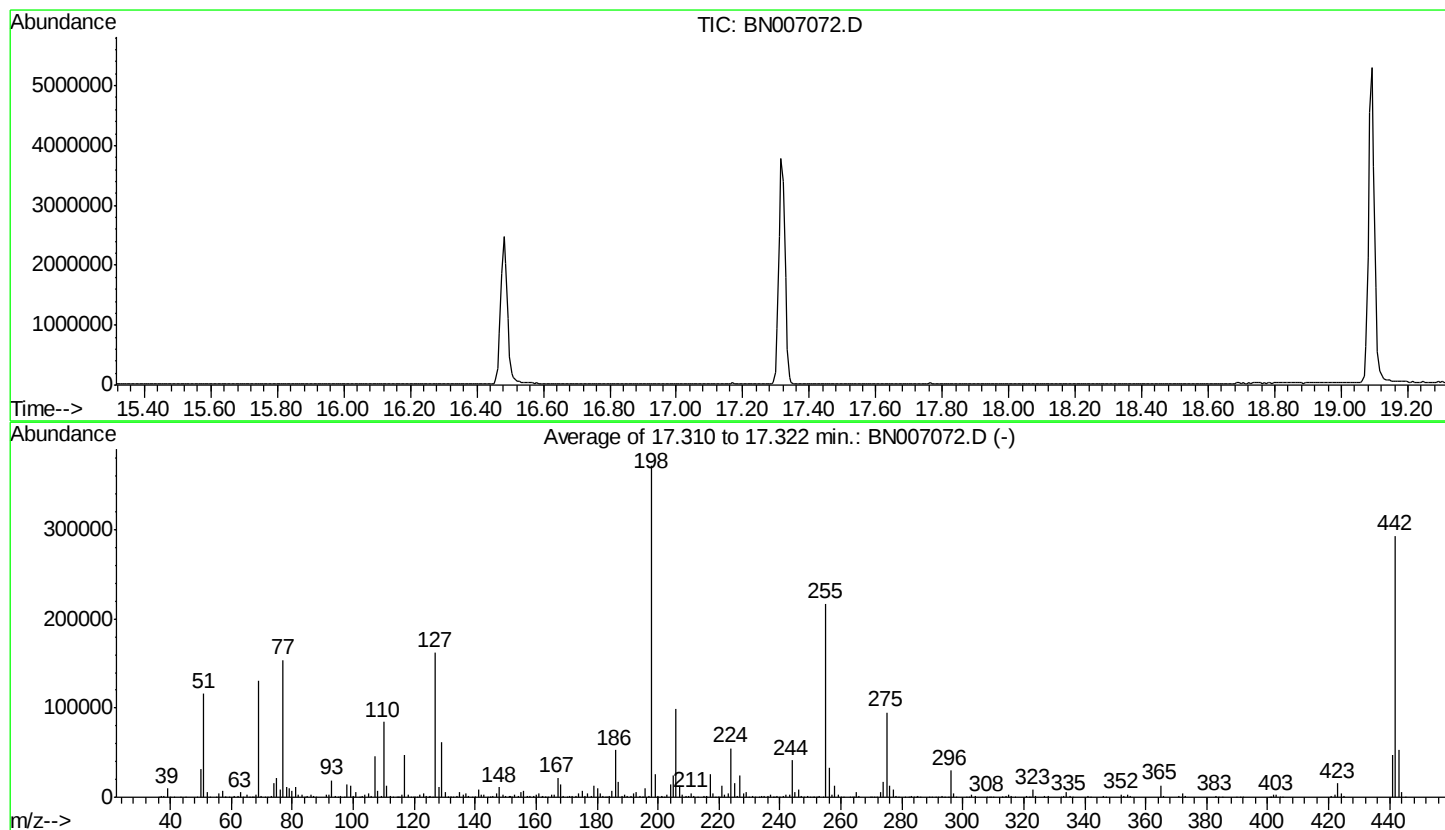

AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2429

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	115684	PASS
68	69	0.00	2	1.9	2526	PASS
69	198	0.00	100	35.1	130510	PASS
70	69	0.00	2	0.6	797	PASS
127	198	10	80	43.6	162218	PASS
197	198	0.00	2	0.5	2016	PASS
198	198	100	100	100.0	371925	PASS
199	198	5	9	7.0	26016	PASS
275	198	10	60	25.6	95093	PASS
365	198	1	100	3.6	13451	PASS
441	198	0.01	100	12.7	47218	PASS
442	198	50	100	78.8	292949	PASS
443	442	15	24	18.2	53341	PASS