
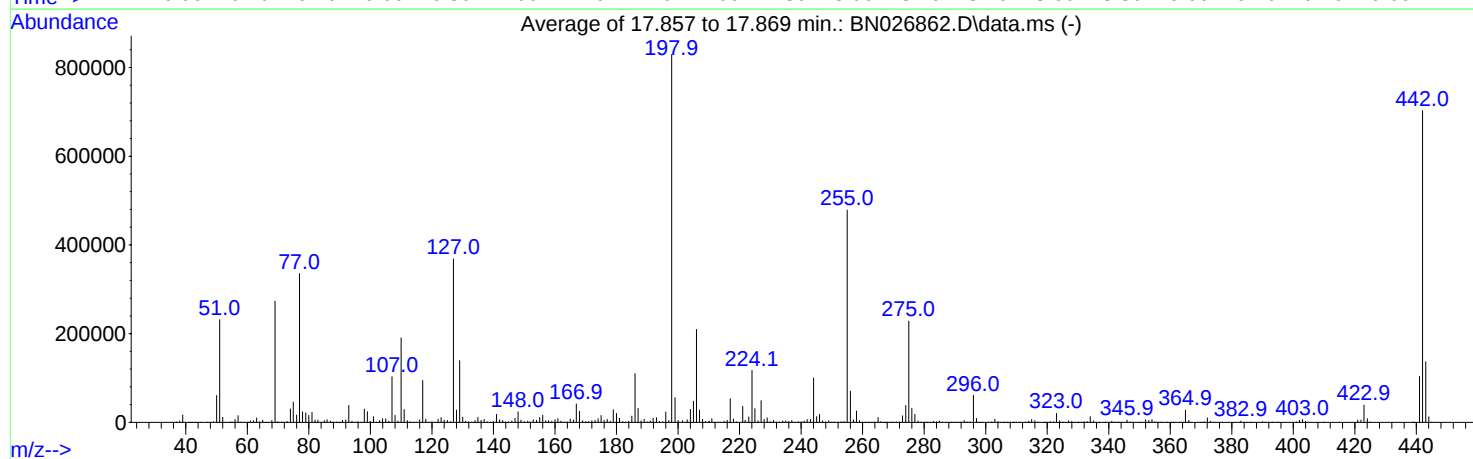


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081023\
 Data File : BN026862.D
 Acq On : 09 Aug 2023 07:50
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 09 17:55:32 2023

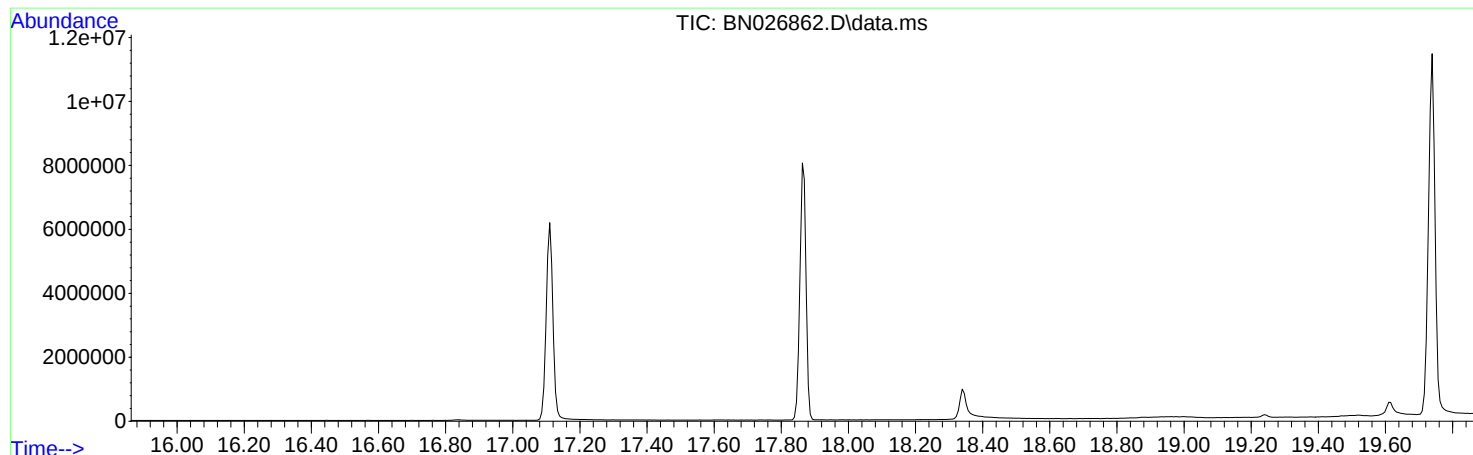




AutoFind: Scans 2545, 2546, 2547; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	231622	PASS
68	69	0.00	2	1.7	4530	PASS
69	198	0.00	100	33.0	273513	PASS
70	69	0.00	2	0.6	1511	PASS
127	198	10	80	44.4	368171	PASS
197	198	0.00	2	0.5	4162	PASS
198	198	100	100	100.0	829291	PASS
199	198	5	9	6.7	55763	PASS
275	198	10	60	27.5	228352	PASS
365	198	1	100	3.3	27293	PASS
441	198	0.01	100	12.5	103387	PASS
442	442	50	100	100.0	703040	PASS
443	442	15	24	19.4	136635	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081023\
Data File : BN026862.D
Acq On : 09 Aug 2023 07:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 08:38:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 08:38:50 2023
Response via : Initial Calibration

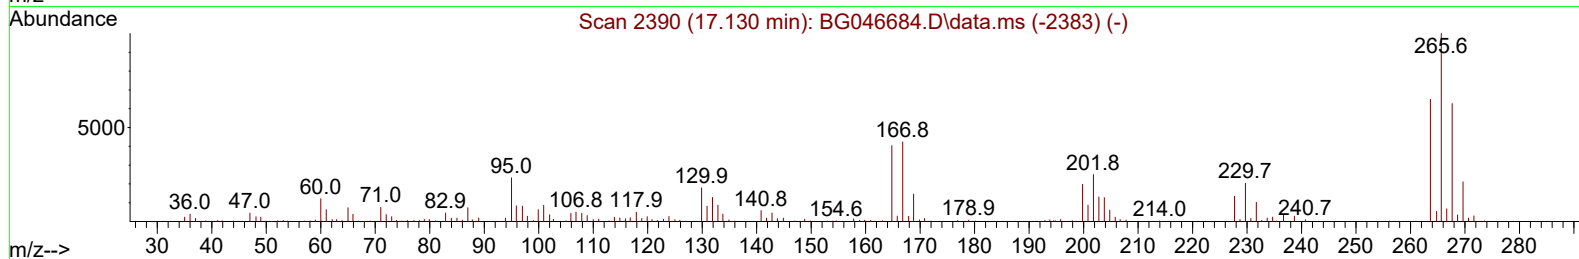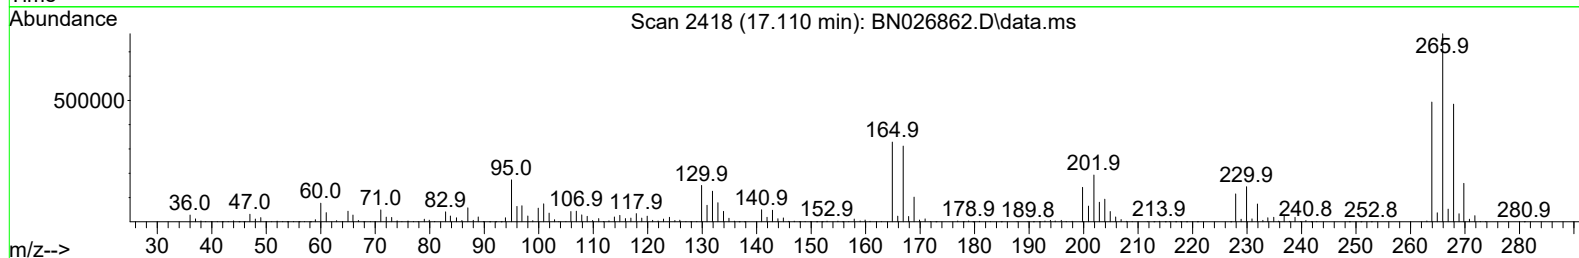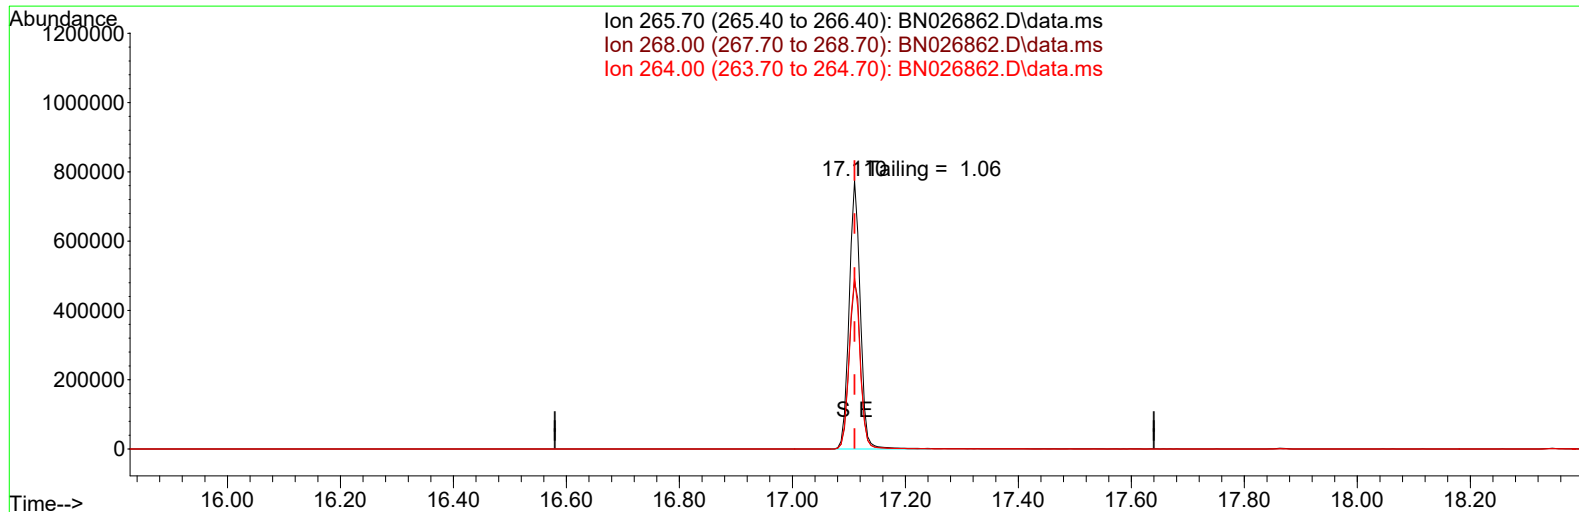

TIC: BN026862.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 27846.22 ng




response 1065116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.53
264.00	61.60	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081023\
Data File : BN026862.D
Acq On : 09 Aug 2023 07:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 09 08:38:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 08:38:50 2023
Response via : Initial Calibration

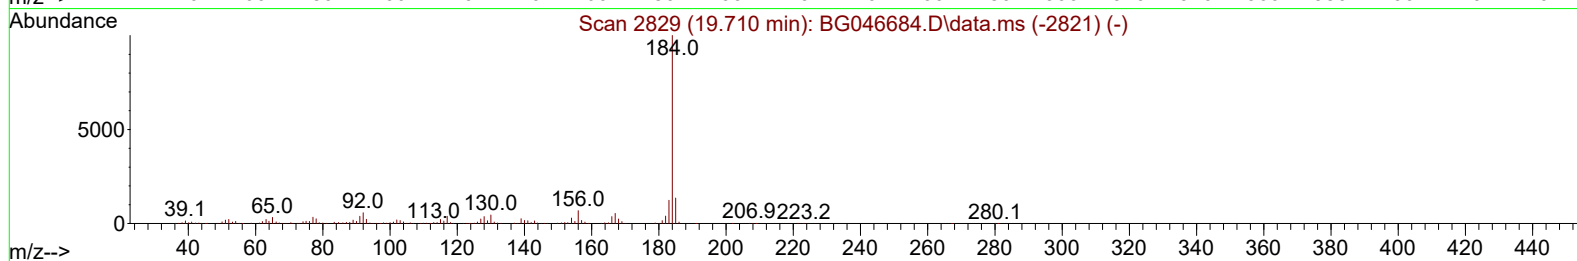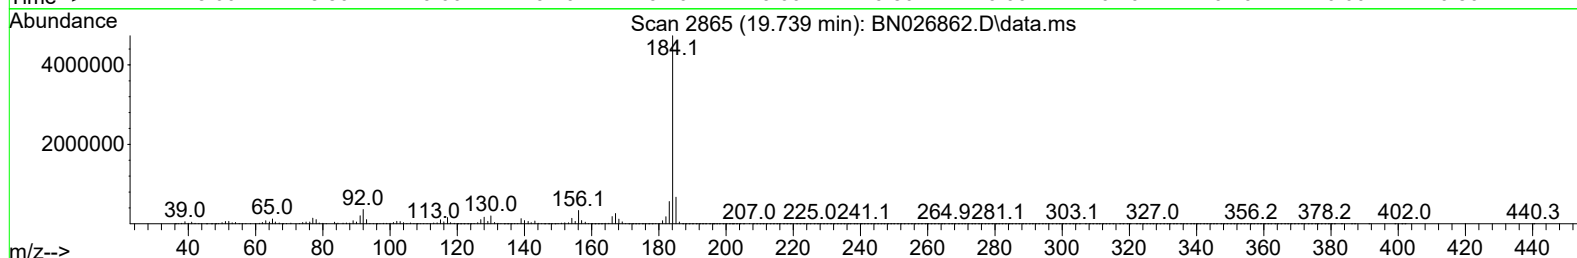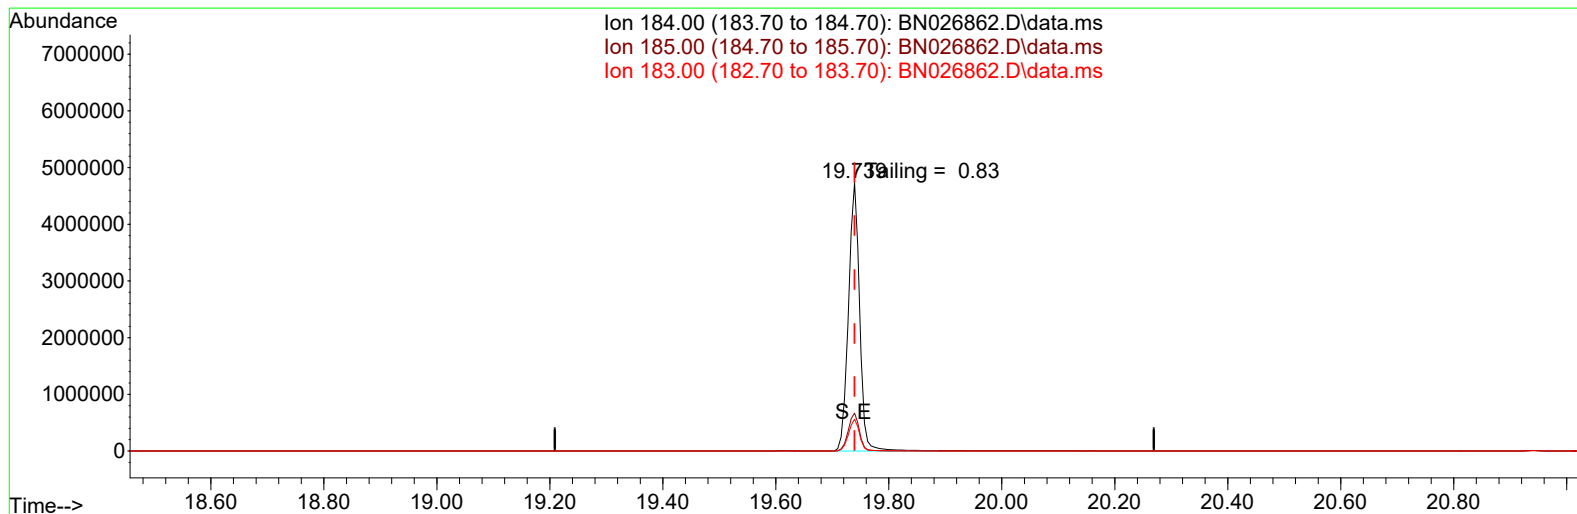

TIC: BN026862.D\data.ms

(77) Benzidine

19.739min (0.000) 447430.77 ng

response 6523720

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_N	<u>BN026862.D</u>
Compound Name	Response	Retention Time
DDT	2896261	20.939
DDD	53908	20.498
DDE	1386	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
55294	2951555	1.87

Instrument :
BNA_N
ClientSampleId :
DFTPP