
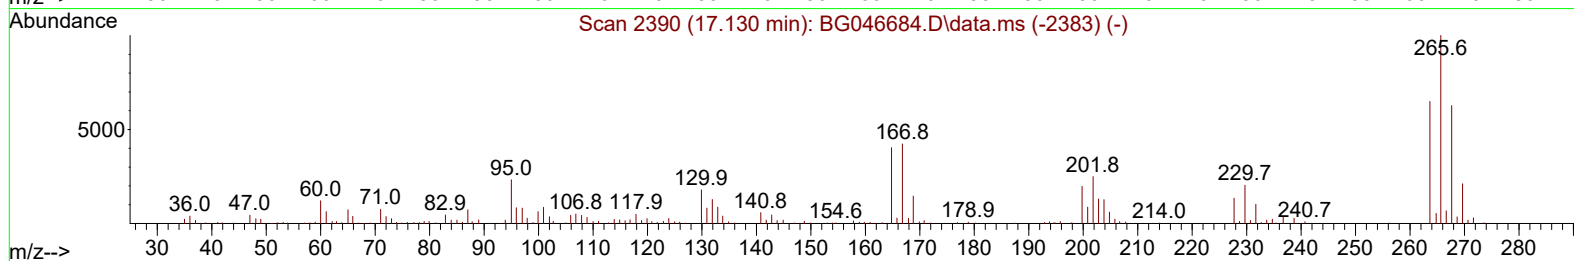
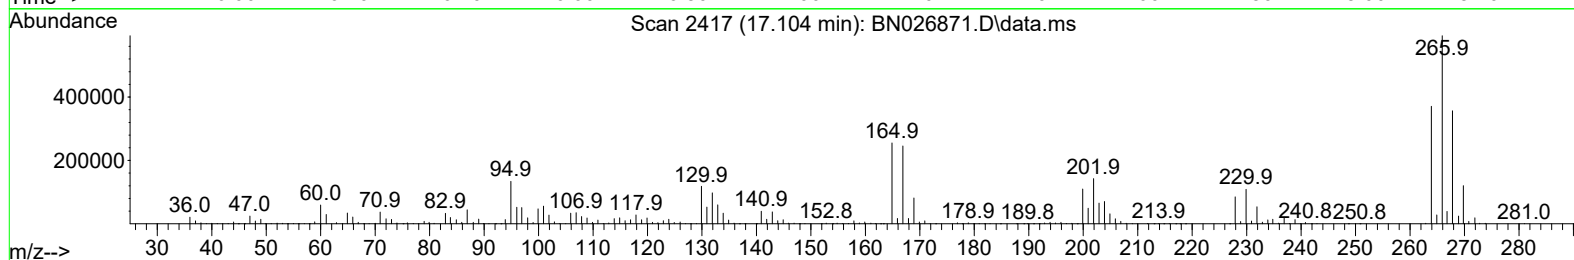


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081123\
Data File : BN026871.D
Acq On : 10 Aug 2023 07:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 02:35:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 02:35:01 2023
Response via : Initial Calibration

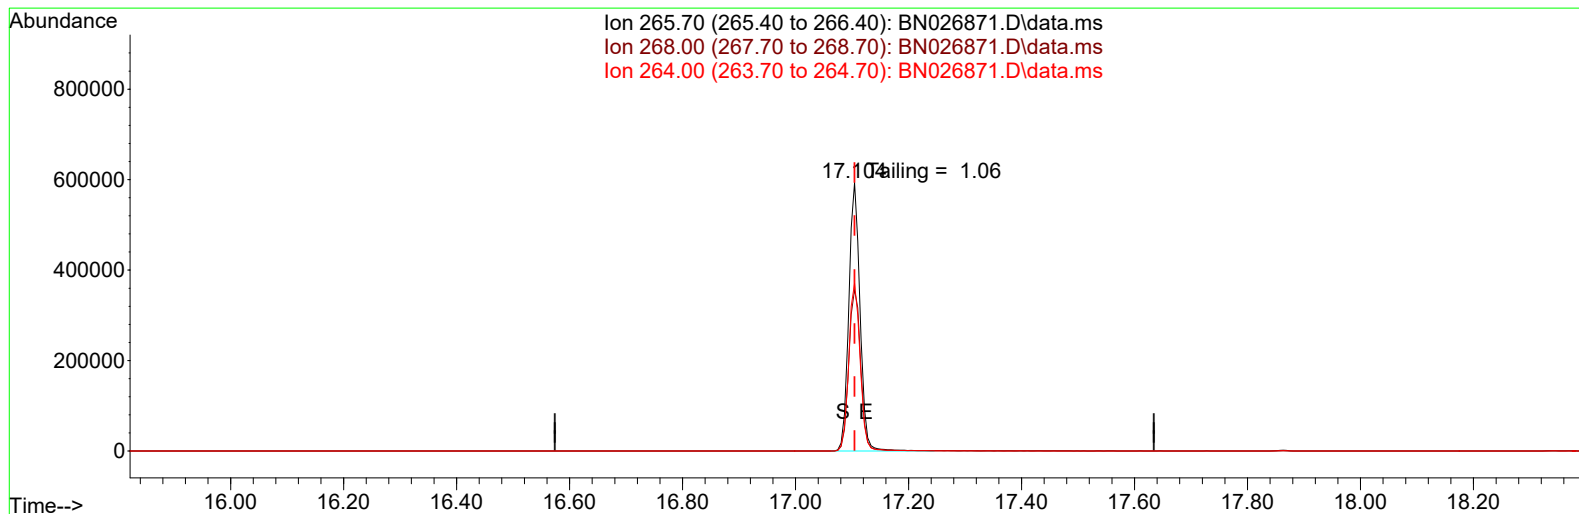

TIC: BN026871.D\data.ms

(70) Pentachlorophenol (C)




17.104min (0.000) 27201.62 ng

response 821865

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.08
264.00	61.60	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081123\
Data File : BN026871.D
Acq On : 10 Aug 2023 07:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 02:35:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 02:35:01 2023
Response via : Initial Calibration

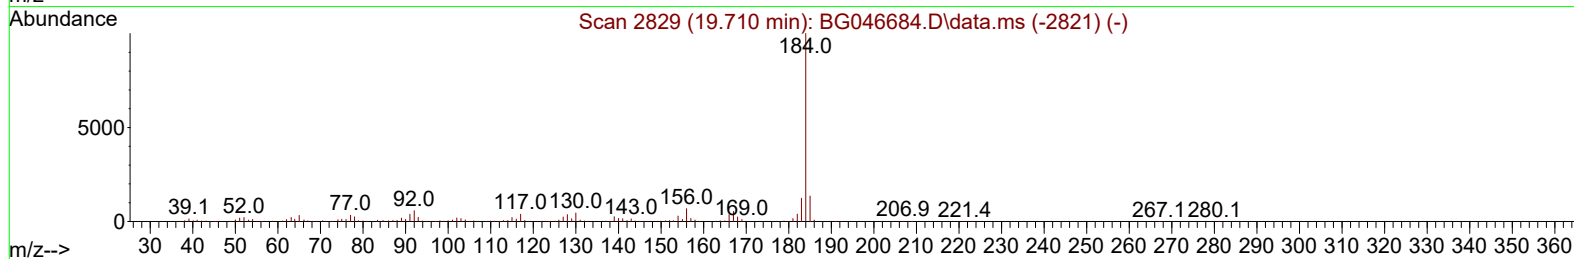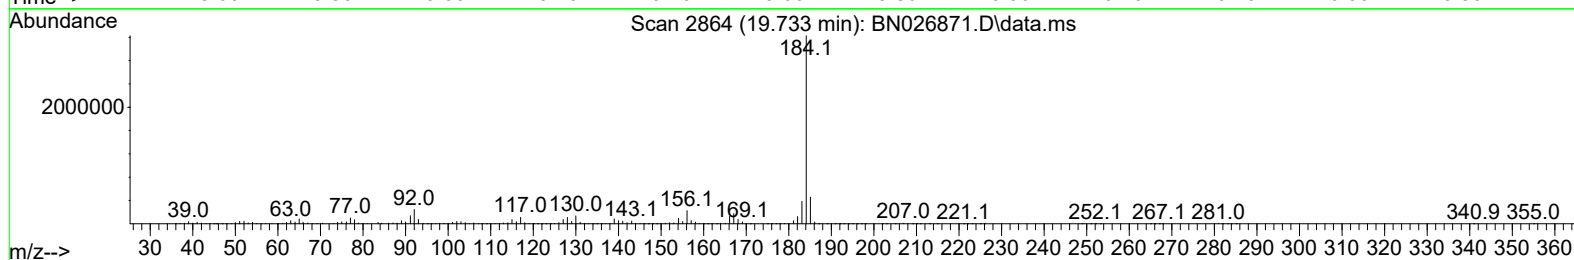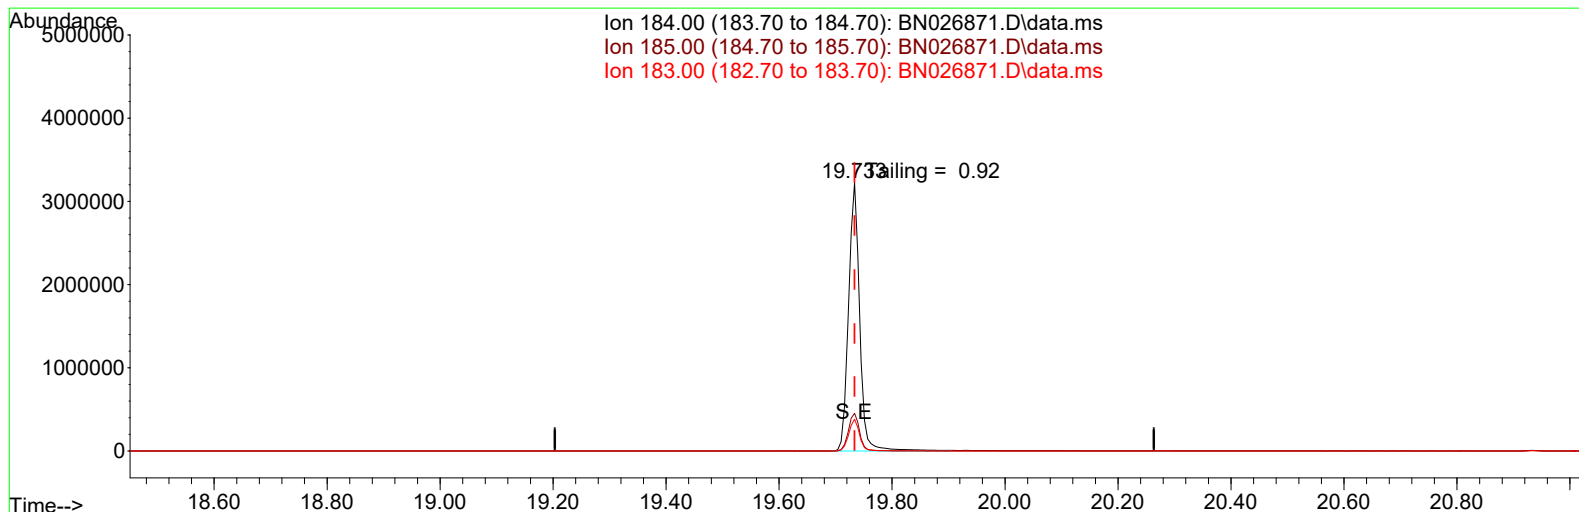

TIC: BN026871.D\data.ms

(77) Benzidine**19.733min (0.000) 2359741.79 ng****response 4437135**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.11
183.00	13.20	11.90
0.00	0.00	0.00