

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081222\
 Data File : BN021197.D
 Acq On : 13 Aug 2022 05:29
 Operator : CG/JU
 Sample : N4165-12
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBY4

Quant Time: Aug 13 06:12:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 13 04:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	3540	0.400	ng/ul	0.00
4) Naphthalene-d8	10.574	136	11241	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.434	164	6949	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.184	188	15463	0.400	ng/ul	0.00
17) Chrysene-d12	21.395	240	10561	0.400	ng/ul	0.00
23) Perylene-d12	23.716	264	10244	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.190	96	23192	5.121	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	6049	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.226	212	16592	0.509	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	438	0.094	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081222\
Data File : BN021197.D
Acq On : 13 Aug 2022 05:29
Operator : CG/JU
Sample : N4165-12
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBY4

Quant Time: Aug 13 06:12:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 04:02:44 2022
Response via : Initial Calibration

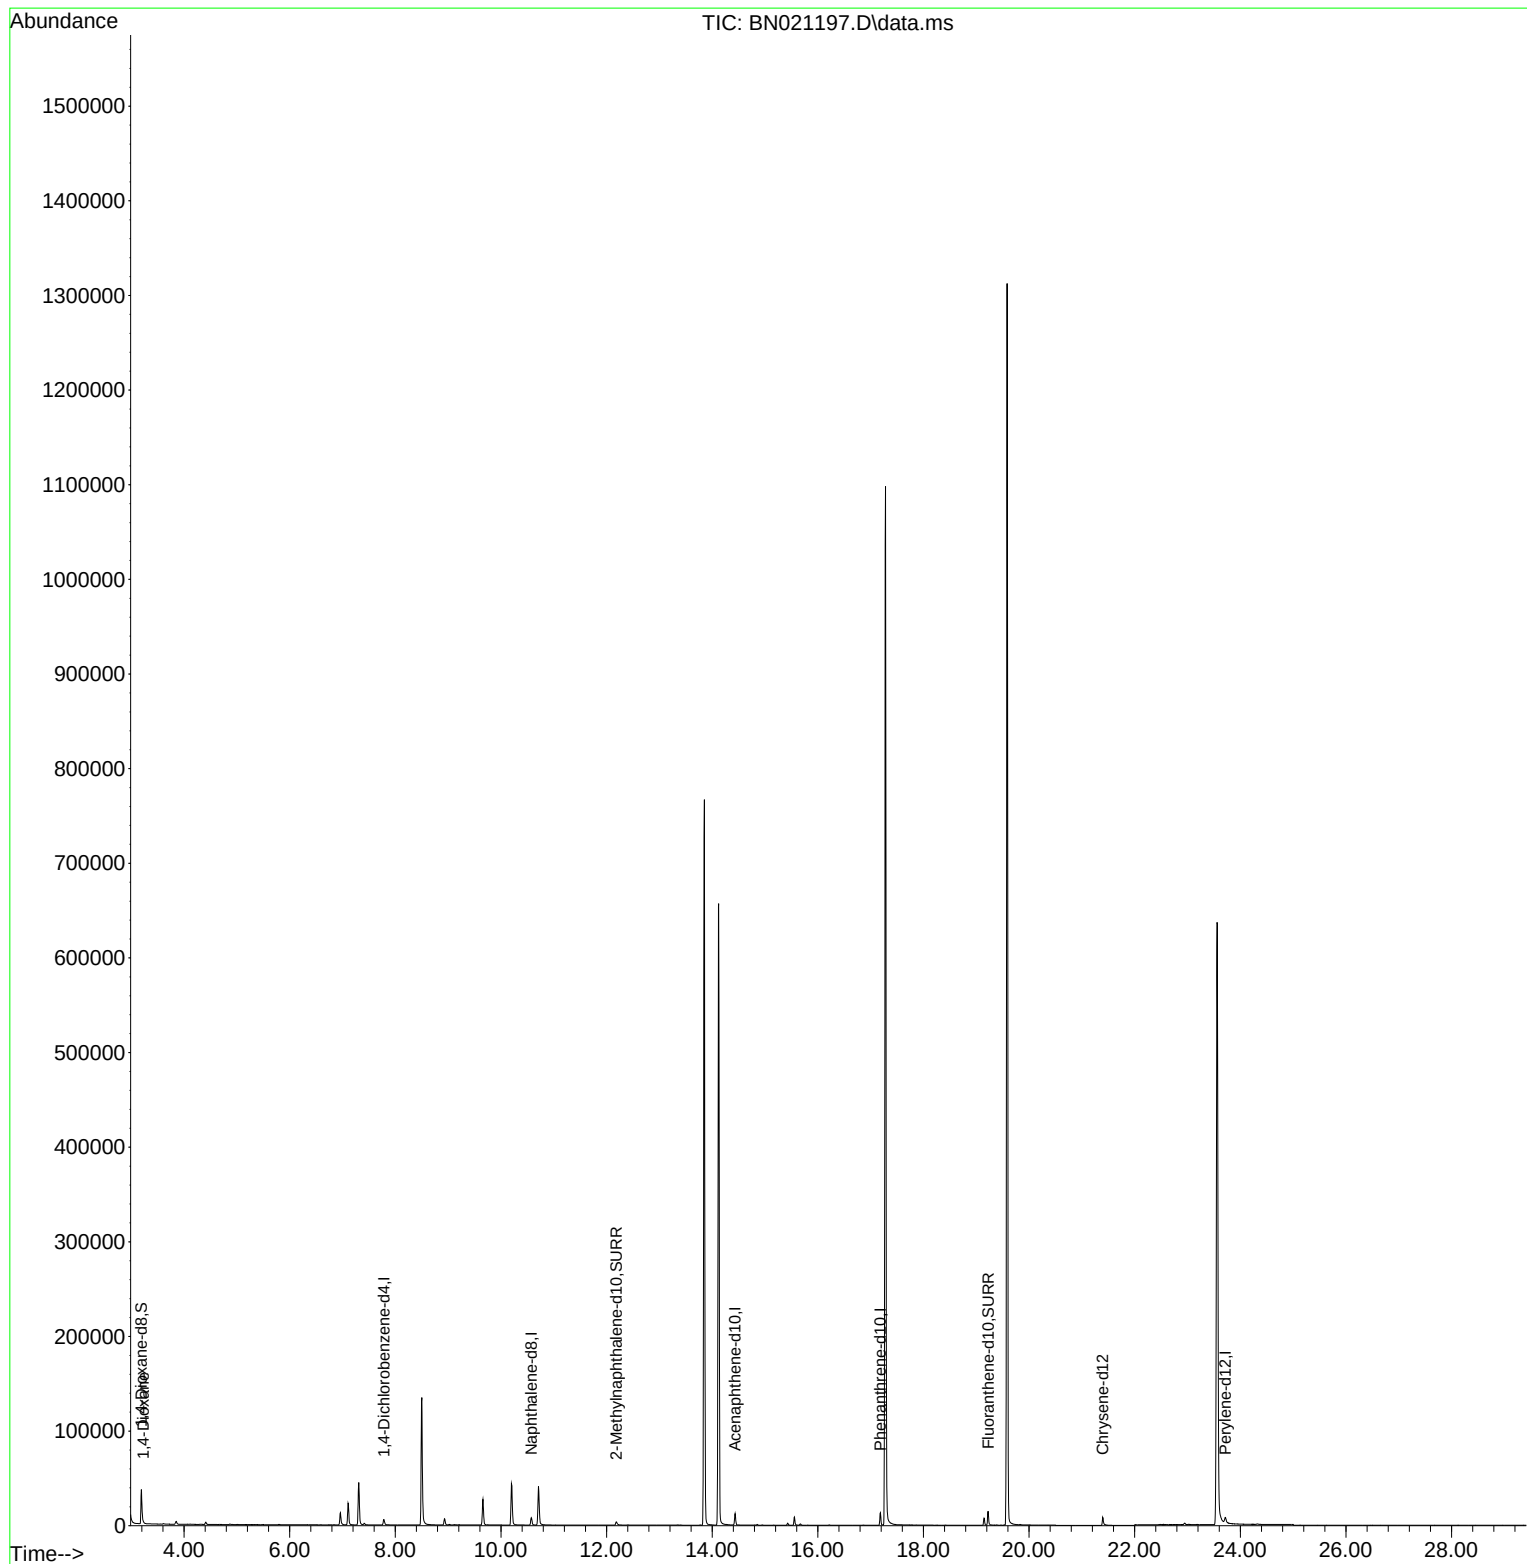

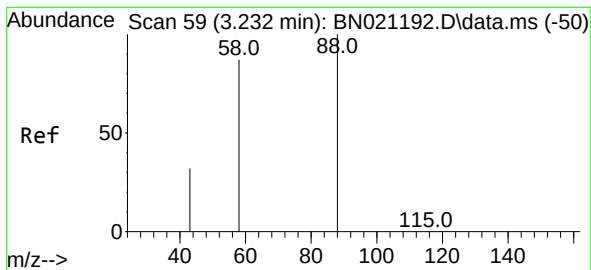

#2

1,4-Dioxane

Concen: 0.094 ng/ul

RT: 3.228 min Scan# 51

Delta R.T. -0.004 min

Lab File: BN021197.D

Acq: 13 Aug 2022 05:29

Instrument :

BNA_N

ClientSampleId :

BGBY4

Tgt Ion: 88 Resp: 438

Ion Ratio Lower Upper

88 100

43 29.6 31.4 47.0#

58 18.6 49.0 73.6#

