

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081222\
 Data File : BN021203.D
 Acq On : 13 Aug 2022 09:06
 Operator : CG/JU
 Sample : N4165-18
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBZ0

Quant Time: Aug 14 23:02:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 13 04:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	3923	0.400	ng/ul	0.00
4) Naphthalene-d8	10.573	136	11785	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.432	164	7070	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.183	188	15561	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	10245	0.400	ng/ul	0.00
23) Perylene-d12	23.716	264	9911	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.190	96	18629	3.712	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.190	152	4612	0.267	ng/ul	0.00
18) Fluoranthene-d10	19.225	212	13714	0.433	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	319	0.062	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081222\
Data File : BN021203.D
Acq On : 13 Aug 2022 09:06
Operator : CG/JU
Sample : N4165-18
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBZ0


Quant Time: Aug 14 23:02:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 04:02:44 2022
Response via : Initial Calibration

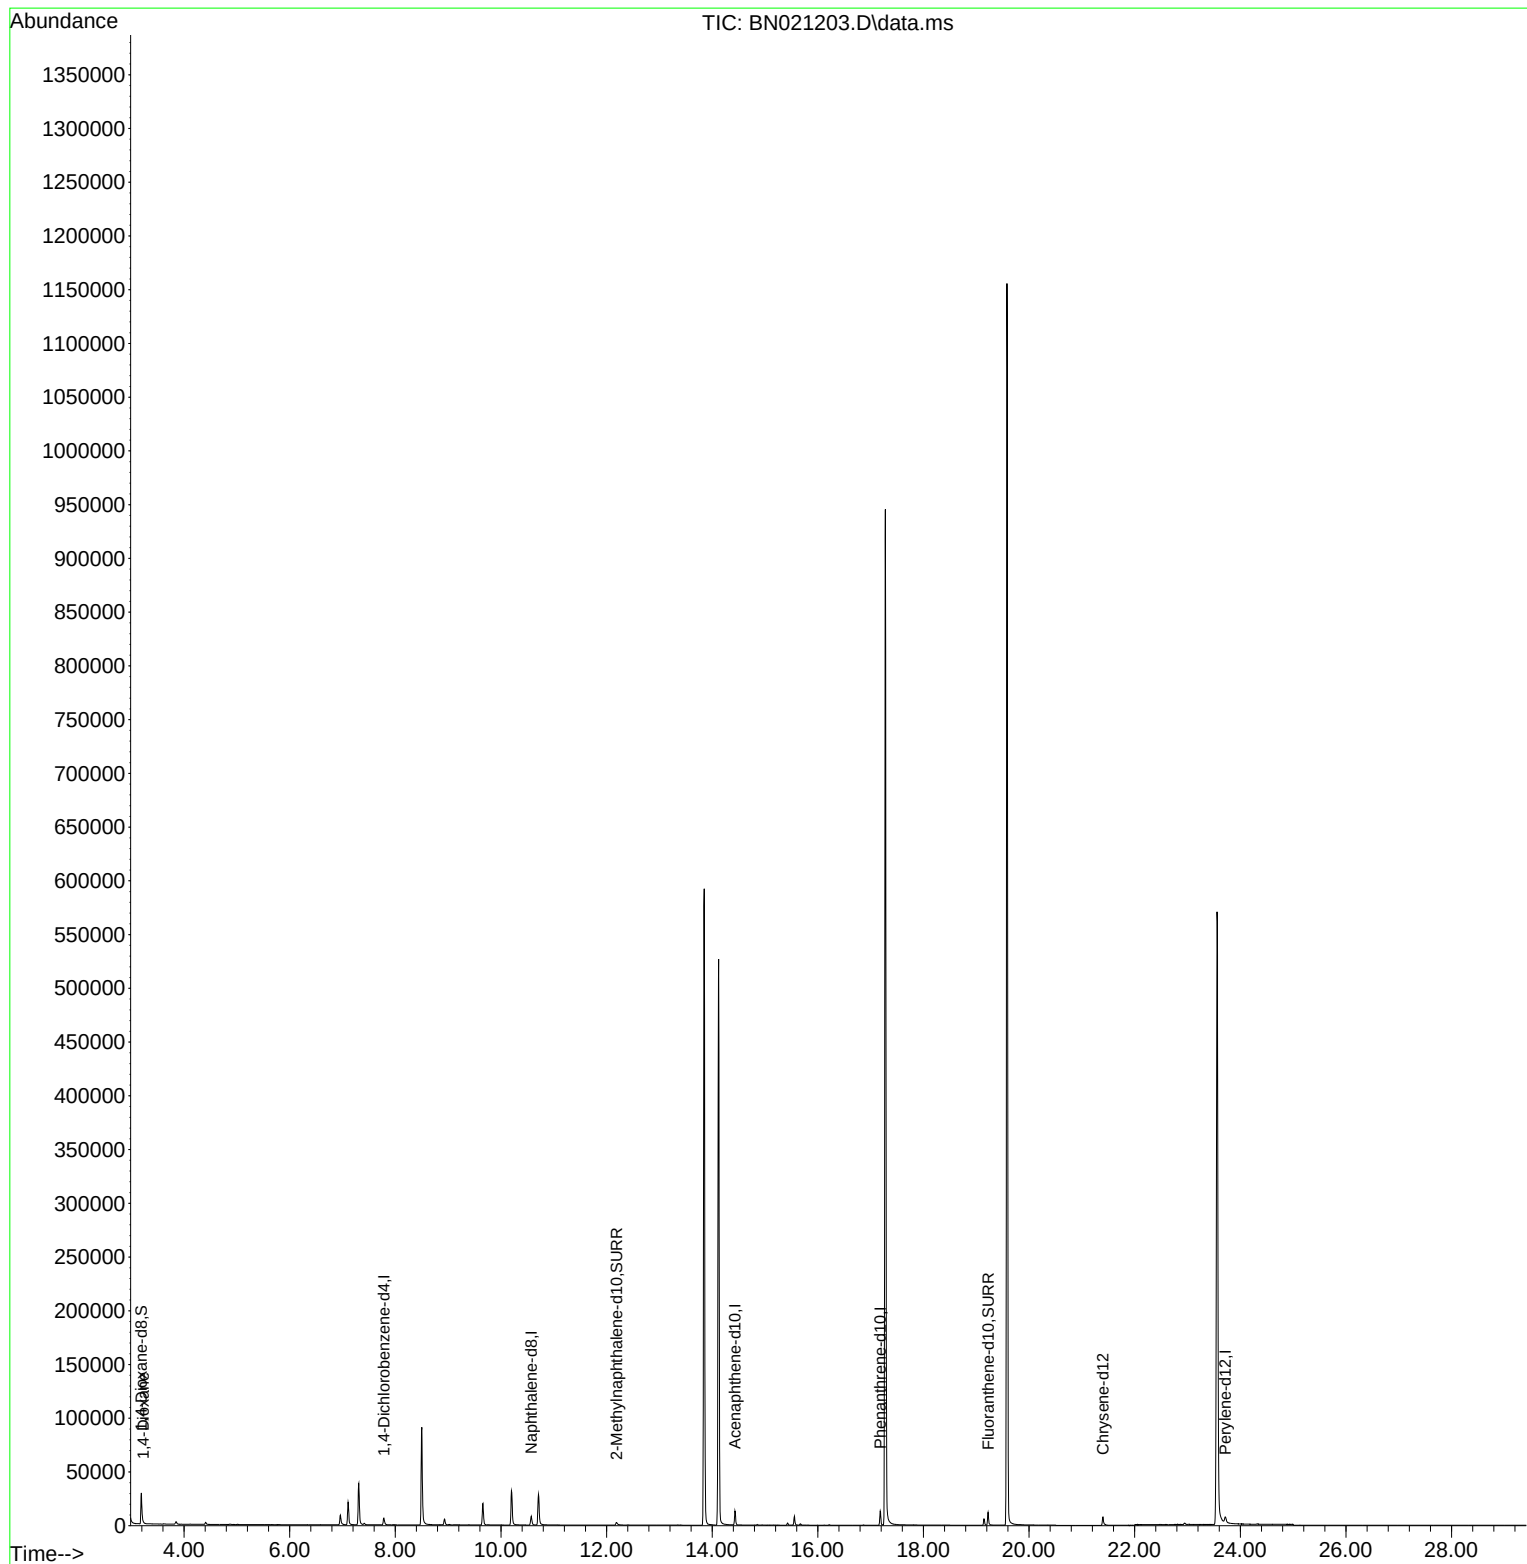

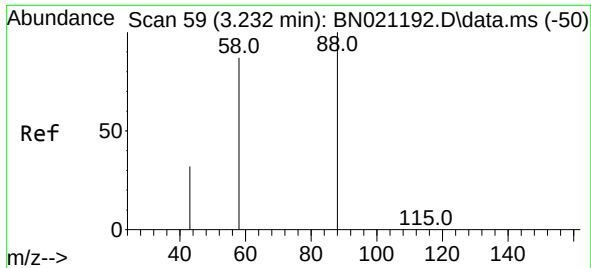

#2
 1,4-Dioxane
 Concen: 0.062 ng/ul
 RT: 3.228 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BN021203.D
 Acq: 13 Aug 2022 09:06

Instrument :
 BNA_N
 ClientSampleId :
 BGBZ0

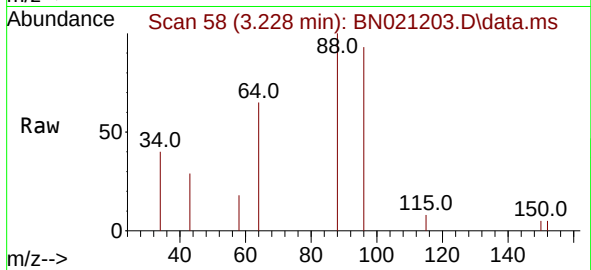

Tgt Ion:	88	Resp:	319
Ion	Ratio	Lower	Upper
88	100		
43	29.2	31.4	47.0#
58	18.4	49.0	73.6#

